

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015687.D
 Acq On : 24 Jun 2023 00:31
 Operator : MA/JU
 Sample : PB153415BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK415

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	43	rVB	52188	68737	2.00%	0.215%
2	3.840	108	111	135	rBV	538740	854319	24.89%	2.677%
3	4.170	165	167	175	rVB2	9522	14099	0.41%	0.044%
4	6.840	617	621	624	rBV6	2392	3777	0.11%	0.012%
5	7.246	683	690	709	rBV	539120	1085385	31.62%	3.401%
6	7.399	710	716	737	rVB	485692	848092	24.71%	2.657%
7	7.605	744	751	767	rBV	672283	1151809	33.56%	3.609%
8	8.075	824	831	846	rBV	428764	761892	22.20%	2.387%
9	8.805	947	955	973	rBV	652035	1304897	38.02%	4.088%
10	8.922	973	975	979	rVB5	3364	5150	0.15%	0.016%
11	9.258	1025	1032	1055	rBV	551973	1058742	30.85%	3.317%
12	9.987	1147	1156	1175	rBV	485287	919728	26.80%	2.882%
13	10.540	1242	1250	1274	rBV	496863	1207798	35.19%	3.784%
14	10.905	1305	1312	1330	rVB	536838	948053	27.62%	2.970%
15	11.057	1330	1338	1364	rBV	443363	1195571	34.83%	3.746%
16	12.522	1579	1587	1588	rBV8	7372	11602	0.34%	0.036%
17	13.610	1766	1772	1778	rVB5	7798	14530	0.42%	0.046%
18	14.134	1854	1861	1876	rBV	1035653	1597510	46.54%	5.005%
19	14.246	1879	1880	1887	rVB7	3805	5494	0.16%	0.017%
20	14.422	1903	1910	1928	rBV	1177109	1902605	55.43%	5.961%
21	14.593	1936	1939	1947	rVB10	2425	5597	0.16%	0.018%
22	14.728	1956	1962	1977	rBV	712343	1049290	30.57%	3.287%
23	14.981	1998	2005	2029	rBV2	141275	567027	16.52%	1.777%
24	15.728	2125	2132	2149	rBV	1259679	2151226	62.67%	6.740%
25	15.875	2151	2157	2170	rBV	274965	558995	16.29%	1.751%
26	17.492	2425	2432	2442	rBV	777198	1170579	34.10%	3.667%
27	17.592	2442	2449	2467	rVV	1395382	2268767	66.10%	7.108%
28	19.392	2753	2755	2761	rVB4	19391	23926	0.70%	0.075%
29	19.816	2821	2827	2840	rBV	1944171	2904602	84.62%	9.100%
30	21.580	3123	3127	3137	rBV	869965	1329430	38.73%	4.165%
31	23.969	3526	3533	3548	rVB2	1516260	3432428	100.00%	10.754%
32	24.139	3556	3562	3573	rVB	662311	1496519	43.60%	4.689%




Sum of corrected areas: 31918176

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015687.D
Acq On : 24 Jun 2023 00:31
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

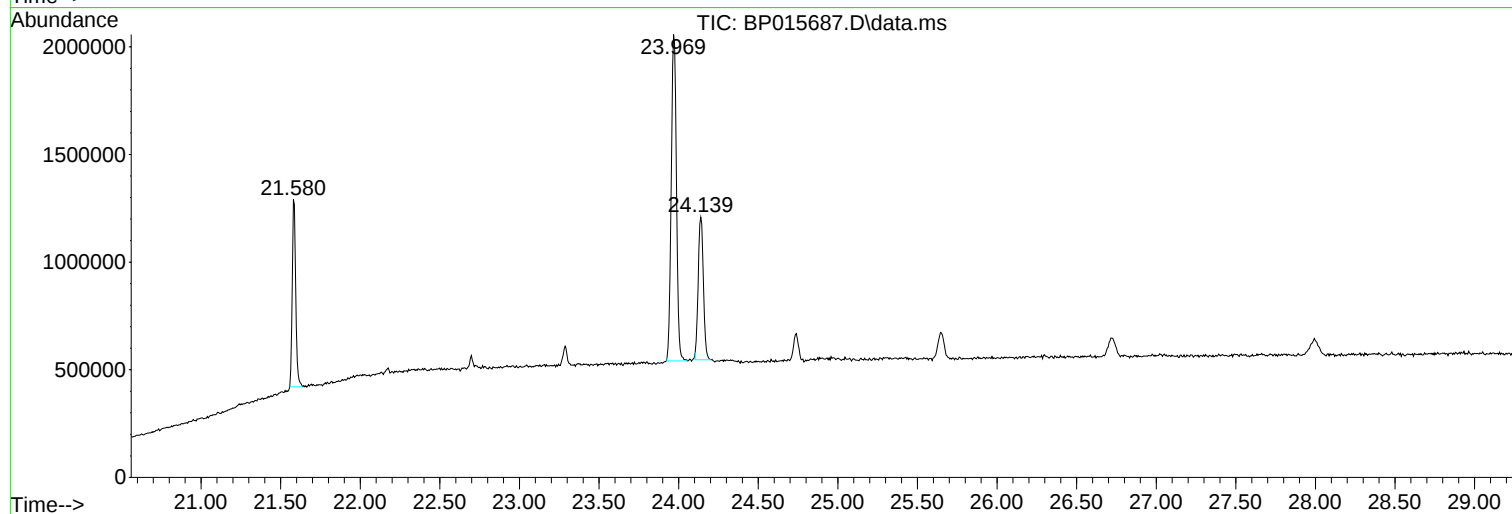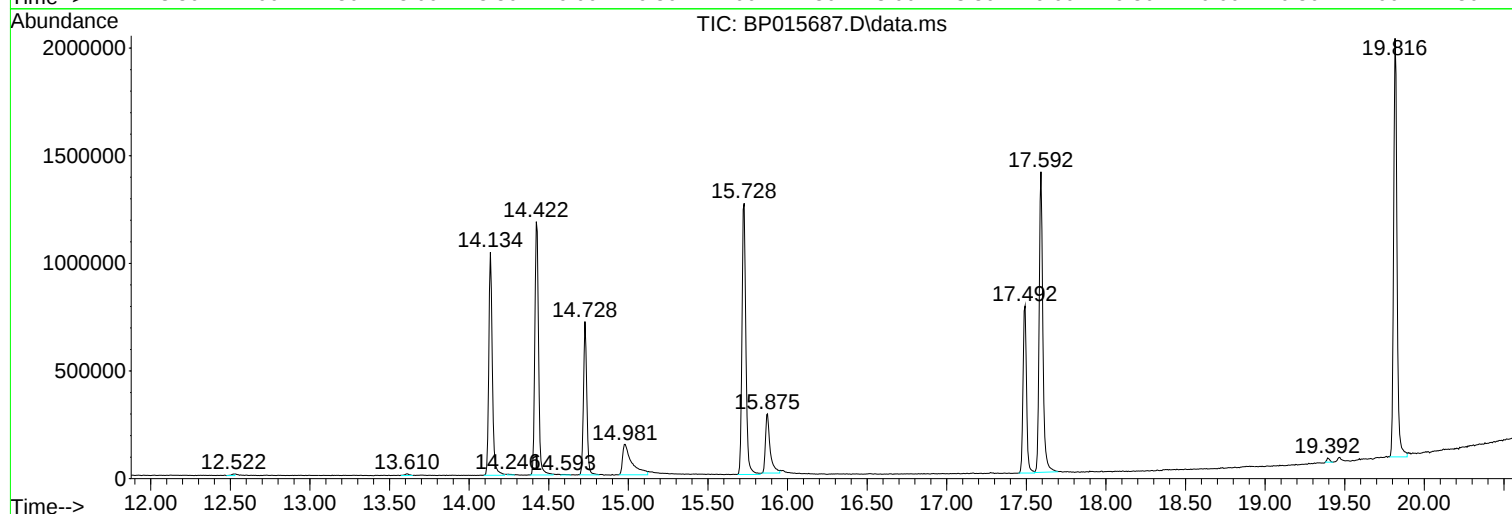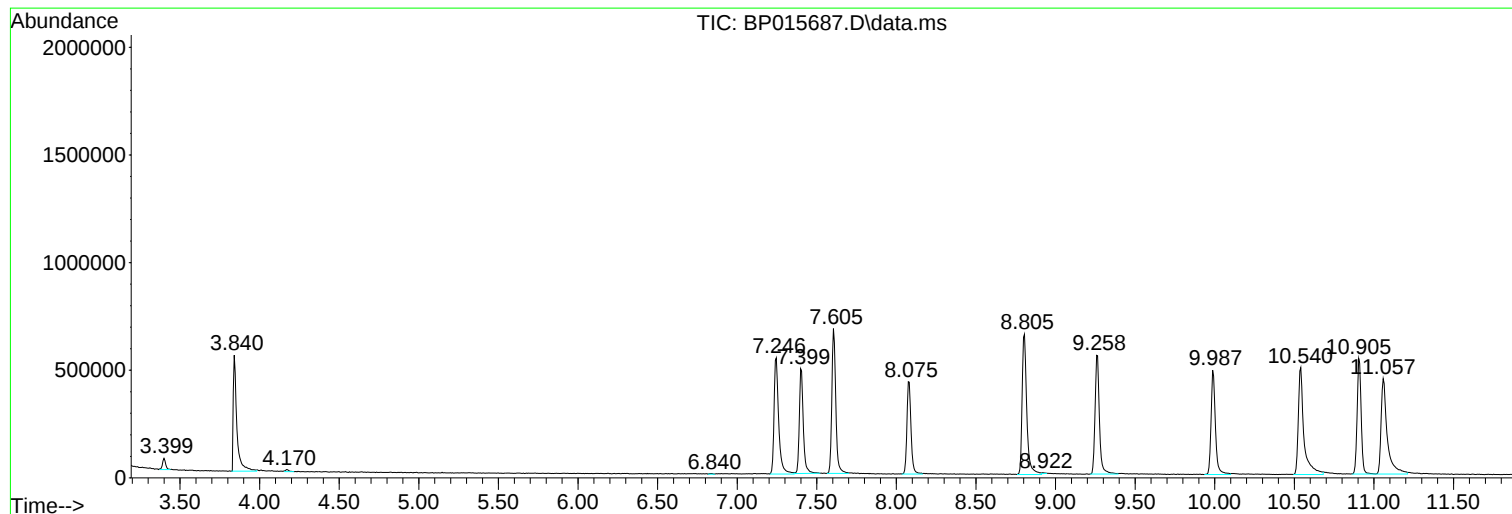

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015687.D
Acq On : 24 Jun 2023 00:31
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015687.D
Acq On : 24 Jun 2023 00:31
Operator : MA/JU
Sample : PB153415BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc