

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
 Data File : BP015702.D
 Acq On : 24 Jun 2023 11:12
 Operator : MA/JU
 Sample : PB153446BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	42	rVB	52033	71396	1.81%	0.186%
2	3.840	108	111	131	rBV	520962	883724	22.46%	2.306%
3	4.164	163	166	172	rVB	9027	13788	0.35%	0.036%
4	7.240	682	689	708	rBV	569422	1135397	28.86%	2.963%
5	7.399	710	716	732	rVB	508592	858495	21.82%	2.240%
6	7.605	744	751	772	rVB	710126	1216870	30.93%	3.175%
7	8.075	824	831	843	rBV	480324	834071	21.20%	2.176%
8	8.799	947	954	974	rBV	715275	1421462	36.13%	3.709%
9	9.257	1025	1032	1052	rBV	616755	1163218	29.57%	3.035%
10	9.987	1149	1156	1170	rBV	533239	1004414	25.53%	2.621%
11	10.534	1242	1249	1274	rBV	559098	1385549	35.22%	3.615%
12	10.904	1304	1312	1326	rBV	629111	1100876	27.98%	2.873%
13	11.057	1328	1338	1365	rBV	523823	1370882	34.85%	3.577%
14	11.534	1416	1419	1427	rVB9	2074	3945	0.10%	0.010%
15	12.528	1583	1588	1595	rBV5	7768	15028	0.38%	0.039%
16	13.604	1765	1771	1778	rVB3	9322	16737	0.43%	0.044%
17	14.134	1850	1861	1875	rBV	1272989	2012199	51.15%	5.250%
18	14.422	1902	1910	1923	rBV	1511130	2356665	59.91%	6.149%
19	14.728	1955	1962	1979	rVV	886072	1362198	34.63%	3.554%
20	14.969	1996	2003	2023	rBV2	207136	756155	19.22%	1.973%
21	15.722	2124	2131	2150	rBV	1674603	2796183	71.08%	7.296%
22	15.869	2150	2156	2170	rBV	413244	810340	20.60%	2.114%
23	17.163	2373	2376	2381	rVB6	4246	4854	0.12%	0.013%
24	17.486	2425	2431	2442	rBV	1075226	1613537	41.02%	4.210%
25	17.592	2442	2449	2470	rVB	1822665	3002478	76.32%	7.834%
26	19.392	2752	2755	2760	rBV3	24475	34143	0.87%	0.089%
27	19.469	2764	2768	2773	rVB4	23395	38747	0.98%	0.101%
28	19.816	2821	2827	2845	rBV	2396376	3619209	92.00%	9.444%
29	21.586	3123	3128	3138	rBV	1096104	1672376	42.51%	4.364%
30	23.974	3527	3534	3546	rVB2	1757496	3933876	100.00%	10.265%
31	24.145	3556	3563	3574	rVB	793722	1815680	46.15%	4.738%




Sum of corrected areas: 38324492

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015702.D
Acq On : 24 Jun 2023 11:12
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

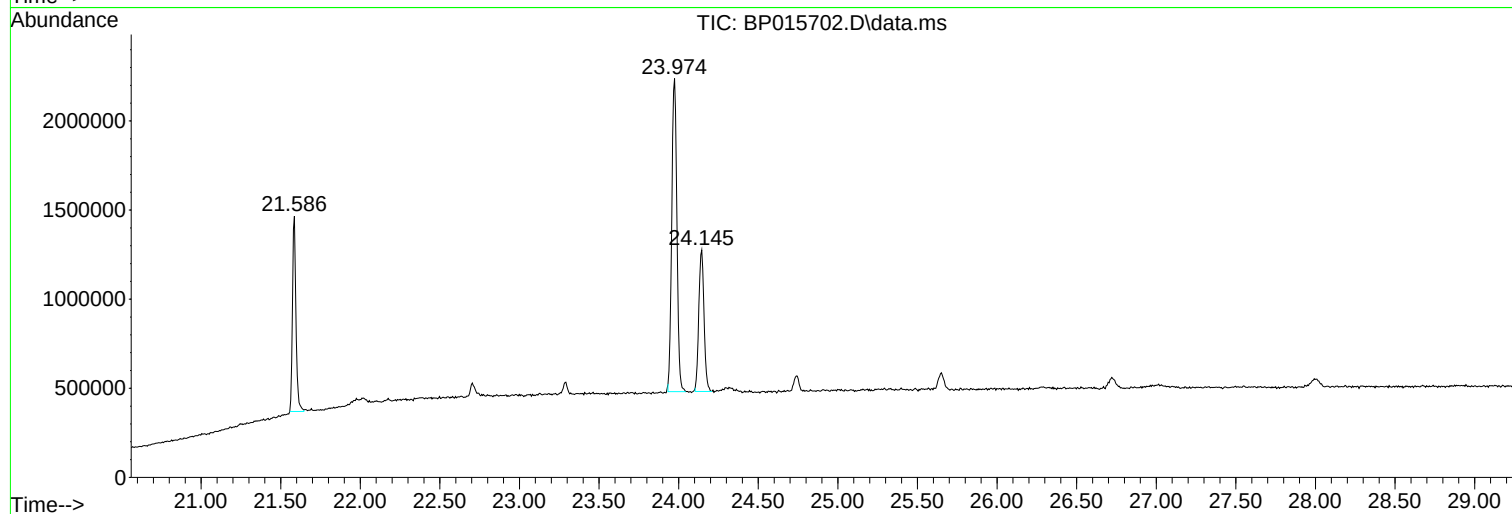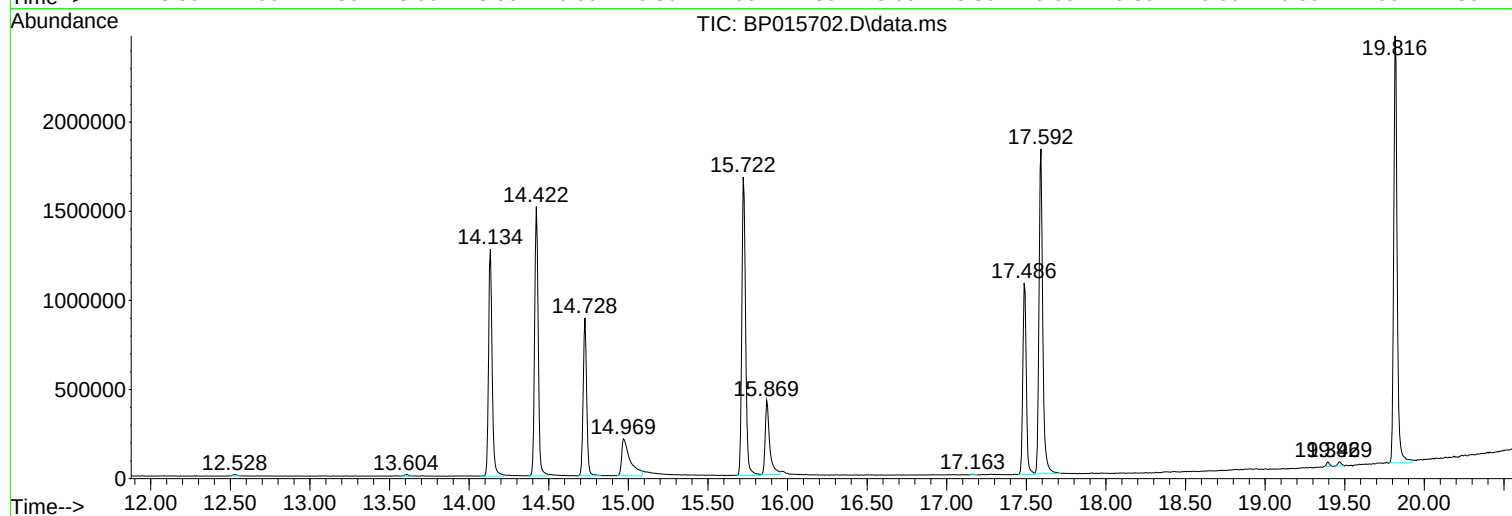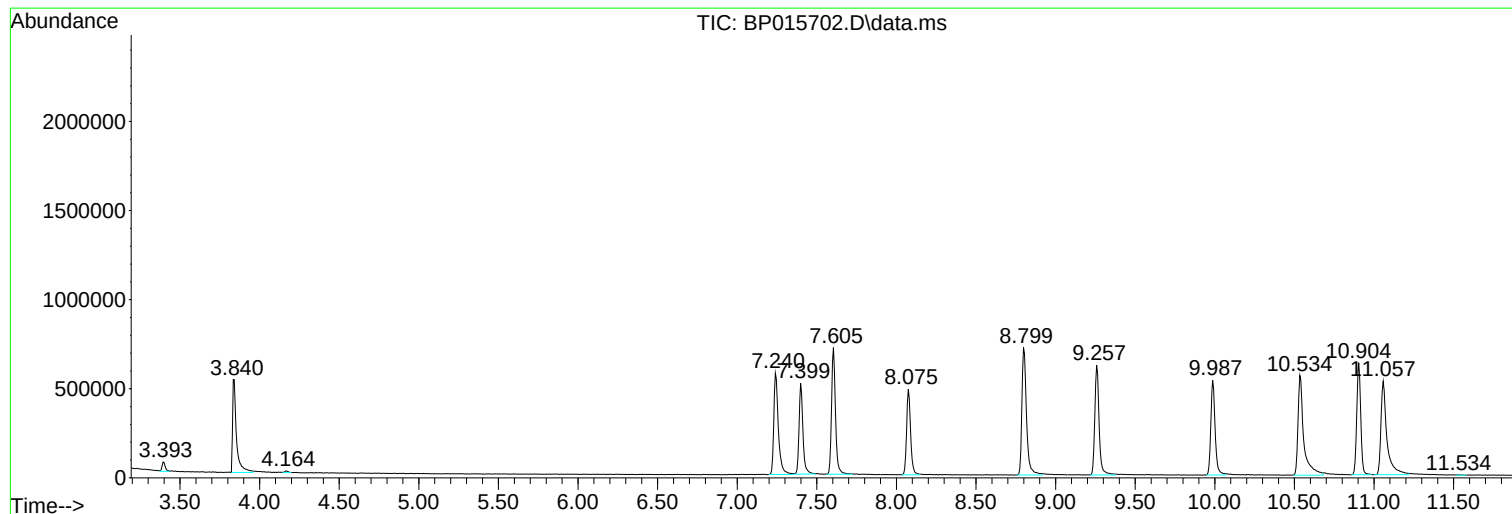

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015702.D
Acq On : 24 Jun 2023 11:12
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062323\
Data File : BP015702.D
Acq On : 24 Jun 2023 11:12
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP060723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------