




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

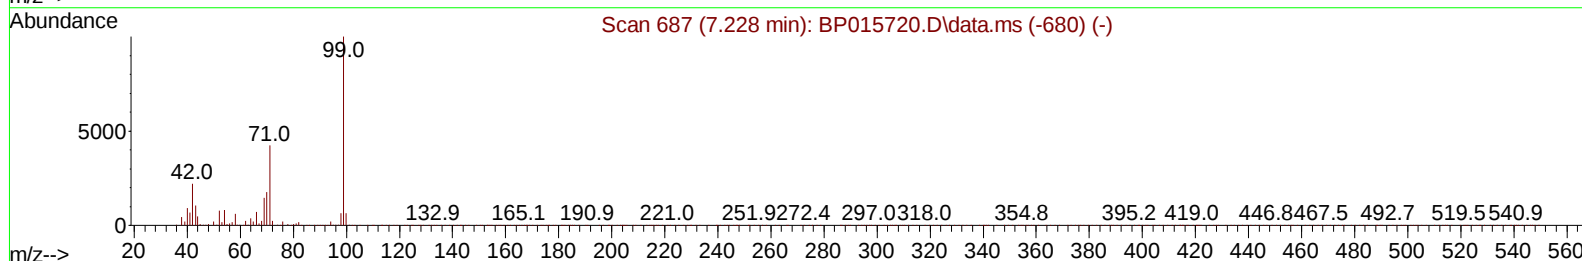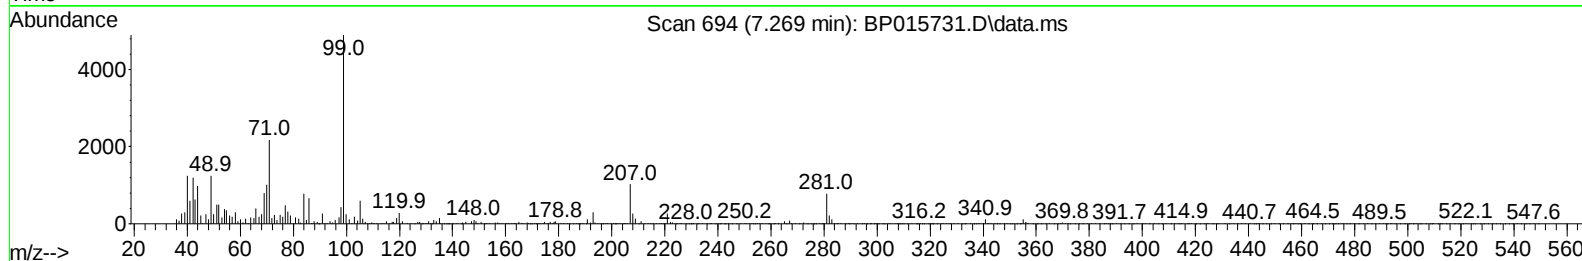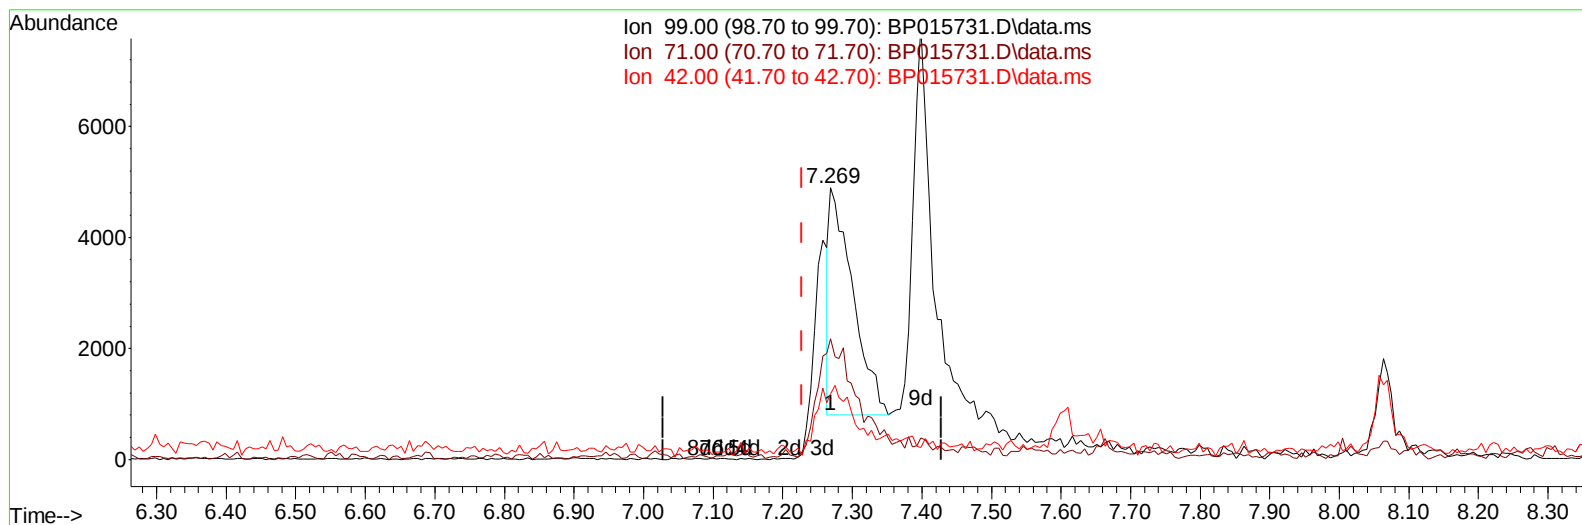

TIC: BP015731.D\data.ms

(7) Phenol-d5 (S)

7.269min (+ 0.041) 0.67 ng/u1

response 9554

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	44.43
42.00	21.90	24.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

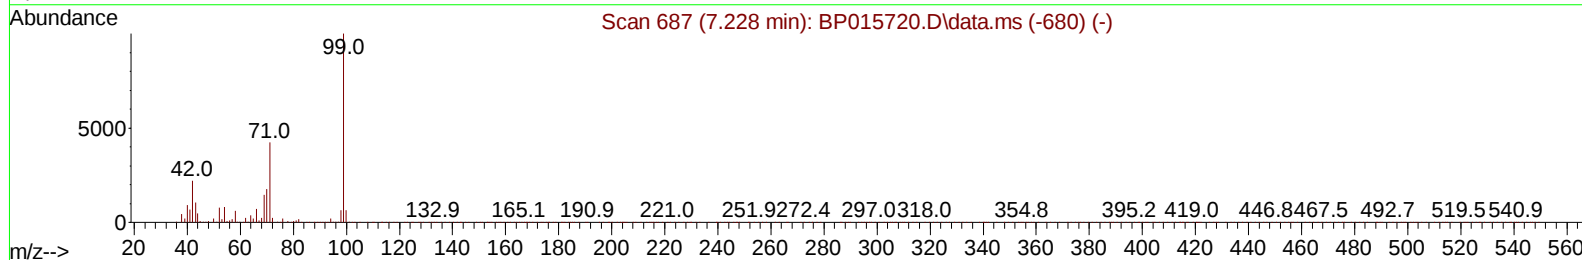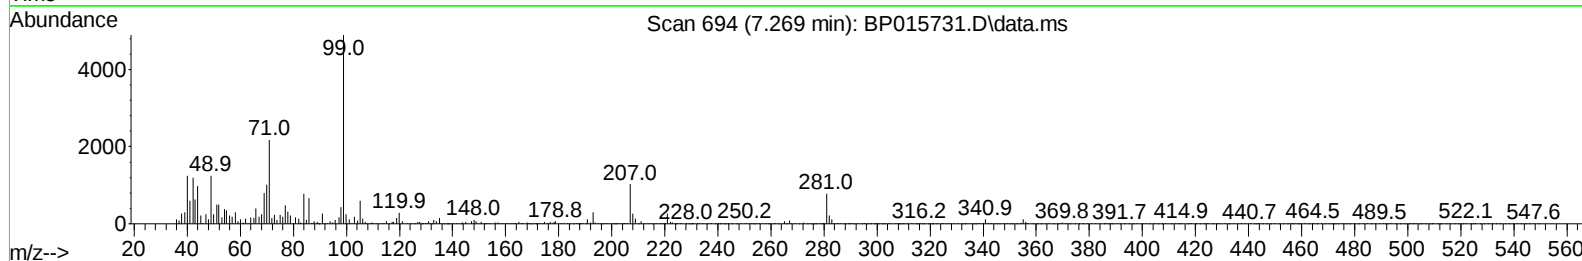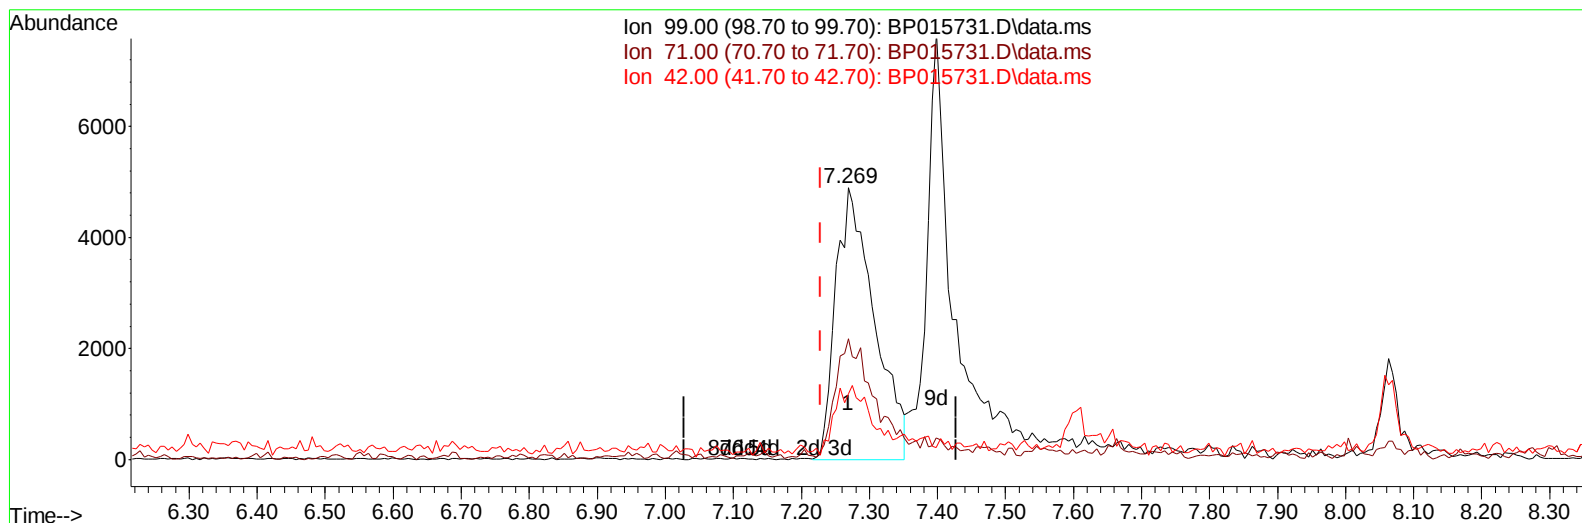

TIC: BP015731.D\data.ms

(7) Phenol-d5 (S)

7.269min (+ 0.041) 1.35 ng/ul m

response 19299

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	44.43
42.00	21.90	24.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

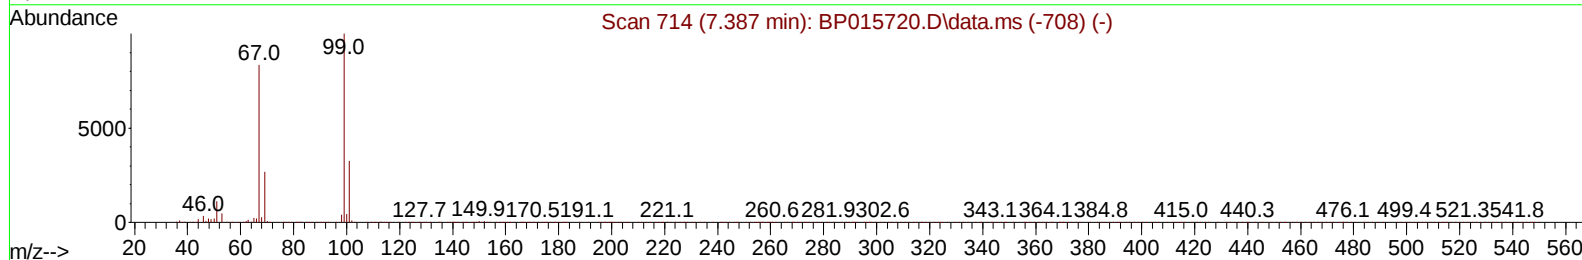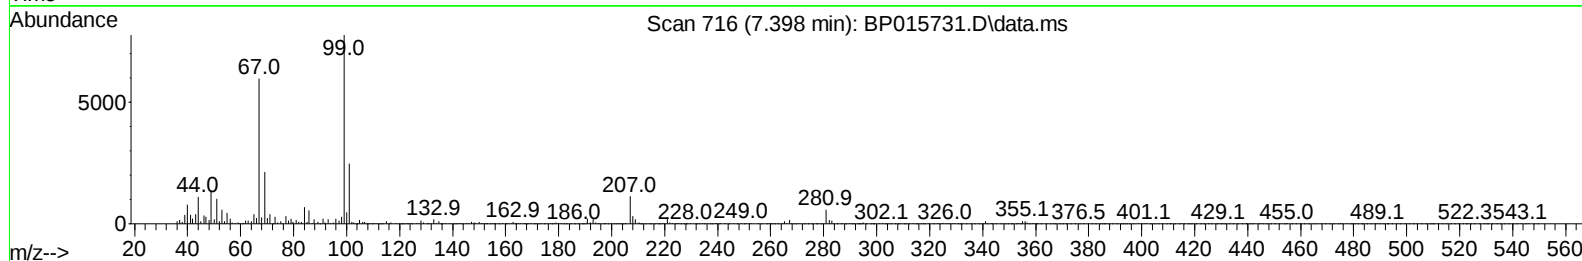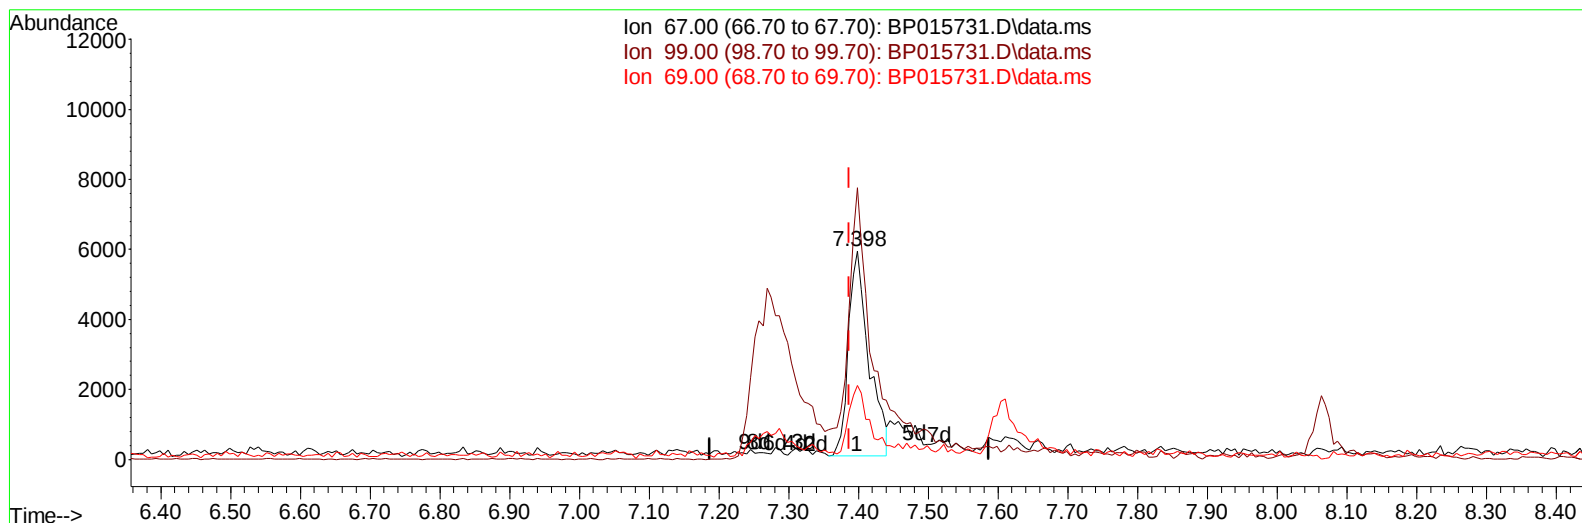

TIC: BP015731.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.398min (+ 0.012) 1.34 ng/u1

response 11903

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	130.22
69.00	32.10	35.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

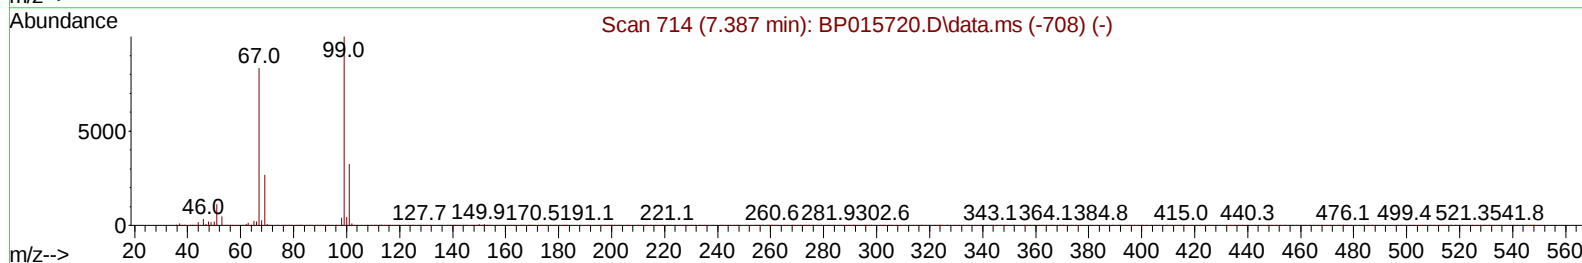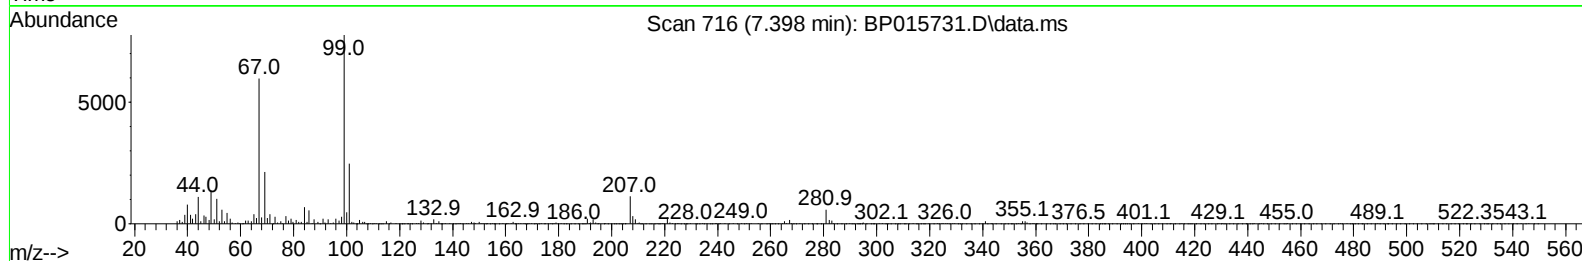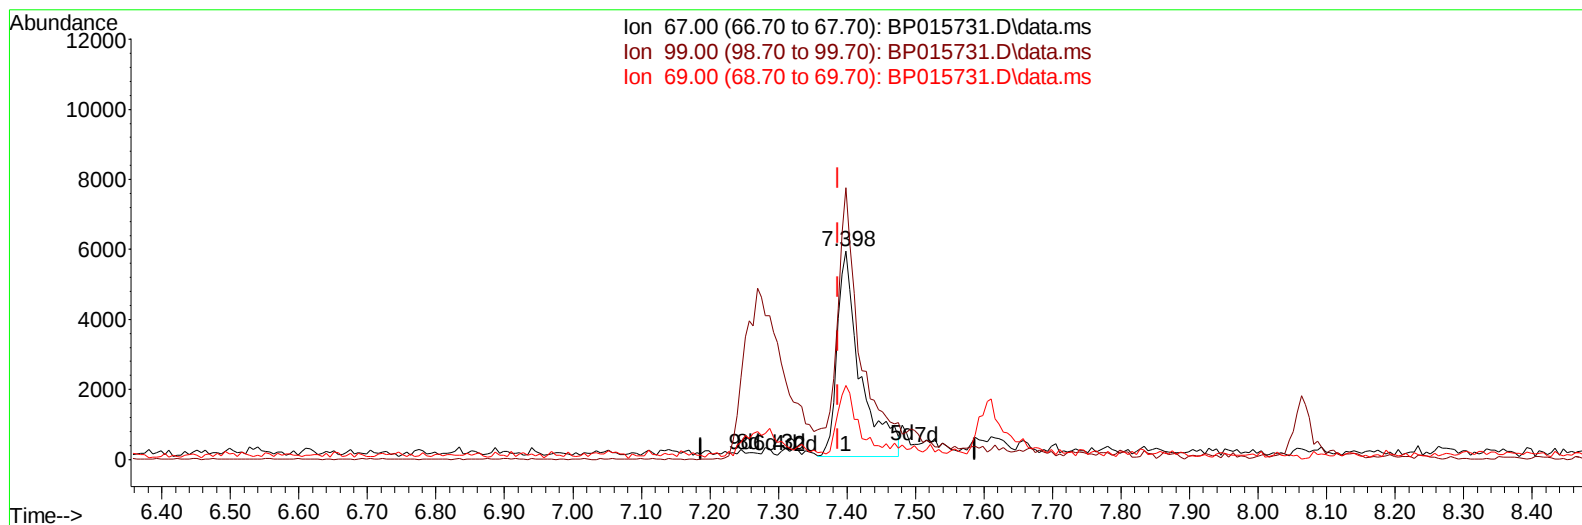

TIC: BP015731.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.398min (+ 0.012) 1.56 ng/ul m

response 13854

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	130.22
69.00	32.10	35.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

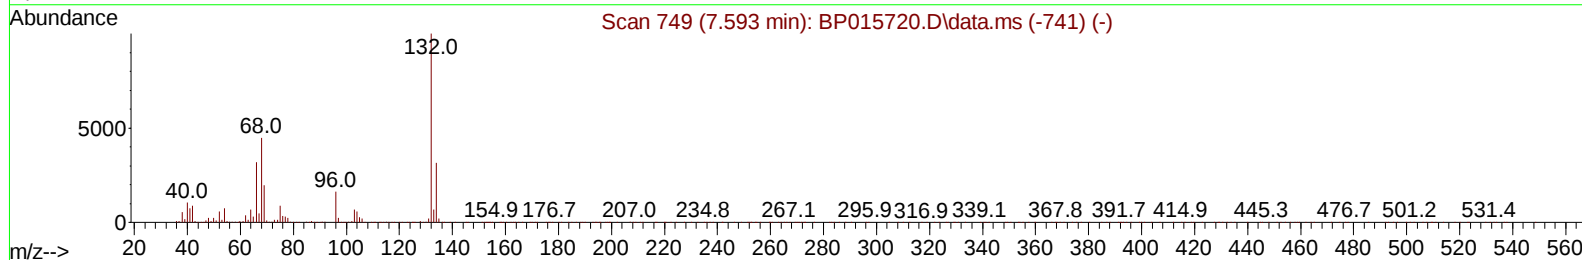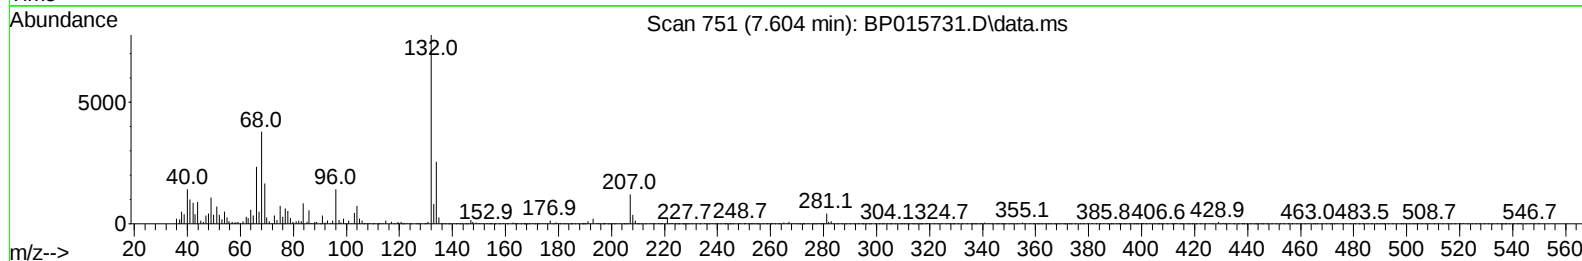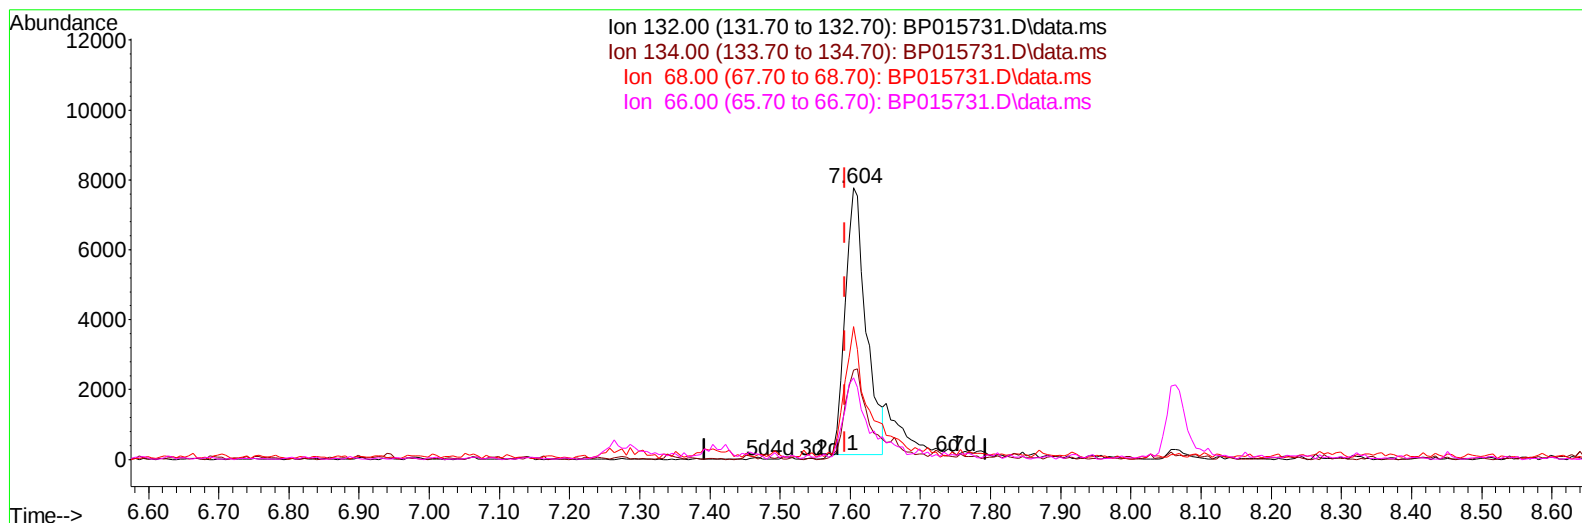

TIC: BP015731.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.604min (+ 0.012) 1.46 ng/u1

response 15770

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.40	32.93
68.00	46.60	48.89
66.00	32.60	30.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

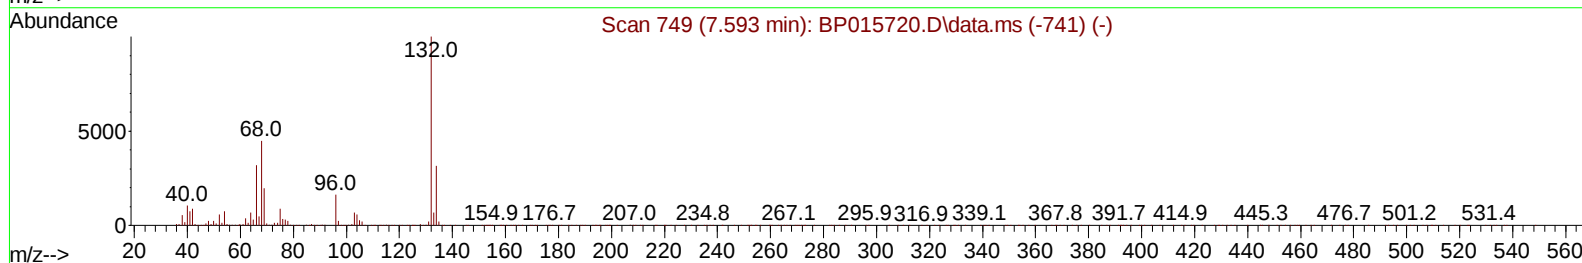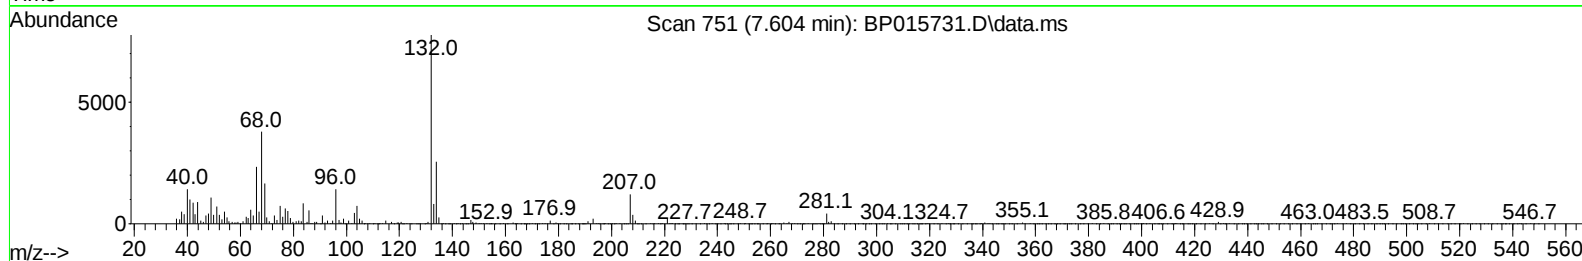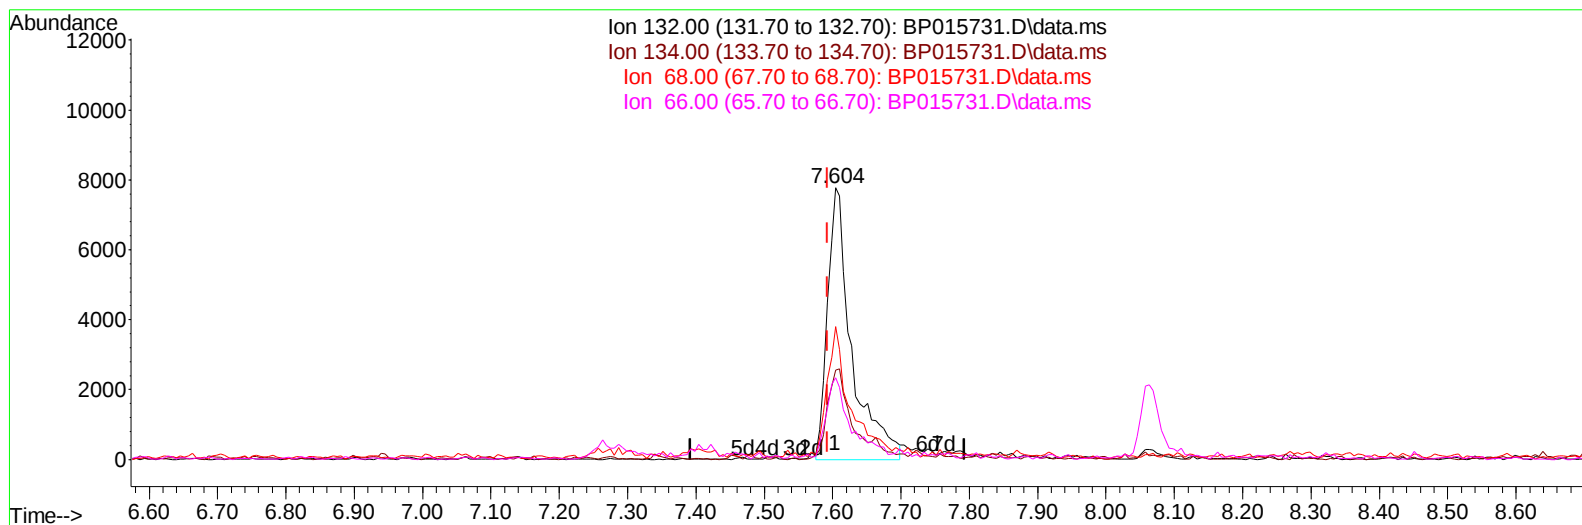

TIC: BP015731.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.604min (+ 0.012) 1.77 ng/ul m

response 19118

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.40	32.93
68.00	46.60	48.89
66.00	32.60	30.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015731.D
Acq On : 27 Jun 2023 00:39
Operator : MA/JU
Sample : 03083-13DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

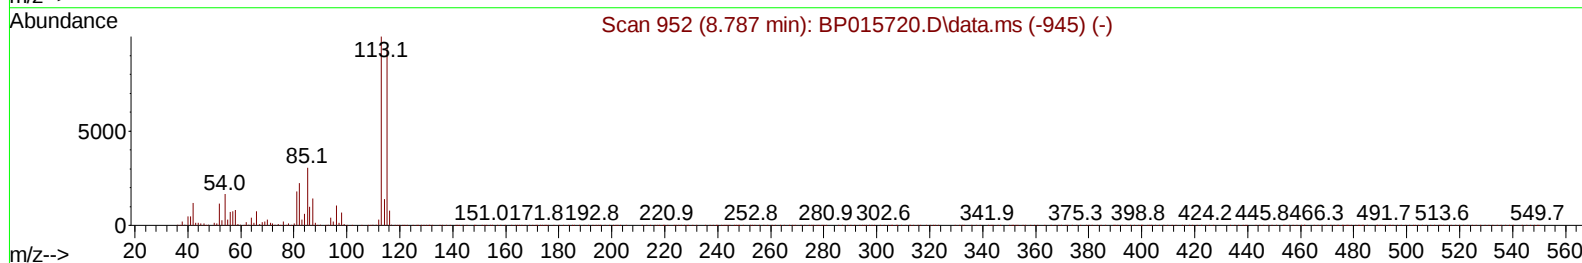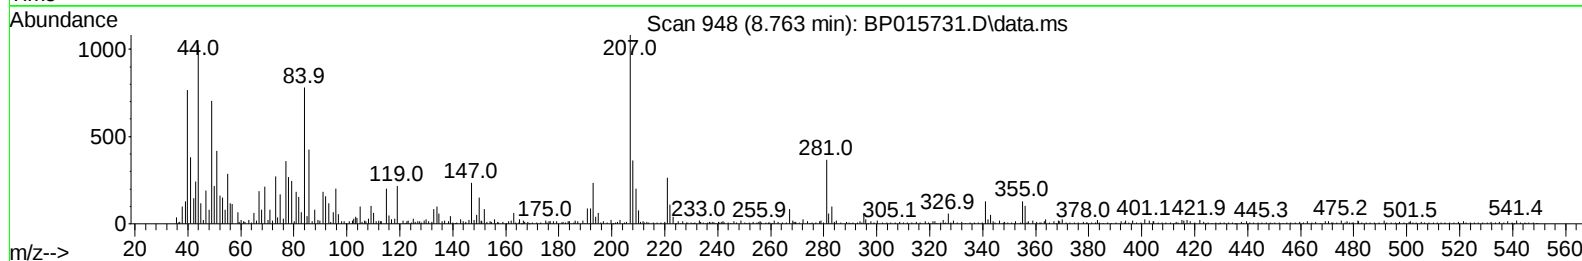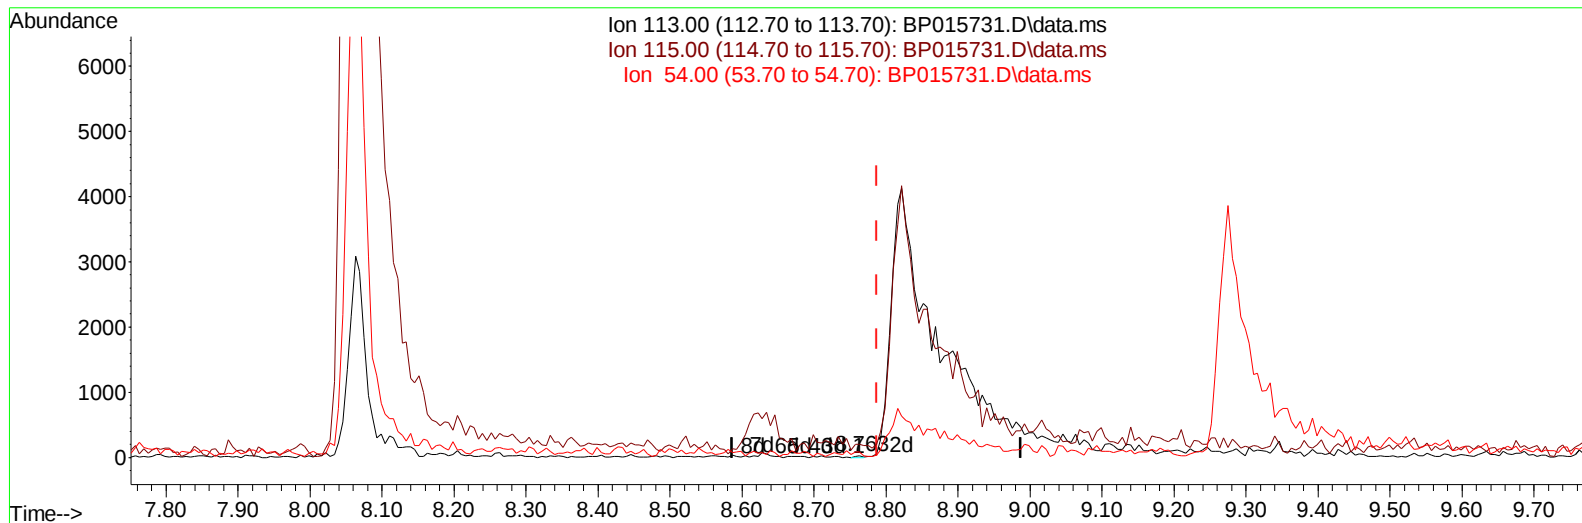

TIC: BP015731.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.763min (-0.024) 0.00 ng/u1

response 19

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	744.44#
54.00	16.10	296.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:29:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

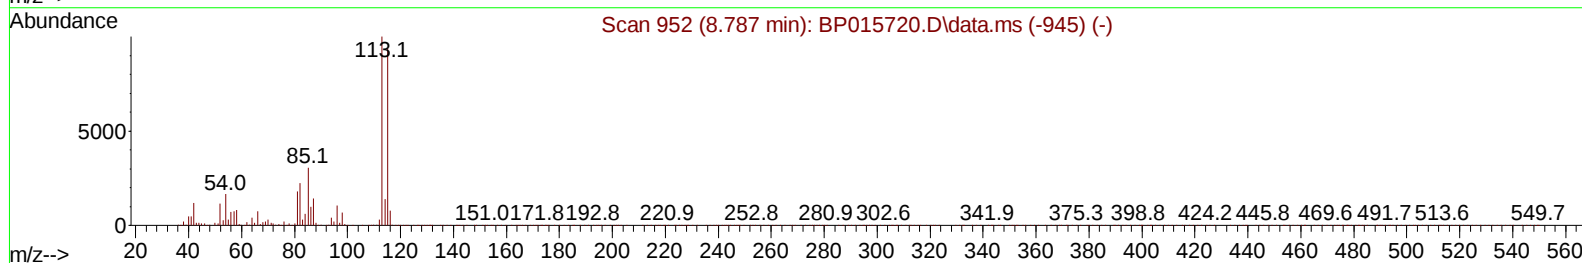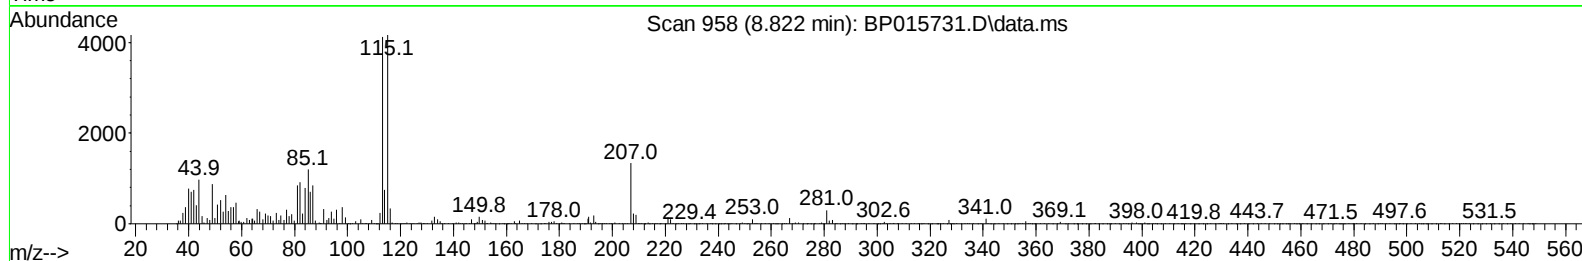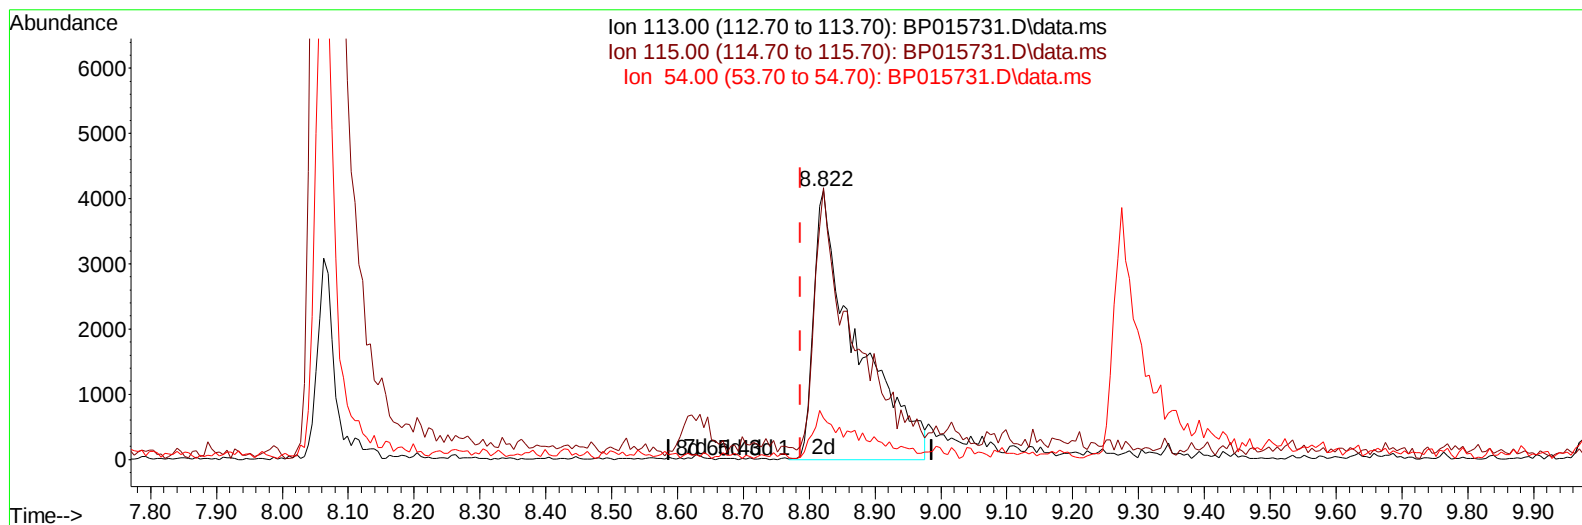

TIC: BP015731.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.822min (+ 0.035) 1.64 ng/ul m

response 18628

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	100.95
54.00	16.10	15.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

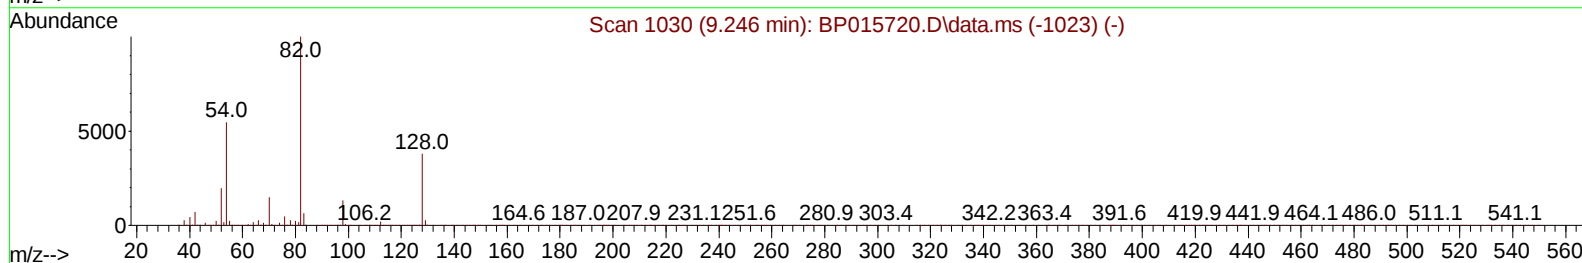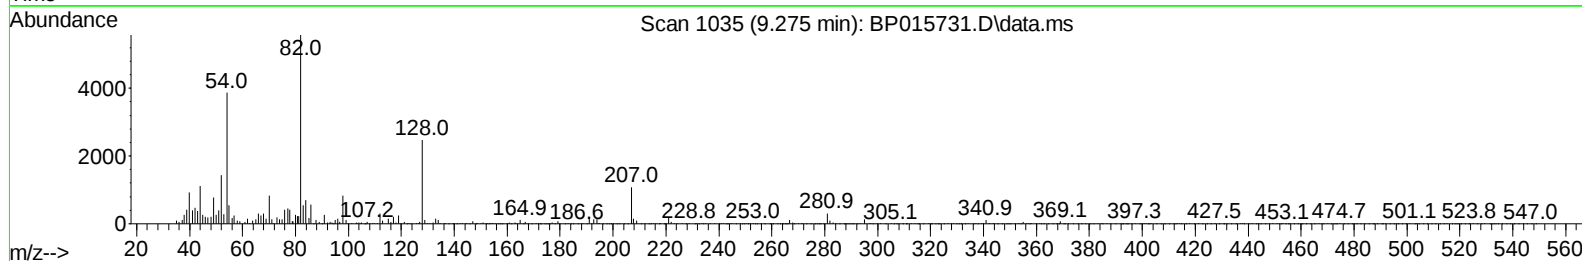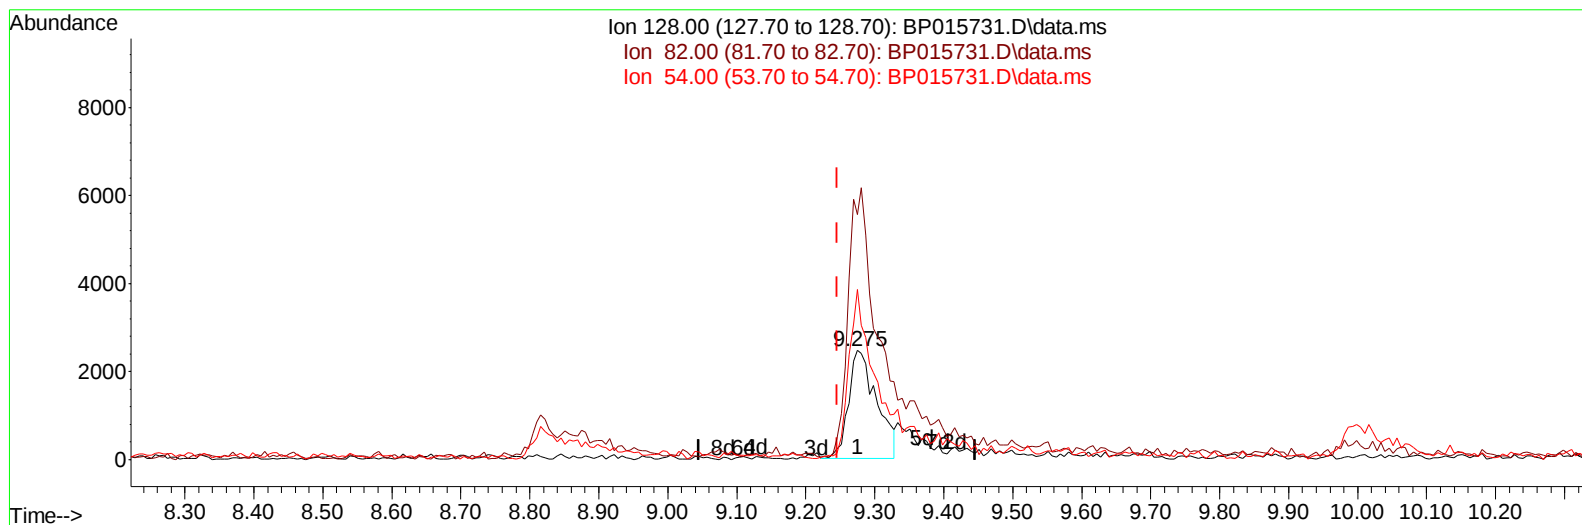

TIC: BP015731.D\data.ms

(21) Nitrobenzene-d5 (S)

9.275min (+ 0.029) 1.30 ng/u1

response 6986

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	224.56
54.00	141.60	155.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

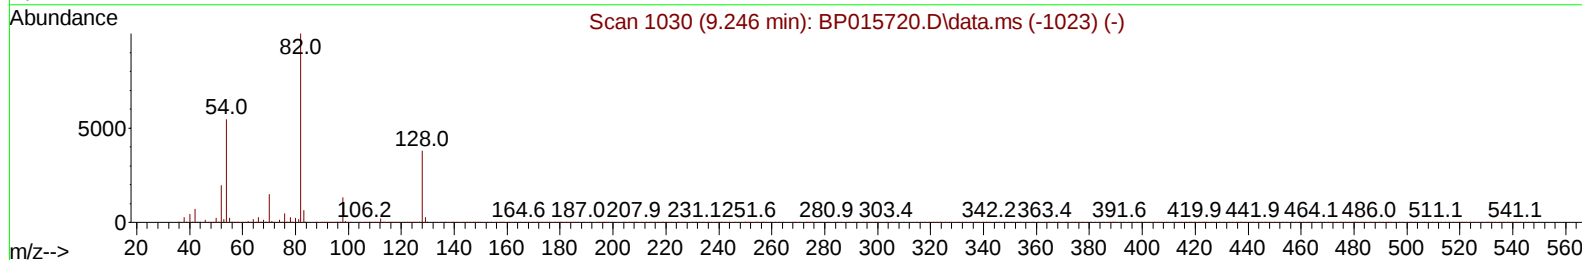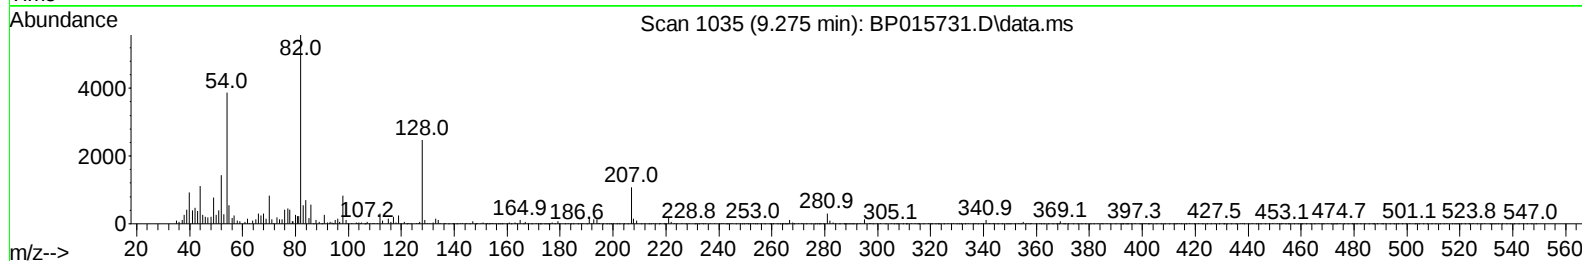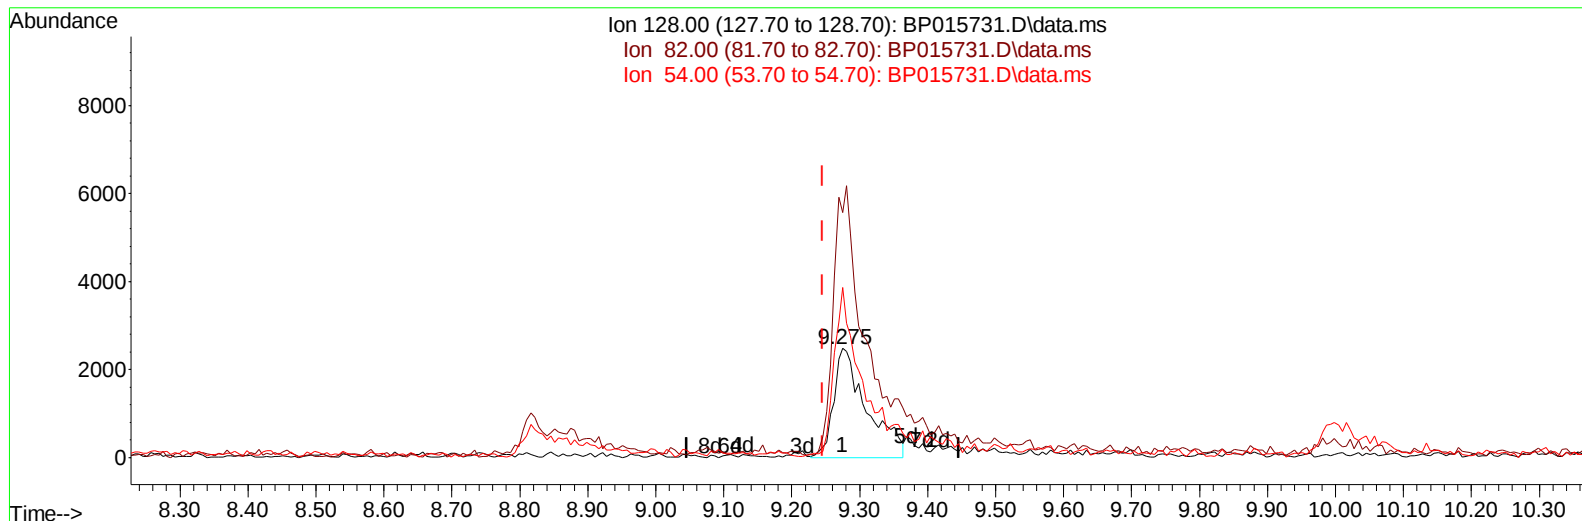

TIC: BP015731.D\data.ms

(21) Nitrobenzene-d5 (S)

9.275min (+ 0.029) 1.56 ng/ul m

response 8390

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	224.56
54.00	141.60	155.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

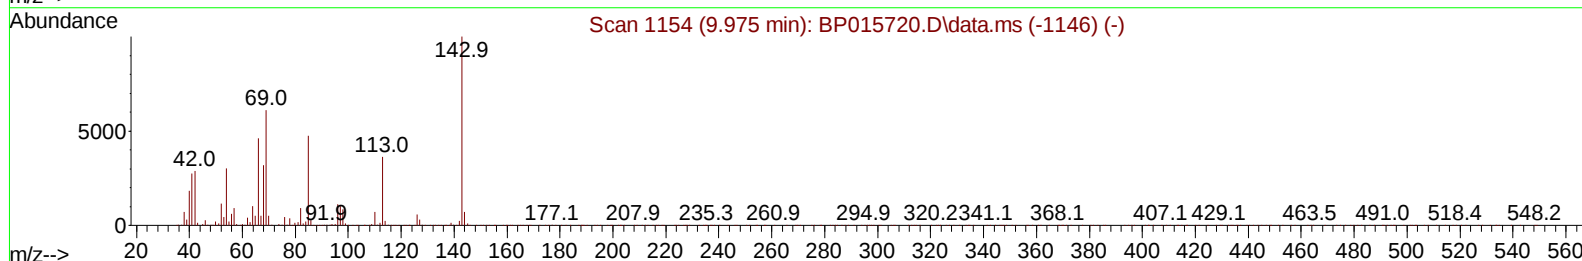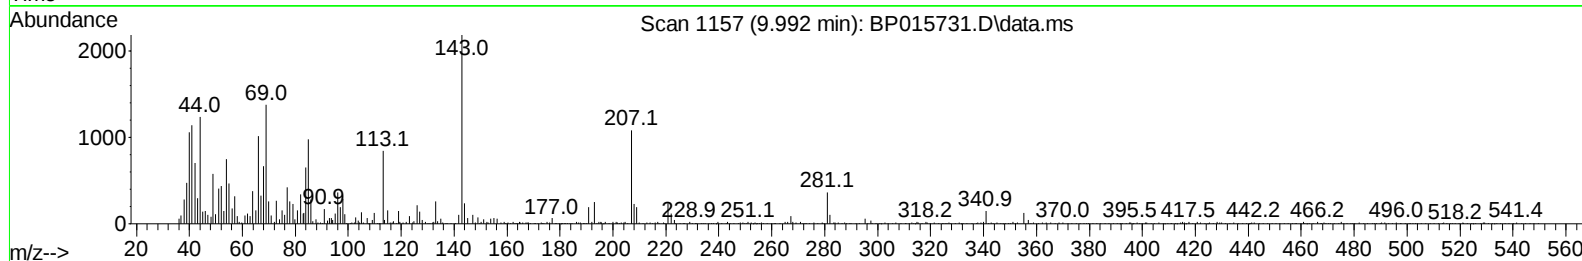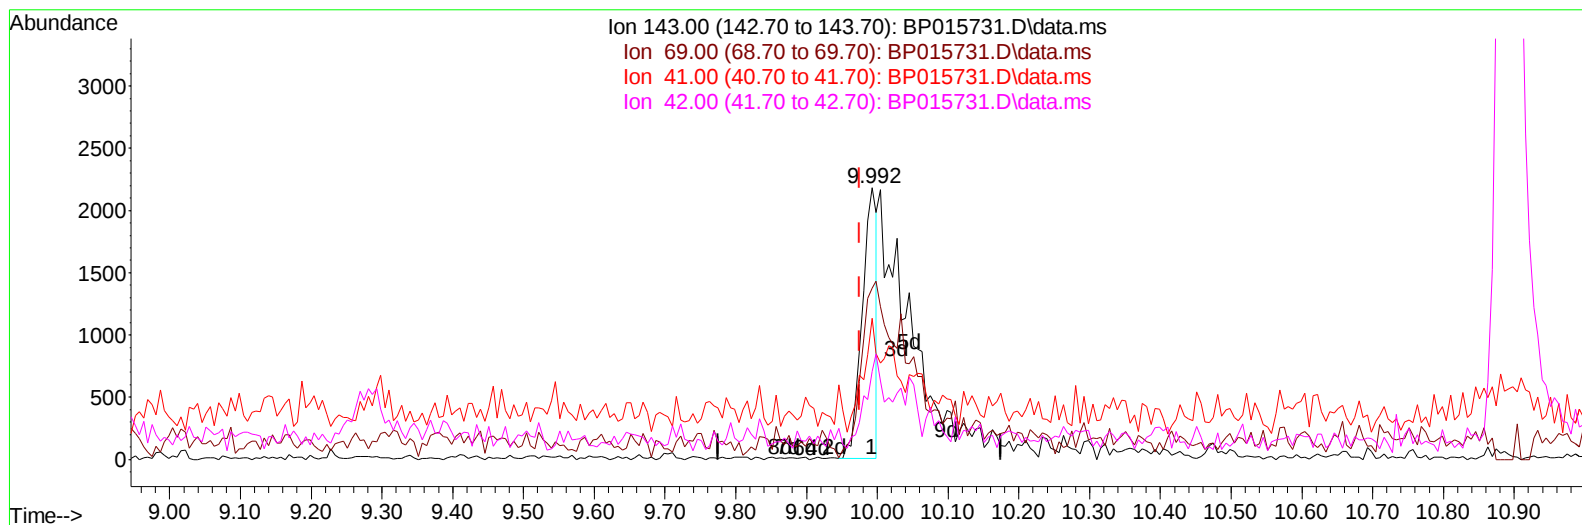

TIC: BP015731.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.992min (+ 0.017) 0.50 ng/u1

response 3165

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	63.09
41.00	26.80	52.09#
42.00	30.50	32.37




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

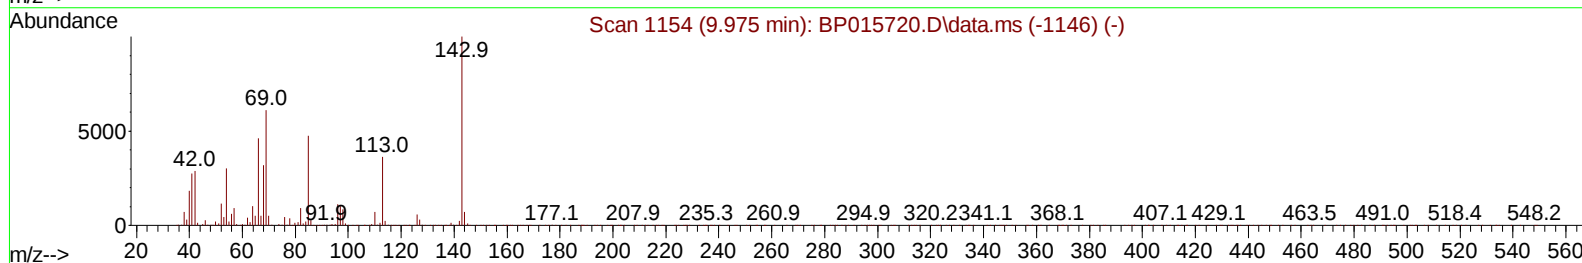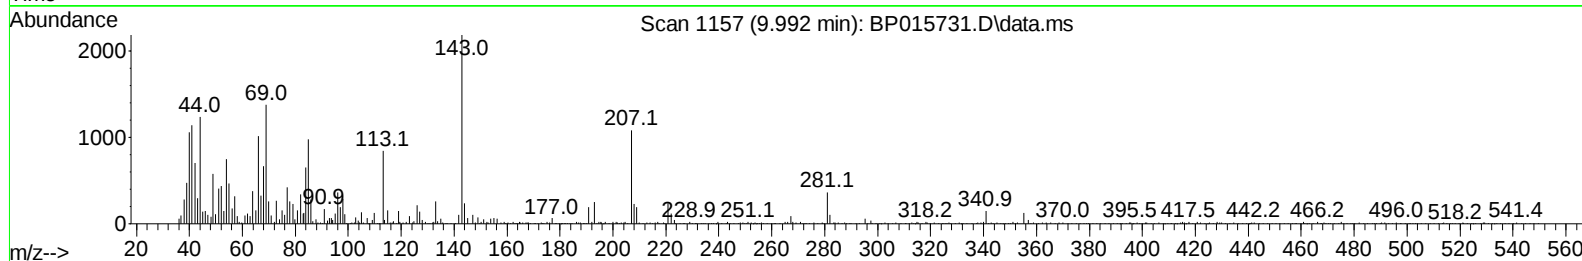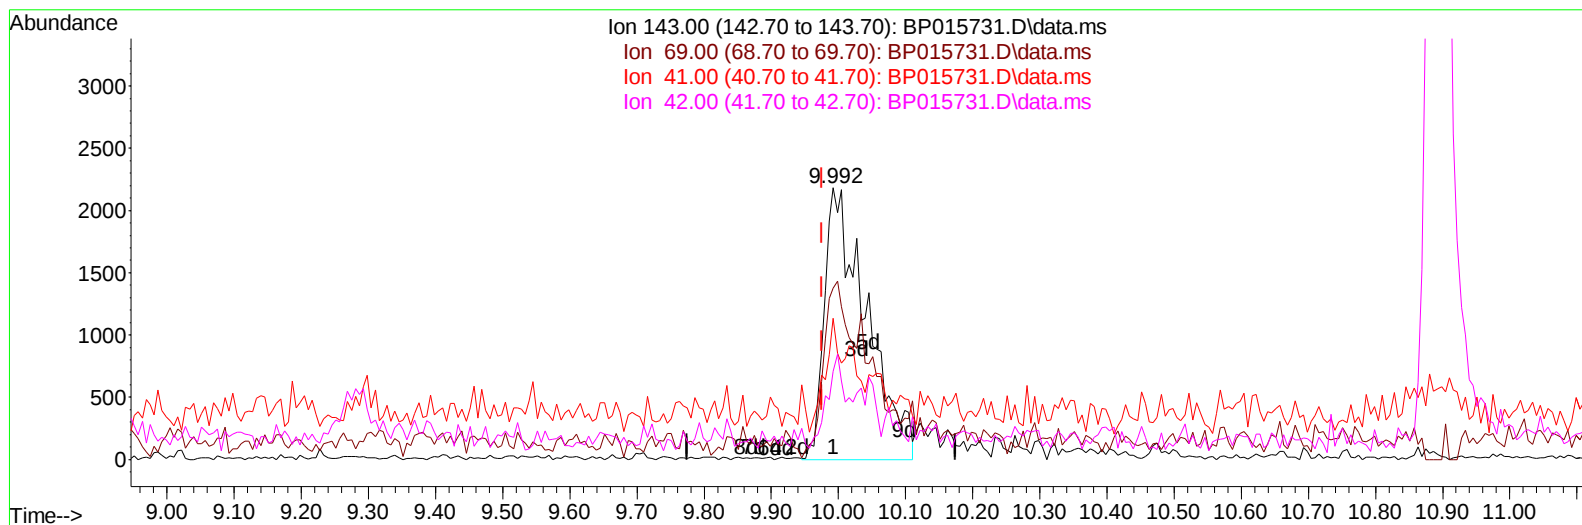

TIC: BP015731.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.992min (+ 0.017) 1.50 ng/ul m

response 9434

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	63.09
41.00	26.80	52.09#
42.00	30.50	32.37




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015731.D
Acq On : 27 Jun 2023 00:39
Operator : MA/JU
Sample : 03083-13DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

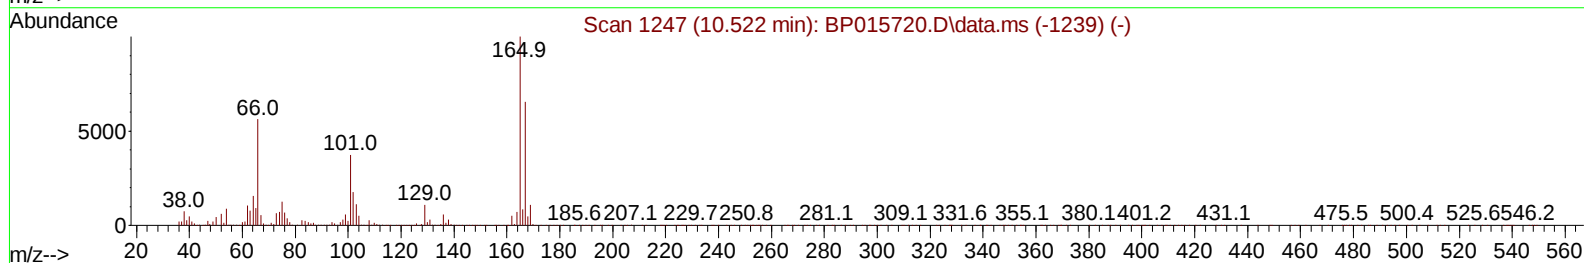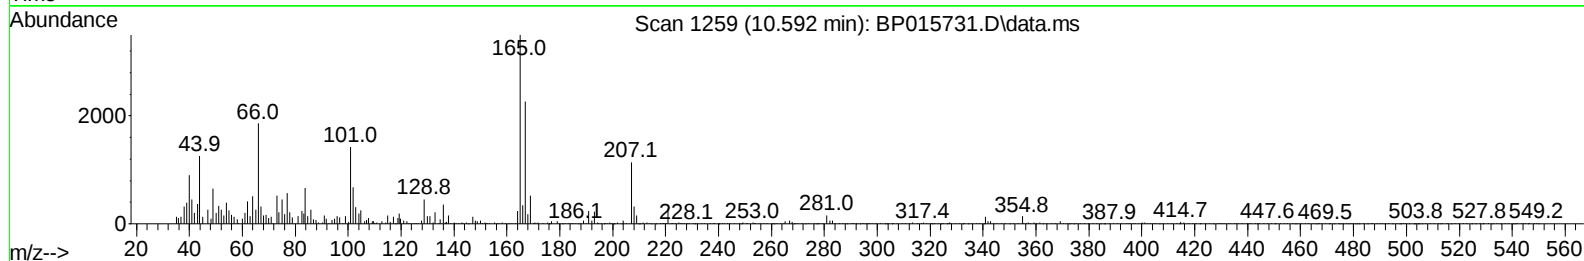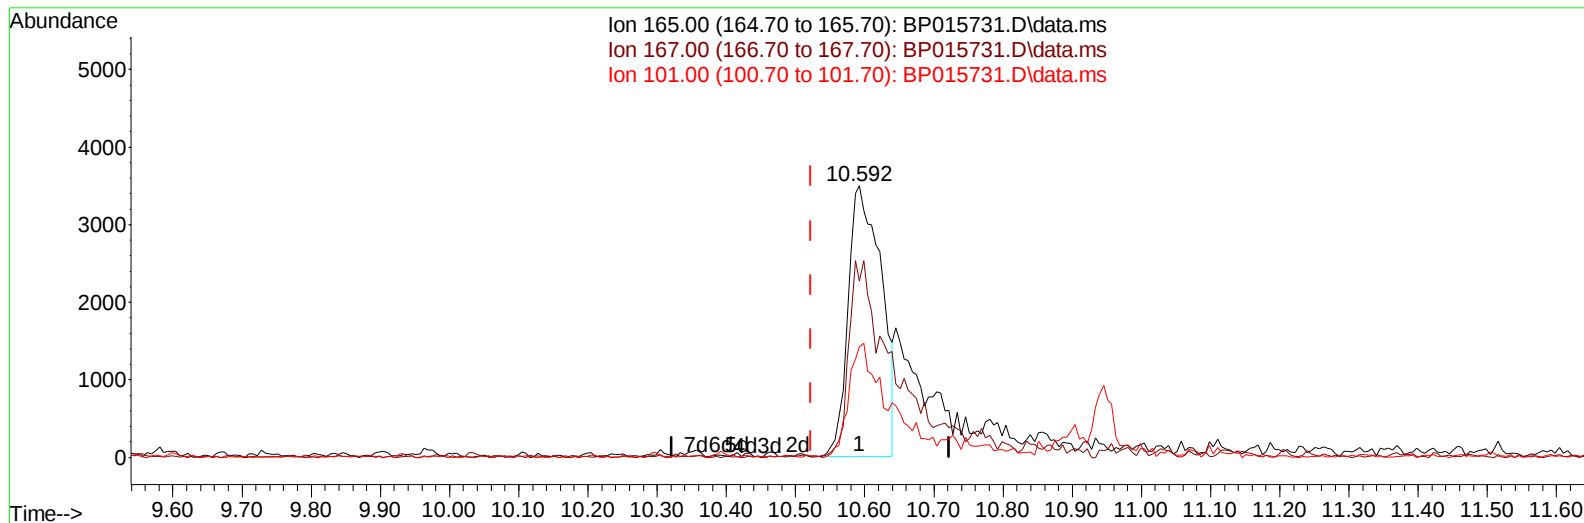

TIC: BP015731.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.592min (+ 0.070) 1.03 ng/u1

response 11536

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	64.88
101.00	37.30	40.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:30:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

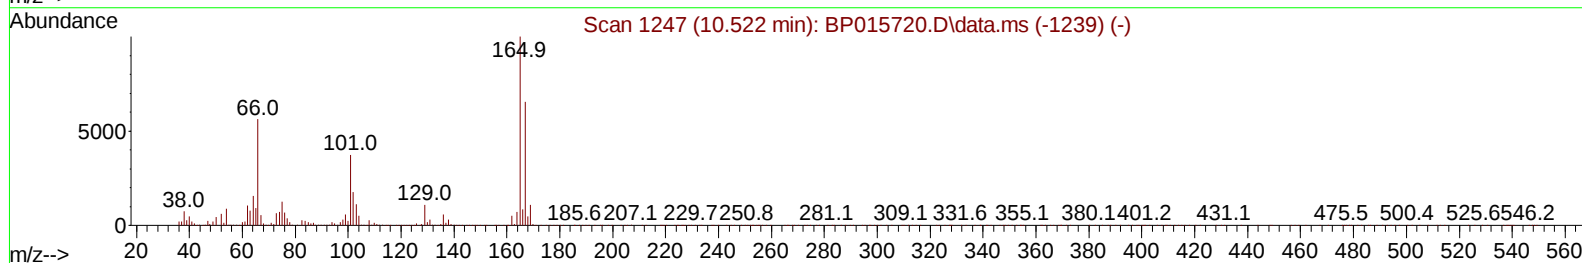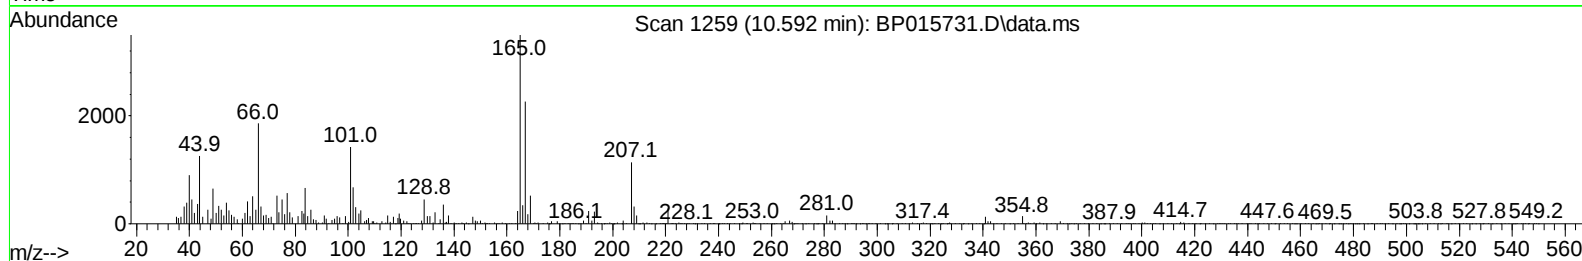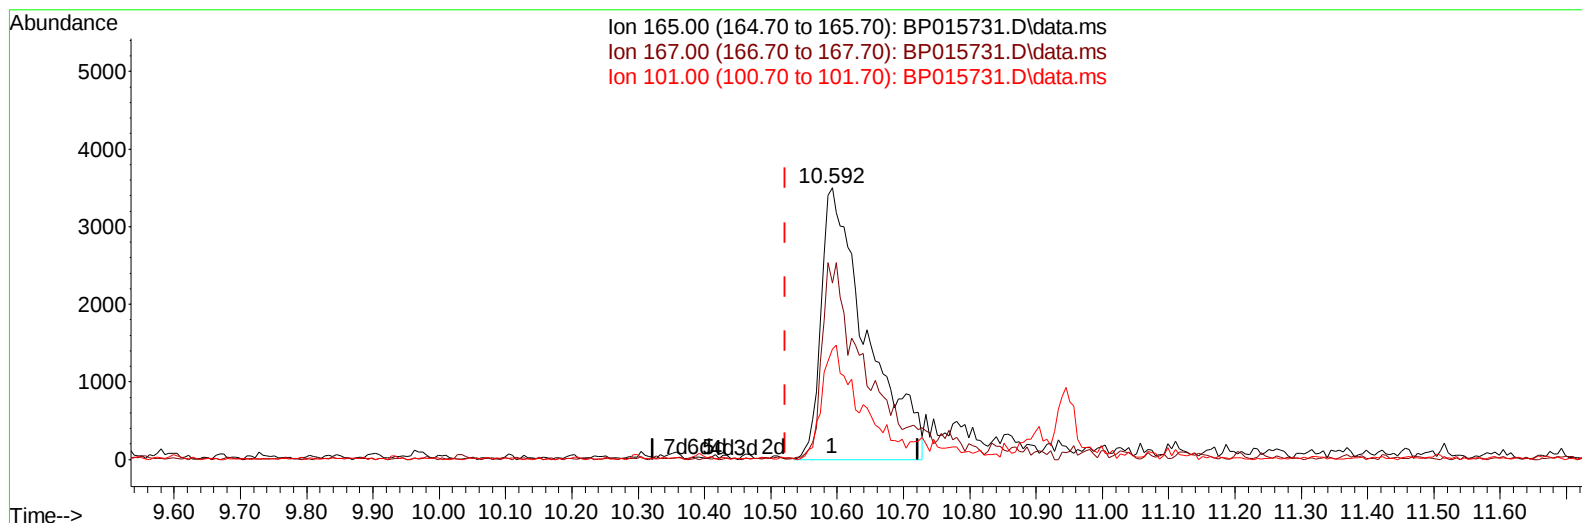

TIC: BP015731.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.592min (+ 0.070) 1.48 ng/ul m

response 16629

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	64.88
101.00	37.30	40.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:32:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

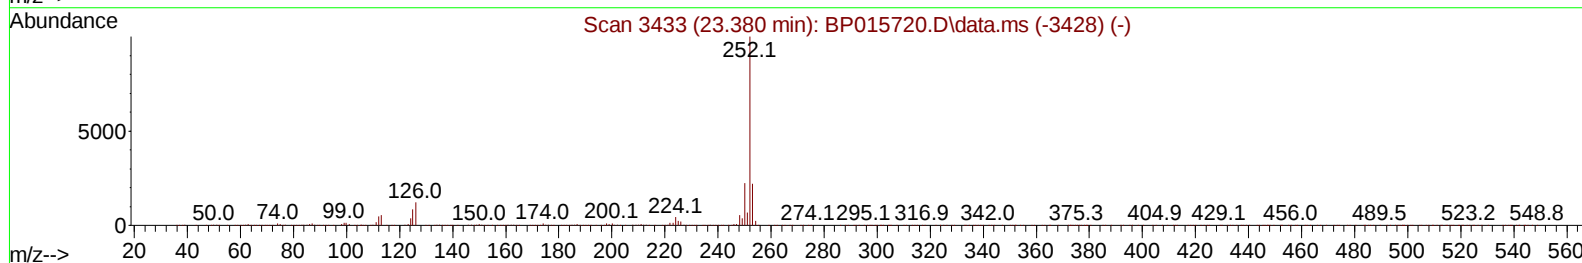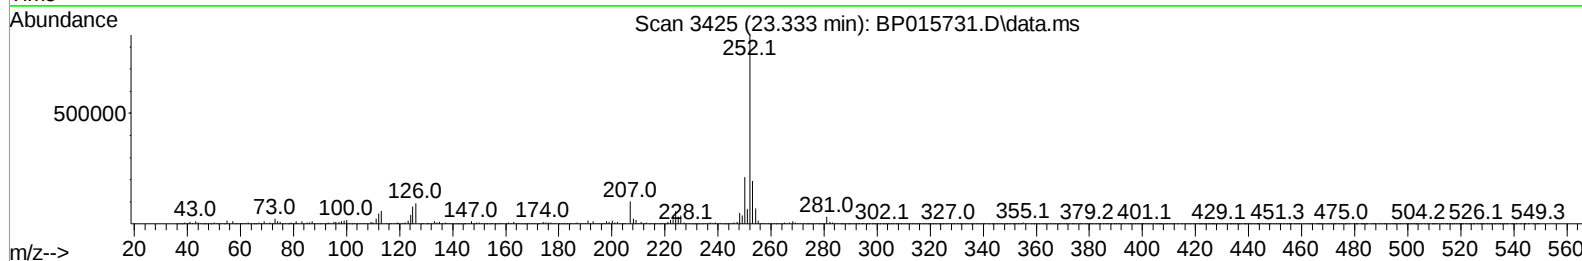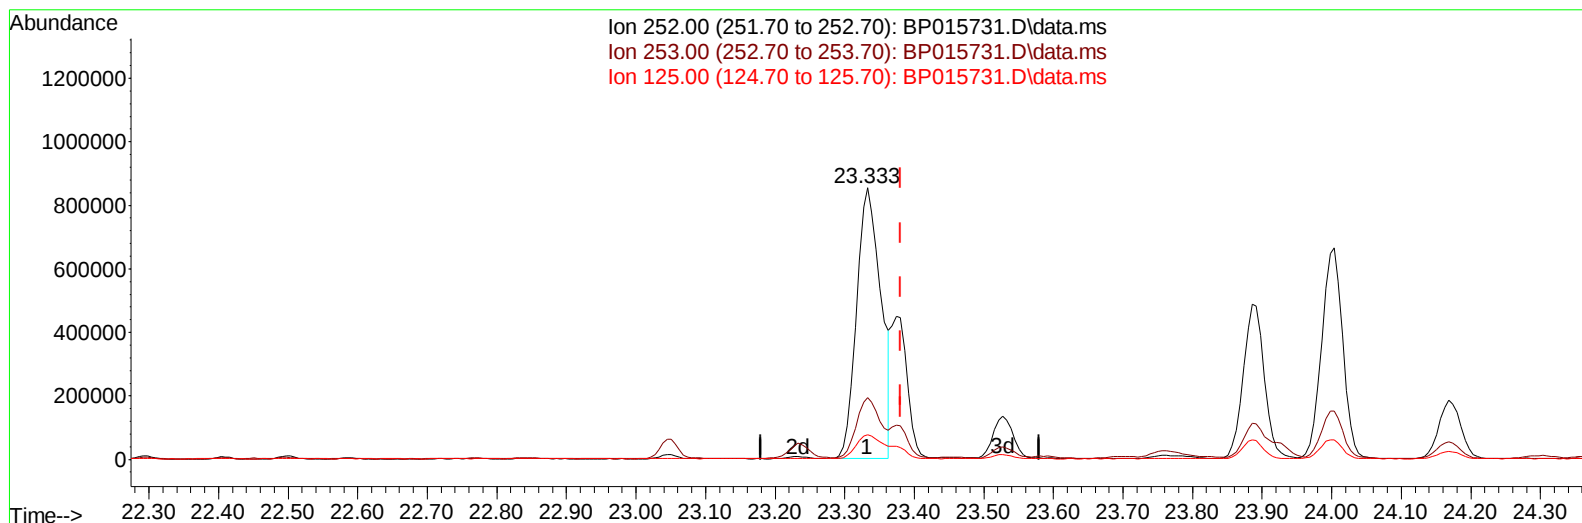

TIC: BP015731.D\data.ms

(91) Benzo(k)fluoranthene

23.333min (-0.047) 45.87 ng/u1

response 2069745

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.20	22.81
125.00	9.10	9.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:32:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

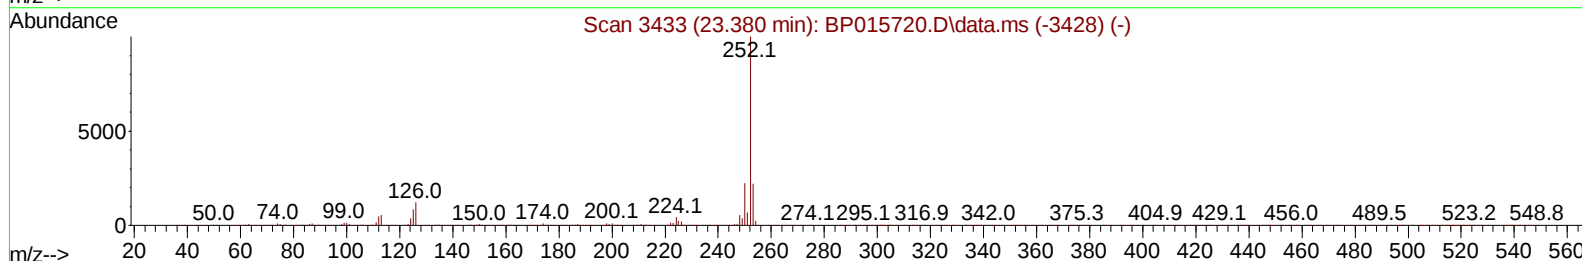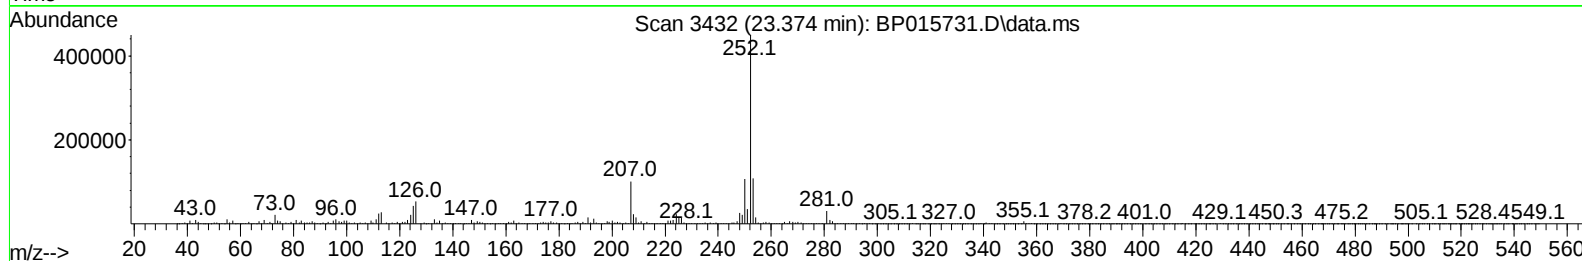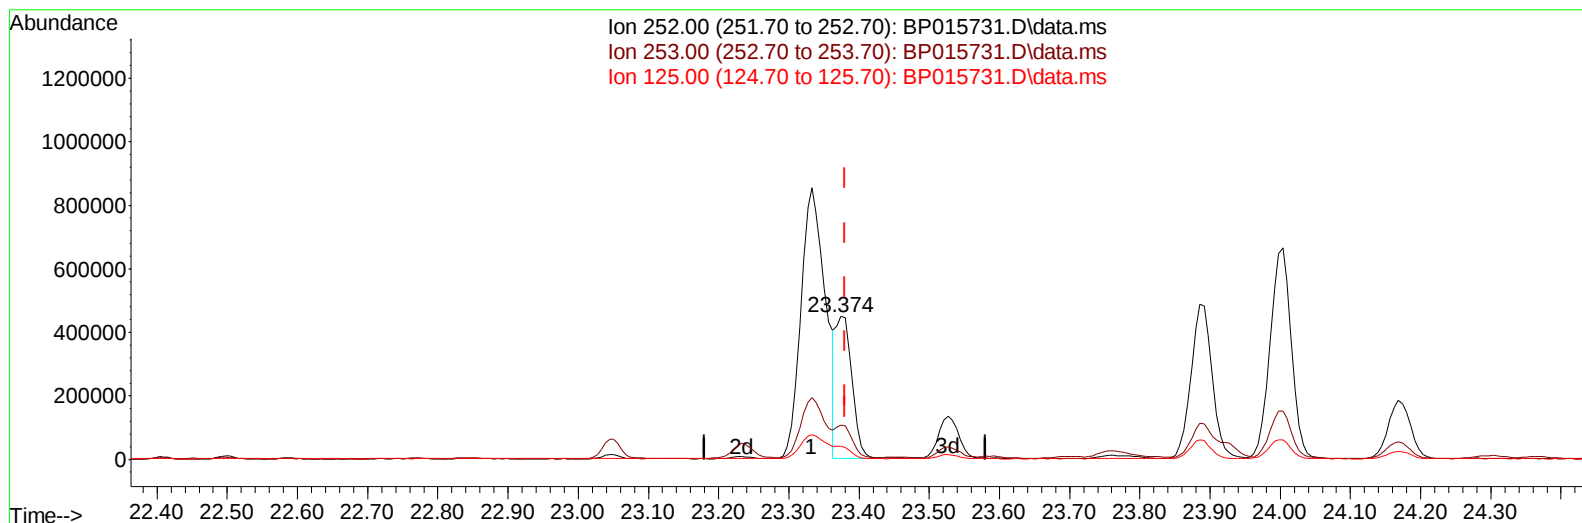

TIC: BP015731.D\data.ms

(91) Benzo(k)fluoranthene

23.374min (-0.006) 15.80 ng/ul m

response 712734

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.20	23.96
125.00	9.10	9.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015731.D
 Acq On : 27 Jun 2023 00:39
 Operator : MA/JU
 Sample : 03083-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:32:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	167653	20.000	ng/ul	0.00
20) Naphthalene-d8	10.892	136	704611	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	444951	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.474	188	939372	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	597588	20.000	ng/ul	0.00
88) Perylene-d12	24.115	264	695045	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	1280	0.275	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.269	99	19299m	1.345	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.398	67	13854m	1.561	ng/ul	0.01
11) 2-Chlorophenol-d4	7.604	132	19118m	1.766	ng/ul	0.01
15) 4-Methylphenol-d8	8.822	113	18628m	1.644	ng/ul	0.04
21) Nitrobenzene-d5	9.275	128	8390m	1.558	ng/ul	0.03
24) 2-Nitrophenol-d4	9.992	143	9434m	1.501	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.592	165	16629m	1.485	ng/ul	0.07
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	14.128	166	72987	2.122	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	79206	2.049	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.710	176	60202	2.126	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.574	188	91975	2.144	ng/ul	0.00
81) Pyrene-d10	19.798	212	90035	2.307	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	72019	2.054	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.945	128	57586	1.503	ng/ul	98
36) 2-Methylnaphthalene	12.569	142	26879	1.066	ng/ul	91
52) Acenaphthene	14.780	153	149992	5.078	ng/ul	97
61) Fluorene	15.769	166	141543	4.256	ng/ul	99
72) Phenanthrene	17.516	178	2609997	51.144	ng/ul	100
74) Anthracene	17.610	178	601427	11.729	ng/ul	99
80) Fluoranthene	19.480	202	4180593	86.205	ng/ul	98
82) Pyrene	19.833	202	3217096	65.032	ng/ul	100
85) Benzo(a)anthracene	21.545	228	1637275	38.948	ng/ul	97
87) Chrysene	21.604	228	1514196	37.966	ng/ul	97
90) Benzo(b)fluoranthene	23.333	252	2069745	46.345	ng/ul	98
91) Benzo(k)fluoranthene	23.374	252	712734m	15.795	ng/ul	
93) Benzo(a)pyrene	24.003	252	1391559	35.660	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.815	276	1111528	20.982	ng/ul	98
95) Dibenzo(a,h)anthracene	26.815	278	314535	7.229	ng/ul#	78
96) Benzo(g,h,i)perylene	27.656	276	1021886	23.448	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015731.D
Acq On : 27 Jun 2023 00:39
Operator : MA/JU
Sample : 03083-13DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL1DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

Quant Time: Jun 27 03:32:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

