




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

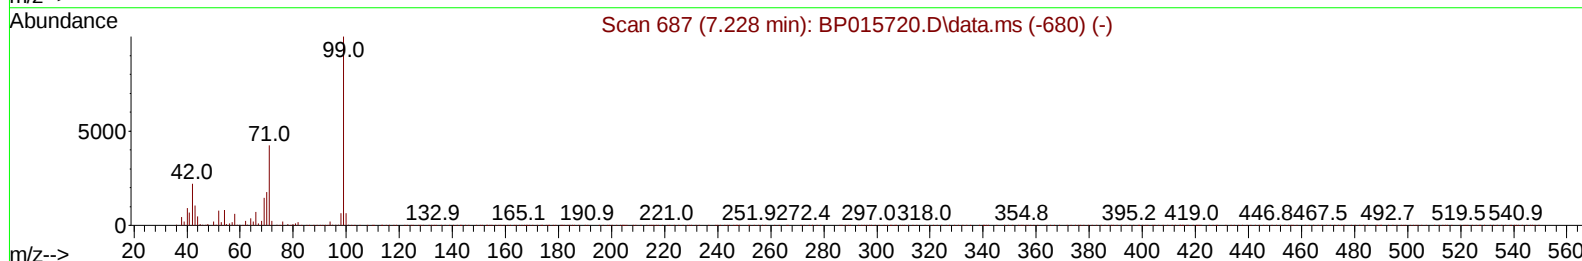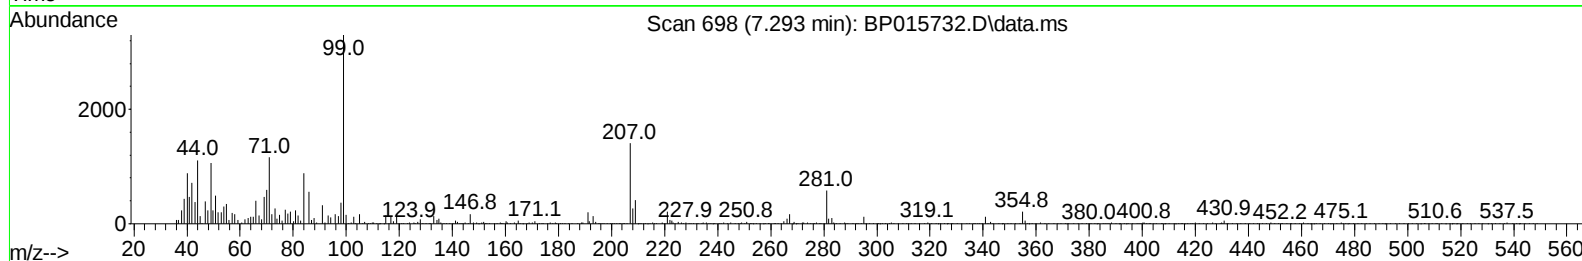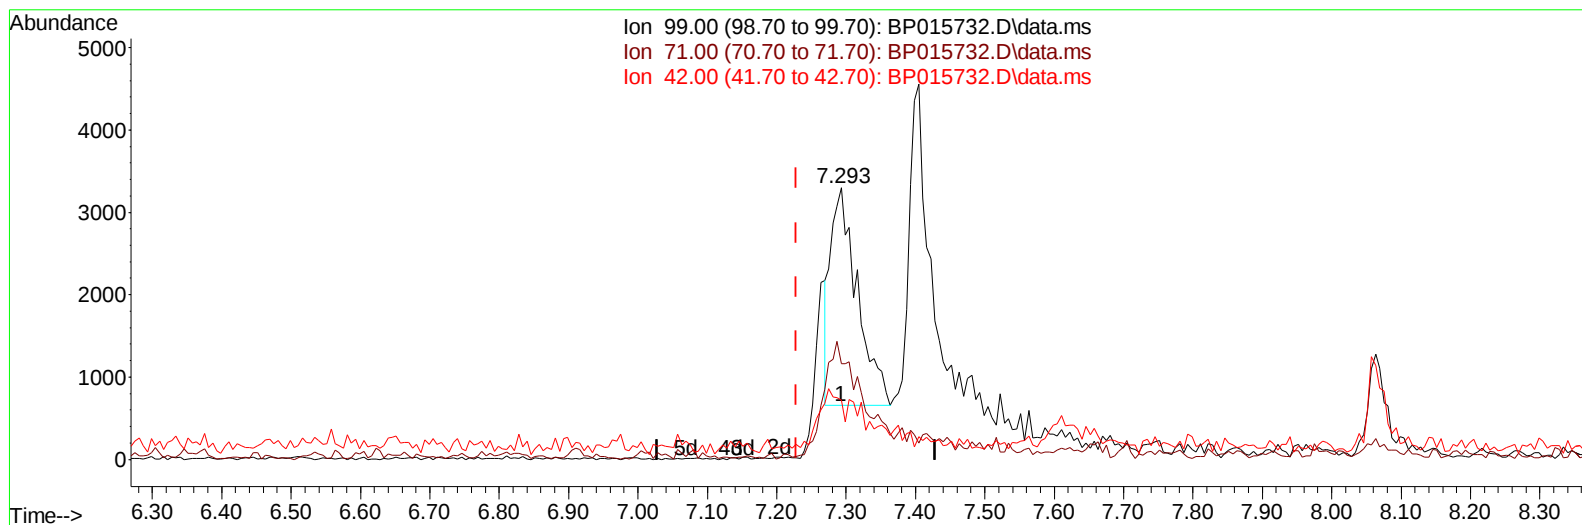

TIC: BP015732.D\data.ms

(7) Phenol-d5 (S)

7.293min (+ 0.065) 0.65 ng/u1

response 7045

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	35.21
42.00	21.90	21.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

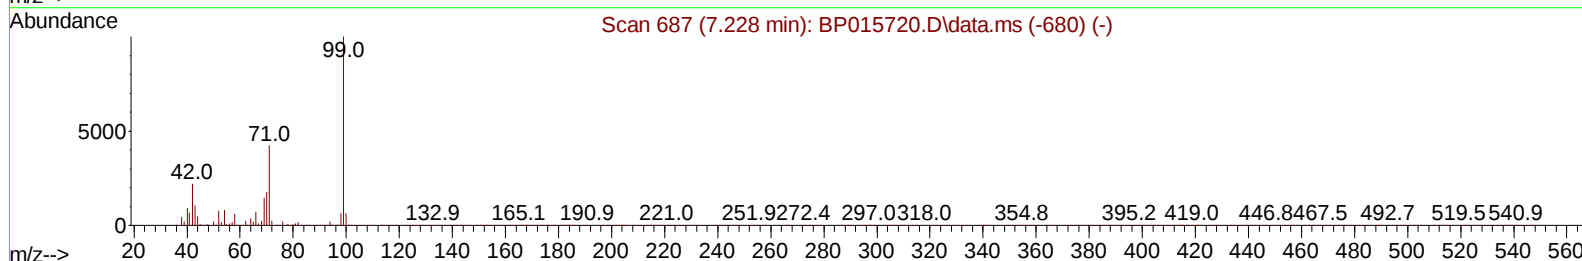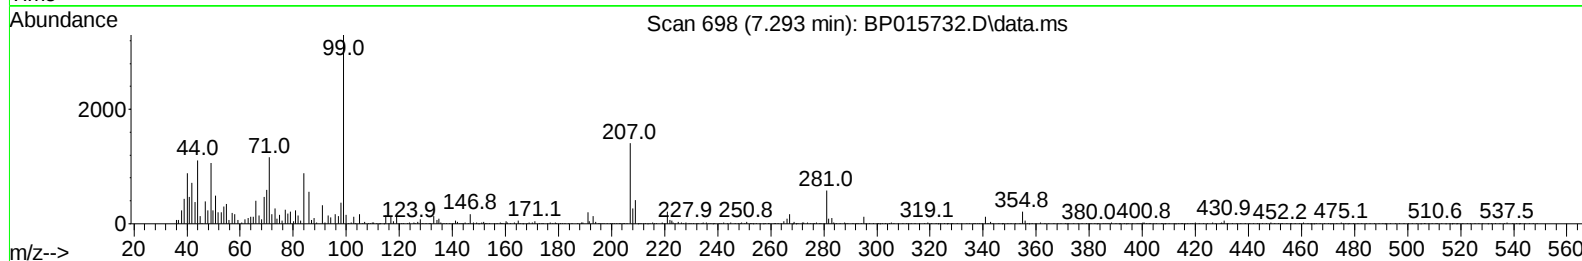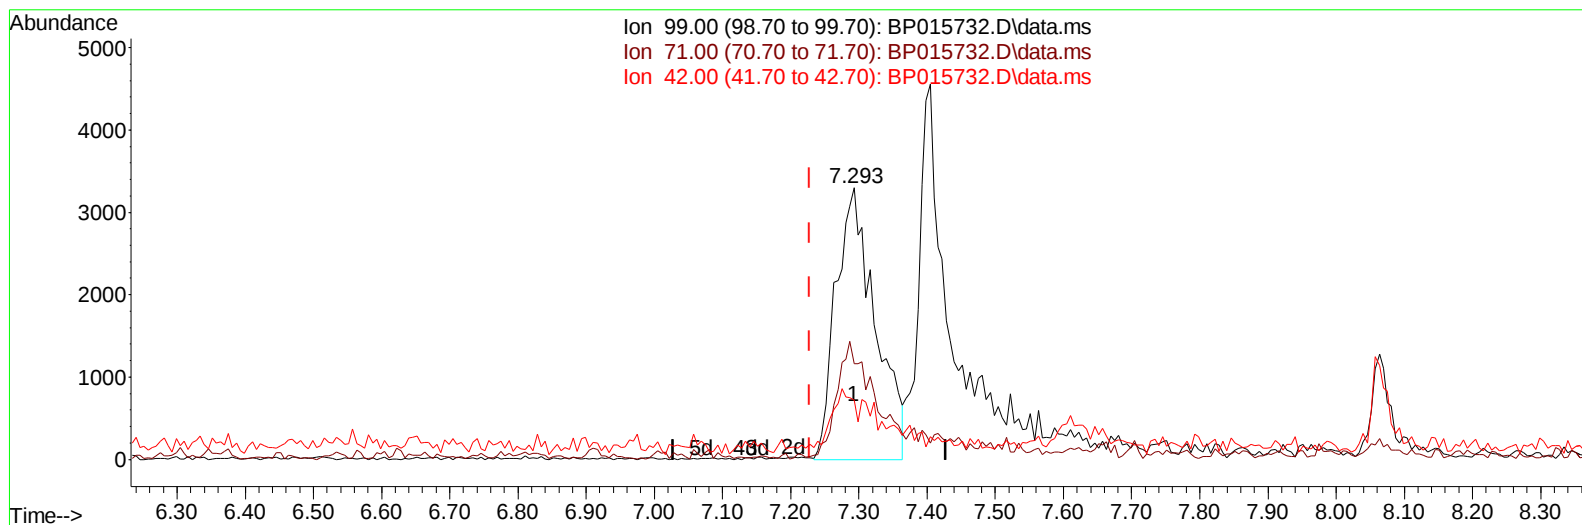

TIC: BP015732.D\data.ms

(7) Phenol-d5 (S)

7.293min (+ 0.065) 1.21 ng/ul m

response 13143

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	35.21
42.00	21.90	21.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

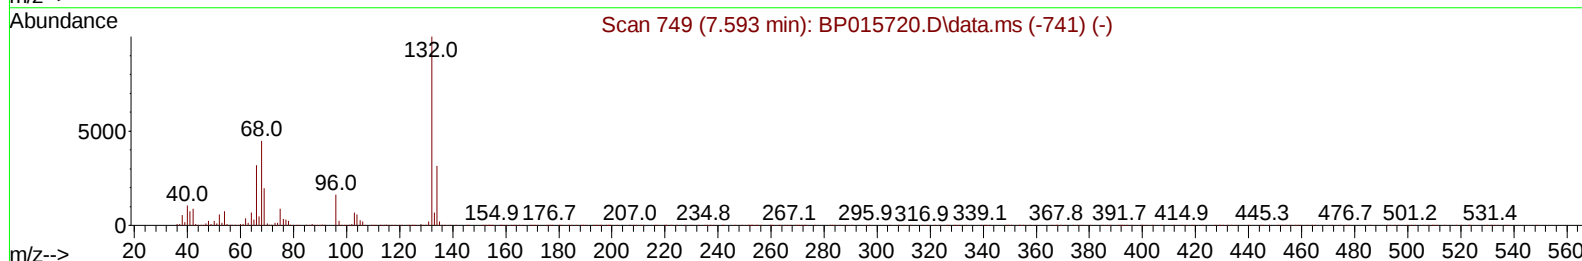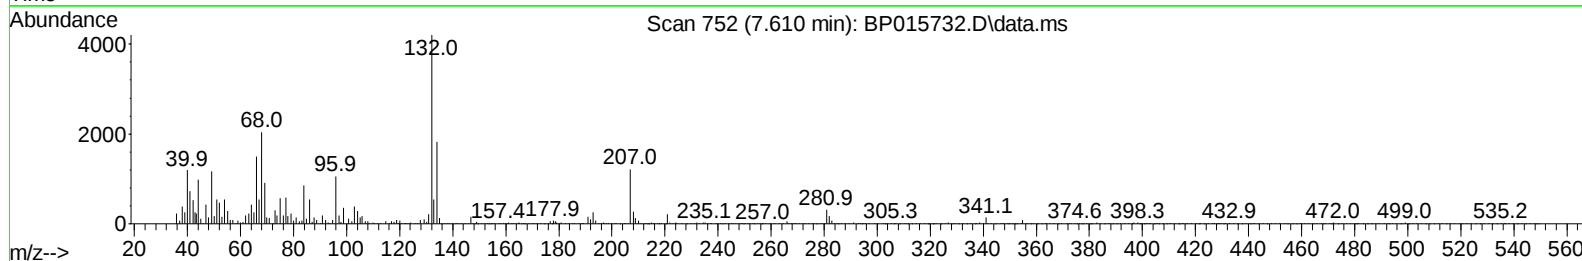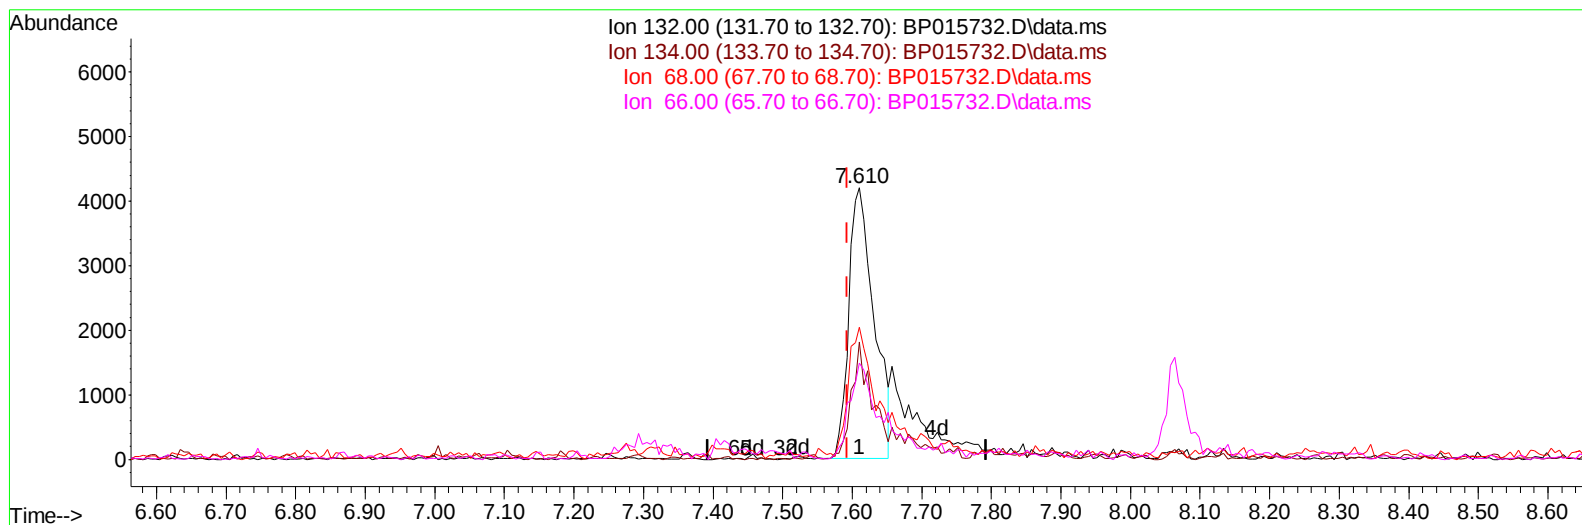

TIC: BP015732.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.610min (+ 0.018) 1.28 ng/u1

response 10498

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.40	43.40#
68.00	46.60	48.61
66.00	32.60	35.52




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

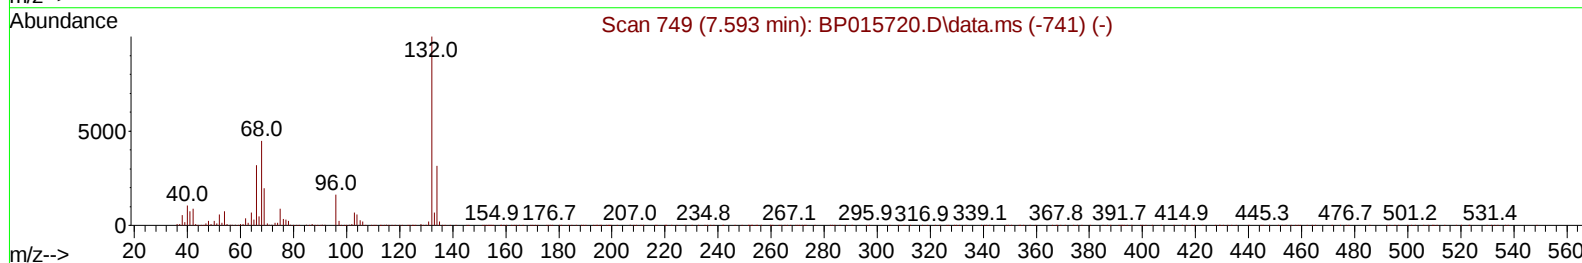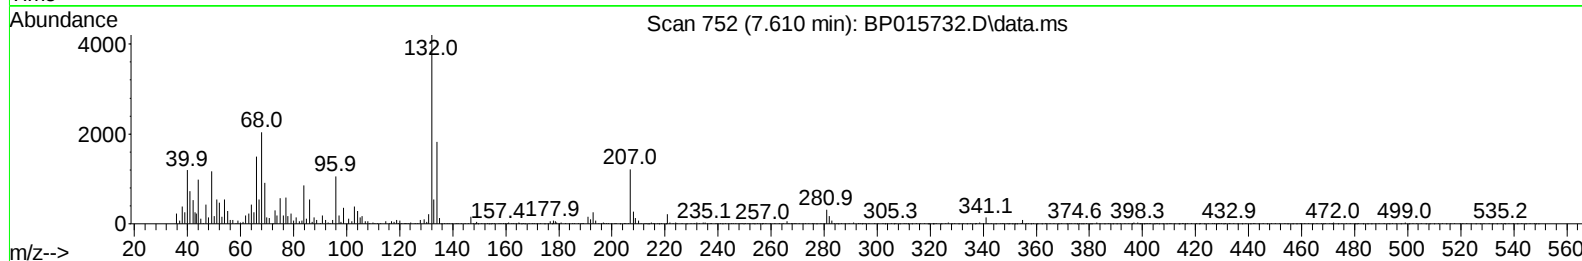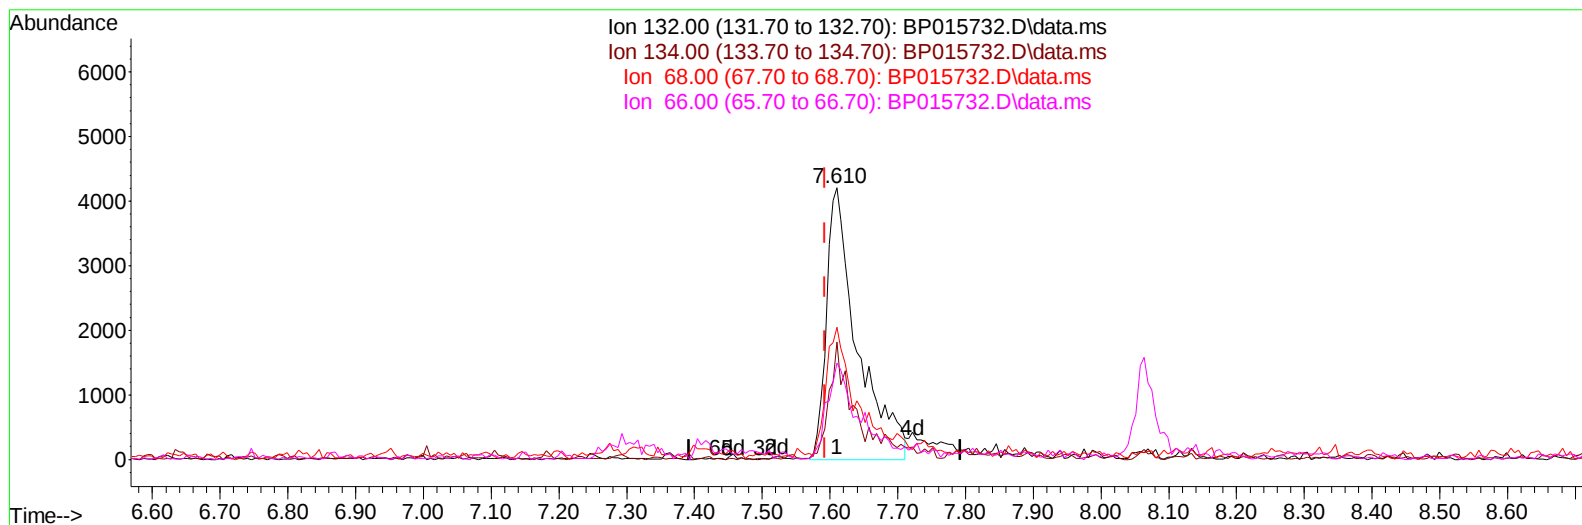

TIC: BP015732.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.610min (+ 0.018) 1.62 ng/ul m

response 13275

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.40	43.40#
68.00	46.60	48.61
66.00	32.60	35.52




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015732.D
Acq On : 27 Jun 2023 01:13
Operator : MA/JU
Sample : 03083-14DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

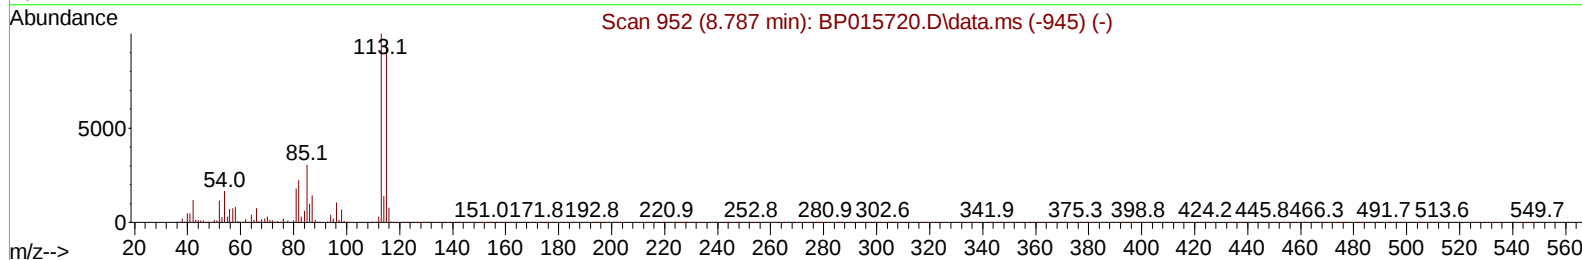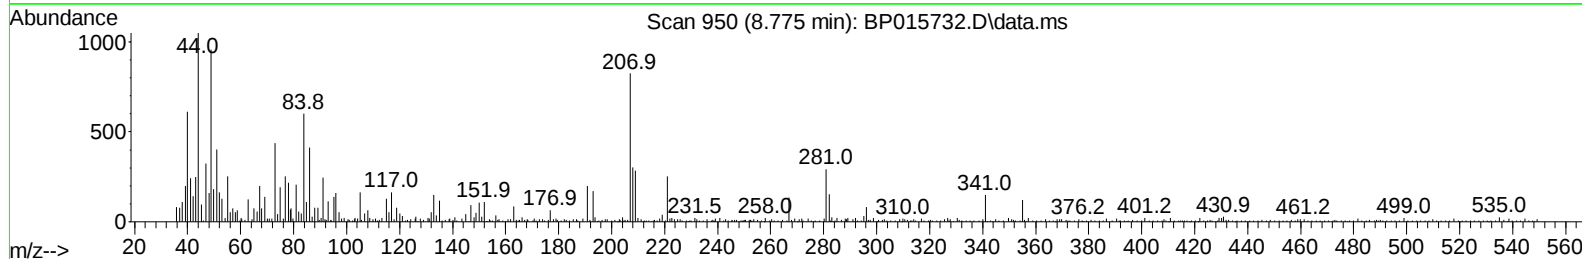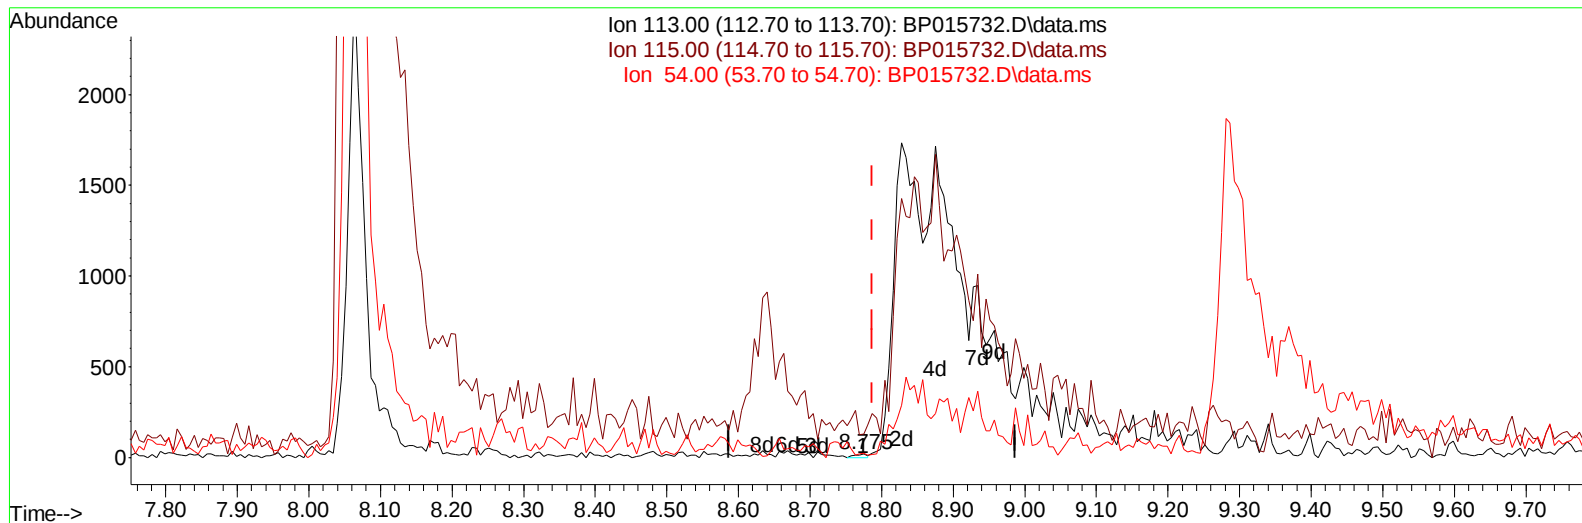

TIC: BP015732.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.775min (-0.012) 0.00 ng/u1

response 22

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	609.52#
54.00	16.10	104.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015732.D
Acq On : 27 Jun 2023 01:13
Operator : MA/JU
Sample : 03083-14DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 02:37:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

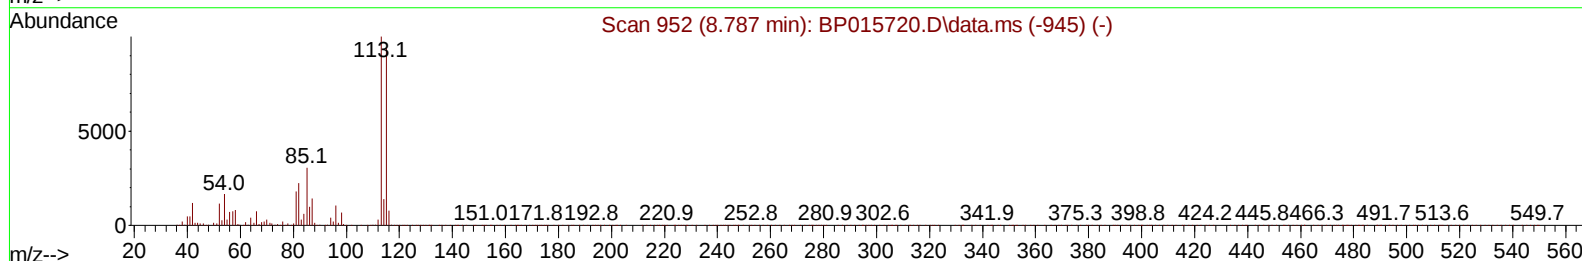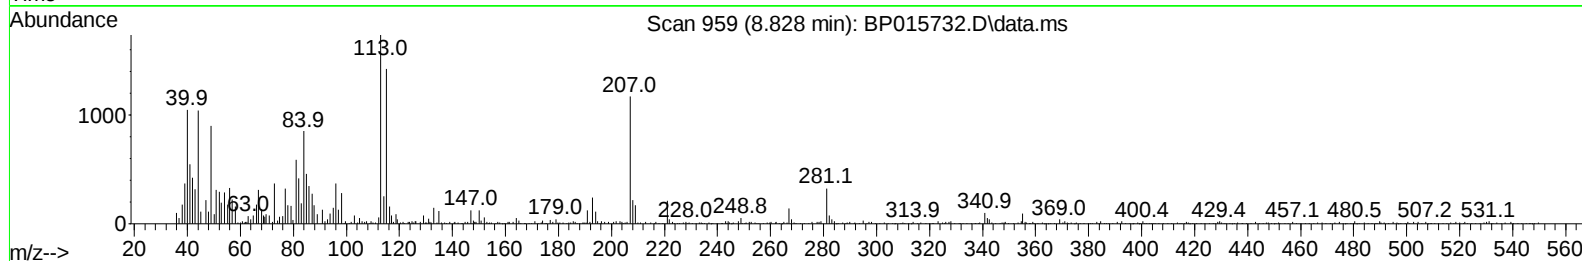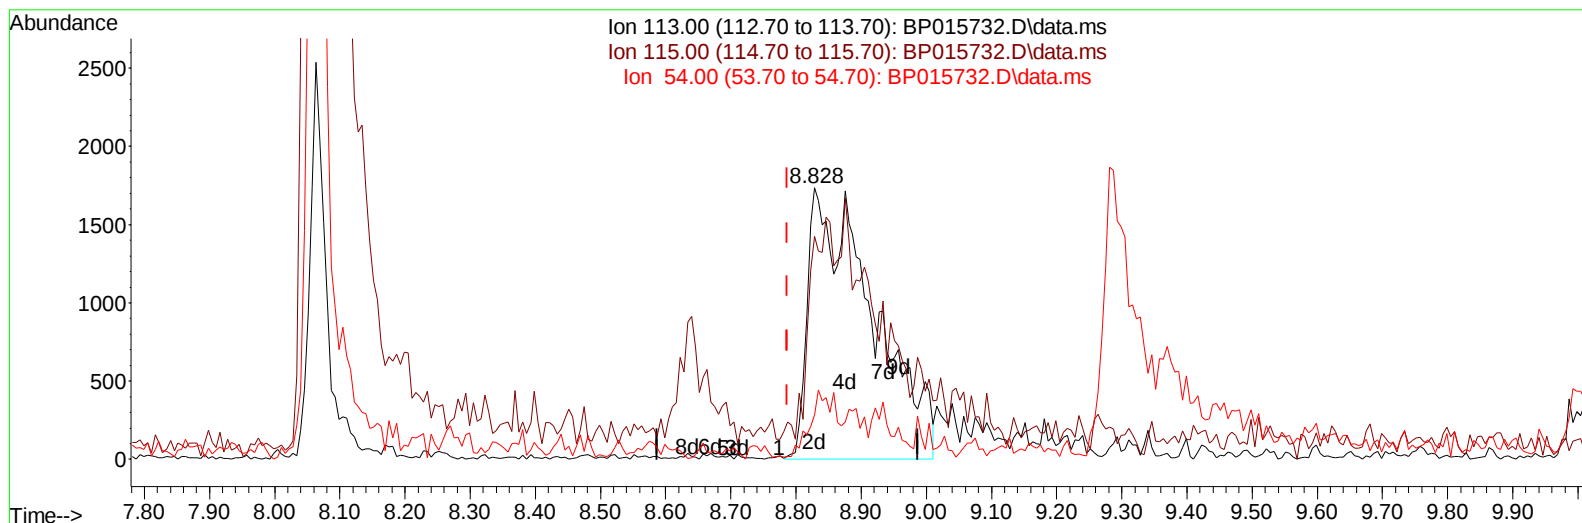

TIC: BP015732.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.828min (+ 0.041) 1.40 ng/ul m

response 12029

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	82.19
54.00	16.10	16.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

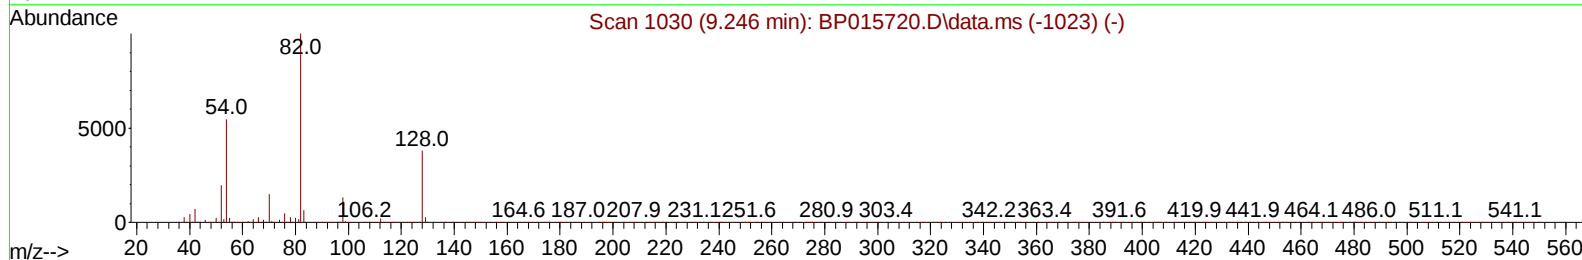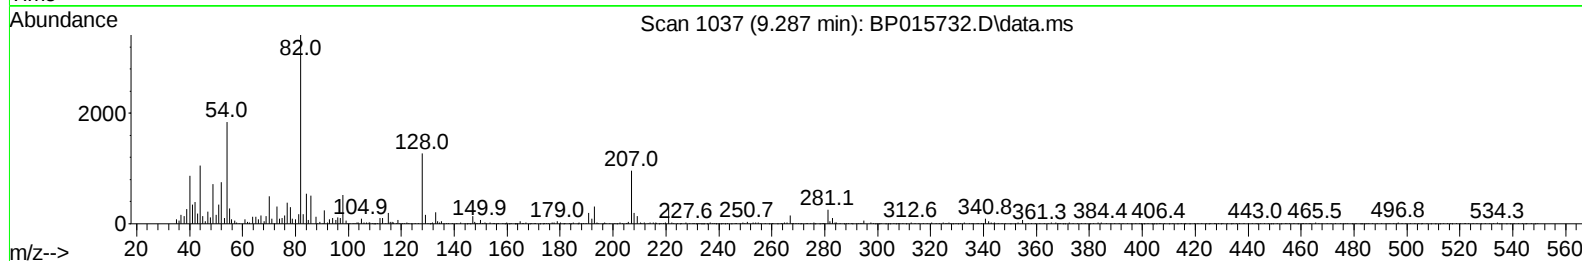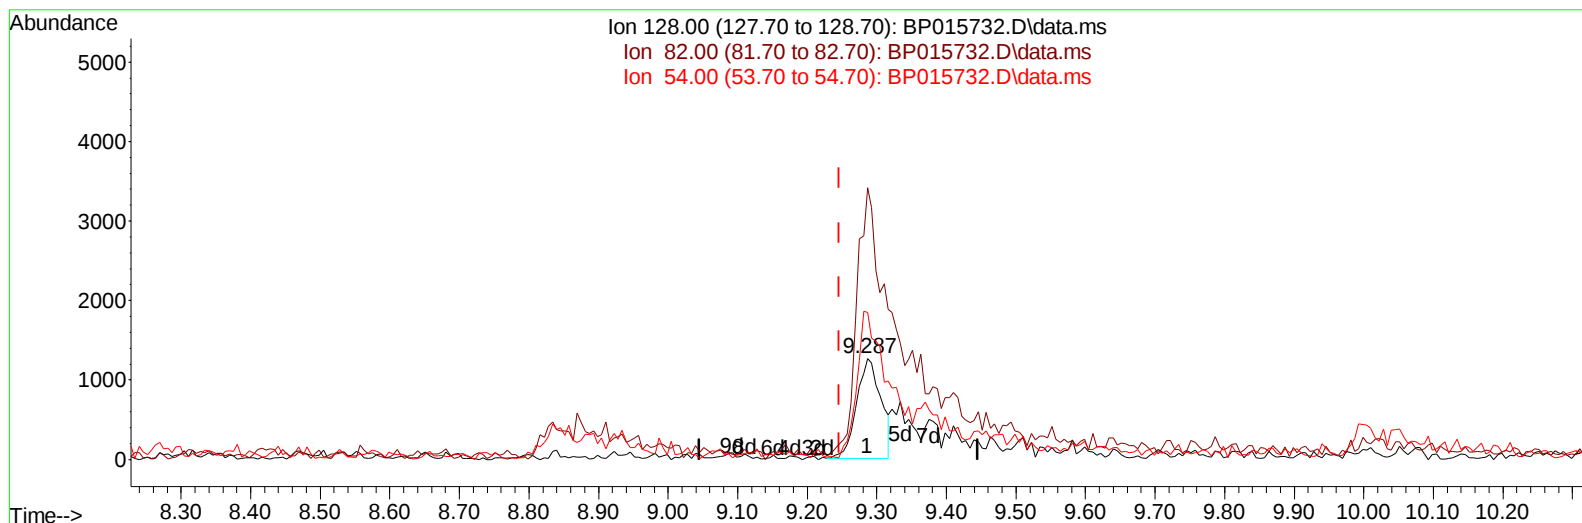

TIC: BP015732.D\data.ms

(21) Nitrobenzene-d5 (S)

9.287min (+ 0.041) 0.81 ng/u1

response 3034

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	268.42
54.00	141.60	144.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

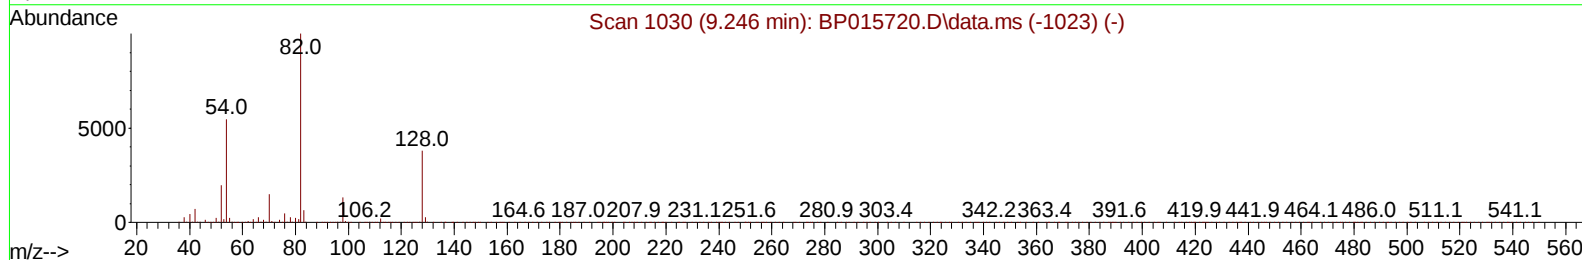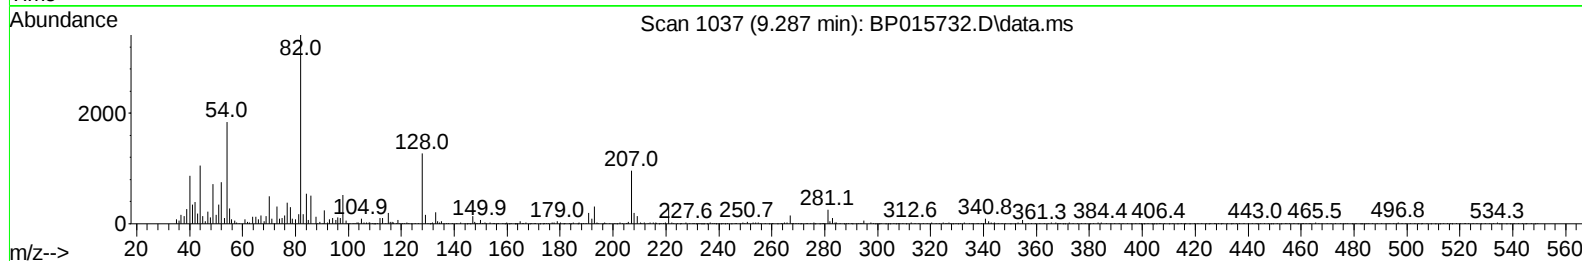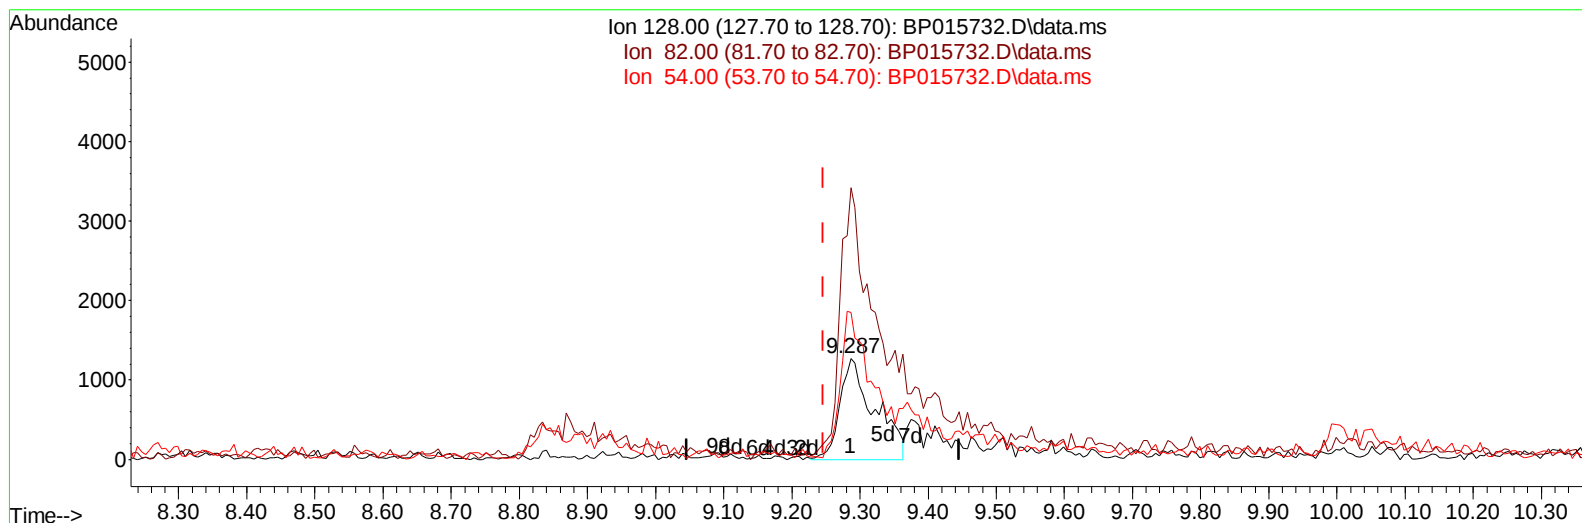

TIC: BP015732.D\data.ms

(21) Nitrobenzene-d5 (S)

9.287min (+ 0.041) 1.20 ng/ul m

response 4491

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	268.42
54.00	141.60	144.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015732.D
Acq On : 27 Jun 2023 01:13
Operator : MA/JU
Sample : 03083-14DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

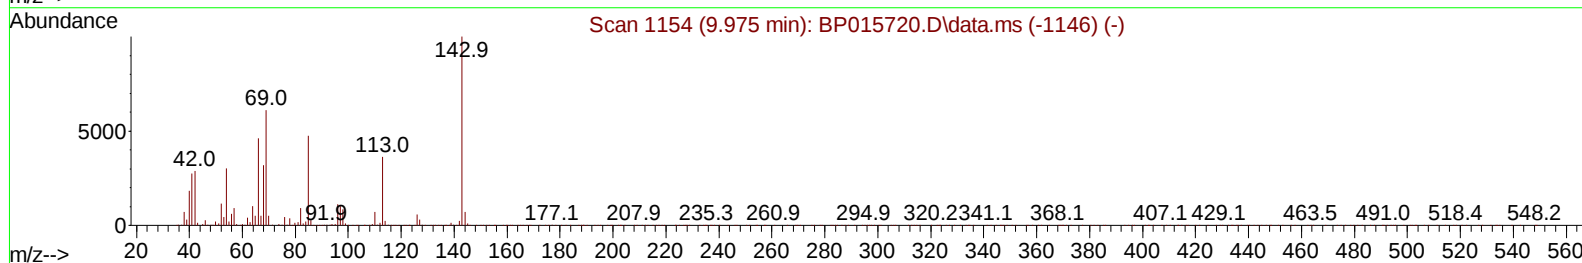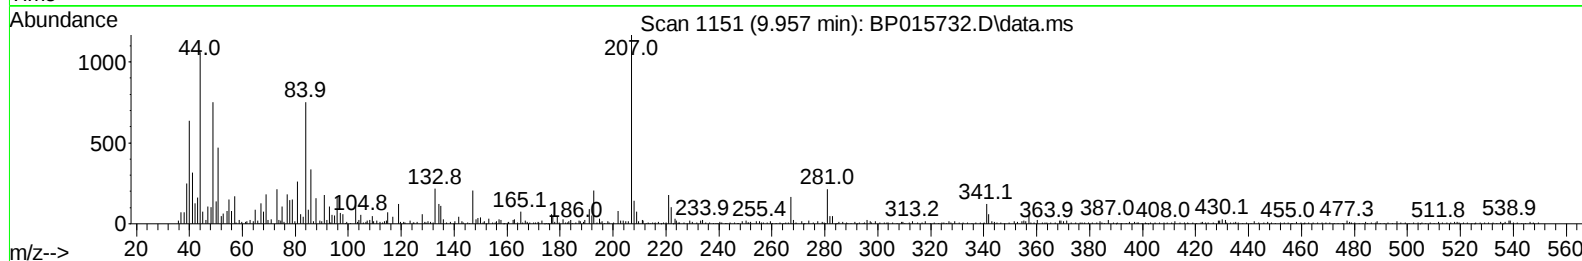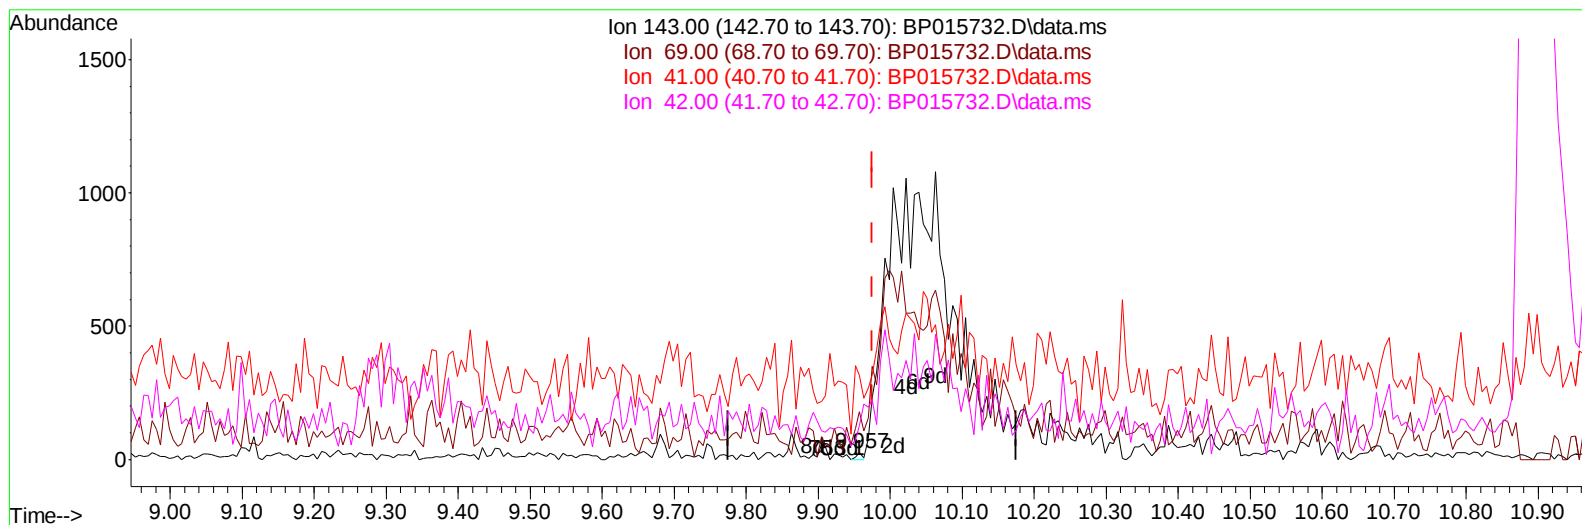

TIC: BP015732.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.957min (-0.018) 0.00 ng/u1

response 14

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	780.77#
41.00	26.80	1219.23#
42.00	30.50	488.46#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

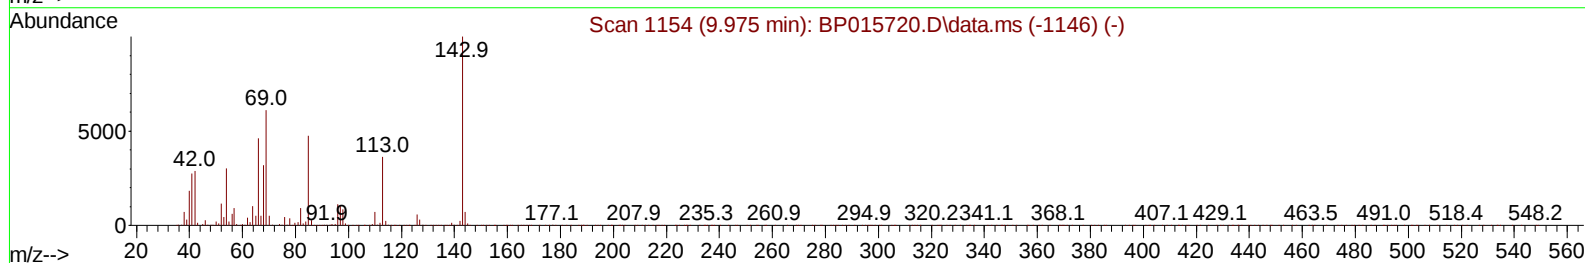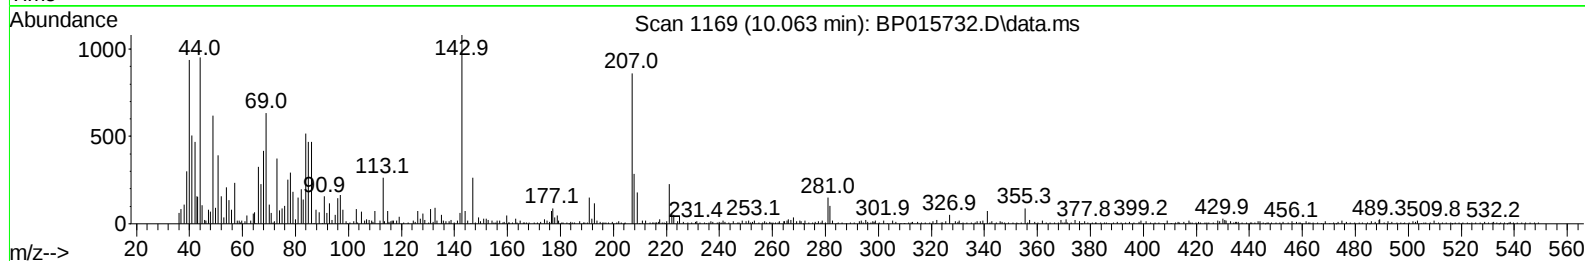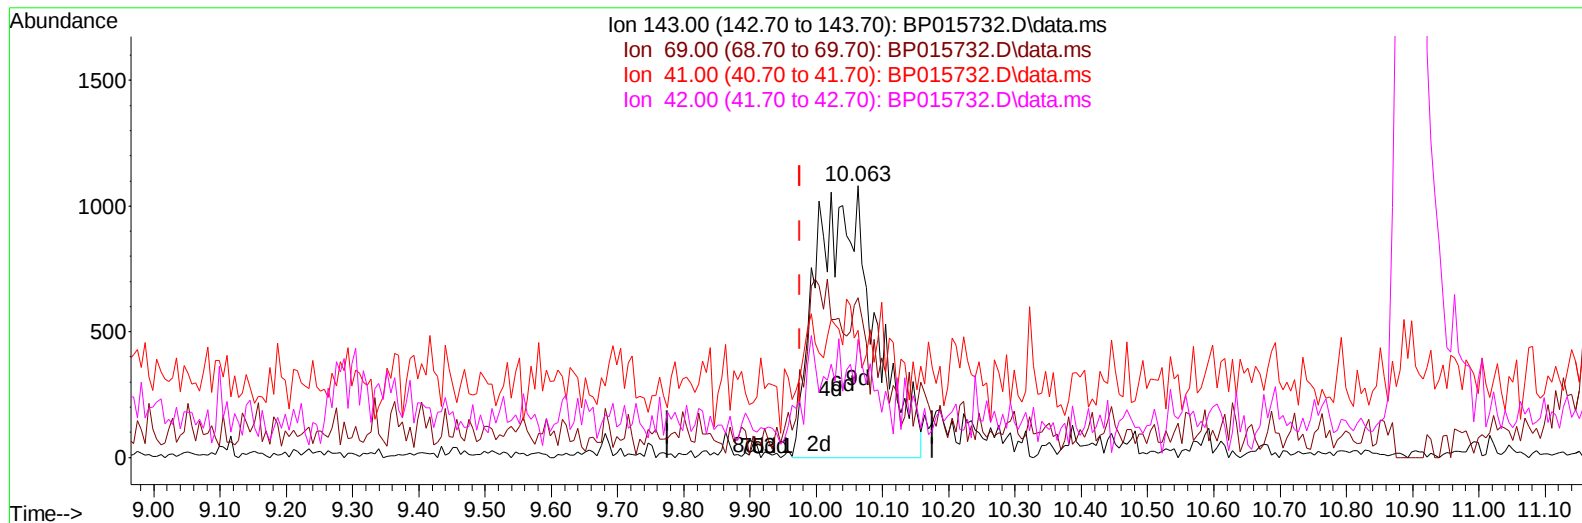

TIC: BP015732.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.063min (+ 0.088) 1.49 ng/ul m

response 6507

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	58.80
41.00	26.80	46.85#
42.00	30.50	43.43#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

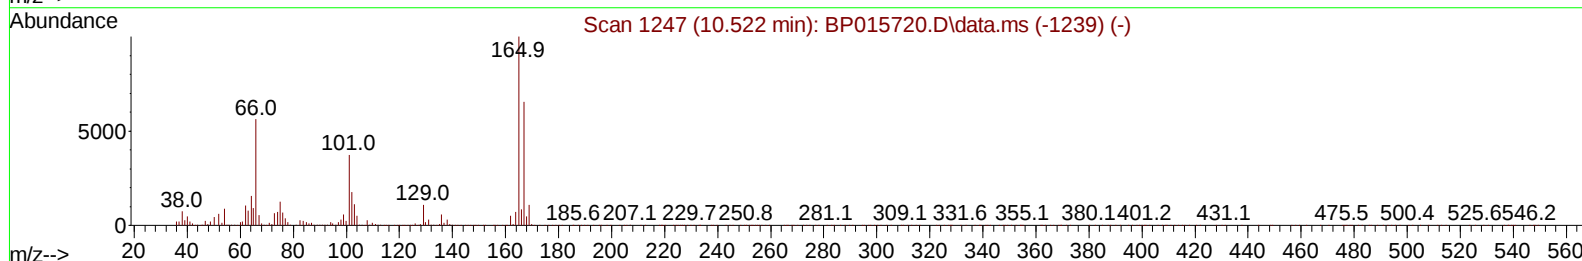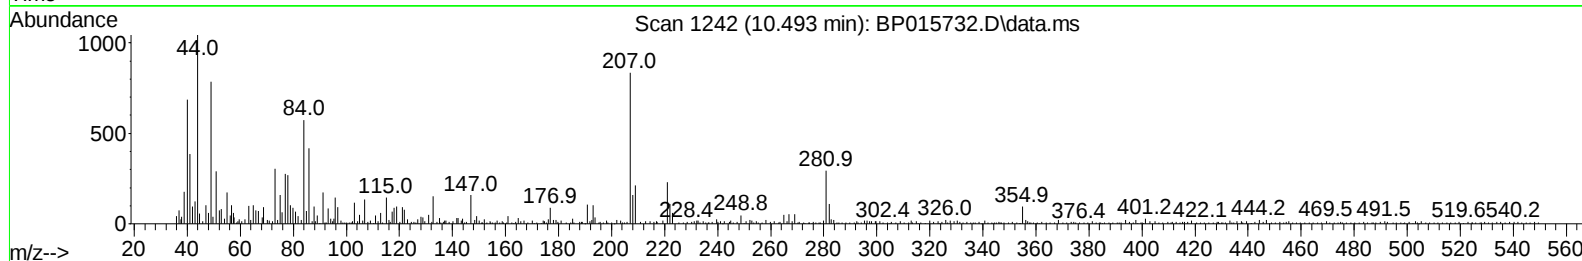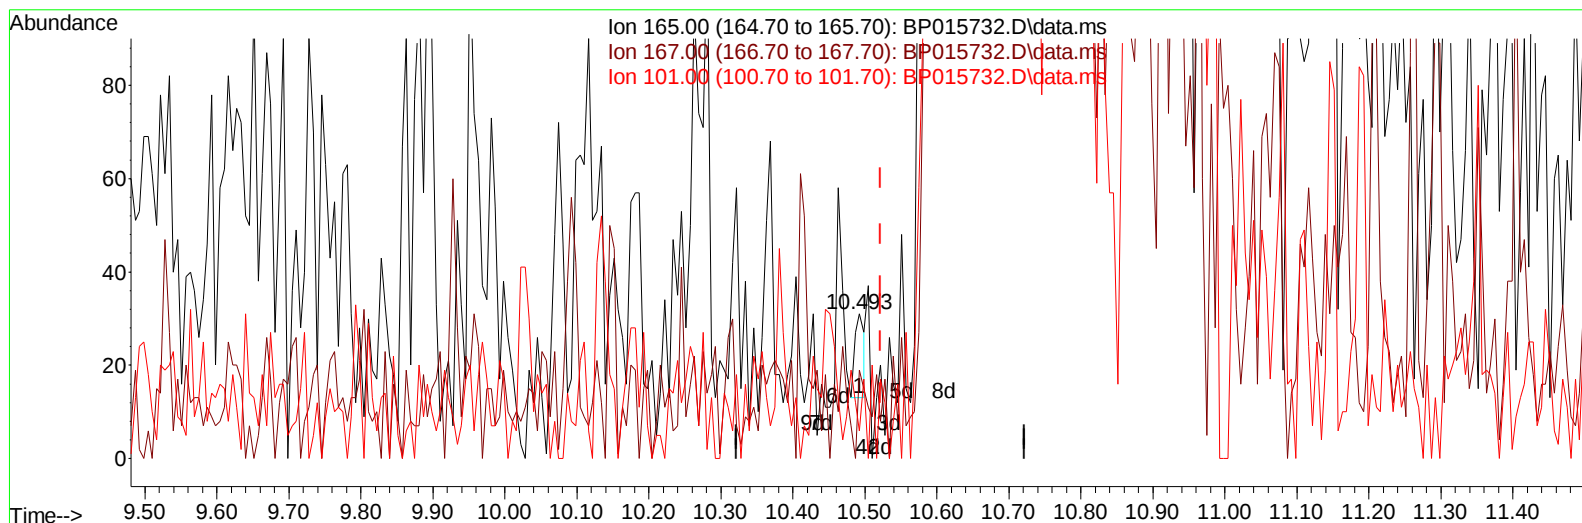

TIC: BP015732.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.493min (-0.029) 0.00 ng/u1

response 16

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	61.29
101.00	37.30	41.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:37:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

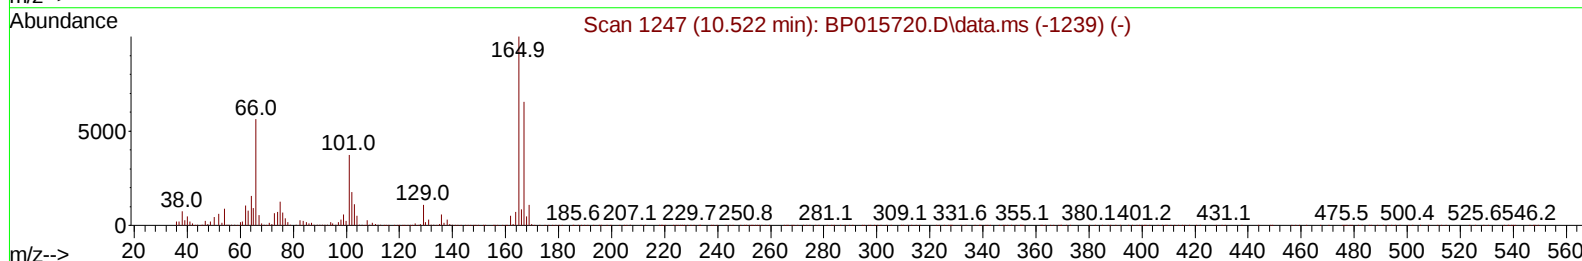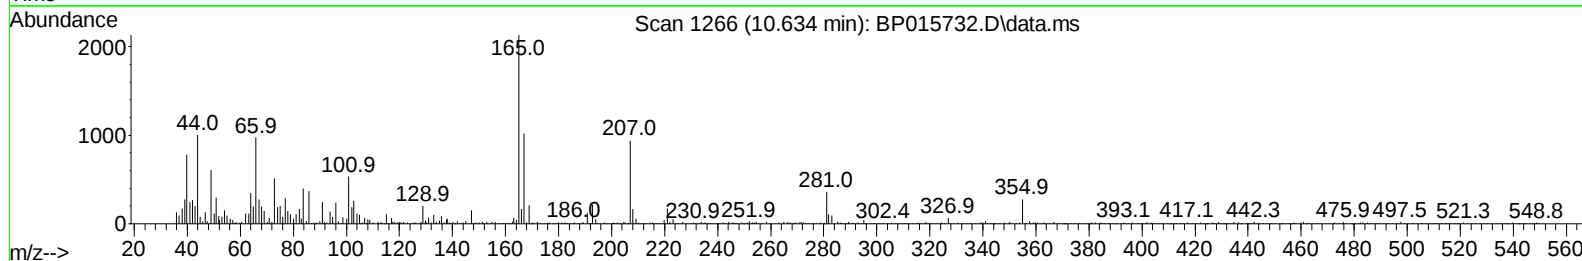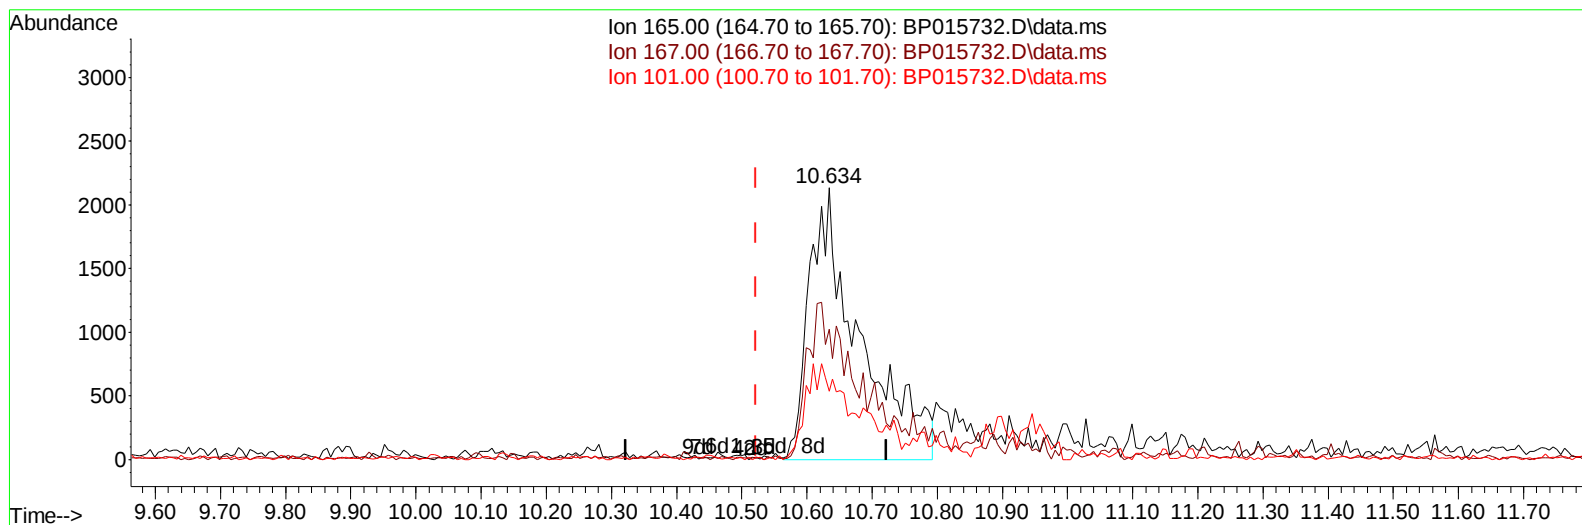

TIC: BP015732.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.634min (+ 0.112) 1.48 ng/ul m

response 11540

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	47.91#
101.00	37.30	25.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:38:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

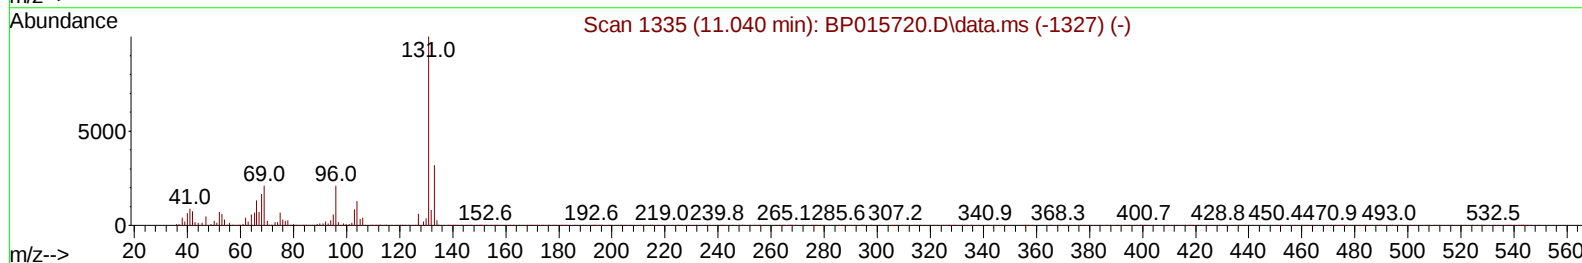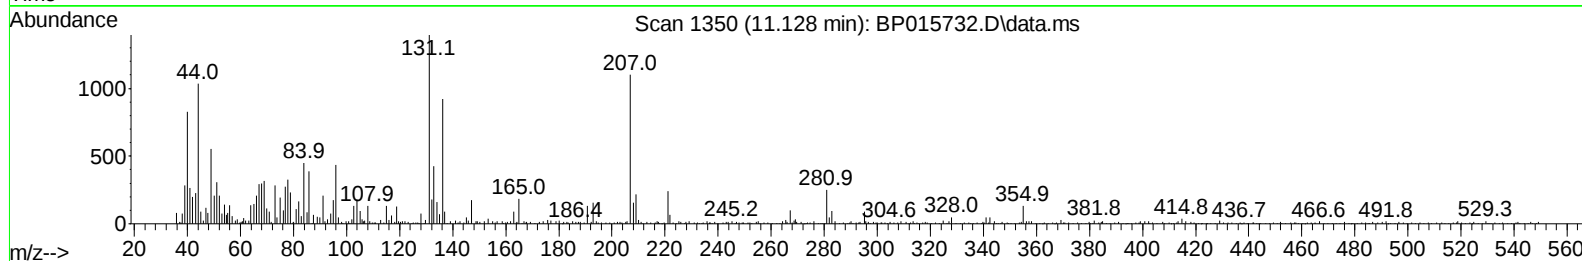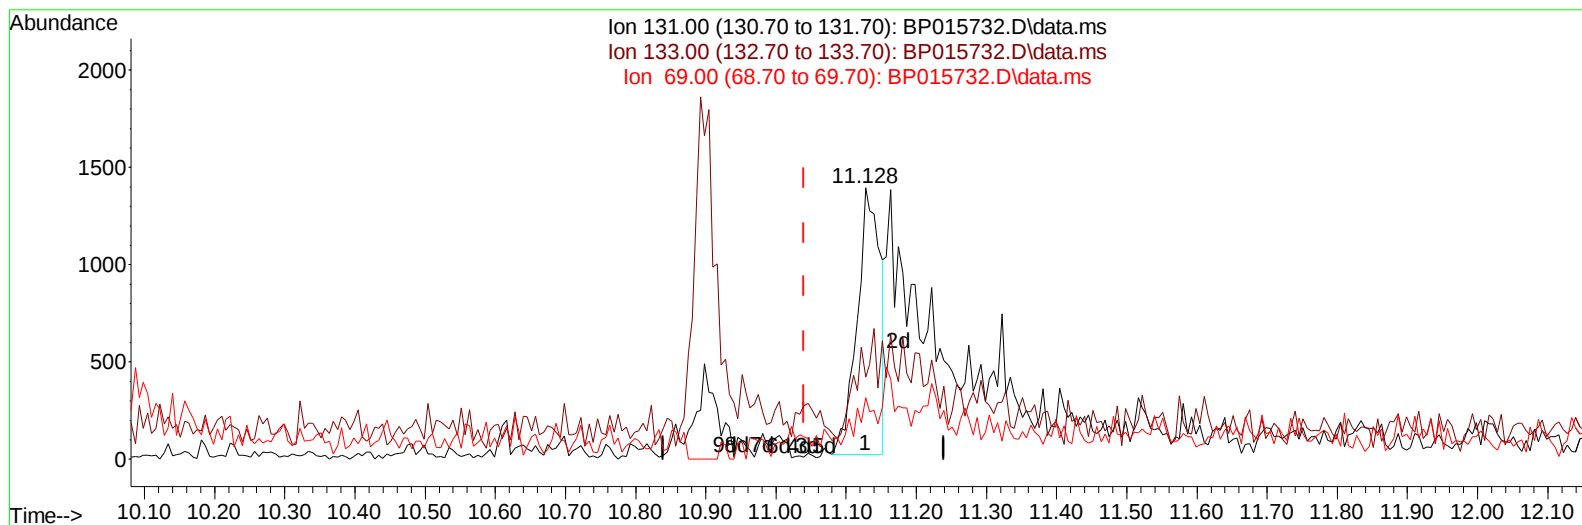

TIC: BP015732.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.128min (+ 0.088) 0.31 ng/u1

response 3078

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	30.39
69.00	22.20	22.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015732.D
Acq On : 27 Jun 2023 01:13
Operator : MA/JU
Sample : 03083-14DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:38:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :mohammad ahmed 06/27/2023

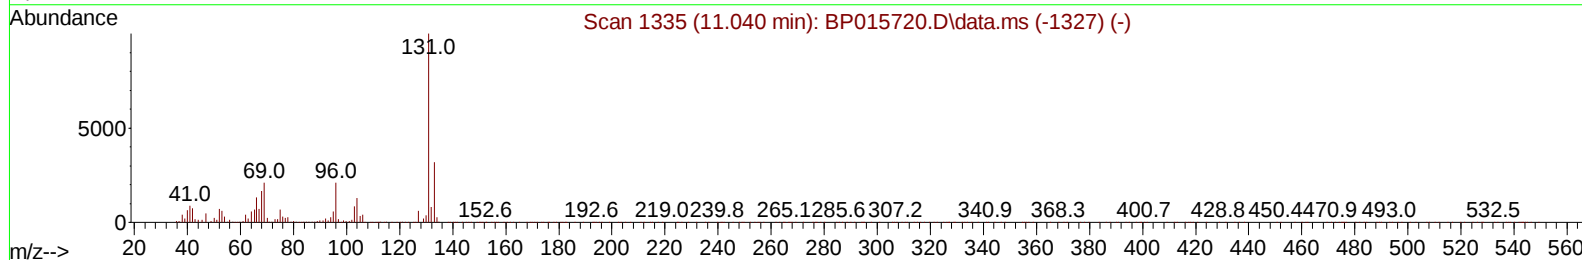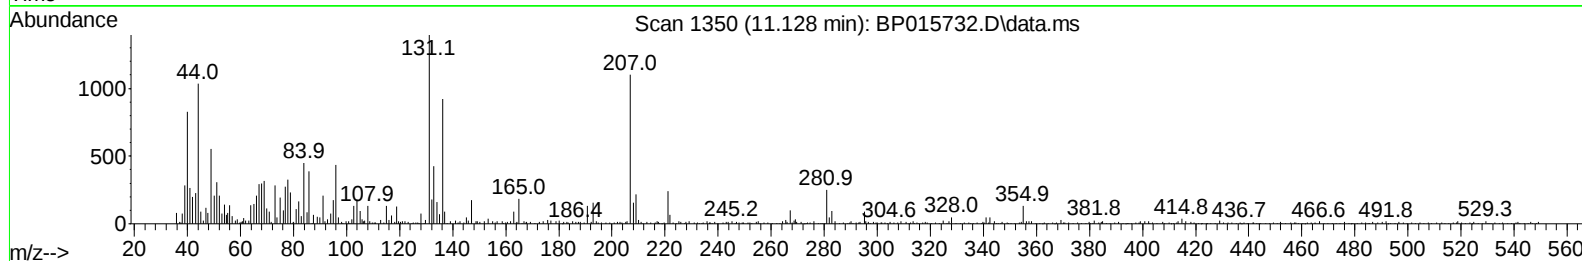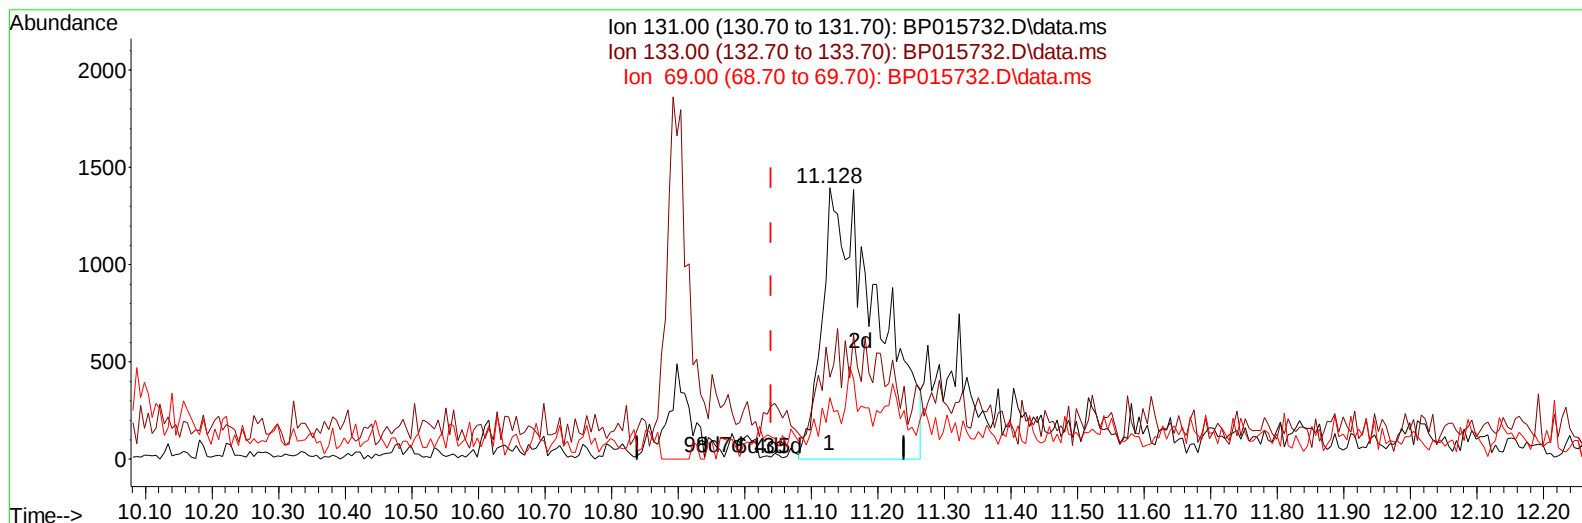

TIC: BP015732.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.128min (+ 0.088) 0.80 ng/ul m

response 8032

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	30.39
69.00	22.20	22.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:38:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

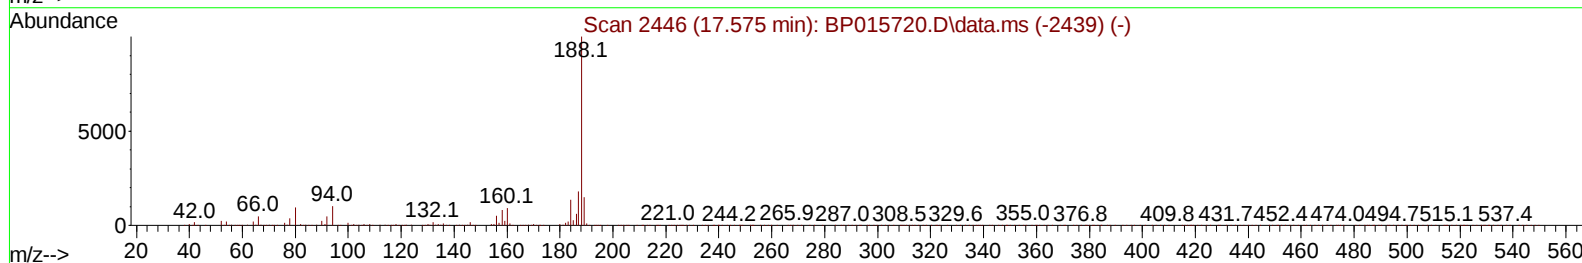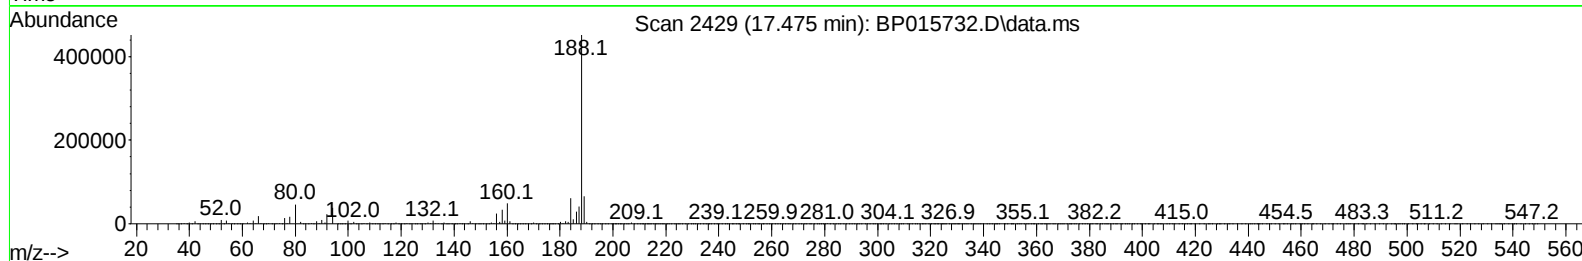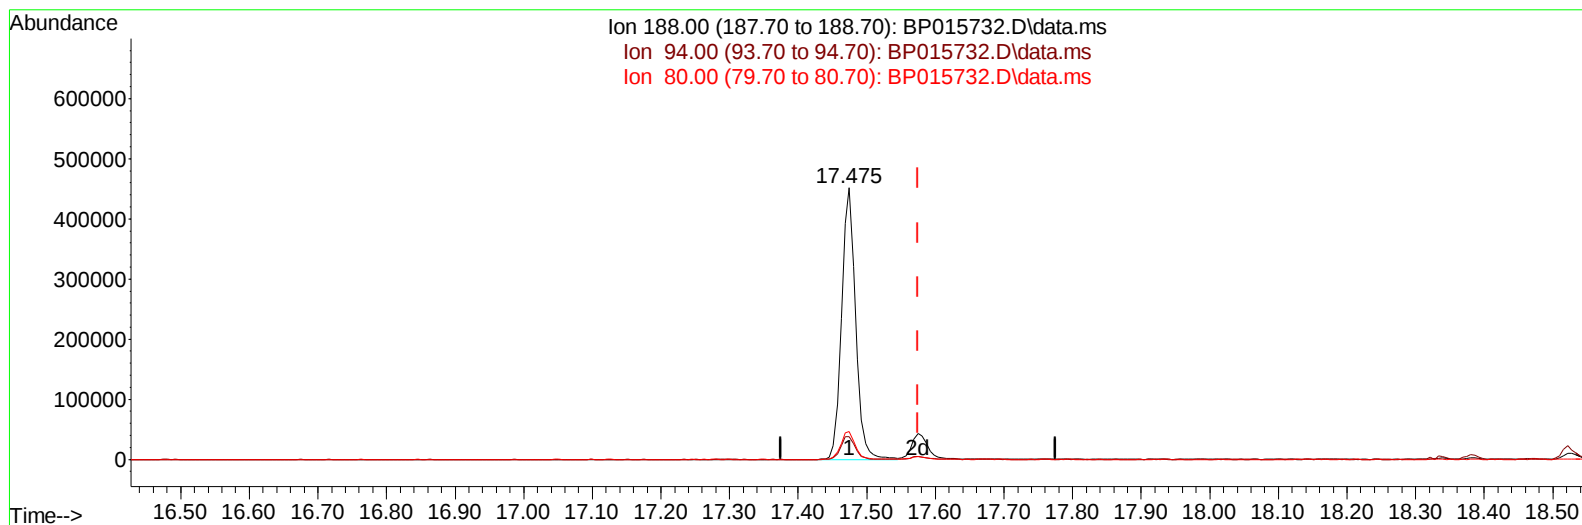

TIC: BP015732.D\data.ms

(73) Anthracene-d10 (S)

17.475min (-0.100) 21.89 ng/u1

response 641616

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.00	8.37
80.00	9.80	10.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:38:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

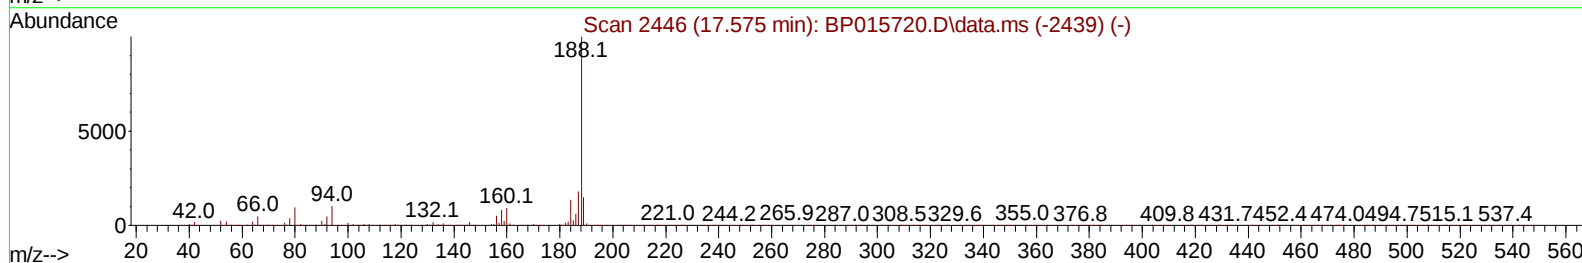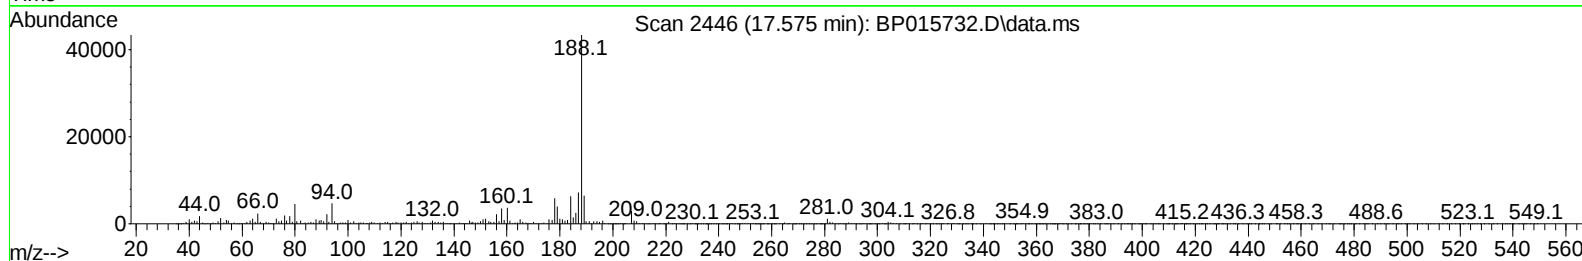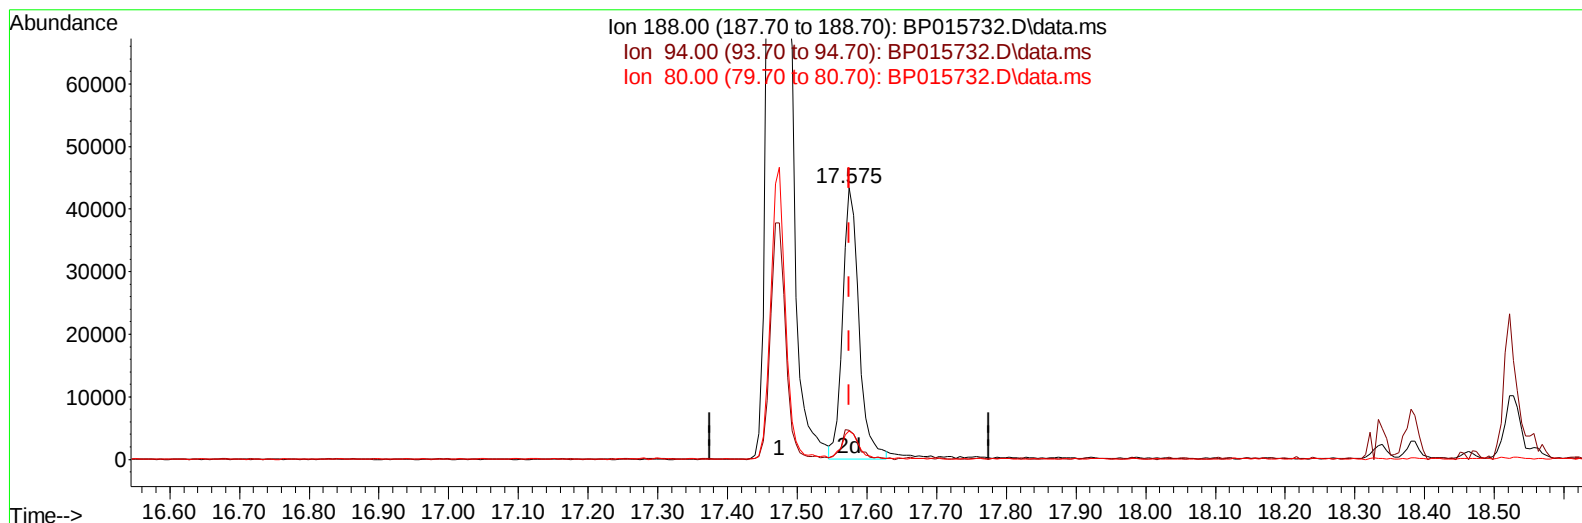

TIC: BP015732.D\data.ms

(73) Anthracene-d10 (S)

17.575min (-0.000) 2.40 ng/u1 m

response 70431

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.00	10.79
80.00	9.80	10.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015732.D
 Acq On : 27 Jun 2023 01:13
 Operator : MA/JU
 Sample : 03083-14DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFL2DL

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:39:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :mohammad ahmed 06/27/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	127146	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	488919	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	294145	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.475	188	641616	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	644488	20.000	ng/ul	0.00
88) Perylene-d12	24.110	264	789484	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.293	99	13143m	1.208	ng/ul	0.06
9) Bis-(2-Chloroethyl)eth...	7.405	67	8018	1.191	ng/ul	0.02
11) 2-Chlorophenol-d4	7.610	132	13275m	1.617	ng/ul	0.02
15) 4-Methylphenol-d8	8.828	113	12029m	1.400	ng/ul	0.04
21) Nitrobenzene-d5	9.287	128	4491m	1.202	ng/ul	0.04
24) 2-Nitrophenol-d4	10.063	143	6507m	1.492	ng/ul	0.09
28) 2,4-Dichlorophenol-d3	10.634	165	11540m	1.485	ng/ul	0.11
31) 4-Chloroaniline-d4	11.128	131	8032m	0.805	ng/ul	0.09
46) Dimethylphthalate-d6	14.134	166	43955	1.933	ng/ul	0.01
49) Acenaphthylene-d8	14.410	160	51903	2.031	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.716	176	41194	2.201	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.575	188	70431m	2.403	ng/ul	0.00
81) Pyrene-d10	19.798	212	82192	1.953	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.945	264	90442	2.271	ng/ul	0.00
Target Compounds						
					Qvalue	
52) Acenaphthene	14.781	153	49221	2.521	ng/ul	95
61) Fluorene	15.775	166	44054	2.004	ng/ul	99
72) Phenanthrene	17.516	178	991806	28.454	ng/ul	100
74) Anthracene	17.610	178	236536	6.753	ng/ul	99
80) Fluoranthene	19.474	202	2259400	43.199	ng/ul	100
82) Pyrene	19.827	202	1884347	35.319	ng/ul	99
85) Benzo(a)anthracene	21.545	228	1189802	26.244	ng/ul	98
87) Chrysene	21.604	228	1057281	24.580	ng/ul	97
90) Benzo(b)fluoranthene	23.333	252	1512185	29.810	ng/ul	98
91) Benzo(k)fluoranthene	23.374	252	495811	9.674	ng/ul	96
93) Benzo(a)pyrene	23.998	252	987534	22.279	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.809	276	701612	11.660	ng/ul	99
95) Dibenzo(a,h)anthracene	26.809	278	201020	4.067	ng/ul#	83
96) Benzo(g,h,i)perylene	27.651	276	613415	12.392	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

