

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015721.D
 Acq On : 26 Jun 2023 19:01
 Operator : MA/JU
 Sample : PB153446BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	43	rVB	52319	69307	2.52%	0.209%
2	3.828	107	109	125	rBV	464402	764576	27.82%	2.310%
3	4.158	161	165	174	rVB3	11000	20020	0.73%	0.060%
4	4.705	255	258	259	rBV3	3156	2953	0.11%	0.009%
5	5.334	363	365	370	rVB6	3081	4580	0.17%	0.014%
6	6.340	531	536	537	rBV5	3088	3459	0.13%	0.010%
7	6.875	625	627	629	rBV3	2739	3111	0.11%	0.009%
8	7.228	679	687	704	rBV	473643	1014857	36.93%	3.067%
9	7.387	706	714	729	rVV	454637	777752	28.30%	2.350%
10	7.593	742	749	766	rBV	616554	1082150	39.37%	3.270%
11	8.063	822	829	845	rBV	484013	882134	32.10%	2.666%
12	8.405	882	887	889	rVB6	2307	3245	0.12%	0.010%
13	8.434	889	892	895	rBV5	2046	3160	0.11%	0.010%
14	8.793	944	953	968	rBV	618254	1273113	46.32%	3.847%
15	9.252	1023	1031	1048	rBV	527001	1057850	38.49%	3.197%
16	9.975	1145	1154	1172	rBV	453564	938521	34.15%	2.836%
17	10.528	1240	1248	1273	rBV	442787	1229726	44.74%	3.716%
18	10.893	1302	1310	1328	rVB	704031	1205632	43.87%	3.643%
19	11.052	1328	1337	1368	rBV	404911	1248603	45.43%	3.773%
20	11.616	1432	1433	1440	rVB7	2344	3078	0.11%	0.009%
21	12.099	1511	1515	1520	rVB8	3260	5343	0.19%	0.016%
22	12.528	1582	1588	1591	rBV3	8358	15845	0.58%	0.048%
23	12.975	1661	1664	1669	rVB7	1830	3456	0.13%	0.010%
24	13.598	1766	1770	1776	rBV7	7402	14631	0.53%	0.044%
25	14.122	1850	1859	1878	rBV	1152277	1902578	69.23%	5.749%
26	14.410	1900	1908	1927	rBV	1408146	2207321	80.32%	6.670%
27	14.716	1951	1960	1971	rBV	968904	1526182	55.53%	4.612%
28	14.969	1997	2003	2020	rBV2	144898	547940	19.94%	1.656%
29	15.634	2112	2116	2120	rBV7	2975	4218	0.15%	0.013%
30	15.716	2122	2130	2148	rBV	1435295	2577107	93.77%	7.788%
31	15.869	2150	2156	2169	rBV	231740	584664	21.27%	1.767%
32	16.498	2261	2263	2266	rBV4	3118	4283	0.16%	0.013%
33	16.892	2328	2330	2334	rVB5	3233	3727	0.14%	0.011%
34	17.134	2368	2371	2373	rBV4	3371	4386	0.16%	0.013%
35	17.157	2373	2375	2378	rVV4	3243	3450	0.13%	0.010%
36	17.263	2391	2393	2398	rBV6	2191	3819	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015721.D
Acq On : 26 Jun 2023 19:01
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	17.475	2423	2429	2441	rBV	1092626	1643578	59.80%	4.967%
38	17.581	2441	2447	2471	rVB	1367925	2571495	93.57%	7.771%
39	19.380	2751	2753	2757	rVB3	18309	20540	0.75%	0.062%
40	19.810	2820	2826	2844	rBV	1494447	2748328	100.00%	8.305%
41	21.574	3121	3126	3137	rBV2	705031	1406912	51.19%	4.251%
42	23.951	3523	3530	3547	rVB2	984717	2426606	88.29%	7.333%
43	24.121	3553	3559	3574	rVB	489400	1278441	46.52%	3.863%




Sum of corrected areas: 33092677

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015721.D
Acq On : 26 Jun 2023 19:01
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

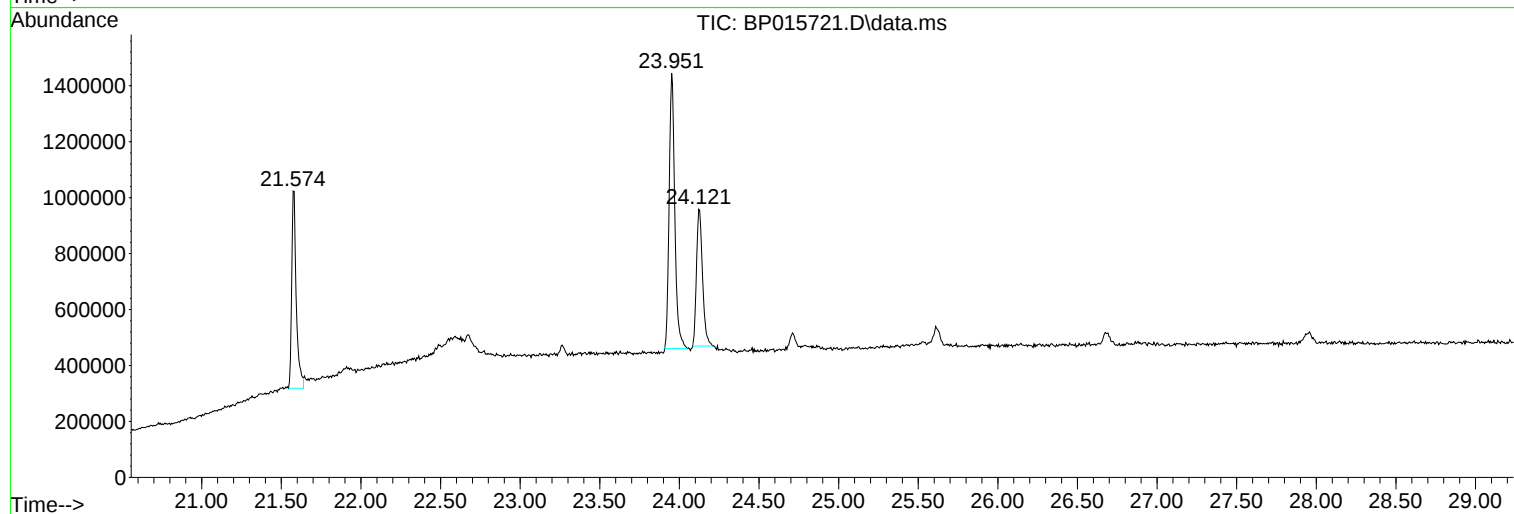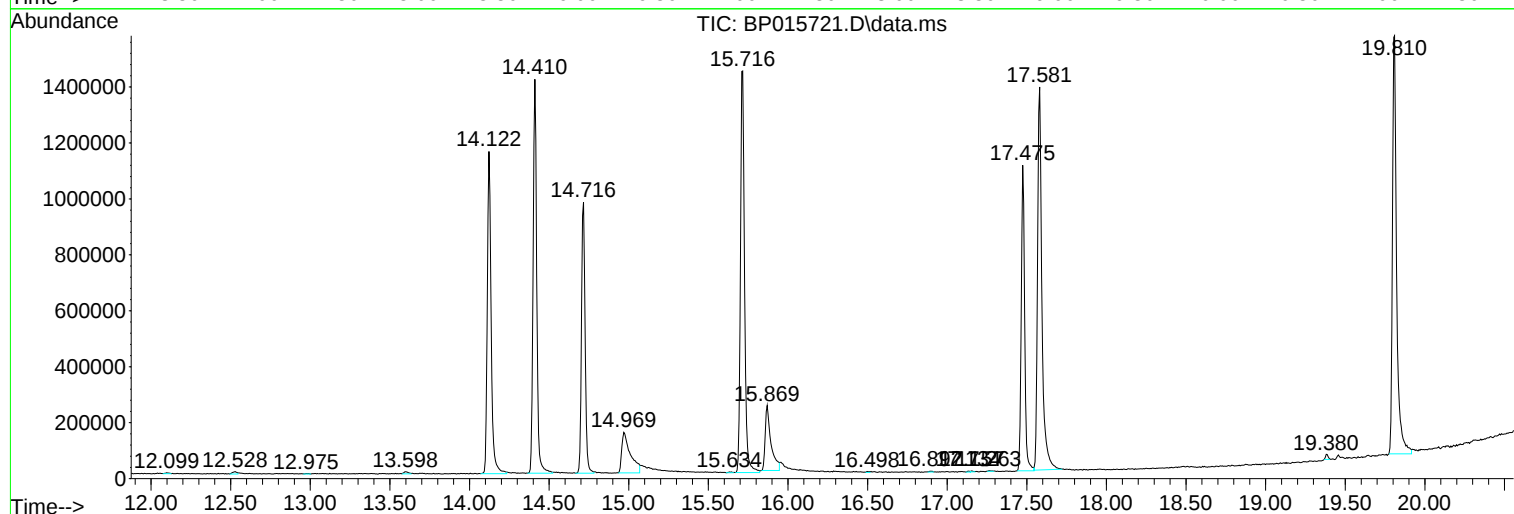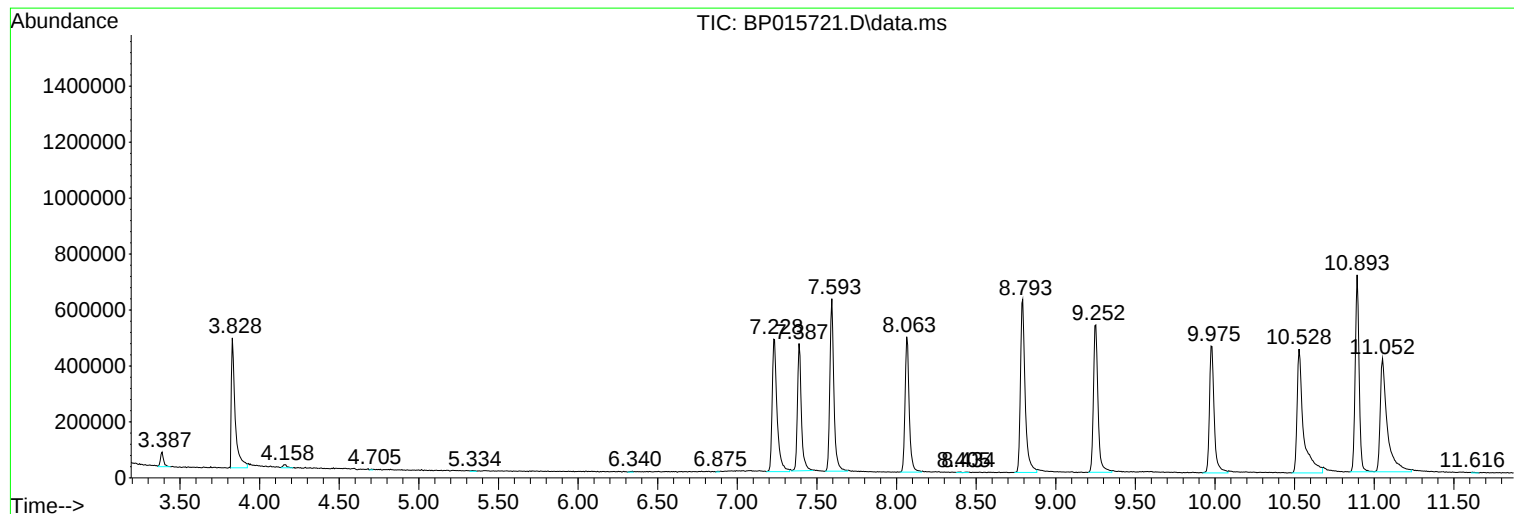

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015721.D
Acq On : 26 Jun 2023 19:01
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015721.D
Acq On : 26 Jun 2023 19:01
Operator : MA/JU
Sample : PB153446BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------