

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015729.D
 Acq On : 26 Jun 2023 23:32
 Operator : MA/JU
 Sample : 03085-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.934	124	127	131	rVB5	7435	9578	0.47%	0.044%
2	4.058	143	148	156	rVB	19780	37177	1.83%	0.170%
3	4.158	162	165	170	rBV2	9571	12597	0.62%	0.058%
4	4.334	193	195	198	rBV4	3447	3625	0.18%	0.017%
5	4.734	259	263	265	rBV5	2555	3695	0.18%	0.017%
6	4.805	274	275	278	rBV3	2039	2268	0.11%	0.010%
7	5.105	324	326	330	rVB4	4551	6332	0.31%	0.029%
8	5.222	344	346	348	rBV3	2425	2277	0.11%	0.010%
9	5.452	383	385	391	rBV7	2899	4343	0.21%	0.020%
10	6.311	527	531	537	rBV9	2720	5202	0.26%	0.024%
11	6.411	544	548	551	rBV6	1342	2575	0.13%	0.012%
12	6.605	579	581	589	rVB8	2694	2391	0.12%	0.011%
13	6.693	591	596	597	rBV5	2675	3368	0.17%	0.015%
14	6.705	597	598	608	rVB9	5587	9787	0.48%	0.045%
15	7.152	671	674	679	rVB7	2764	4332	0.21%	0.020%
16	7.234	681	688	708	rVV	224665	525686	25.83%	2.405%
17	7.387	708	714	731	rVB	210478	381566	18.75%	1.746%
18	7.593	742	749	764	rBV	308502	567697	27.89%	2.597%
19	8.063	821	829	842	rBV	545139	961777	47.25%	4.400%
20	8.575	915	916	921	rVB5	1867	2678	0.13%	0.012%
21	8.799	945	954	968	rBV	233684	543141	26.68%	2.485%
22	8.910	969	973	991	rVV	39638	102444	5.03%	0.469%
23	9.063	995	999	1002	rVB6	1935	2523	0.12%	0.012%
24	9.252	1024	1031	1047	rBV	228316	484477	23.80%	2.217%
25	9.599	1088	1090	1092	rBV3	2718	3003	0.15%	0.014%
26	9.646	1096	1098	1101	rBV3	2119	2645	0.13%	0.012%
27	9.981	1147	1155	1171	rBV	190323	430010	21.13%	1.967%
28	10.228	1193	1197	1200	rVB6	1969	3058	0.15%	0.014%
29	10.257	1200	1202	1205	rBV4	1955	2120	0.10%	0.010%
30	10.352	1214	1218	1219	rBV4	2478	2967	0.15%	0.014%
31	10.540	1242	1250	1275	rBV	174202	578427	28.42%	2.647%
32	10.893	1300	1310	1324	rBV	661513	1216774	59.78%	5.567%
33	11.063	1331	1339	1363	rBV	138425	472225	23.20%	2.161%
34	11.504	1411	1414	1417	rBV5	1887	2366	0.12%	0.011%
35	11.875	1476	1477	1485	rVB8	1904	3633	0.18%	0.017%
36	11.957	1488	1491	1495	rBV6	1637	3094	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
 Data File : BP015729.D
 Acq On : 26 Jun 2023 23:32
 Operator : MA/JU
 Sample : 03085-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	12.040	1502	1505	1508	rBV5	1642	2620	0.13%	0.012%
38	12.357	1556	1559	1561	rBV4	2263	2133	0.10%	0.010%
39	12.681	1607	1614	1615	rBV7	1583	3167	0.16%	0.014%
40	12.987	1663	1666	1668	rBV3	1564	2270	0.11%	0.010%
41	13.063	1675	1679	1682	rBV6	3028	5135	0.25%	0.023%
42	13.104	1682	1686	1689	rVB6	2377	4466	0.22%	0.020%
43	13.210	1699	1704	1706	rBV6	1350	2220	0.11%	0.010%
44	13.316	1720	1722	1725	rVB4	2436	2579	0.13%	0.012%
45	13.587	1762	1768	1776	rBV6	11825	25509	1.25%	0.117%
46	13.698	1783	1787	1789	rBV5	7531	9540	0.47%	0.044%
47	13.775	1795	1800	1803	rBV7	1722	3447	0.17%	0.016%
48	14.022	1837	1842	1847	rVB4	24127	35380	1.74%	0.162%
49	14.122	1852	1859	1872	rBV	487006	805230	39.56%	3.684%
50	14.210	1872	1874	1884	rVB	5088	11196	0.55%	0.051%
51	14.410	1901	1908	1922	rBV	606111	976558	47.98%	4.468%
52	14.610	1939	1942	1945	rBV5	2448	2429	0.12%	0.011%
53	14.657	1945	1950	1953	rBV7	8472	12974	0.64%	0.059%
54	14.716	1953	1960	1977	rVV	907797	1442517	70.87%	6.600%
55	14.998	2002	2008	2026	rBV4	47171	227772	11.19%	1.042%
56	15.340	2064	2066	2068	rBV3	3365	3463	0.17%	0.016%
57	15.716	2123	2130	2143	rBV	638883	1159720	56.98%	5.306%
58	15.869	2150	2156	2167	rBV2	100868	242342	11.91%	1.109%
59	16.087	2189	2193	2198	rVB3	10524	16738	0.82%	0.077%
60	16.181	2205	2209	2214	rVB8	9643	16003	0.79%	0.073%
61	16.734	2301	2303	2307	rBV5	3596	4632	0.23%	0.021%
62	17.104	2364	2366	2369	rBV4	4501	4483	0.22%	0.021%
63	17.475	2423	2429	2440	rBV	1100332	1664300	81.77%	7.615%
64	17.575	2440	2446	2462	rVB	654825	1167889	57.38%	5.344%
65	18.333	2571	2575	2581	rBV2	51703	92651	4.55%	0.424%
66	19.804	2820	2825	2833	rBV	1006874	1567382	77.00%	7.171%
67	21.569	3120	3125	3134	rBV	1248102	1970876	96.83%	9.017%
68	23.945	3523	3529	3538	rVB2	835465	1931332	94.89%	8.837%
69	24.116	3552	3558	3569	rVB	914066	2035437	100.00%	9.313%




Sum of corrected areas: 21856248

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015729.D
Acq On : 26 Jun 2023 23:32
Operator : MA/JU
Sample : 03085-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

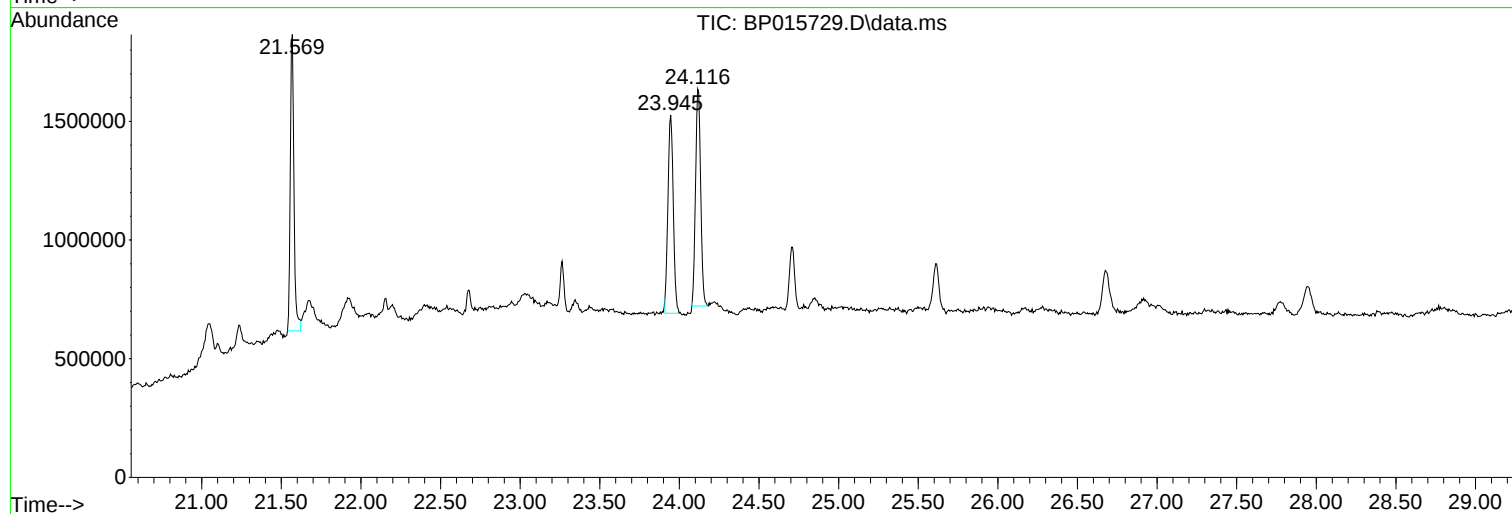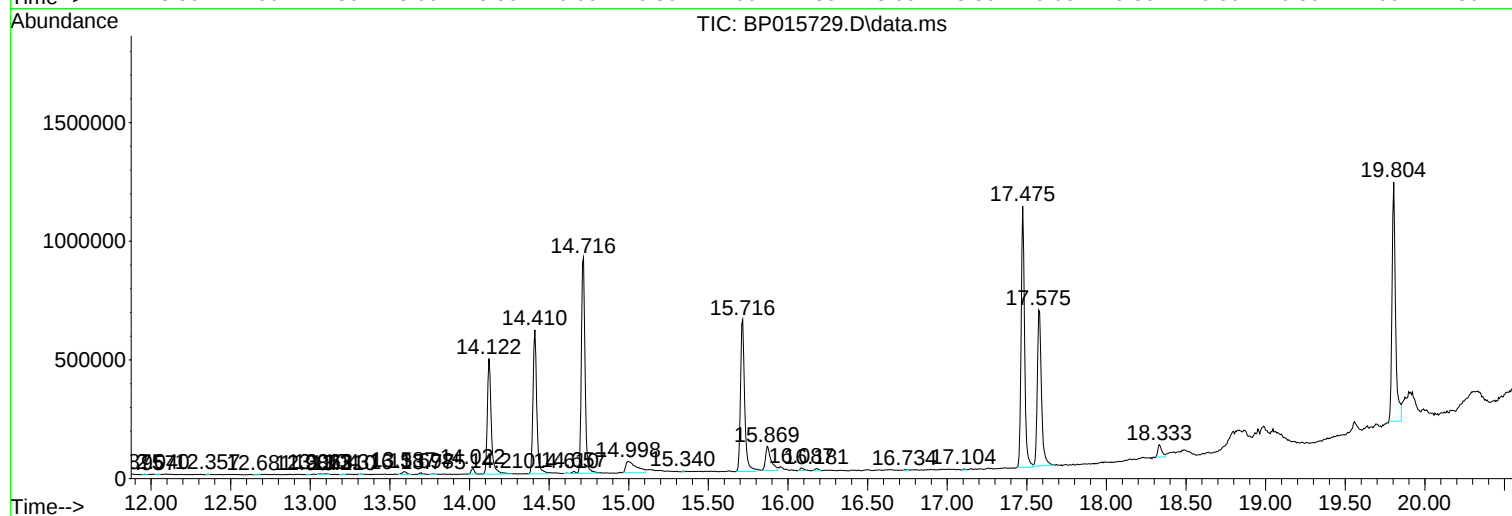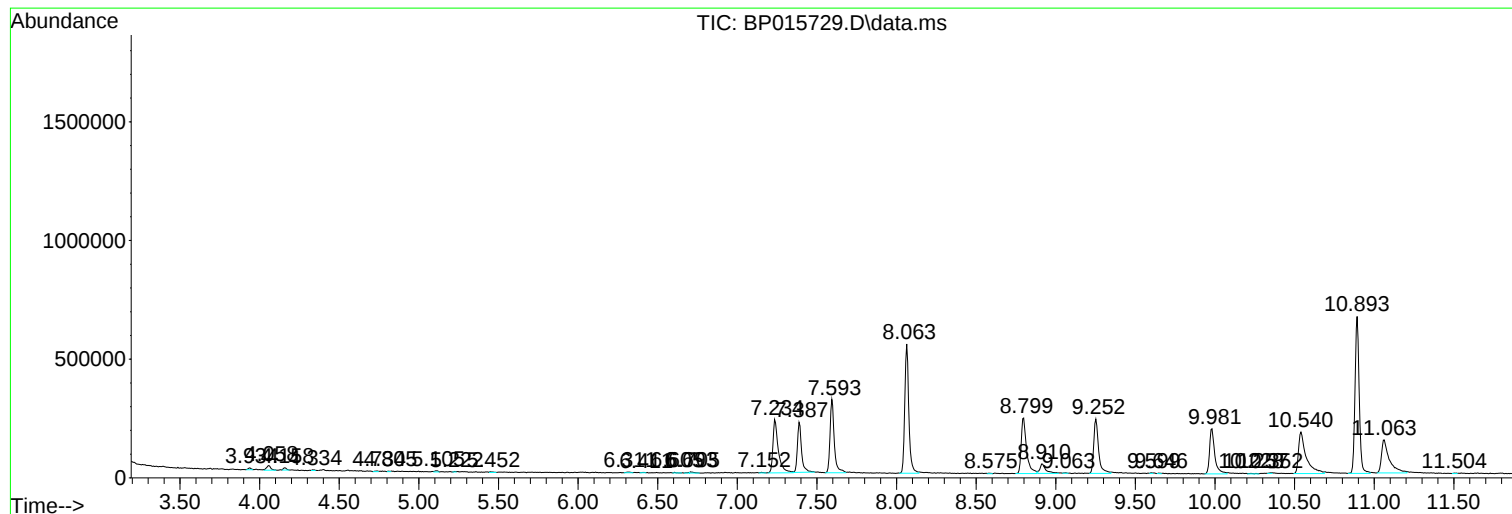

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015729.D
Acq On : 26 Jun 2023 23:32
Operator : MA/JU
Sample : 03085-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFP5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Aceto phenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.910	2.13 ng/ul	102444	1,4-Dichlorobenzene-d4	8.063

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetophenone			120	C8H8O	000098-86-2	90
2	Acetophenone			120	C8H8O	000098-86-2	90
3	Acetophenone			120	C8H8O	000098-86-2	90
4	Acetophenone			120	C8H8O	000098-86-2	90
5	Acetophenone			120	C8H8O	000098-86-2	87

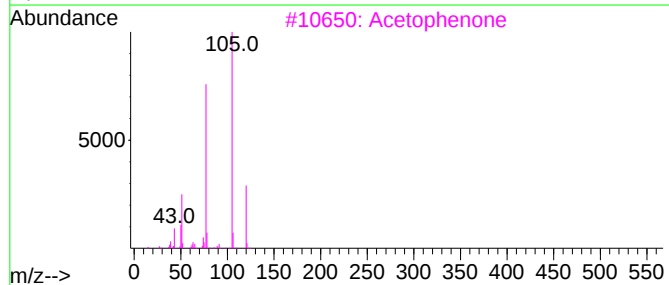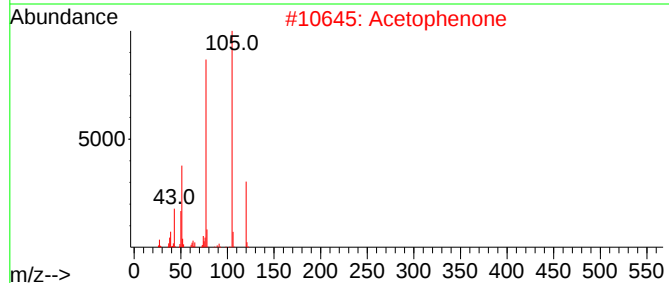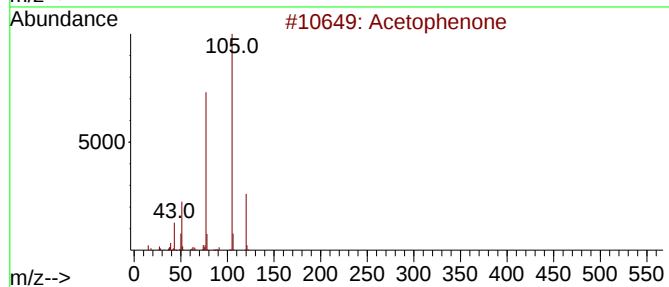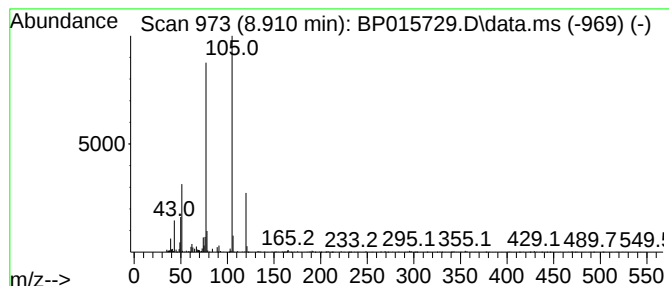

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062623\
Data File : BP015729.D
Acq On : 26 Jun 2023 23:32
Operator : MA/JU
Sample : 03085-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Aceto phenone	8.910	2.1	ng/ul	102444	1	8.063	961777	20.0