

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015738.D
 Acq On : 27 Jun 2023 10:06
 Operator : MA/JU
 Sample : PB153469BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK469

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	39	rVB	37394	49039	1.93%	0.182%
2	3.828	106	109	126	rBV	382291	620467	24.40%	2.305%
3	4.158	161	165	172	rVB3	12730	20174	0.79%	0.075%
4	5.128	325	330	333	rBV7	2618	4204	0.17%	0.016%
5	6.152	502	504	508	rVB5	3027	4234	0.17%	0.016%
6	7.228	681	687	705	rBV	348764	800434	31.47%	2.974%
7	7.387	708	714	729	rVB	347560	606163	23.83%	2.252%
8	7.593	742	749	764	rBV	464448	850973	33.46%	3.162%
9	8.063	822	829	847	rBV	499556	906352	35.64%	3.368%
10	8.505	902	904	908	rVB5	2928	3666	0.14%	0.014%
11	8.793	946	953	970	rBV	431849	972528	38.24%	3.614%
12	9.016	988	991	994	rVB5	1817	2547	0.10%	0.009%
13	9.246	1022	1030	1050	rBV	381204	804266	31.62%	2.988%
14	9.975	1146	1154	1169	rBV	316143	681939	26.81%	2.534%
15	10.534	1239	1249	1273	rBV	295469	906835	35.66%	3.370%
16	10.893	1302	1310	1324	rBV	628933	1143986	44.98%	4.251%
17	11.057	1330	1338	1361	rBV	262320	849193	33.39%	3.155%
18	12.363	1555	1560	1564	rBV8	1538	3439	0.14%	0.013%
19	12.516	1582	1586	1592	rBV7	5399	12662	0.50%	0.047%
20	13.257	1709	1712	1716	rBV6	1616	3261	0.13%	0.012%
21	13.592	1764	1769	1776	rVB10	5878	9454	0.37%	0.035%
22	14.122	1851	1859	1885	rVV	731758	1283674	50.47%	4.770%
23	14.410	1901	1908	1927	rVV	911574	1490996	58.62%	5.540%
24	14.716	1952	1960	1977	rVV	800593	1314445	51.68%	4.884%
25	14.822	1977	1978	1983	rVV5	2957	3315	0.13%	0.012%
26	14.987	2000	2006	2025	rBV2	76805	338650	13.32%	1.258%
27	15.622	2111	2114	2117	rBV4	2061	2679	0.11%	0.010%
28	15.710	2120	2129	2144	rBV	962923	1708145	67.16%	6.347%
29	15.875	2151	2157	2167	rBV2	147370	365305	14.36%	1.357%
30	16.186	2208	2210	2213	rVB4	3016	3132	0.12%	0.012%
31	16.292	2226	2228	2232	rVB5	2863	2989	0.12%	0.011%
32	17.475	2422	2429	2440	rBV	869169	1398428	54.98%	5.196%
33	17.575	2440	2446	2472	rVB2	955049	1770003	69.59%	6.577%
34	19.380	2751	2753	2758	rVB4	14824	18574	0.73%	0.069%
35	19.804	2819	2825	2846	rBV	1296915	2123465	83.49%	7.890%
36	21.569	3120	3125	3136	rBV2	878234	1525124	59.97%	5.667%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015738.D
Acq On : 27 Jun 2023 10:06
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	23.945	3522	3529	3546	rVB2	1097716	2543349	100.00%	9.450%
38	24.110	3551	3557	3573	rVB	718995	1764885	69.39%	6.558%




Sum of corrected areas: 26912974

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015738.D
Acq On : 27 Jun 2023 10:06
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

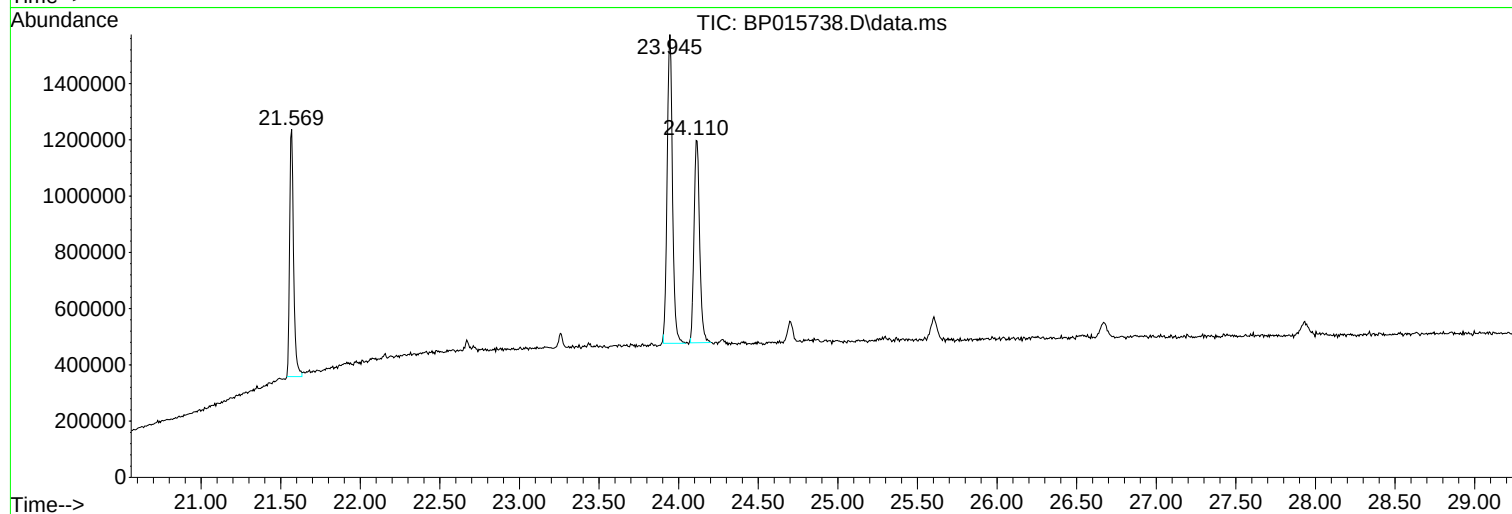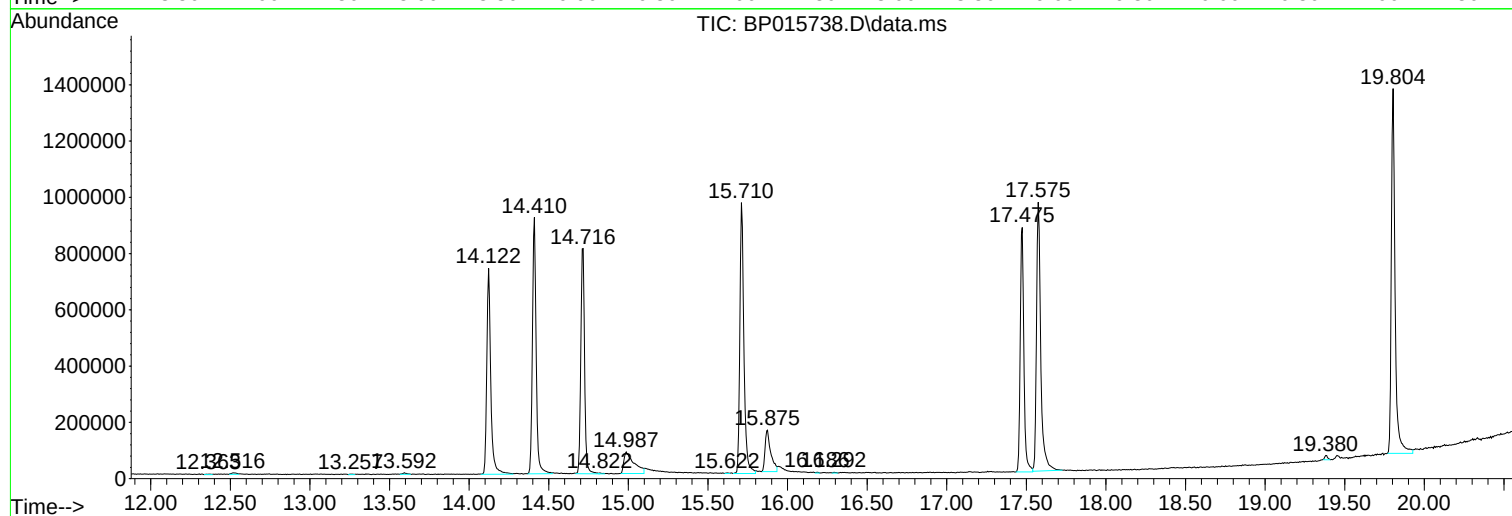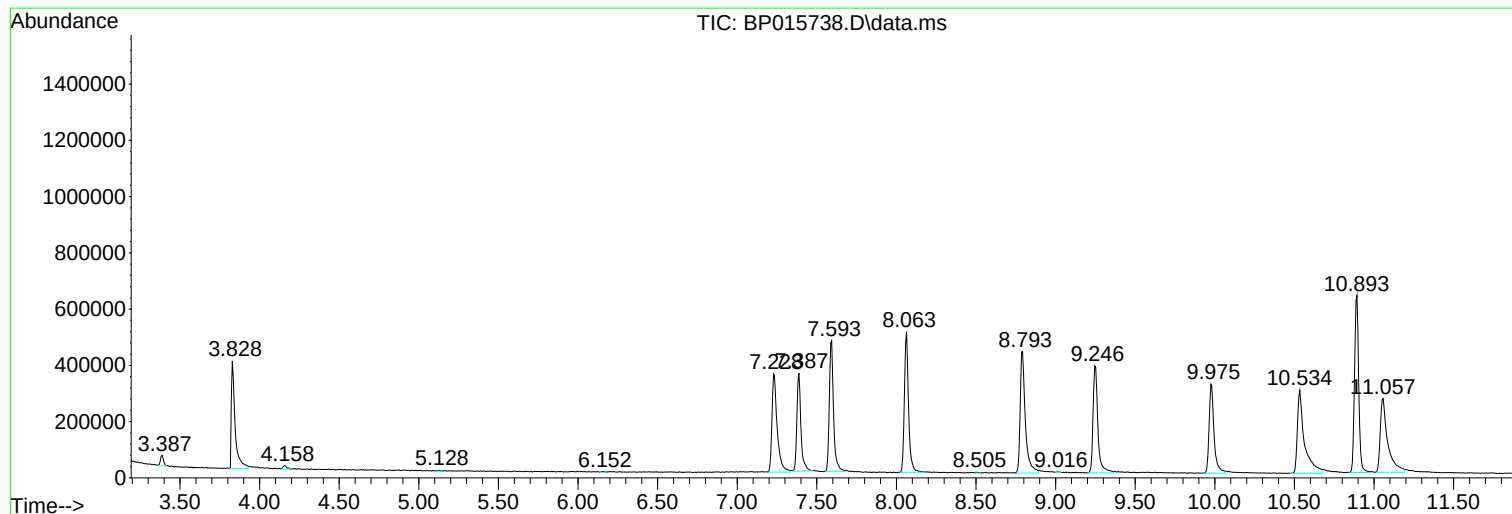

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015738.D
Acq On : 27 Jun 2023 10:06
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015738.D
Acq On : 27 Jun 2023 10:06
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------