

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015754.D
 Acq On : 27 Jun 2023 19:11
 Operator : MA/JU
 Sample : 03411-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.899	120	121	124	rBV3	4047	2184	0.11%	0.025%
2	4.158	162	165	170	rVB3	8819	13253	0.67%	0.150%
3	4.352	196	198	200	rBV3	2368	2191	0.11%	0.025%
4	5.728	430	432	435	rVB3	1837	2071	0.10%	0.023%
5	6.158	502	505	506	rVB3	3028	2628	0.13%	0.030%
6	6.181	506	509	511	rBV3	2280	2900	0.15%	0.033%
7	6.428	547	551	554	rBV6	1857	2943	0.15%	0.033%
8	6.481	558	560	563	rVB4	2898	2810	0.14%	0.032%
9	6.675	589	593	597	rVB7	2376	3670	0.18%	0.042%
10	6.840	616	621	624	rBV6	1292	2515	0.13%	0.028%
11	7.611	750	752	756	rBV5	1988	2522	0.13%	0.029%
12	8.069	822	830	856	rBV	323762	835178	41.92%	9.462%
13	8.311	869	871	873	rVB3	3020	2215	0.11%	0.025%
14	8.340	873	876	878	rVB4	3069	2777	0.14%	0.031%
15	8.369	878	881	888	rVB9	1553	3278	0.16%	0.037%
16	8.675	931	933	934	rBV2	2678	2718	0.14%	0.031%
17	9.016	988	991	994	rVB5	1849	2071	0.10%	0.023%
18	9.399	1054	1056	1059	rVB4	1976	2307	0.12%	0.026%
19	9.516	1072	1076	1077	rBV4	2428	2324	0.12%	0.026%
20	9.599	1086	1090	1092	rBV5	1727	2250	0.11%	0.025%
21	9.799	1123	1124	1131	rVB7	1635	2342	0.12%	0.027%
22	9.910	1142	1143	1148	rBV5	1878	2752	0.14%	0.031%
23	10.805	1291	1295	1300	rVB8	1457	2592	0.13%	0.029%
24	10.899	1300	1311	1338	rBV	333592	1055300	52.97%	11.956%
25	11.346	1385	1387	1392	rVB5	2470	3663	0.18%	0.042%
26	11.734	1450	1453	1455	rBV4	1940	2149	0.11%	0.024%
27	12.075	1507	1511	1512	rBV4	2096	2110	0.11%	0.024%
28	12.193	1528	1531	1534	rBV5	1951	2040	0.10%	0.023%
29	12.216	1534	1535	1539	rVV4	1415	2008	0.10%	0.023%
30	12.340	1553	1556	1559	rBV5	2048	3077	0.15%	0.035%
31	13.128	1687	1690	1693	rVB5	1890	2239	0.11%	0.025%
32	13.316	1717	1722	1725	rVB7	1520	2783	0.14%	0.032%
33	13.610	1764	1772	1777	rBV9	6010	14018	0.70%	0.159%
34	13.946	1825	1829	1830	rBV4	1808	2193	0.11%	0.025%
35	14.075	1848	1851	1855	rBV5	2139	3881	0.19%	0.044%
36	14.716	1952	1960	1979	rBV	609243	1326884	66.60%	15.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015754.D
 Acq On : 27 Jun 2023 19:11
 Operator : MA/JU
 Sample : 03411-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	15.098	2022	2025	2029	rBV6	1432	2640	0.13%	0.030%
38	15.163	2034	2036	2039	rVV4	1955	2928	0.15%	0.033%
39	15.216	2043	2045	2048	rBV4	2337	2718	0.14%	0.031%
40	15.434	2078	2082	2086	rBV7	1713	2891	0.15%	0.033%
41	15.622	2110	2114	2120	rVB8	3463	8446	0.42%	0.096%
42	15.675	2120	2123	2126	rBV4	2778	4254	0.21%	0.048%
43	16.134	2196	2201	2202	rBV5	3058	4130	0.21%	0.047%
44	16.475	2256	2259	2263	rVB6	2604	3943	0.20%	0.045%
45	17.363	2405	2410	2411	rBV5	3209	5346	0.27%	0.061%
46	17.422	2417	2420	2421	rBV3	2495	2546	0.13%	0.029%
47	17.481	2424	2430	2450	rVV	678464	1551889	77.89%	17.582%
48	21.563	3119	3124	3136	rBV	1071879	1917378	96.23%	21.723%
49	24.116	3551	3558	3572	rVB	816843	1992445	100.00%	22.574%




Sum of corrected areas: 8826390

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015754.D
Acq On : 27 Jun 2023 19:11
Operator : MA/JU
Sample : 03411-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

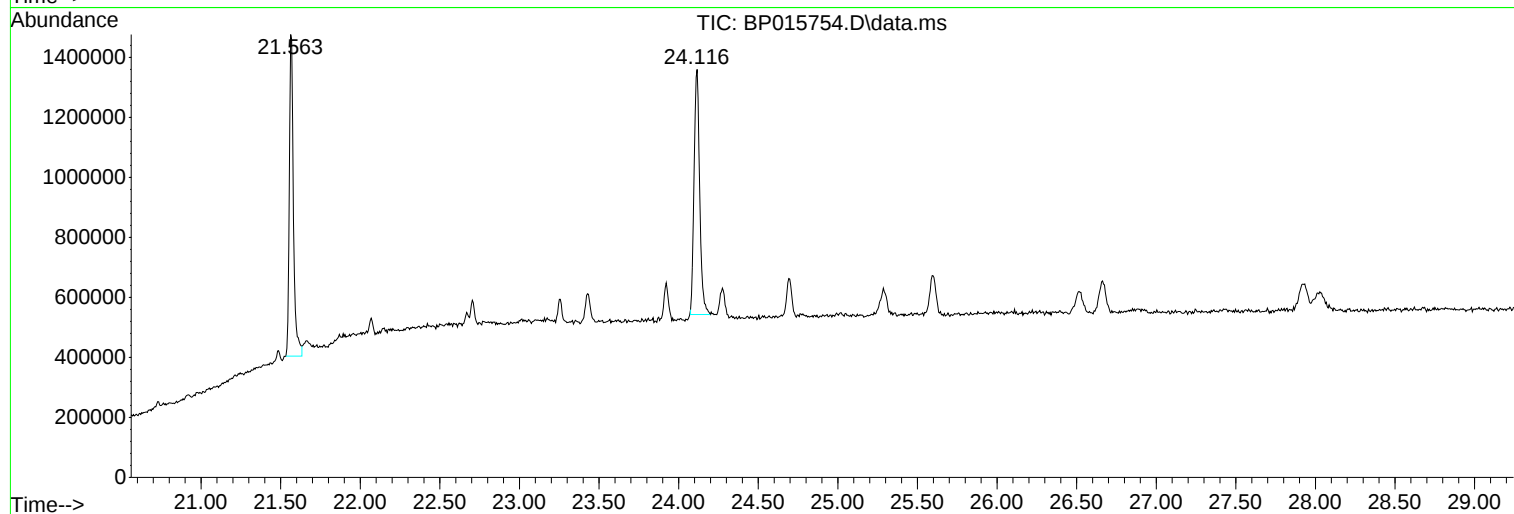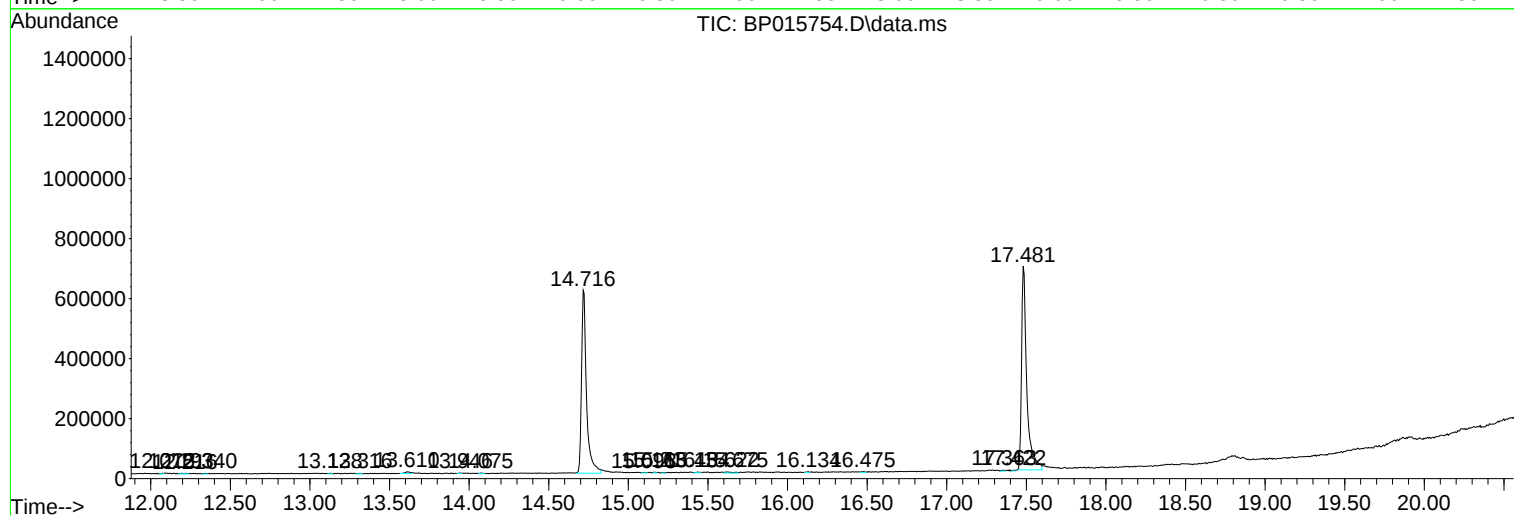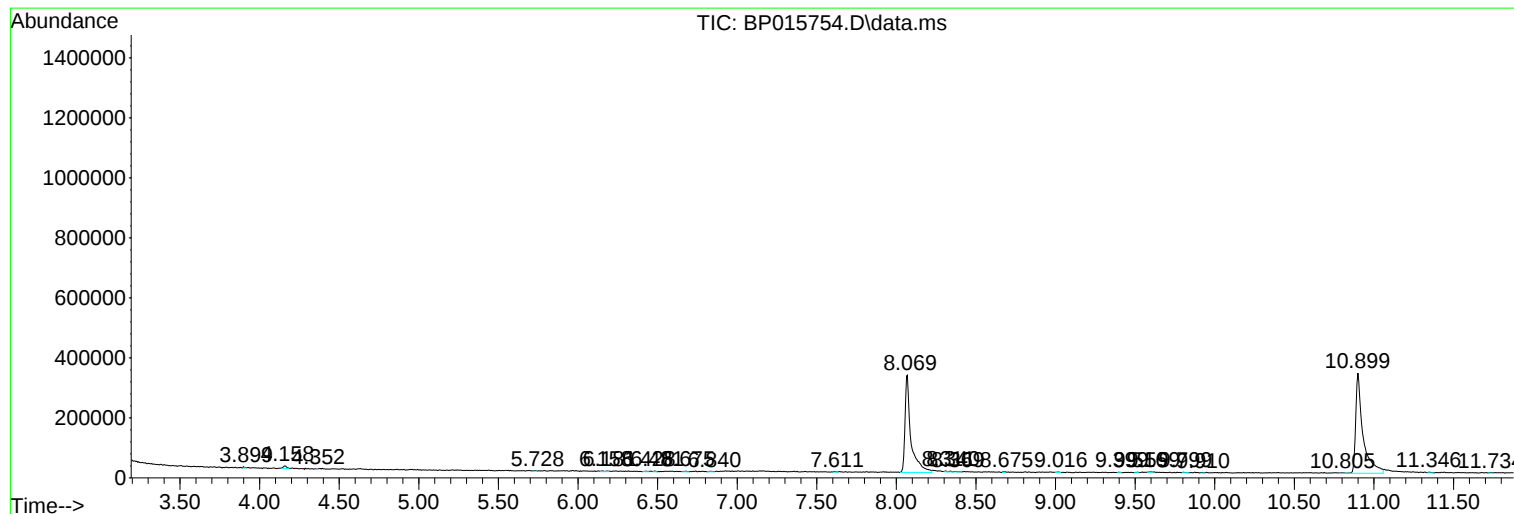

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015754.D
Acq On : 27 Jun 2023 19:11
Operator : MA/JU
Sample : 03411-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015754.D
Acq On : 27 Jun 2023 19:11
Operator : MA/JU
Sample : 03411-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------