

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015755.D
 Acq On : 27 Jun 2023 19:44
 Operator : MA/JU
 Sample : 03411-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.675	81	83	86	rBV4	4130	4866	0.28%	0.054%
2	4.158	159	165	168	rBV2	10654	16432	0.94%	0.181%
3	4.334	193	195	196	rBV2	2479	1893	0.11%	0.021%
4	4.940	296	298	302	rBV4	2527	3936	0.22%	0.043%
5	6.046	484	486	488	rVB3	2042	1904	0.11%	0.021%
6	6.287	525	527	531	rBV5	1920	2258	0.13%	0.025%
7	6.422	548	550	551	rBV2	2249	2076	0.12%	0.023%
8	6.810	614	616	620	rVB4	1847	2177	0.12%	0.024%
9	6.875	625	627	632	rVB6	1313	2112	0.12%	0.023%
10	7.028	649	653	656	rBV6	2382	4217	0.24%	0.046%
11	7.416	715	719	722	rBV6	2288	2859	0.16%	0.031%
12	7.610	750	752	757	rBV6	1309	1774	0.10%	0.020%
13	8.063	821	829	851	rBV	378584	926523	52.85%	10.199%
14	8.516	905	906	911	rVB5	2232	2274	0.13%	0.025%
15	8.646	925	928	930	rVB4	1682	1847	0.11%	0.020%
16	8.898	968	971	973	rBV4	1487	1943	0.11%	0.021%
17	8.951	977	980	982	rBV4	1461	1880	0.11%	0.021%
18	9.198	1017	1022	1024	rBV5	1507	2382	0.14%	0.026%
19	9.375	1051	1052	1057	rVB5	1814	1789	0.10%	0.020%
20	9.434	1057	1062	1066	rVB8	2492	4024	0.23%	0.044%
21	9.581	1085	1087	1089	rVV3	1862	2112	0.12%	0.023%
22	9.634	1093	1096	1098	rVB4	2206	2784	0.16%	0.031%
23	9.928	1143	1146	1147	rBV3	1861	1945	0.11%	0.021%
24	10.187	1187	1190	1193	rBV4	1960	2028	0.12%	0.022%
25	10.481	1236	1240	1241	rBV4	1739	2046	0.12%	0.023%
26	10.604	1259	1261	1265	rVB5	1249	1935	0.11%	0.021%
27	10.775	1289	1290	1293	rBV3	2153	1948	0.11%	0.021%
28	10.810	1293	1296	1298	rVV4	1757	2298	0.13%	0.025%
29	10.898	1303	1311	1339	rBV	407107	1282560	73.16%	14.118%
30	11.287	1376	1377	1382	rVB5	2205	2939	0.17%	0.032%
31	11.610	1431	1432	1437	rVB5	2242	2098	0.12%	0.023%
32	11.645	1437	1438	1441	rBV3	2463	2174	0.12%	0.024%
33	11.728	1450	1452	1455	rBV4	1475	1883	0.11%	0.021%
34	11.875	1474	1477	1479	rBV3	1404	1936	0.11%	0.021%
35	12.204	1530	1533	1535	rBV4	2190	2462	0.14%	0.027%
36	12.551	1589	1592	1594	rVV4	1685	1786	0.10%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015755.D
 Acq On : 27 Jun 2023 19:44
 Operator : MA/JU
 Sample : 03411-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	12.657	1608	1610	1613	rBV4	1221	1763	0.10%	0.019%
38	12.804	1634	1635	1640	rBV5	1355	1974	0.11%	0.022%
39	12.863	1640	1645	1647	rBV5	1378	1812	0.10%	0.020%
40	13.287	1712	1717	1719	rBV6	1960	2669	0.15%	0.029%
41	13.386	1732	1734	1737	rBV3	1465	1952	0.11%	0.021%
42	13.422	1737	1740	1742	rVB4	1922	2050	0.12%	0.023%
43	13.622	1768	1774	1775	rBV6	3311	4675	0.27%	0.051%
44	13.639	1775	1777	1780	rVV4	2444	2752	0.16%	0.030%
45	13.675	1780	1783	1785	rVB4	1708	2198	0.13%	0.024%
46	13.804	1802	1805	1807	rBV4	1473	1916	0.11%	0.021%
47	13.969	1831	1833	1837	rVB5	2351	3121	0.18%	0.034%
48	14.186	1867	1870	1874	rBV6	1938	3429	0.20%	0.038%
49	14.328	1891	1894	1897	rBV6	1929	2748	0.16%	0.030%
50	14.416	1905	1909	1910	rVB4	1713	2171	0.12%	0.024%
51	14.657	1948	1950	1953	rBV4	1633	2118	0.12%	0.023%
52	14.716	1953	1960	1985	rBV	761156	1632909	93.15%	17.974%
53	15.063	2016	2019	2023	rBV6	1527	2071	0.12%	0.023%
54	15.492	2089	2092	2095	rBV5	1380	1784	0.10%	0.020%
55	15.580	2105	2107	2111	rVB5	1980	2277	0.13%	0.025%
56	15.610	2111	2112	2115	rVV3	1617	2155	0.12%	0.024%
57	15.639	2115	2117	2120	rVB4	2298	2425	0.14%	0.027%
58	16.028	2181	2183	2185	rBV3	1915	1797	0.10%	0.020%
59	16.098	2192	2195	2197	rBV3	1932	1813	0.10%	0.020%
60	16.122	2197	2199	2201	rBV3	1742	1866	0.11%	0.021%
61	16.233	2215	2218	2222	rBV6	1745	3092	0.18%	0.034%
62	16.457	2255	2256	2263	rBV7	1272	2482	0.14%	0.027%
63	16.745	2300	2305	2307	rBV5	2703	4310	0.25%	0.047%
64	16.857	2322	2324	2329	rBV5	3437	5657	0.32%	0.062%
65	17.145	2371	2373	2376	rBV4	2135	2482	0.14%	0.027%
66	17.269	2391	2394	2398	rBV6	4055	6147	0.35%	0.068%
67	17.486	2423	2431	2462	rBV	706049	1737927	99.14%	19.130%
68	21.568	3120	3125	3139	rBV2	889961	1579023	90.07%	17.381%
69	24.115	3552	3558	3573	rVB	719028	1753026	100.00%	19.296%




Sum of corrected areas: 9084691

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015755.D
Acq On : 27 Jun 2023 19:44
Operator : MA/JU
Sample : 03411-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

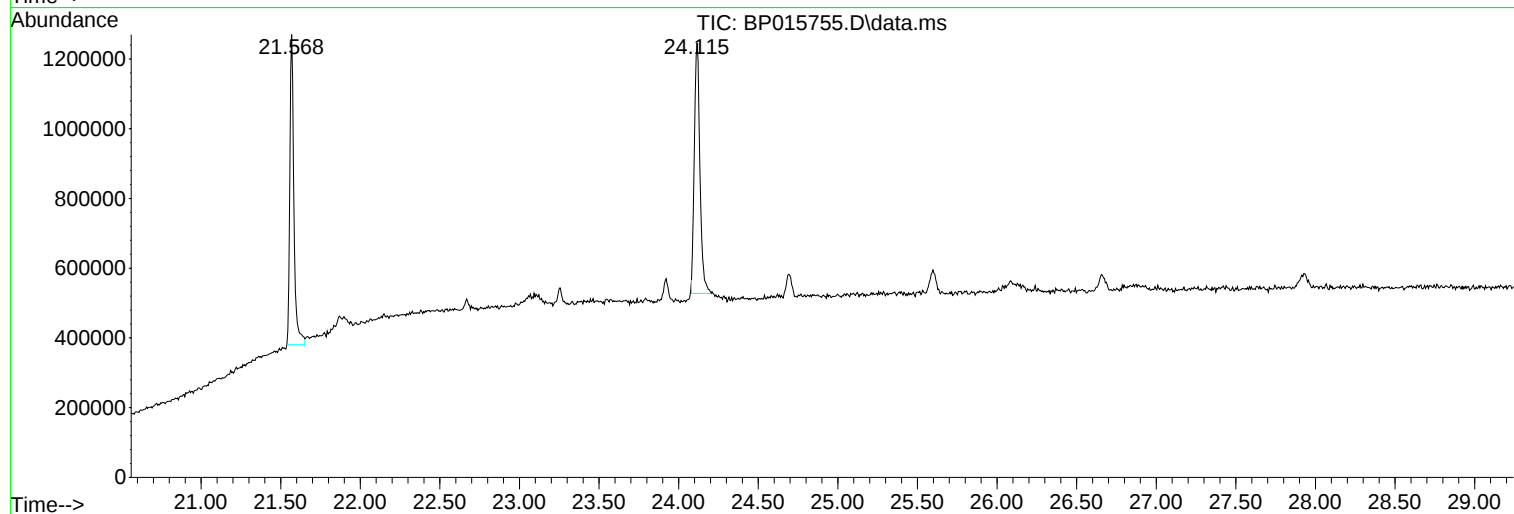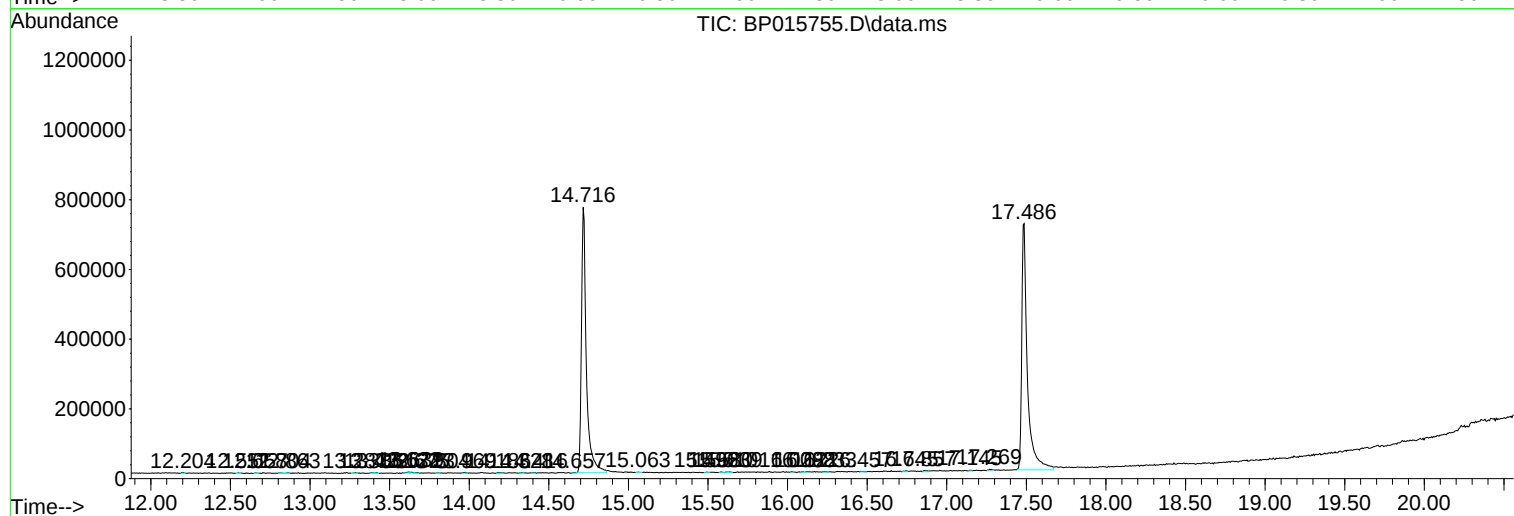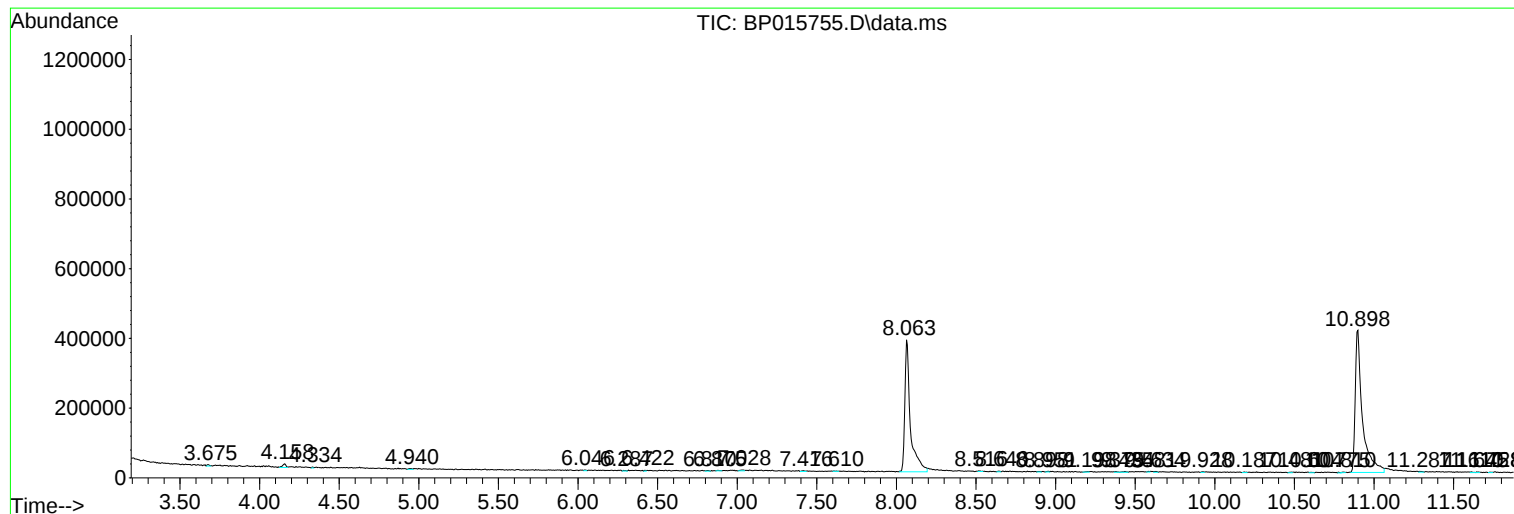

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015755.D
Acq On : 27 Jun 2023 19:44
Operator : MA/JU
Sample : 03411-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015755.D
Acq On : 27 Jun 2023 19:44
Operator : MA/JU
Sample : 03411-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------