

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
 Data File : BP015758.D
 Acq On : 27 Jun 2023 22:00
 Operator : MA/JU
 Sample : PB153469BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK469

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	43	rVB	43773	63563	2.14%	0.219%
2	3.828	106	109	130	rBV	414575	690560	23.25%	2.379%
3	4.152	161	164	168	rBV	12905	16373	0.55%	0.056%
4	6.328	532	534	539	rVB5	3065	4051	0.14%	0.014%
5	7.234	681	688	707	rBV	336934	821855	27.68%	2.831%
6	7.387	707	714	732	rVB	341064	627769	21.14%	2.163%
7	7.587	742	748	763	rBV	477622	888429	29.92%	3.061%
8	8.064	821	829	846	rBV	496019	960073	32.33%	3.308%
9	8.793	946	953	975	rBV	419497	988203	33.28%	3.405%
10	9.093	1001	1004	1008	rVB6	1888	2976	0.10%	0.010%
11	9.252	1023	1031	1048	rBV	369358	799689	26.93%	2.755%
12	9.981	1145	1155	1172	rBV	295510	681569	22.95%	2.348%
13	10.540	1242	1250	1282	rBV	262465	928342	31.26%	3.198%
14	10.787	1291	1292	1298	rVB6	2142	3023	0.10%	0.010%
15	10.887	1302	1309	1326	rBV	604135	1165135	39.23%	4.014%
16	11.057	1330	1338	1369	rBV	245767	856527	28.84%	2.951%
17	11.469	1405	1408	1413	rBV7	2477	4603	0.16%	0.016%
18	12.099	1512	1515	1518	rBV4	2141	3091	0.10%	0.011%
19	12.522	1583	1587	1595	rBV7	5141	10491	0.35%	0.036%
20	13.593	1764	1769	1775	rBV9	6841	14498	0.49%	0.050%
21	14.122	1853	1859	1883	rVV	735262	1307388	44.03%	4.504%
22	14.410	1900	1908	1927	rBV2	888214	1541665	51.91%	5.311%
23	14.710	1952	1959	1978	rBV	841000	1345992	45.33%	4.637%
24	14.993	1999	2007	2022	rBV4	81381	354197	11.93%	1.220%
25	15.710	2122	2129	2144	rBV	919969	1799798	60.61%	6.201%
26	15.875	2151	2157	2183	rBV2	162830	478555	16.11%	1.649%
27	16.298	2226	2229	2231	rBV4	2163	3089	0.10%	0.011%
28	16.404	2242	2247	2248	rBV5	2086	3255	0.11%	0.011%
29	17.469	2422	2428	2440	rBV	955569	1566082	52.74%	5.395%
30	17.575	2440	2446	2465	rVB2	1016342	1951506	65.72%	6.723%
31	19.381	2749	2753	2758	rBV6	20694	31655	1.07%	0.109%
32	19.804	2819	2825	2842	rBV	1471065	2474046	83.31%	8.524%
33	21.569	3120	3125	3138	rBV	1066614	1749365	58.91%	6.027%
34	23.939	3521	3528	3542	rVB2	1223487	2969636	100.00%	10.231%
35	24.110	3551	3557	3570	rVB	798451	1919084	64.62%	6.612%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015758.D
Acq On : 27 Jun 2023 22:00
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 29026133

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015758.D
Acq On : 27 Jun 2023 22:00
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

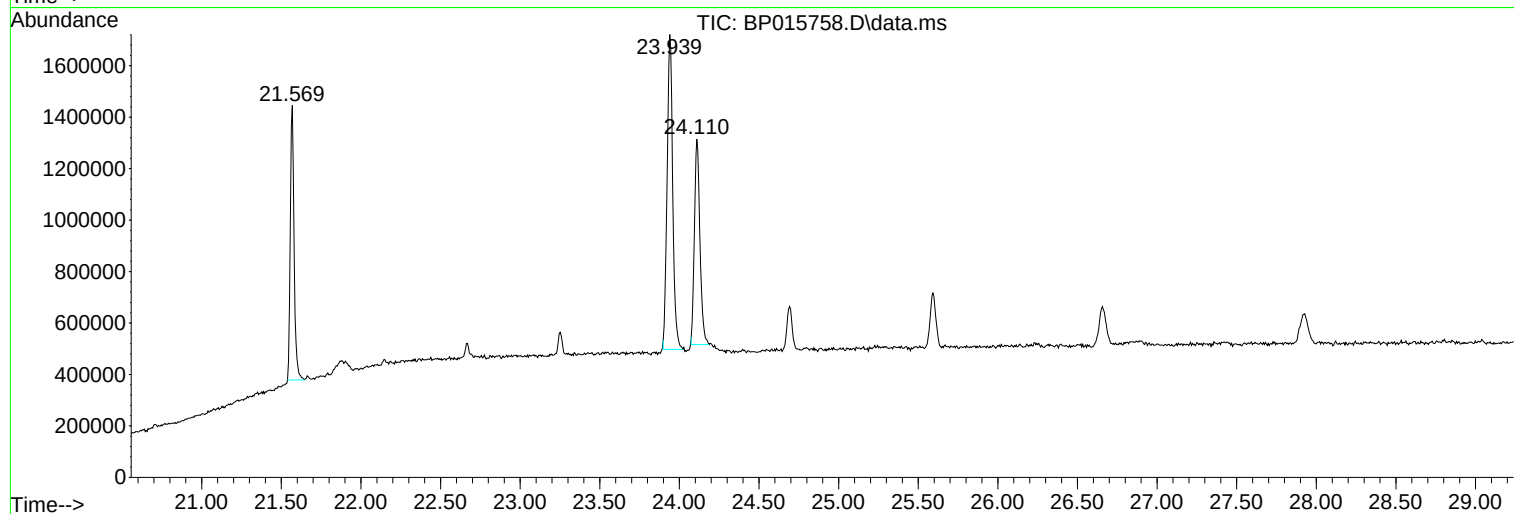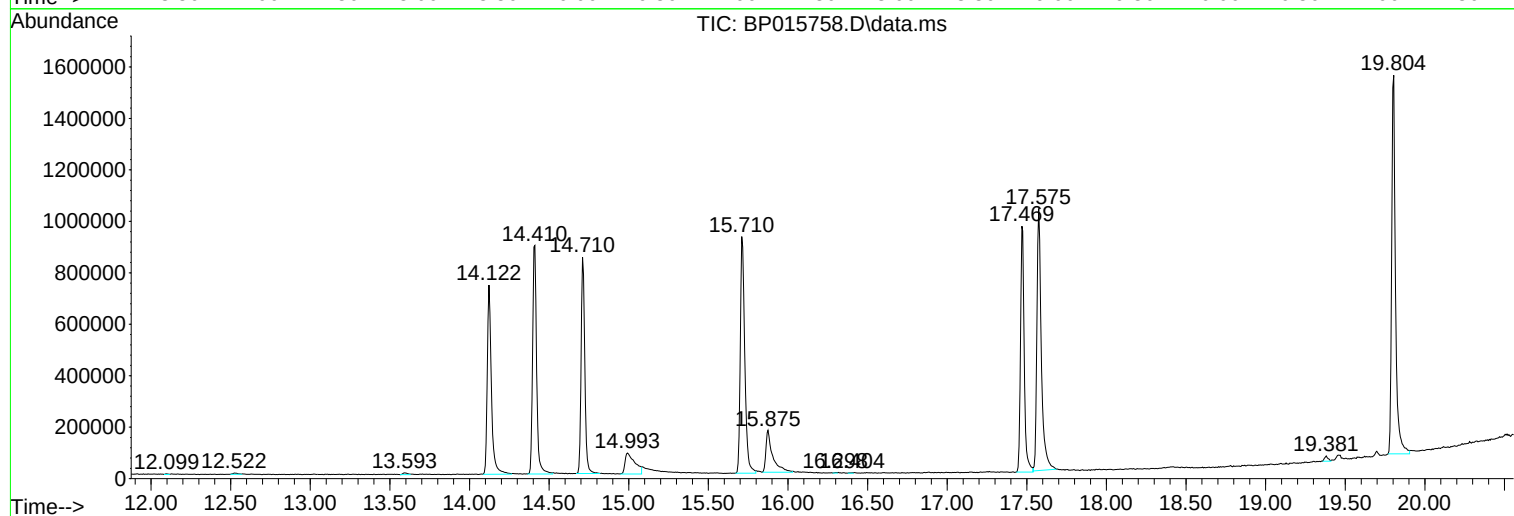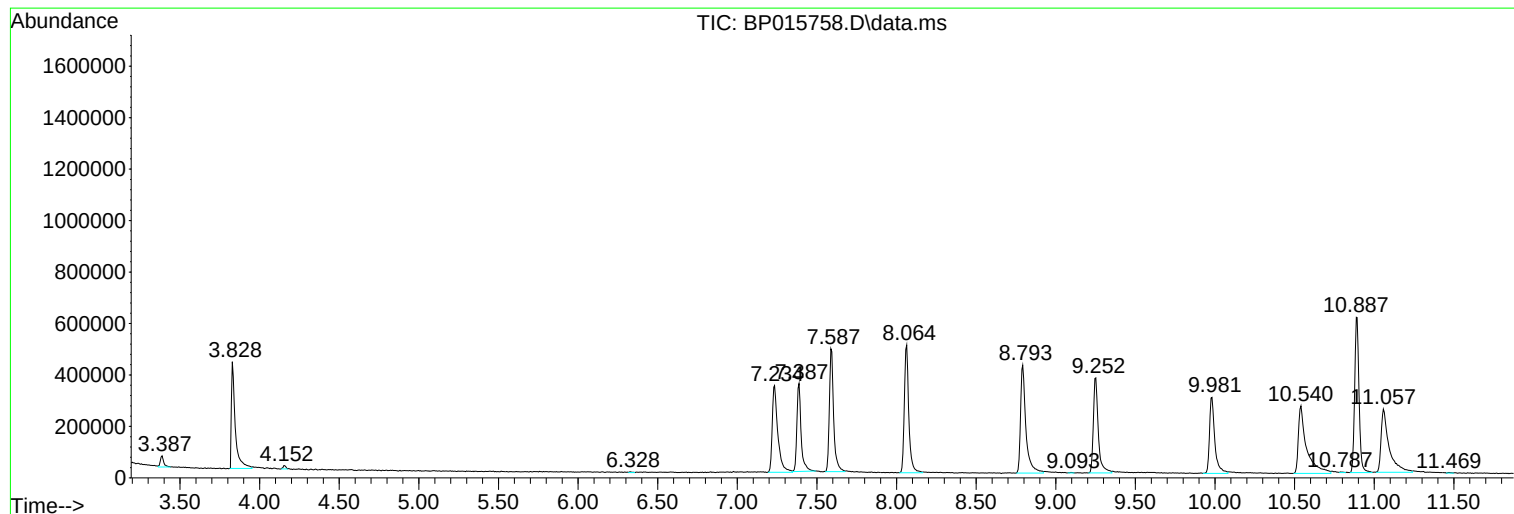

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015758.D
Acq On : 27 Jun 2023 22:00
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062723\
Data File : BP015758.D
Acq On : 27 Jun 2023 22:00
Operator : MA/JU
Sample : PB153469BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK469

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc