

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
 Data File : BP015771.D
 Acq On : 28 Jun 2023 10:26
 Operator : MA/JU
 Sample : 03101-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EZEM0

Quant Time: Jun 28 22:03:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 00:56:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	191927	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	701874	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	362183	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	711270	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	688958	20.000	ng/ul	0.00
88) Perylene-d12	24.103	264	874389	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	22508	4.219	ng/uL	0.00
4) Pyridine-d5	3.828	84	201876	15.013	ng/ul	0.00
7) Phenol-d5	7.234	99	332508	20.248	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	235798	23.209	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	288240	23.252	ng/ul	0.00
15) 4-Methylphenol-d8	8.793	113	224147	17.278	ng/ul	0.00
21) Nitrobenzene-d5	9.245	128	125878	23.467	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	140577	22.455	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.539	165	213833	19.167	ng/ul	0.02
31) 4-Chloroaniline-d4	11.063	131	238795	16.663	ng/ul	0.02
46) Dimethylphthalate-d6	14.122	166	673965	24.075	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	770557	24.486	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	55	0.015	ng/ul	0.00
60) Fluorene-d10	15.710	176	545000	23.644	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.010	200	295	0.067	ng/ul	0.15
73) Anthracene-d10	17.574	188	790184	24.321	ng/ul	0.00
81) Pyrene-d10	19.798	212	1006375	22.370	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	1158723	26.270	ng/ul	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.510	178	545607	14.120	ng/ul	99
74) Anthracene	17.610	178	85656	2.206	ng/ul	97
77) Carbazole	17.898	167	62748	1.917	ng/ul	98
80) Fluoranthene	19.474	202	1013101	18.120	ng/ul	98
82) Pyrene	19.827	202	772133	13.538	ng/ul	96
85) Benzo(a)anthracene	21.545	228	285639	5.894	ng/ul	97
87) Chrysene	21.598	228	304326	6.618	ng/ul	97
90) Benzo(b)fluoranthene	23.321	252	401600	7.148	ng/ul	96
91) Benzo(k)fluoranthene	23.368	252	128012	2.255	ng/ul#	92
93) Benzo(a)pyrene	23.992	252	252433	5.142	ng/ul#	94
94) Indeno(1,2,3-cd)pyrene	26.809	276	194851	2.924	ng/ul	98
96) Benzo(g,h,i)perylene	27.644	276	178484	3.255	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
Data File : BP015771.D
Acq On : 28 Jun 2023 10:26
Operator : MA/JU
Sample : 03101-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EZEM0

Quant Time: Jun 28 22:03:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 00:56:58 2023
Response via : Initial Calibration

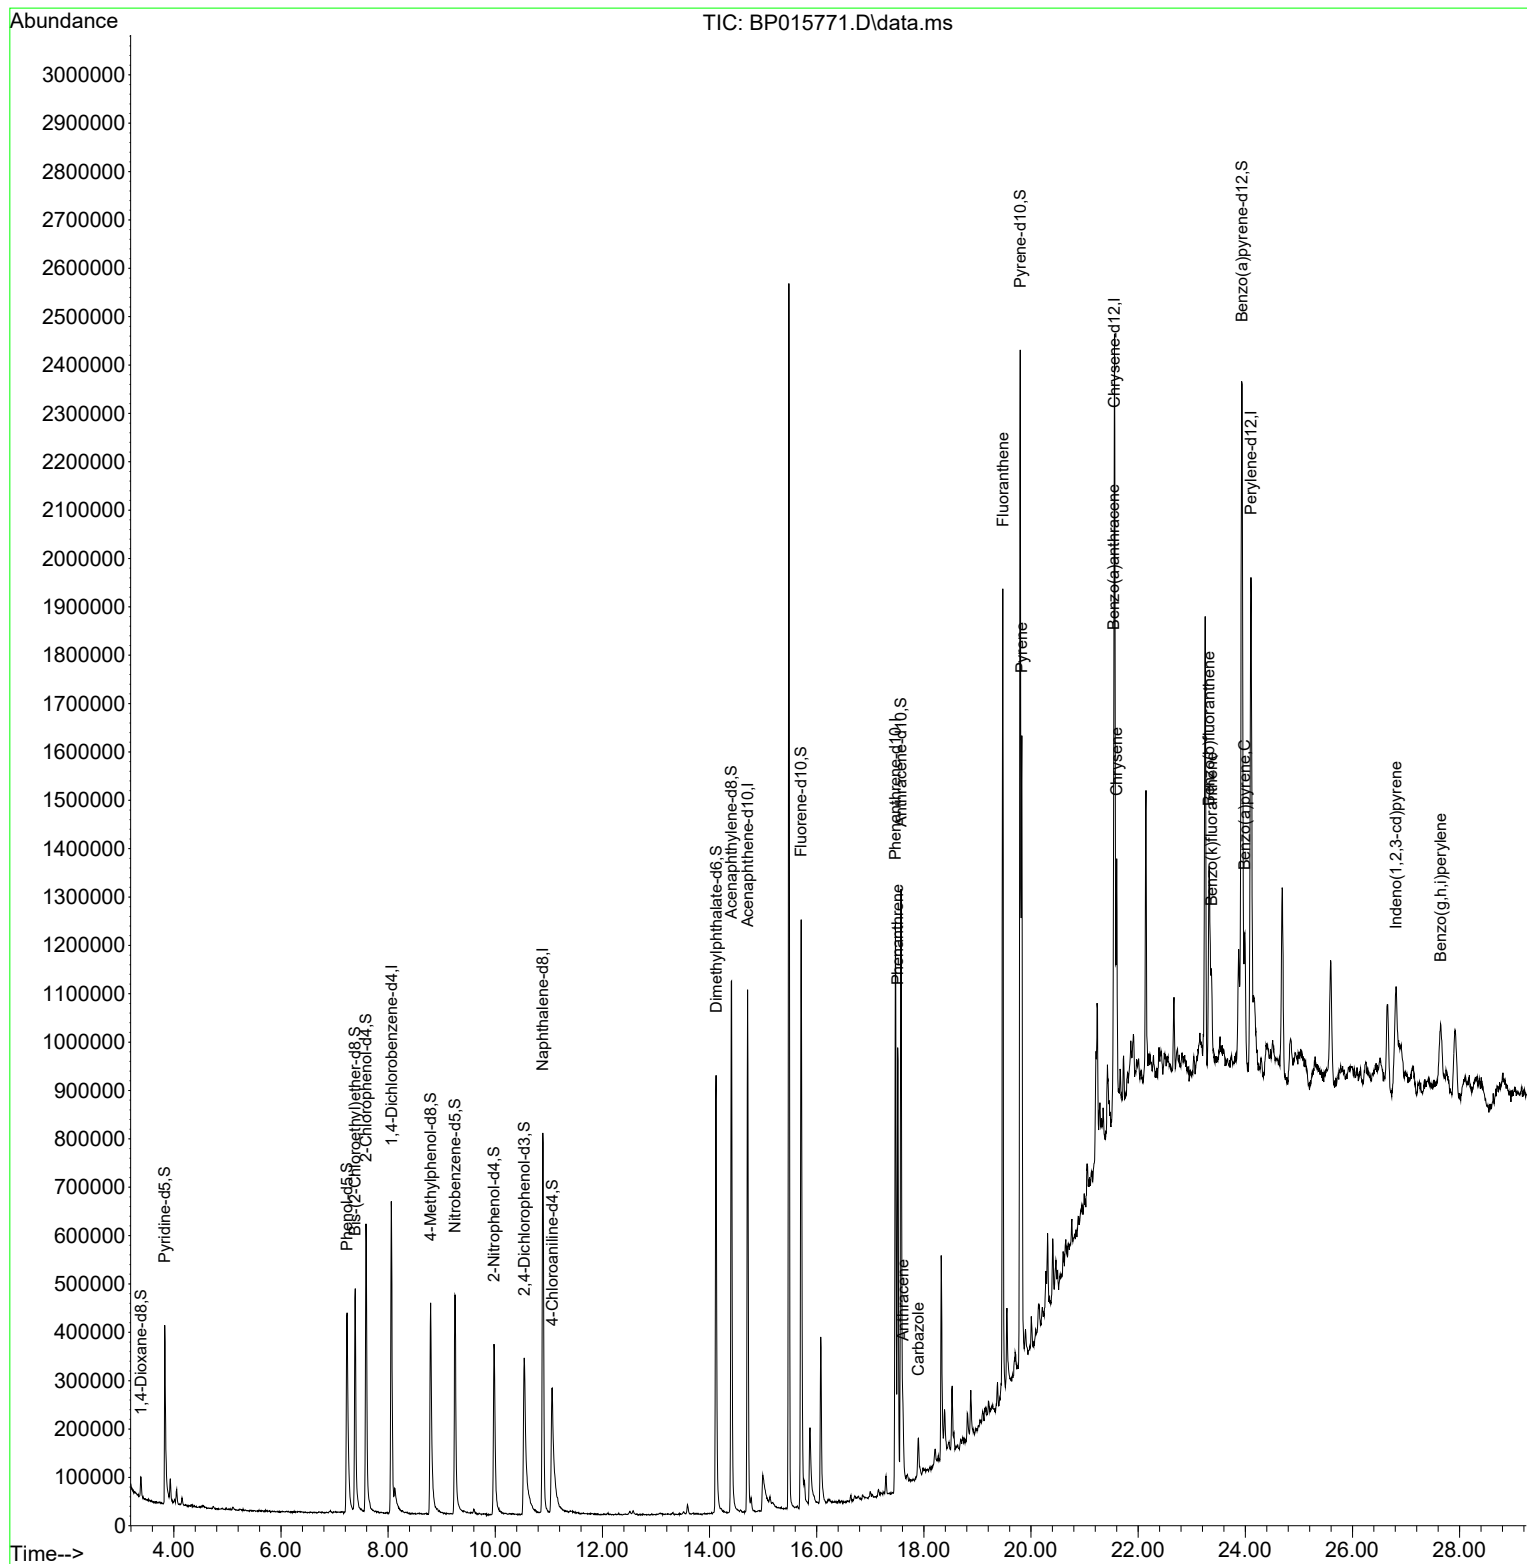

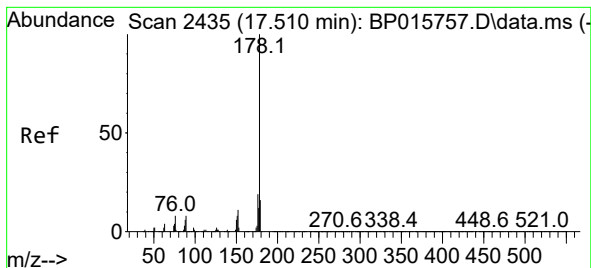

#72

Phenanthrene

Concen: 14.120 ng/ul

RT: 17.510 min Scan# 2435

Delta R.T. -0.006 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Instrument :

BNA_P

ClientSampleId :

EZEM0





Tgt Ion:178 Resp: 545607

Ion Ratio Lower Upper

178 100

179 15.7 12.4 18.6

176 19.0 15.6 23.4

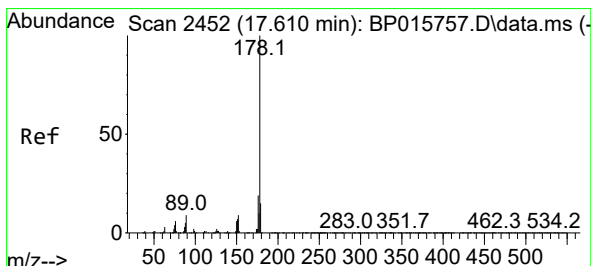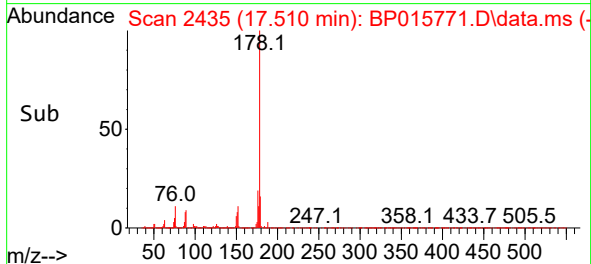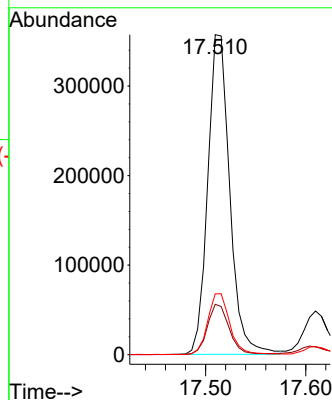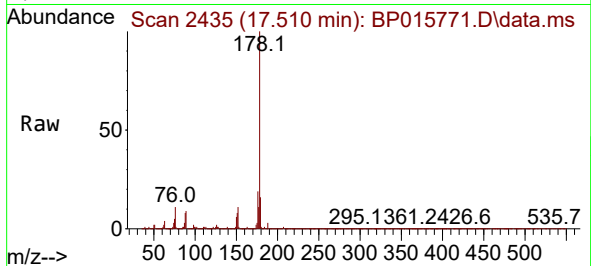

#74

Anthracene

Concen: 2.206 ng/ul

RT: 17.610 min Scan# 2452

Delta R.T. -0.000 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26




Tgt Ion:178 Resp: 85656


Ion Ratio Lower Upper

178 100

179 17.4 12.1 18.1

176 18.7 14.6 22.0


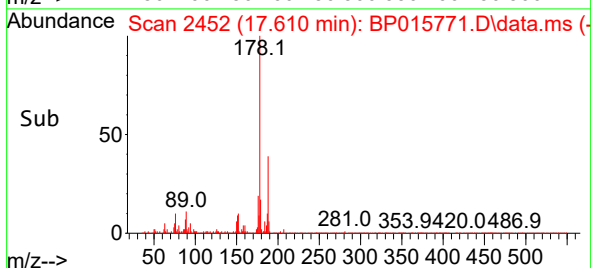
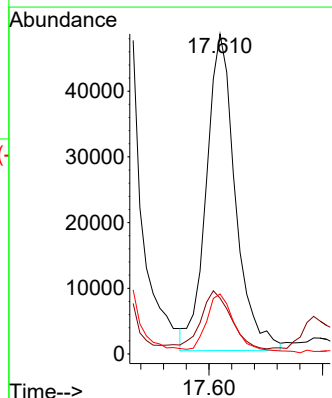
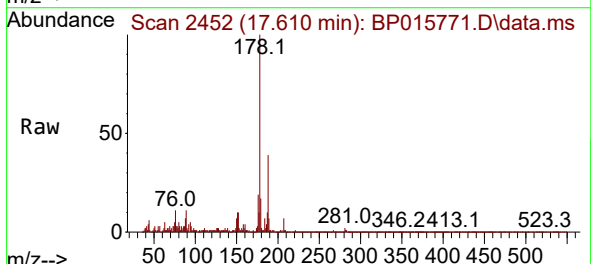


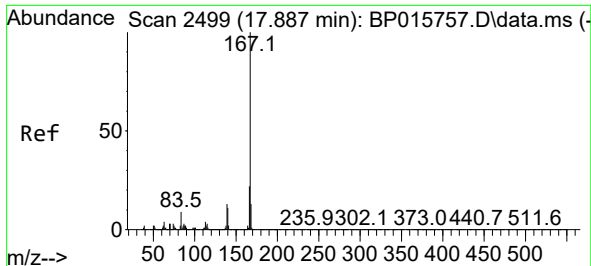

#77
Carbazole
Concen: 1.917 ng/ul
RT: 17.898 min Scan# 2499
Delta R.T. 0.012 min
Lab File: BP015771.D
Acq: 28 Jun 2023 10:26




Instrument :
BNA_P
ClientSampleId :
EZEM0


Tgt Ion:167 Resp: 62748
Ion Ratio Lower Upper
167 100
166 22.7 17.4 26.0
139 14.9 11.0 16.4

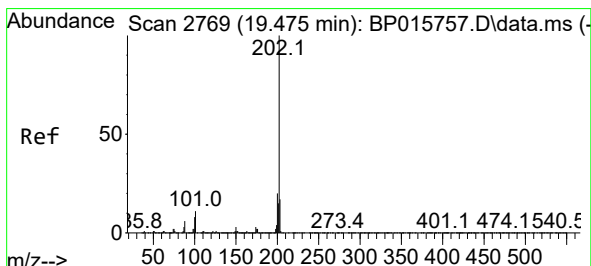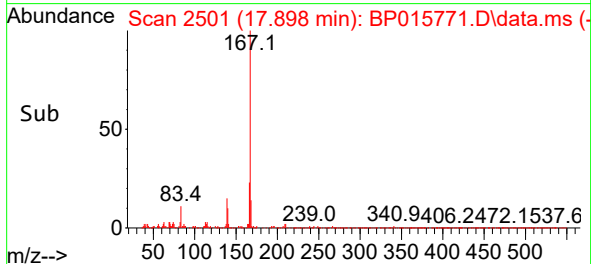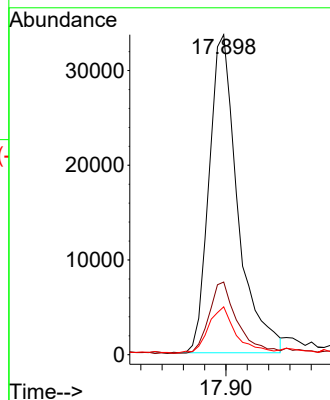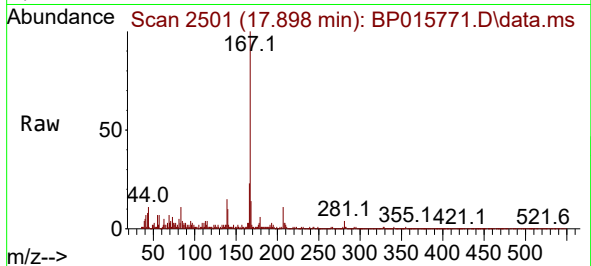

#80
Fluoranthene
Concen: 18.120 ng/ul
RT: 19.474 min Scan# 2769
Delta R.T. -0.000 min
Lab File: BP015771.D
Acq: 28 Jun 2023 10:26

Tgt Ion:202 Resp: 1013101
Ion Ratio Lower Upper
202 100
101 11.2 8.3 12.5
100 8.8 6.6 9.8

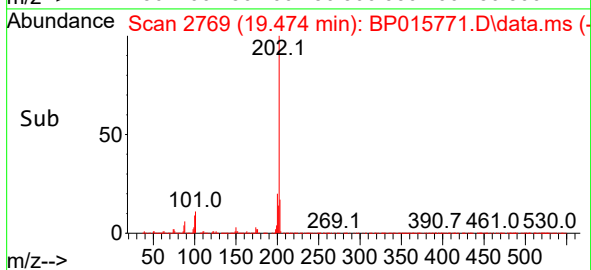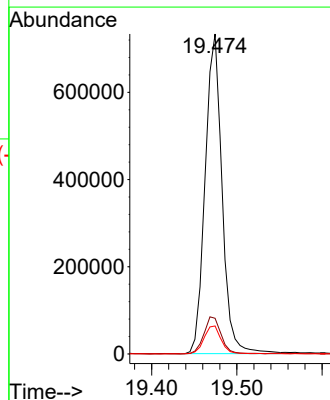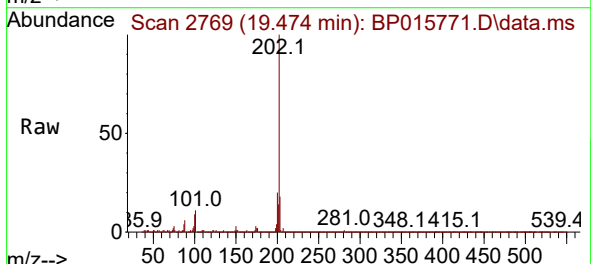

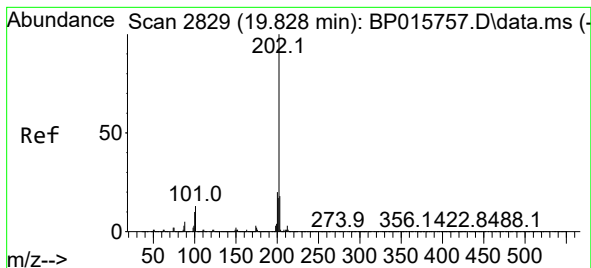

#82

Pyrene

Concen: 13.538 ng/ul

RT: 19.827 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Instrument :

BNA_P

ClientSampleId :

EZEM0





Tgt Ion:202 Resp: 772133

Ion Ratio Lower Upper

202 100

101 12.8 9.3 13.9

100 11.0 7.6 11.4

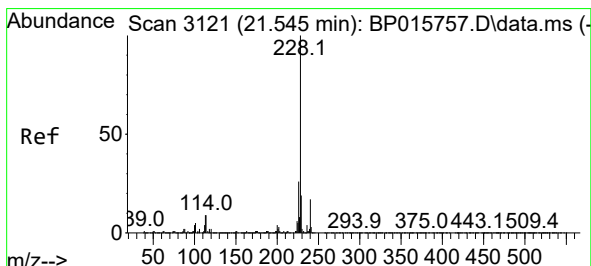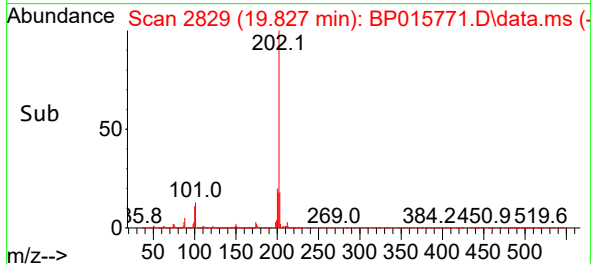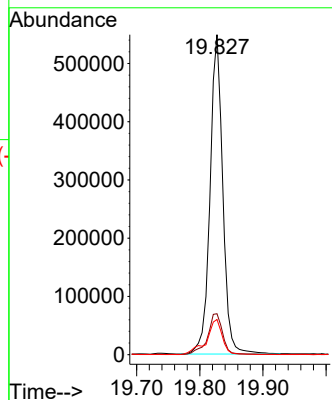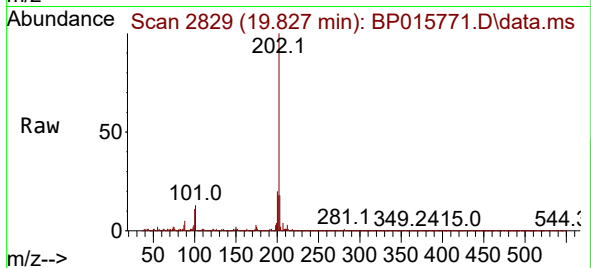

#85

Benzo(a)anthracene

Concen: 5.894 ng/ul

RT: 21.545 min Scan# 3121

Delta R.T. -0.000 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26




Tgt Ion:228 Resp: 285639


Ion Ratio Lower Upper

228 100

229 20.5 15.3 22.9

226 28.4 21.4 32.0

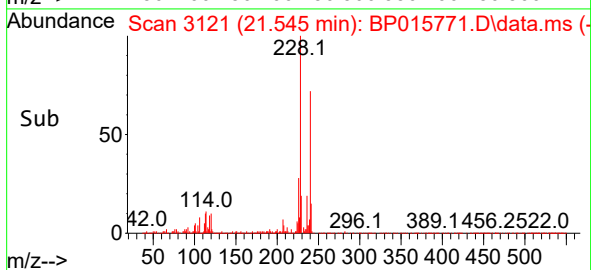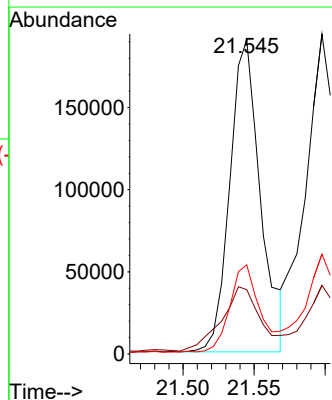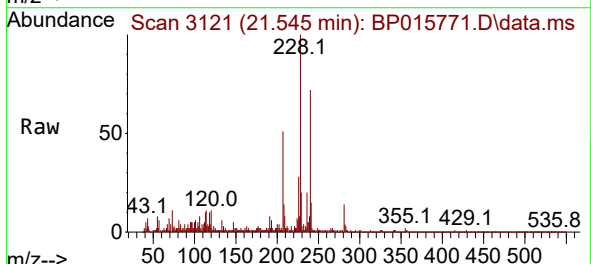

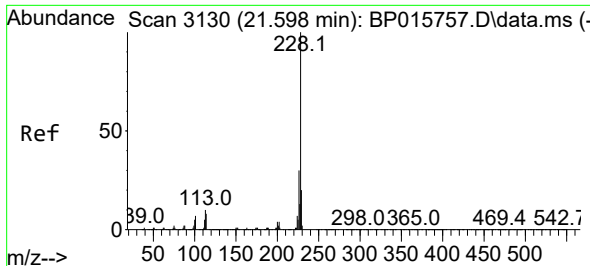

#87

Chrysene

Concen: 6.618 ng/ul

RT: 21.598 min Scan# 3130

Delta R.T. -0.006 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Instrument :

BNA_P

ClientSampleId :

EZEM0





Tgt Ion:228 Resp: 304326

Ion Ratio Lower Upper

228 100

226 31.2 24.3 36.5

229 21.5 15.5 23.3

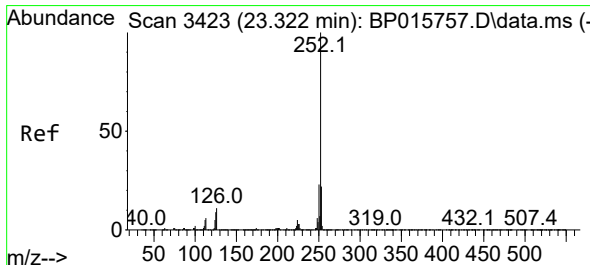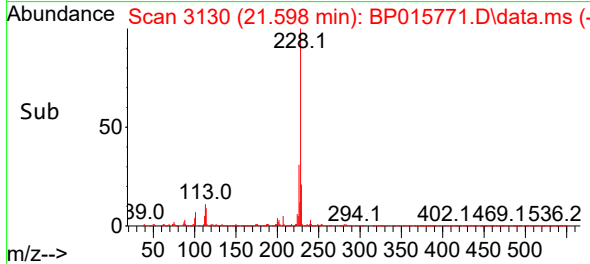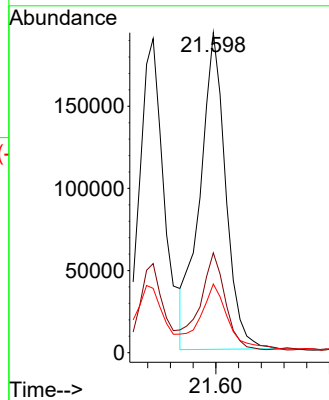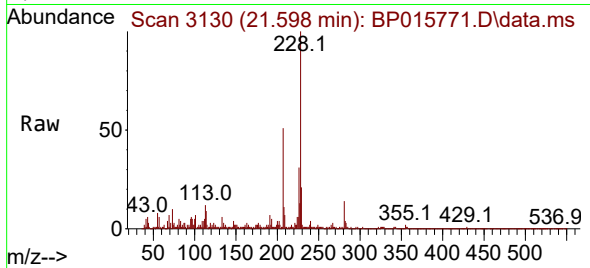

#90

Benzo(b)fluoranthene

Concen: 7.148 ng/ul

RT: 23.321 min Scan# 3423

Delta R.T. -0.006 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26




Tgt Ion:252 Resp: 401600


Ion Ratio Lower Upper

252 100

253 23.4 17.3 25.9

125 11.0 7.5 11.3

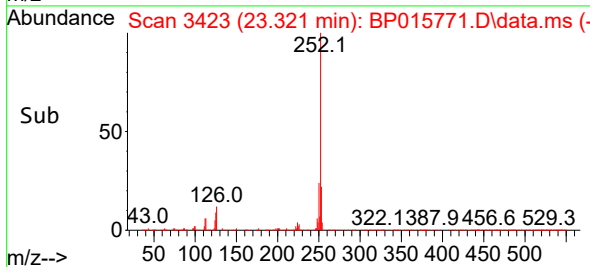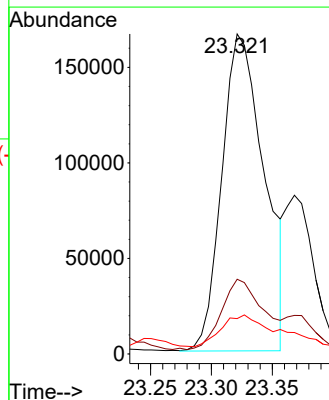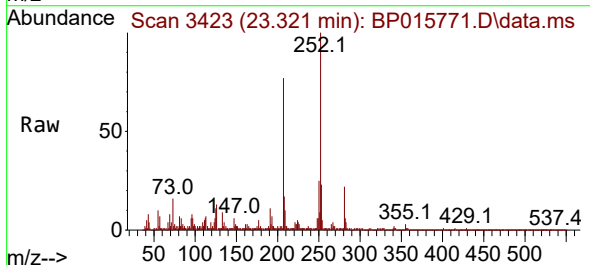

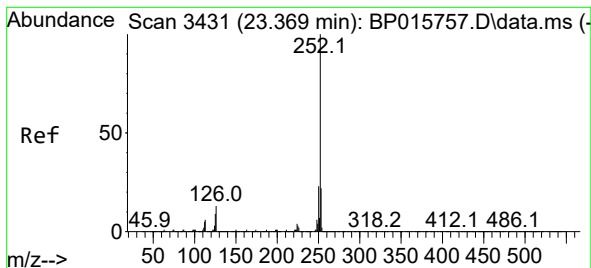

#91

Benzo(k)fluoranthene

Concen: 2.255 ng/ul

RT: 23.368 min Scan# 3431

Delta R.T. -0.012 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Instrument :

BNA_P

ClientSampleId :

EZEM0





Tgt Ion:252 Resp: 128012

Ion Ratio Lower Upper

252 100

253 24.3 17.0 25.4

125 13.5 7.3 10.9#

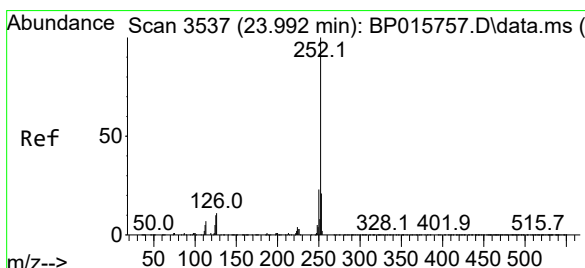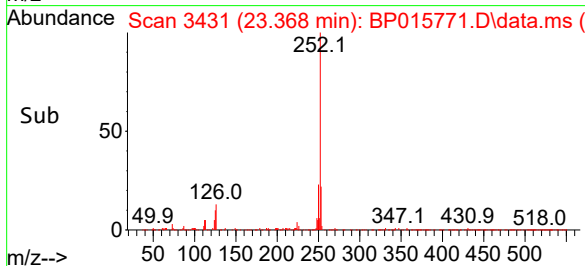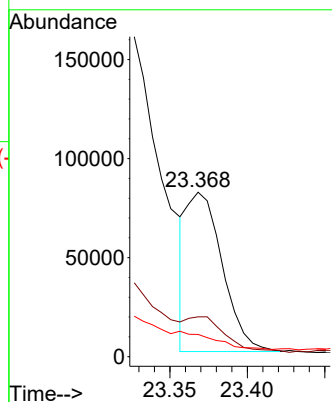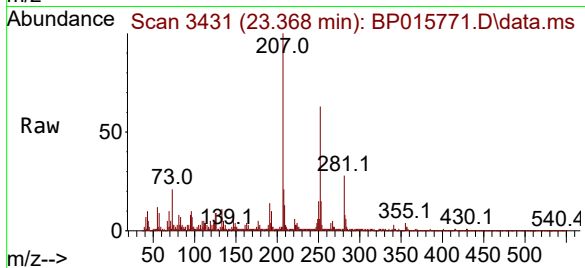

#93

Benzo(a)pyrene

Concen: 5.142 ng/ul

RT: 23.992 min Scan# 3537

Delta R.T. -0.012 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26




Tgt Ion:252 Resp: 252433


Ion Ratio Lower Upper

252 100

253 24.2 17.7 26.5

125 13.3 8.2 12.2#

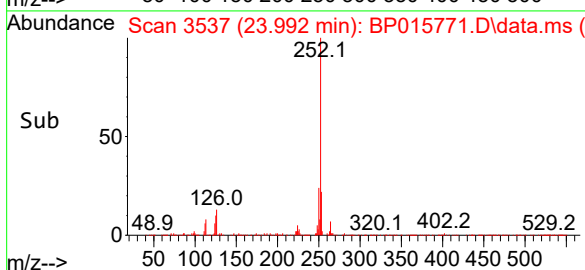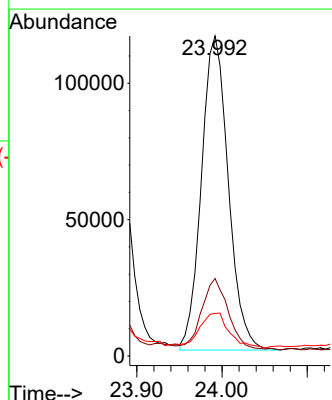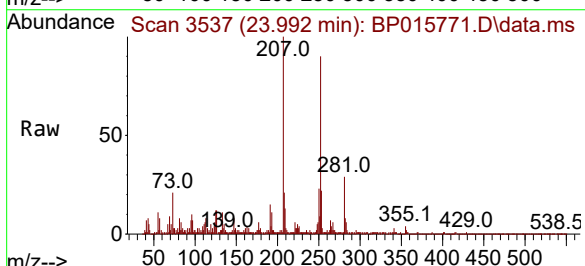

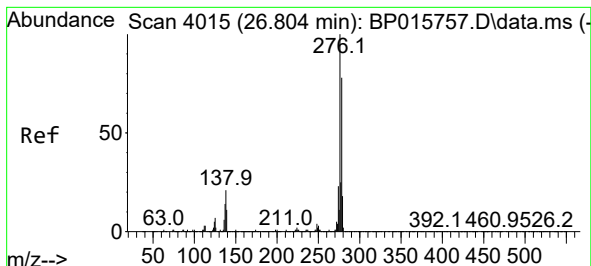

#94

Indeno(1,2,3-cd)pyrene

Concen: 2.924 ng/ul

RT: 26.809 min Scan# 4015

Delta R.T. -0.006 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Instrument :

BNA_P

ClientSampleId :

EZEM0





Tgt Ion:276 Resp: 194851

Ion Ratio Lower Upper

276 100

138 22.0 15.7 23.5

277 24.5 19.6 29.4

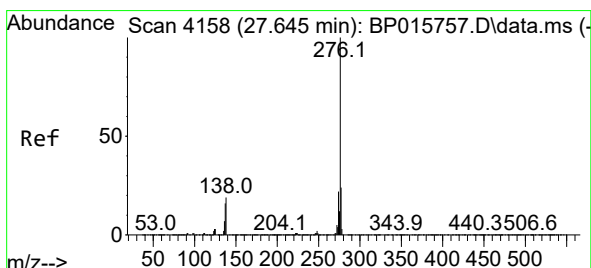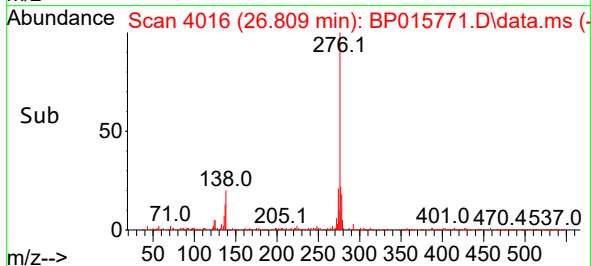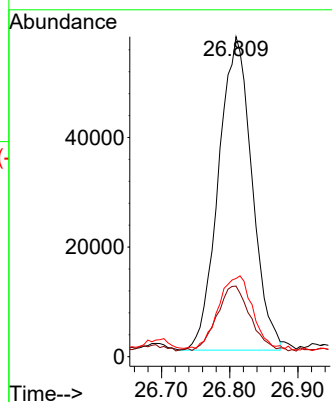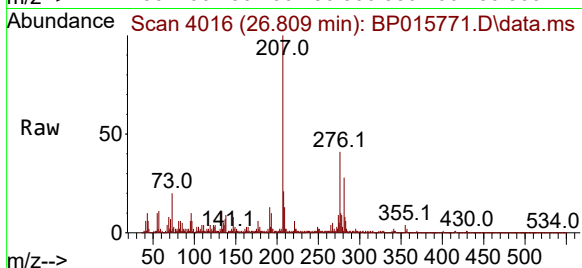

#96

Benzo(g,h,i)perylene

Concen: 3.255 ng/ul

RT: 27.644 min Scan# 4158

Delta R.T. -0.012 min

Lab File: BP015771.D

Acq: 28 Jun 2023 10:26

Tgt Ion:276 Resp: 178484

Ion Ratio Lower Upper

276 100

138 22.8 15.1 22.7#

277 24.4 18.8 28.2

