

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
 Data File : BP015769.D
 Acq On : 28 Jun 2023 09:18
 Operator : MA/JU
 Sample : PB153625BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015769.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	43	rVB	50776	72820	2.45%	0.204%
2	3.828	107	109	128	rBV	503606	836781	28.10%	2.349%
3	4.152	161	164	172	rVB	20139	31268	1.05%	0.088%
4	6.911	630	633	635	rBV4	2710	3788	0.13%	0.011%
5	7.228	679	687	707	rBV	450108	1098949	36.90%	3.086%
6	7.387	708	714	733	rVB	469565	883239	29.66%	2.480%
7	7.587	741	748	766	rBV	635207	1177733	39.55%	3.307%
8	8.058	821	828	846	rBV	647671	1282189	43.06%	3.600%
9	8.787	943	952	976	rBV	574618	1355035	45.50%	3.805%
10	9.122	1006	1009	1014	rVB6	2074	3955	0.13%	0.011%
11	9.252	1021	1031	1049	rBV	493952	1088678	36.56%	3.057%
12	9.975	1148	1154	1169	rVV	389506	879056	29.52%	2.468%
13	10.069	1169	1170	1181	rVB10	8029	16026	0.54%	0.045%
14	10.540	1241	1250	1290	rBV	341852	1253253	42.08%	3.519%
15	10.887	1302	1309	1327	rBV	878874	1658258	55.68%	4.656%
16	11.057	1330	1338	1365	rBV	339742	1163658	39.08%	3.267%
17	12.528	1580	1588	1596	rBV9	6772	17535	0.59%	0.049%
18	13.546	1755	1761	1762	rBV6	2808	3751	0.13%	0.011%
19	13.593	1765	1769	1776	rVV5	8456	14743	0.50%	0.041%
20	14.122	1852	1859	1877	rVV	865143	1629137	54.71%	4.574%
21	14.410	1901	1908	1926	rBV	1151517	1975753	66.35%	5.547%
22	14.710	1952	1959	1980	rBV	1130136	1842718	61.88%	5.174%
23	14.998	2001	2008	2025	rBV4	78874	380844	12.79%	1.069%
24	15.716	2122	2130	2147	rBV	1123859	2216891	74.44%	6.224%
25	15.881	2152	2158	2182	rVV2	143077	475667	15.97%	1.336%
26	16.998	2345	2348	2351	rBV5	3233	4811	0.16%	0.014%
27	17.145	2370	2373	2375	rBV4	2862	3981	0.13%	0.011%
28	17.387	2412	2414	2419	rBV5	2771	4267	0.14%	0.012%
29	17.475	2422	2429	2440	rVV	1129181	1882310	63.21%	5.285%
30	17.575	2440	2446	2472	rVB2	1086041	2265523	76.08%	6.361%
31	19.381	2750	2753	2758	rBV5	20929	27993	0.94%	0.079%
32	19.804	2819	2825	2845	rBV	1530797	2760683	92.70%	7.751%
33	21.569	3120	3125	3135	rBV2	1153445	2039890	68.50%	5.727%
34	23.939	3521	3528	3544	rVB3	1196102	2977962	100.00%	8.361%
35	24.110	3551	3557	3572	rVB	893804	2287352	76.81%	6.422%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
Data File : BP015769.D
Acq On : 28 Jun 2023 09:18
Operator : MA/JU
Sample : PB153625BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK625

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 35616497

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
Data File : BP015769.D
Acq On : 28 Jun 2023 09:18
Operator : MA/JU
Sample : PB153625BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK625

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

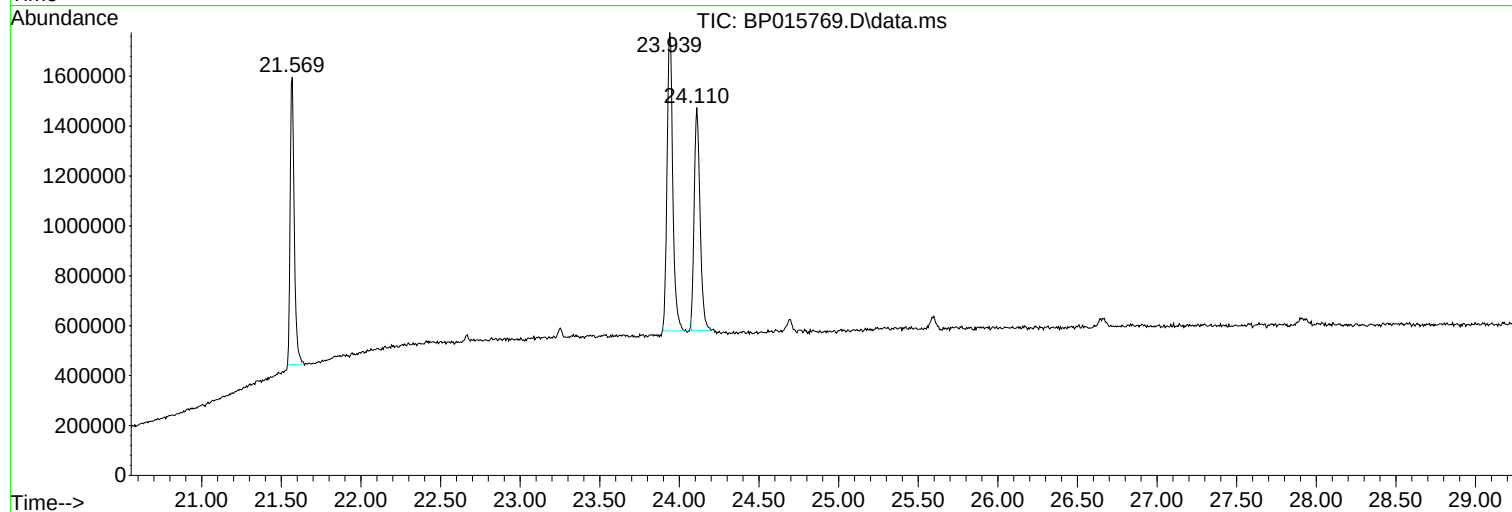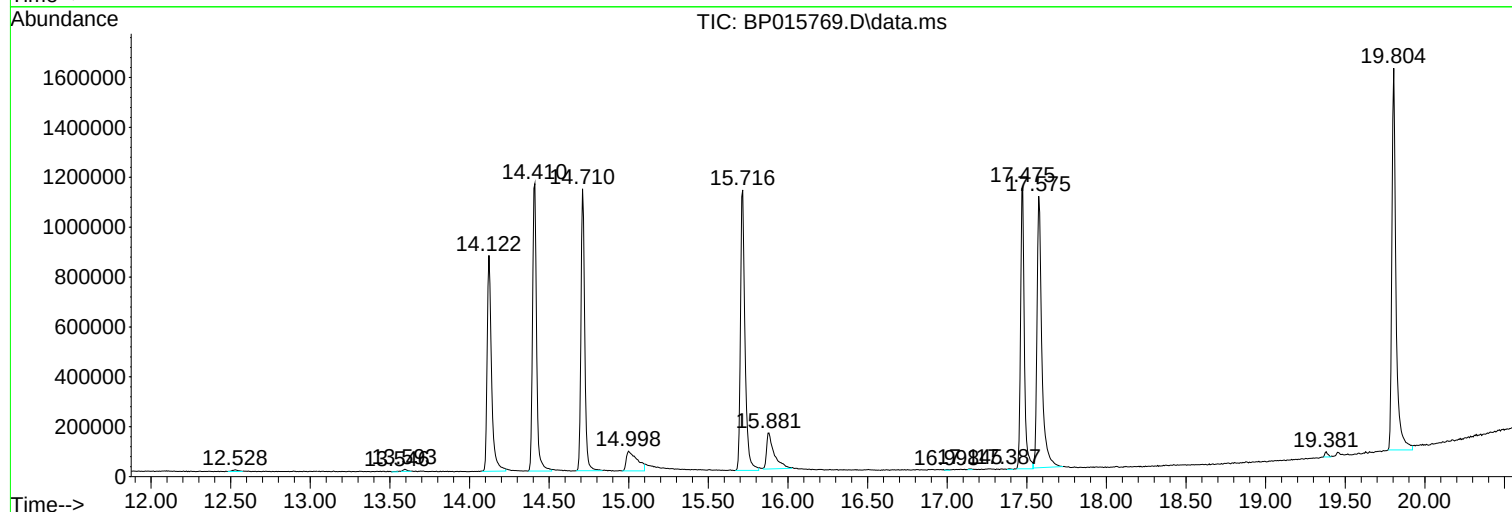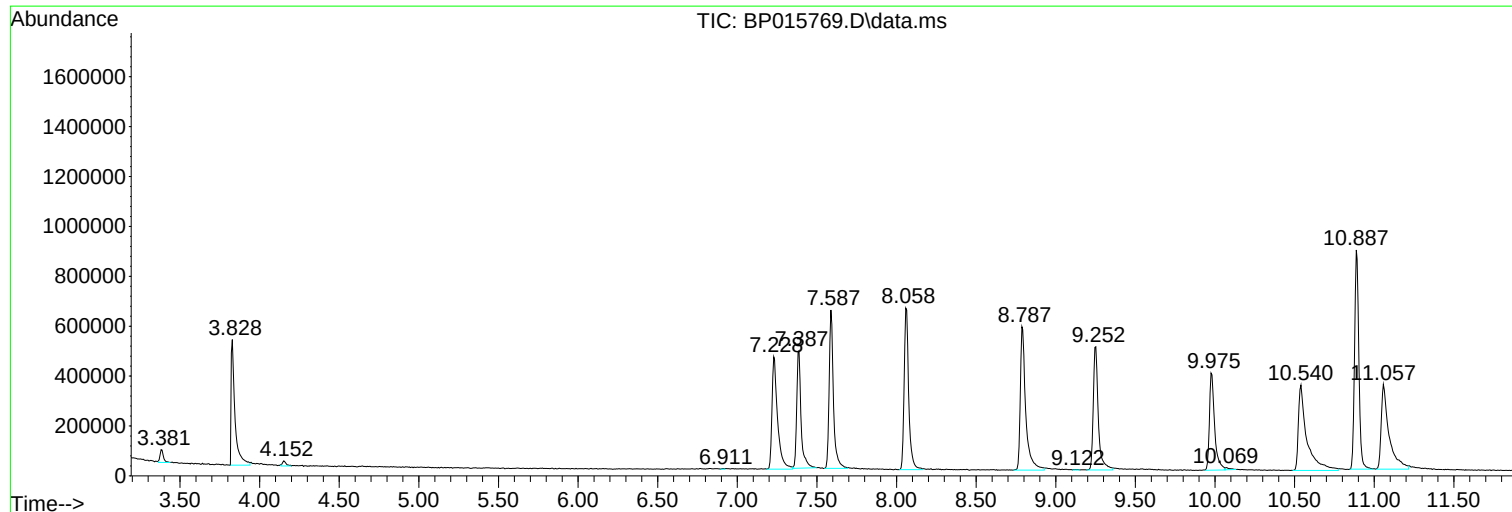

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
Data File : BP015769.D
Acq On : 28 Jun 2023 09:18
Operator : MA/JU
Sample : PB153625BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK625

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062823\
Data File : BP015769.D
Acq On : 28 Jun 2023 09:18
Operator : MA/JU
Sample : PB153625BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK625

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc