

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
 Data File : BP015798.D
 Acq On : 29 Jun 2023 07:52
 Operator : MA/JU
 Sample : PB153627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	40	rVB	82905	106216	2.34%	0.187%
2	3.822	105	108	124	rBV	855686	1443328	31.75%	2.541%
3	4.152	160	164	168	rVB	24480	34025	0.75%	0.060%
4	7.228	680	687	706	rBV	772879	1806143	39.73%	3.180%
5	7.381	707	713	729	rVB	847722	1491012	32.80%	2.625%
6	7.587	741	748	772	rVB	1046089	1906080	41.93%	3.356%
7	8.057	819	828	845	rBV	795325	1536193	33.80%	2.704%
8	8.787	945	952	972	rVV	1039389	2299443	50.59%	4.048%
9	9.246	1022	1030	1046	rBV	879530	1823655	40.12%	3.211%
10	9.510	1072	1075	1078	rBV5	3495	4628	0.10%	0.008%
11	9.975	1146	1154	1178	rVV	707981	1521118	33.46%	2.678%
12	10.534	1241	1249	1272	rBV	640974	2083817	45.84%	3.669%
13	10.887	1301	1309	1323	rBV	1198916	2193459	48.25%	3.862%
14	11.051	1329	1337	1362	rBV	682754	2138227	47.04%	3.764%
15	12.028	1500	1503	1508	rVB7	2769	4669	0.10%	0.008%
16	12.081	1508	1512	1515	rBV6	3246	5170	0.11%	0.009%
17	12.516	1581	1586	1592	rVV	13240	26258	0.58%	0.046%
18	12.893	1646	1650	1653	rVB6	2892	5054	0.11%	0.009%
19	12.934	1653	1657	1660	rBV6	3136	4941	0.11%	0.009%
20	13.587	1764	1768	1776	rVB5	13812	24273	0.53%	0.043%
21	13.692	1783	1786	1789	rBV5	3154	4877	0.11%	0.009%
22	14.116	1851	1858	1885	rBV	1789898	3138761	69.05%	5.526%
23	14.404	1899	1907	1927	rBV2	2296497	3774472	83.04%	6.645%
24	14.704	1952	1958	1977	rBV	1627770	2649982	58.30%	4.665%
25	14.987	1999	2006	2027	rBV3	169397	807961	17.77%	1.422%
26	15.704	2121	2128	2150	rBV	2297322	4326816	95.19%	7.617%
27	15.869	2150	2156	2180	rVV	305509	887913	19.53%	1.563%
28	17.469	2421	2428	2439	rBV	1697305	2654848	58.40%	4.674%
29	17.569	2439	2445	2468	rVB2	2175912	4126002	90.77%	7.264%
30	18.404	2584	2587	2588	rBV3	7219	7772	0.17%	0.014%
31	19.380	2749	2753	2759	rVB5	26487	41157	0.91%	0.072%
32	19.451	2762	2765	2773	rVV3	27679	53995	1.19%	0.095%
33	19.798	2818	2824	2838	rBV	2562972	4377982	96.31%	7.708%
34	21.563	3119	3124	3136	rBV2	1338351	2348956	51.68%	4.135%
35	23.933	3520	3527	3540	rVB2	1827200	4545585	100.00%	8.003%
36	24.104	3550	3556	3571	rVB	1015756	2596681	57.13%	4.572%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015798.D
Acq On : 29 Jun 2023 07:52
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 56801469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015798.D
Acq On : 29 Jun 2023 07:52
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

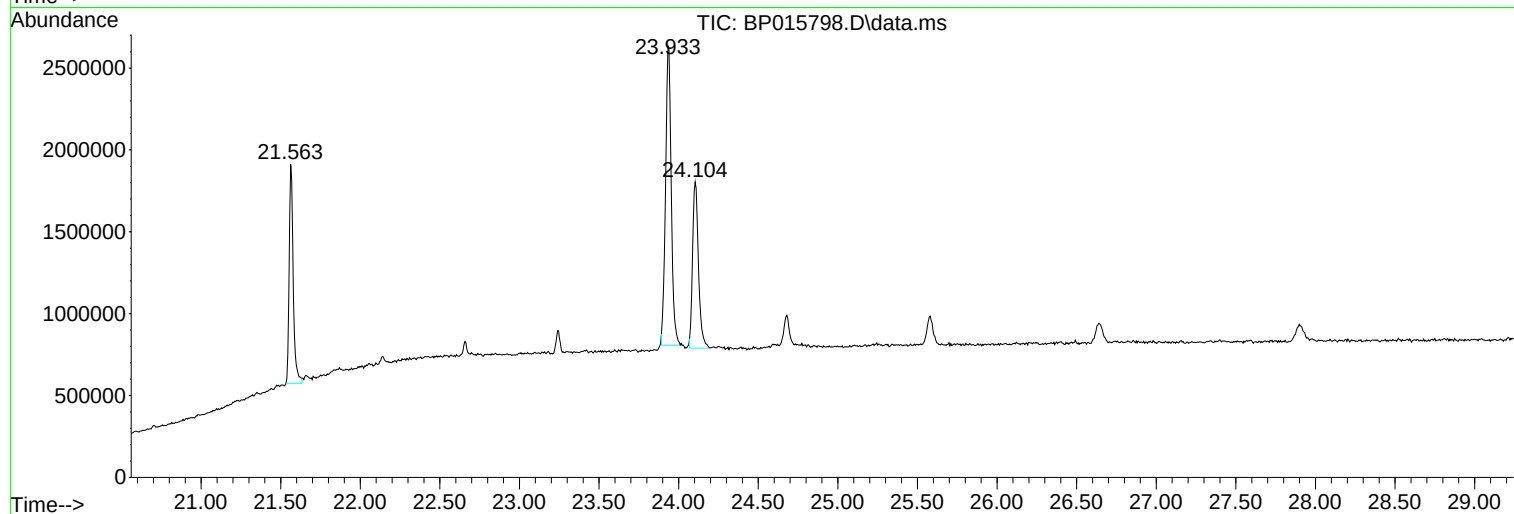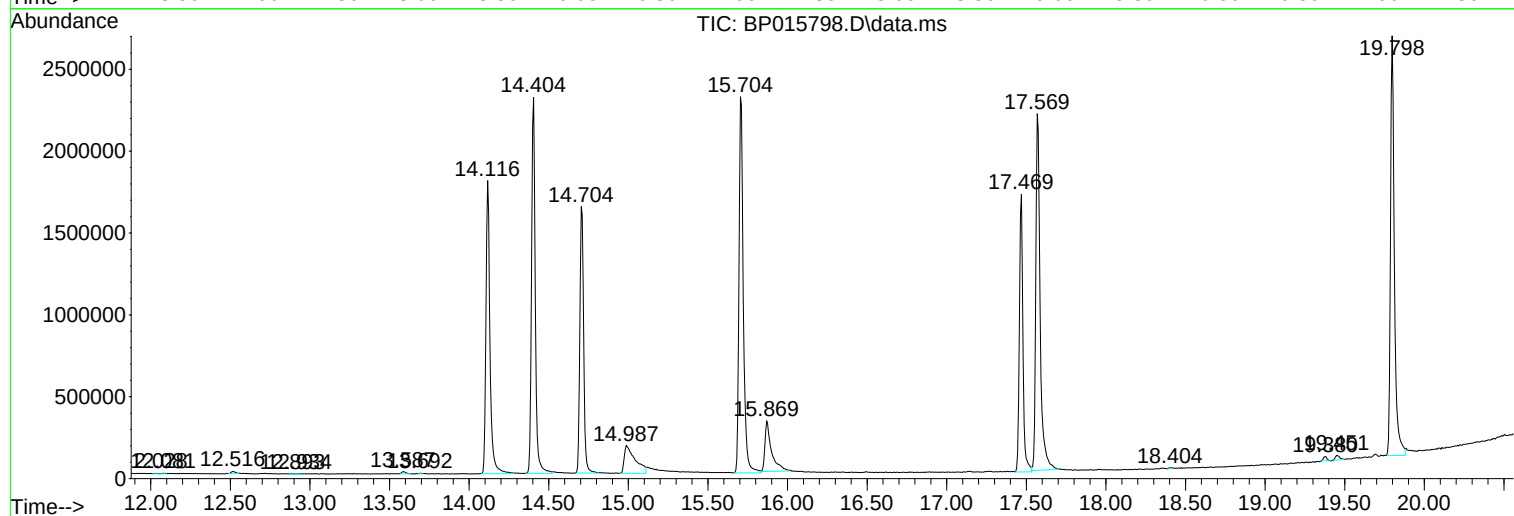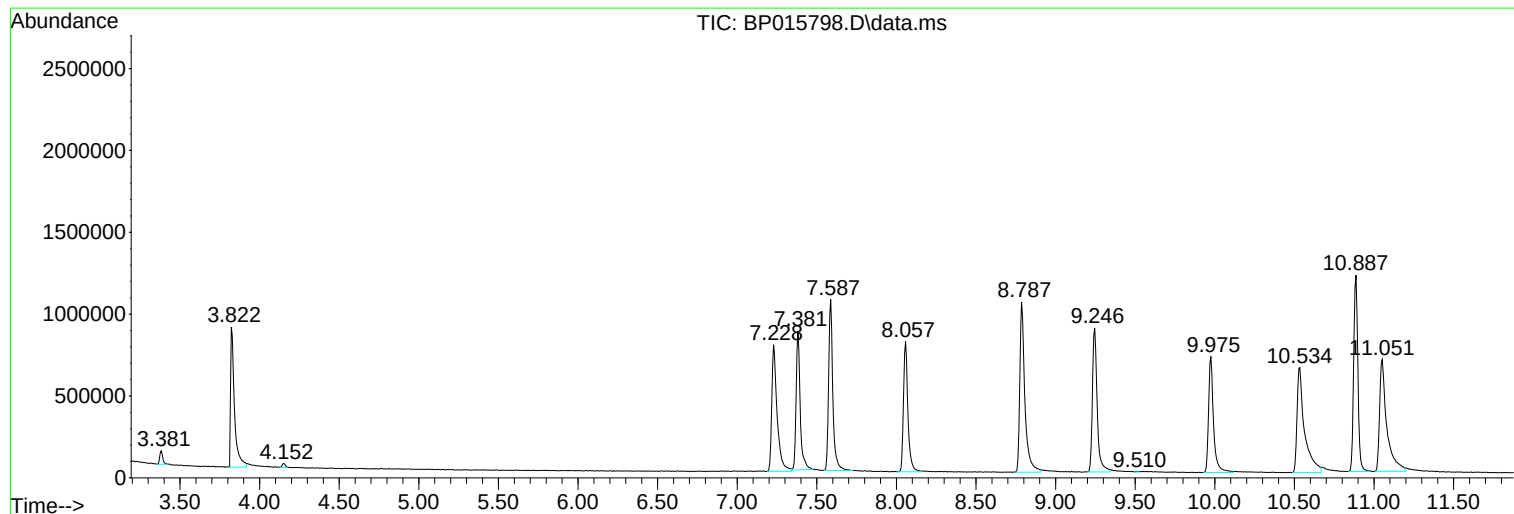

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015798.D
Acq On : 29 Jun 2023 07:52
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015798.D
Acq On : 29 Jun 2023 07:52
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------