

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
 Data File : BP015815.D
 Acq On : 29 Jun 2023 18:04
 Operator : MA/JU
 Sample : PB153627BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	43	rVB	87185	115595	2.32%	0.226%
2	3.828	106	109	133	rBV	785301	1343373	26.93%	2.630%
3	4.152	160	164	169	rBV	22066	30032	0.60%	0.059%
4	7.234	681	688	707	rBV	670054	1649414	33.07%	3.229%
5	7.381	707	713	730	rVV	758969	1365117	27.37%	2.672%
6	7.587	741	748	773	rVB	951296	1773359	35.56%	3.472%
7	8.057	821	828	842	rBV	759873	1442943	28.93%	2.825%
8	8.793	945	953	979	rBV	836376	2012140	40.34%	3.939%
9	9.246	1021	1030	1061	rBV	748092	1621938	32.52%	3.175%
10	9.975	1146	1154	1178	rBV	543149	1294263	25.95%	2.534%
11	10.540	1242	1250	1282	rBV	483113	1777539	35.64%	3.480%
12	10.887	1301	1309	1329	rBV	1004304	1895094	38.00%	3.710%
13	11.057	1331	1338	1371	rBV	514161	1746103	35.01%	3.418%
14	12.522	1580	1587	1594	rBV4	11677	24490	0.49%	0.048%
15	13.587	1764	1768	1773	rBV4	15561	27999	0.56%	0.055%
16	14.122	1852	1859	1883	rBV	1245942	2369148	47.50%	4.638%
17	14.404	1900	1907	1926	rBV	1754047	2954037	59.23%	5.783%
18	14.710	1951	1959	1978	rBV	1278159	2097652	42.06%	4.106%
19	14.998	2002	2008	2042	rBV3	141552	816987	16.38%	1.599%
20	15.710	2122	2129	2146	rBV	1758160	3421319	68.60%	6.698%
21	15.875	2151	2157	2183	rVV2	239353	752598	15.09%	1.473%
22	16.498	2259	2263	2268	rBV8	3943	6019	0.12%	0.012%
23	17.469	2421	2428	2439	rBV	1422591	2280441	45.72%	4.464%
24	17.569	2439	2445	2469	rVB2	1845990	3619046	72.56%	7.085%
25	19.451	2762	2765	2770	rVB4	25922	41261	0.83%	0.081%
26	19.798	2818	2824	2842	rBV	2649586	4401526	88.25%	8.617%
27	21.563	3119	3124	3135	rBV	1455127	2448015	49.08%	4.792%
28	23.933	3519	3527	3543	rVB	1945254	4987593	100.00%	9.764%
29	24.104	3549	3556	3570	rVB	1080742	2766511	55.47%	5.416%




Sum of corrected areas: 51081552

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015815.D
Acq On : 29 Jun 2023 18:04
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

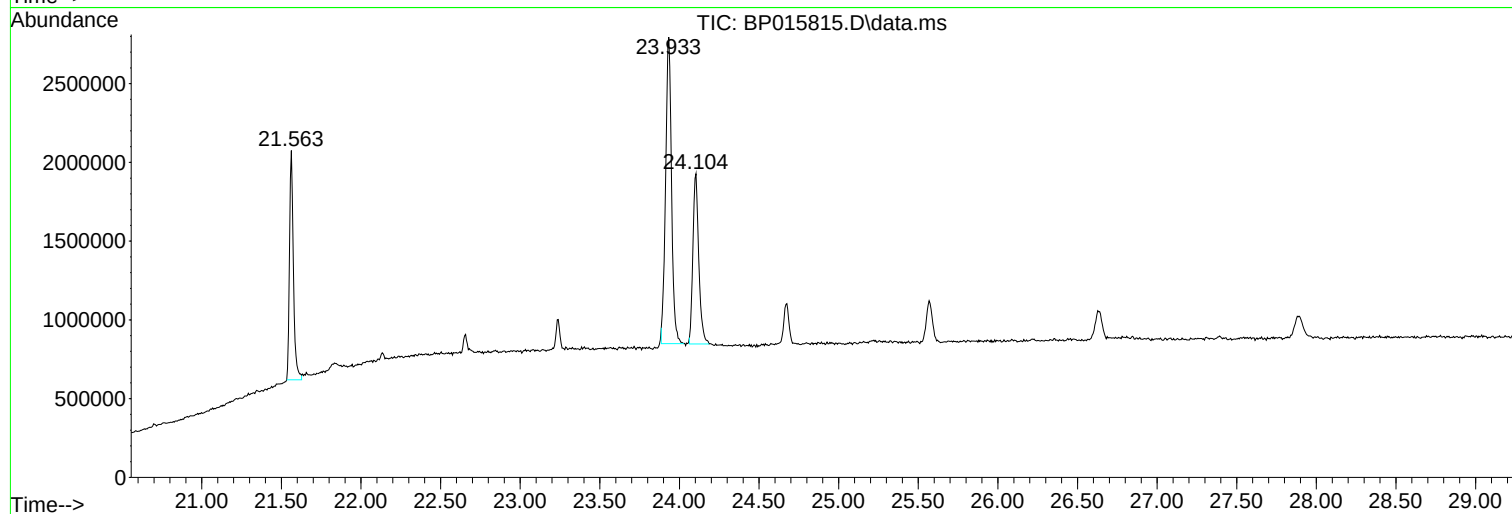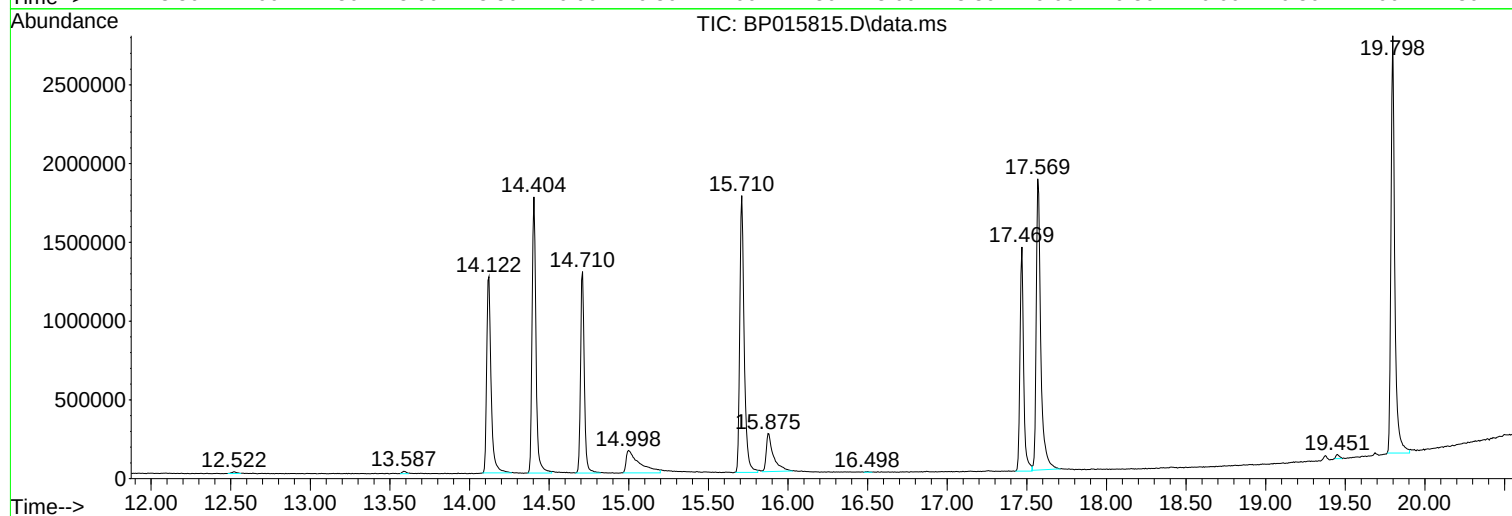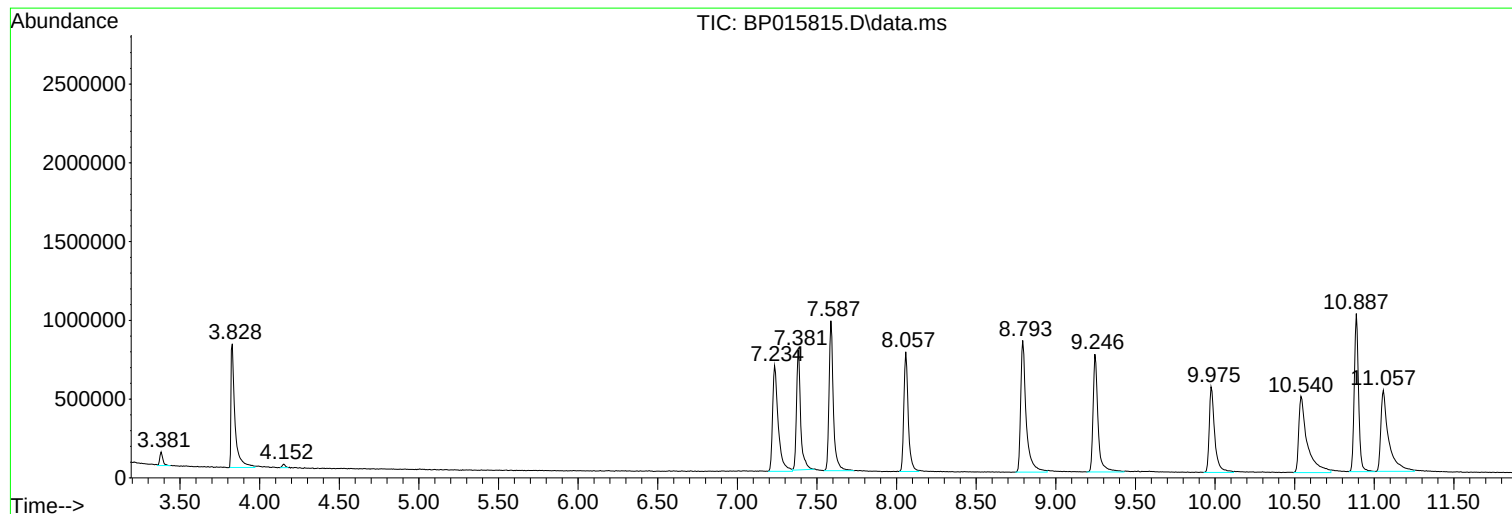

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015815.D
Acq On : 29 Jun 2023 18:04
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015815.D
Acq On : 29 Jun 2023 18:04
Operator : MA/JU
Sample : PB153627BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK627

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------