

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
 Data File : BP015816.D
 Acq On : 29 Jun 2023 18:38
 Operator : MA/JU
 Sample : PB153514BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK514

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	39	rBV	98666	137286	1.85%	0.167%
2	3.822	105	108	135	rBV	1146775	1996447	26.85%	2.432%
3	4.152	160	164	170	rVB	28593	42978	0.58%	0.052%
4	7.228	680	687	707	rBV	1113537	2505827	33.70%	3.052%
5	7.381	707	713	739	rVB	1143366	2063519	27.75%	2.513%
6	7.587	741	748	767	rVV	1409187	2561621	34.45%	3.120%
7	8.057	819	828	842	rBV	898489	1719285	23.12%	2.094%
8	8.787	945	952	977	rBV	1515815	3188258	42.88%	3.883%
9	9.240	1022	1029	1057	rBV	1266647	2563018	34.47%	3.122%
10	9.969	1146	1153	1177	rBV	1012159	2126142	28.60%	2.590%
11	10.528	1238	1248	1280	rBV	1006047	3082846	41.46%	3.755%
12	10.887	1301	1309	1324	rBV	1414961	2559692	34.43%	3.118%
13	11.046	1329	1336	1371	rBV	1025402	3067155	41.25%	3.736%
14	12.516	1580	1586	1593	rBV3	17440	39528	0.53%	0.048%
15	13.587	1763	1768	1778	rVB3	19932	39061	0.53%	0.048%
16	13.692	1781	1786	1789	rBV7	5099	9308	0.13%	0.011%
17	14.116	1851	1858	1881	rBV	2676220	4553299	61.24%	5.546%
18	14.404	1899	1907	1929	rBV	3451730	5590442	75.19%	6.809%
19	14.704	1951	1958	1973	rBV	2144850	3309339	44.51%	4.031%
20	14.969	1997	2003	2038	rBV	408609	1774251	23.86%	2.161%
21	15.704	2120	2128	2148	rBV	3851078	6644600	89.37%	8.093%
22	15.863	2149	2155	2167	rBV	682216	1543671	20.76%	1.880%
23	16.486	2259	2261	2269	rVB9	5730	9218	0.12%	0.011%
24	17.139	2367	2372	2374	rBV6	7421	10979	0.15%	0.013%
25	17.463	2421	2427	2438	rBV	2544866	3730809	50.18%	4.544%
26	17.569	2438	2445	2472	rVB	3999662	7054545	94.88%	8.592%
27	19.369	2748	2751	2757	rBV2	51985	69924	0.94%	0.085%
28	19.445	2760	2764	2771	rBV	47698	84268	1.13%	0.103%
29	19.792	2817	2823	2844	rBV	4513737	7434857	100.00%	9.055%
30	21.557	3118	3123	3137	rBV	1718859	3182187	42.80%	3.876%
31	23.933	3519	3527	3541	rVB2	2560477	6264455	84.26%	7.630%
32	24.104	3549	3556	3572	rVB	1191059	3144443	42.29%	3.830%




Sum of corrected areas: 82103258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015816.D
Acq On : 29 Jun 2023 18:38
Operator : MA/JU
Sample : PB153514BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

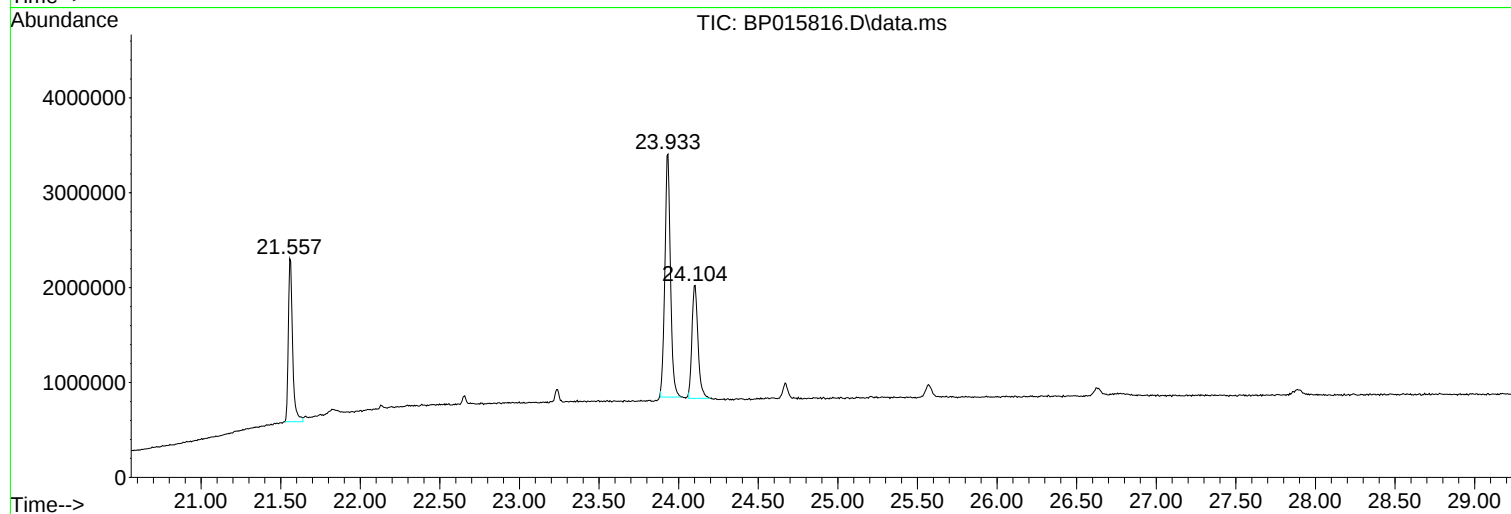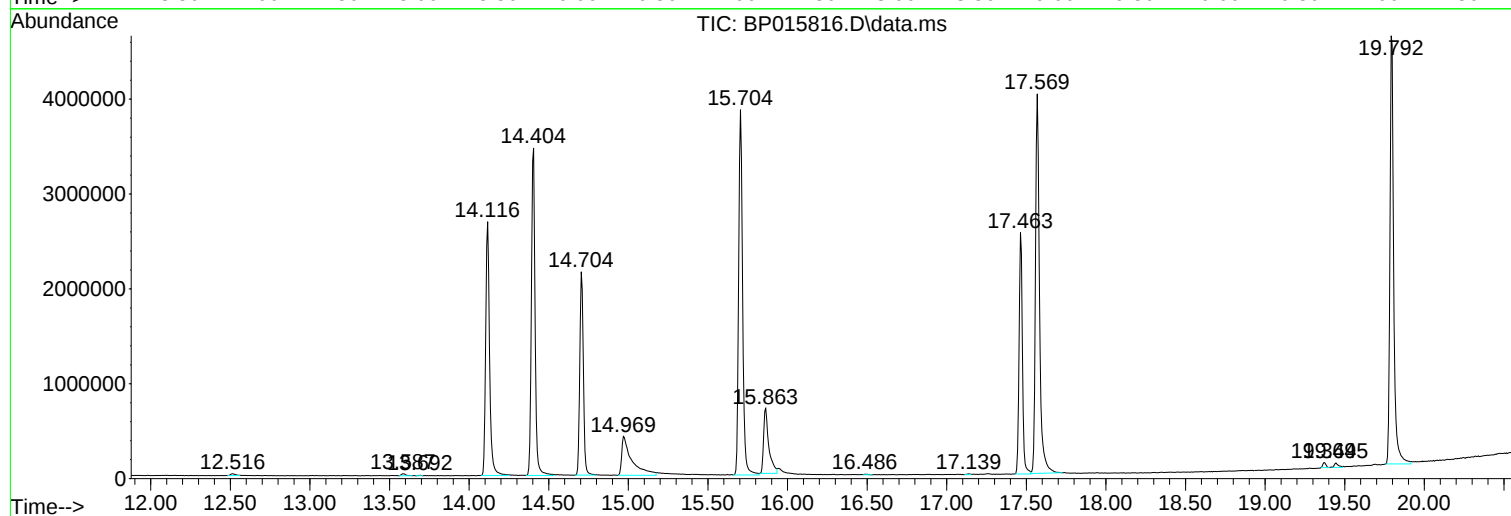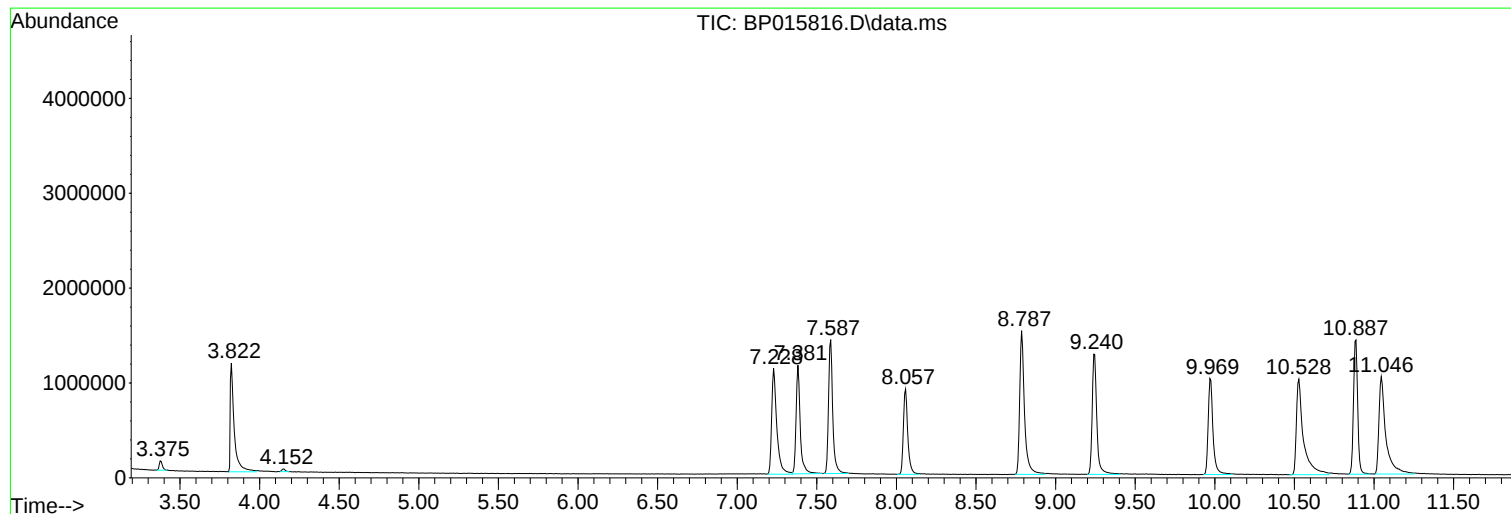

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015816.D
Acq On : 29 Jun 2023 18:38
Operator : MA/JU
Sample : PB153514BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062923\
Data File : BP015816.D
Acq On : 29 Jun 2023 18:38
Operator : MA/JU
Sample : PB153514BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc