

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015898.D
 Acq On : 01 Jul 2023 23:19
 Operator : MA/JU
 Sample : 03242-14
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGB5

Quant Time: Jul 02 02:45:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 02:29:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	283264	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1211965	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.704	164	676304	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1189846	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	846909	20.000	ng/ul	# 0.00
88) Perylene-d12	24.098	264	1007362	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	16270	2.067	ng/uL	0.00
4) Pyridine-d5	3.816	84	974	0.049	ng/ul	0.00
7) Phenol-d5	7.240	99	285090	11.763	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.381	67	208914	13.933	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	241931	13.224	ng/ul	0.00
15) 4-Methylphenol-d8	8.804	113	159756	8.344	ng/ul	0.02
21) Nitrobenzene-d5	9.251	128	117795	12.718	ng/ul	0.02
24) 2-Nitrophenol-d4	9.975	143	125563	11.615	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.563	165	204771	10.630	ng/ul	0.04
31) 4-Chloroaniline-d4	11.087	131	85953	3.473	ng/ul	0.05
46) Dimethylphthalate-d6	14.116	166	710896	13.600	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	782716	13.320	ng/ul	0.00
54) 4-Nitrophenol-d4	14.975	143	47	0.007	ng/ul	0.00
60) Fluorene-d10	15.704	176	565345	13.135	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	69	0.009	ng/ul	-0.02
73) Anthracene-d10	17.569	188	700465	12.888	ng/ul	0.00
81) Pyrene-d10	19.792	212	723680	13.086	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	673437	13.252	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.281	94	29304	1.165	ng/ul	95
16) Acetophenone	8.910	105	96096	3.053	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015898.D
Acq On : 01 Jul 2023 23:19
Operator : MA/JU
Sample : 03242-14
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGB5

Quant Time: Jul 02 02:45:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 02:29:46 2023
Response via : Initial Calibration




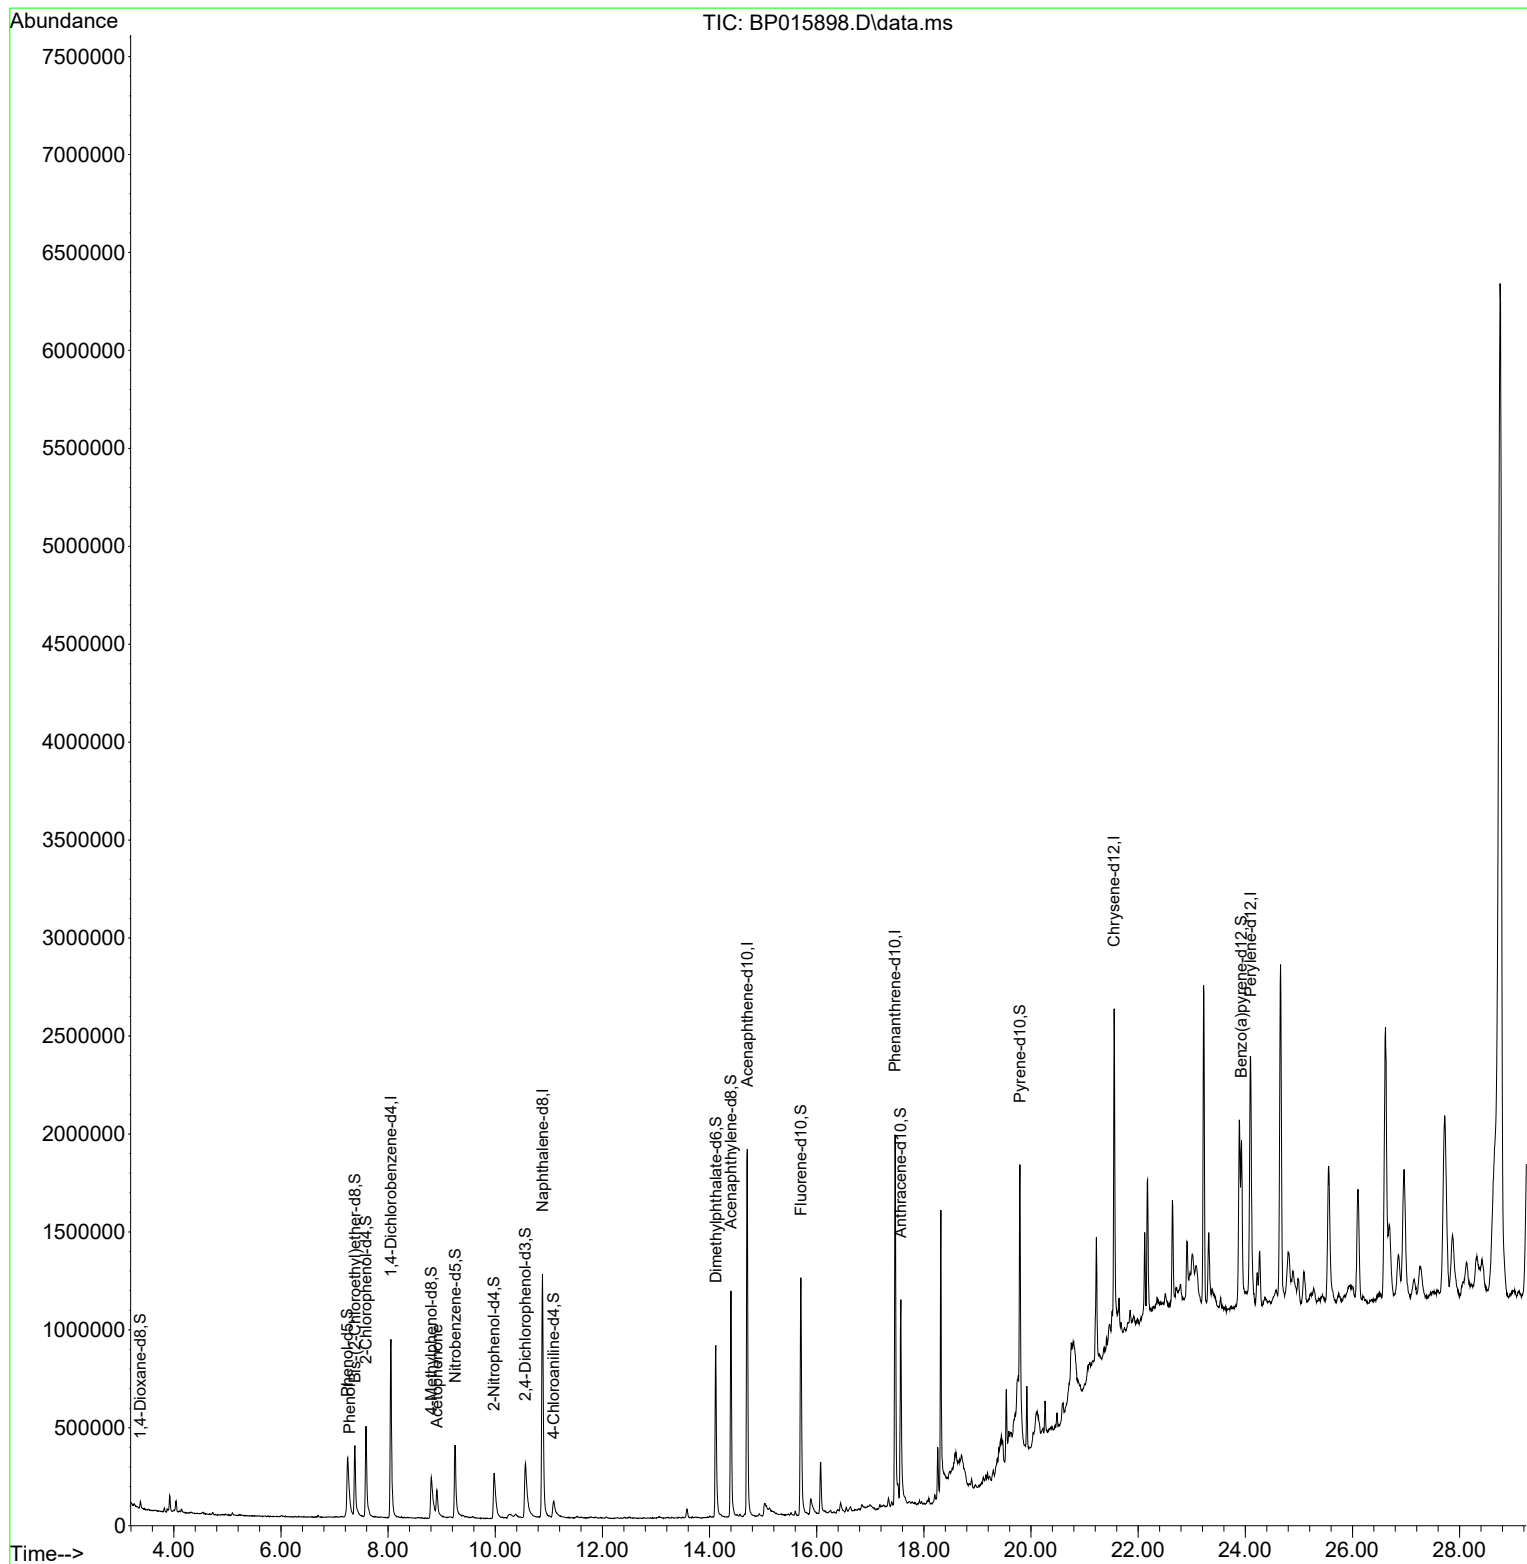


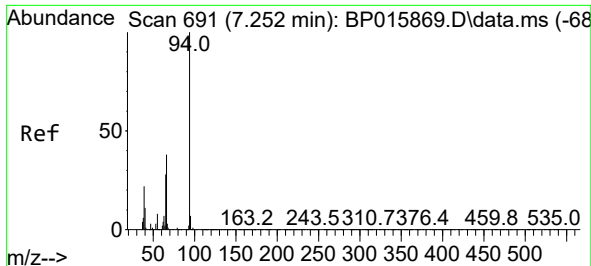

#8
Phenol
Concen: 1.165 ng/ul
RT: 7.281 min Scan# 691
Delta R.T. 0.023 min
Lab File: BP015898.D
Acq: 01 Jul 2023 23:19

Instrument :
BNA_P
ClientSampleId :
DCGB5

Tgt Ion: 94	Resp: 29304
Ion Ratio	Lower Upper
94 100	
65 28.0	26.4 39.6
66 48.5	37.3 55.9

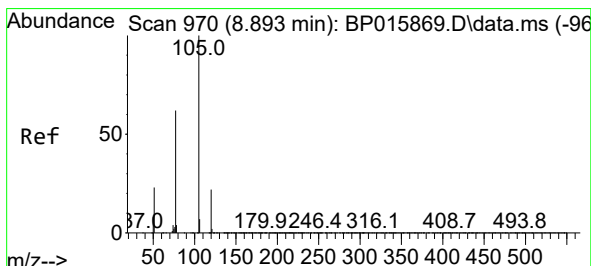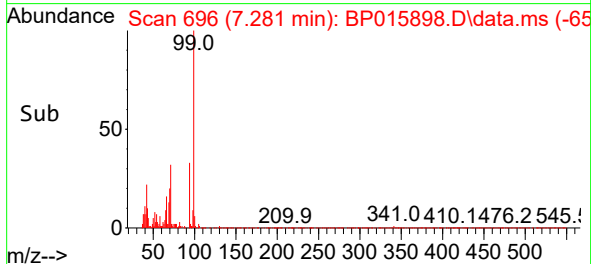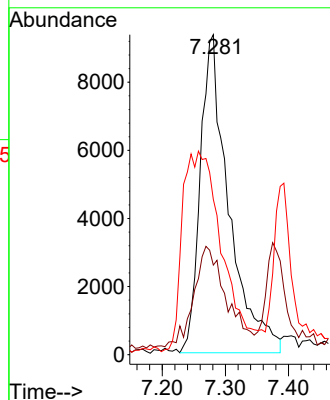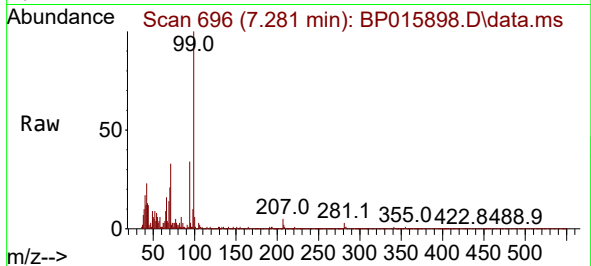

#16
Acetophenone
Concen: 3.053 ng/ul
RT: 8.910 min Scan# 973
Delta R.T. 0.017 min
Lab File: BP015898.D
Acq: 01 Jul 2023 23:19

Tgt Ion: 105	Resp: 96096
Ion Ratio	Lower Upper
105 100	
77 83.3	65.0 97.4
51 32.5	25.1 37.7

