

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015899.D
 Acq On : 01 Jul 2023 23:53
 Operator : MA/JU
 Sample : 03242-21
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC2

Quant Time: Jul 02 02:45:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 02:29:46 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	301299	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1331299	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	791816	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1536209	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.557	240	949834	20.000	ng/ul	0.00
88) Perylene-d12	24.098	264	1107300	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	18328	2.189	ng/uL	0.00
4) Pyridine-d5	3.828	84	540	0.026	ng/ul	0.01
7) Phenol-d5	7.246	99	335947	13.032	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.375	67	243447	15.264	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	279688	14.372	ng/ul	0.00
15) 4-Methylphenol-d8	8.799	113	215070	10.560	ng/ul	0.01
21) Nitrobenzene-d5	9.246	128	142459	14.002	ng/ul	0.01
24) 2-Nitrophenol-d4	9.975	143	153330	12.912	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.551	165	240238	11.353	ng/ul	0.03
31) 4-Chloroaniline-d4	11.069	131	229121	8.429	ng/ul	0.03
46) Dimethylphthalate-d6	14.110	166	886994	14.493	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	1011523	14.703	ng/ul	0.00
54) 4-Nitrophenol-d4	15.010	143	60340	7.471	ng/ul	0.04
60) Fluorene-d10	15.698	176	747555	14.834	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.887	200	39104	4.139	ng/ul	0.02
73) Anthracene-d10	17.569	188	988137	14.082	ng/ul	0.00
81) Pyrene-d10	19.792	212	1004313	16.193	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	858697	15.373	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.916	105	36712	1.097	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015899.D
 Acq On : 01 Jul 2023 23:53
 Operator : MA/JU
 Sample : 03242-21
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC2

Quant Time: Jul 02 02:45:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 02:29:46 2023
 Response via : Initial Calibration

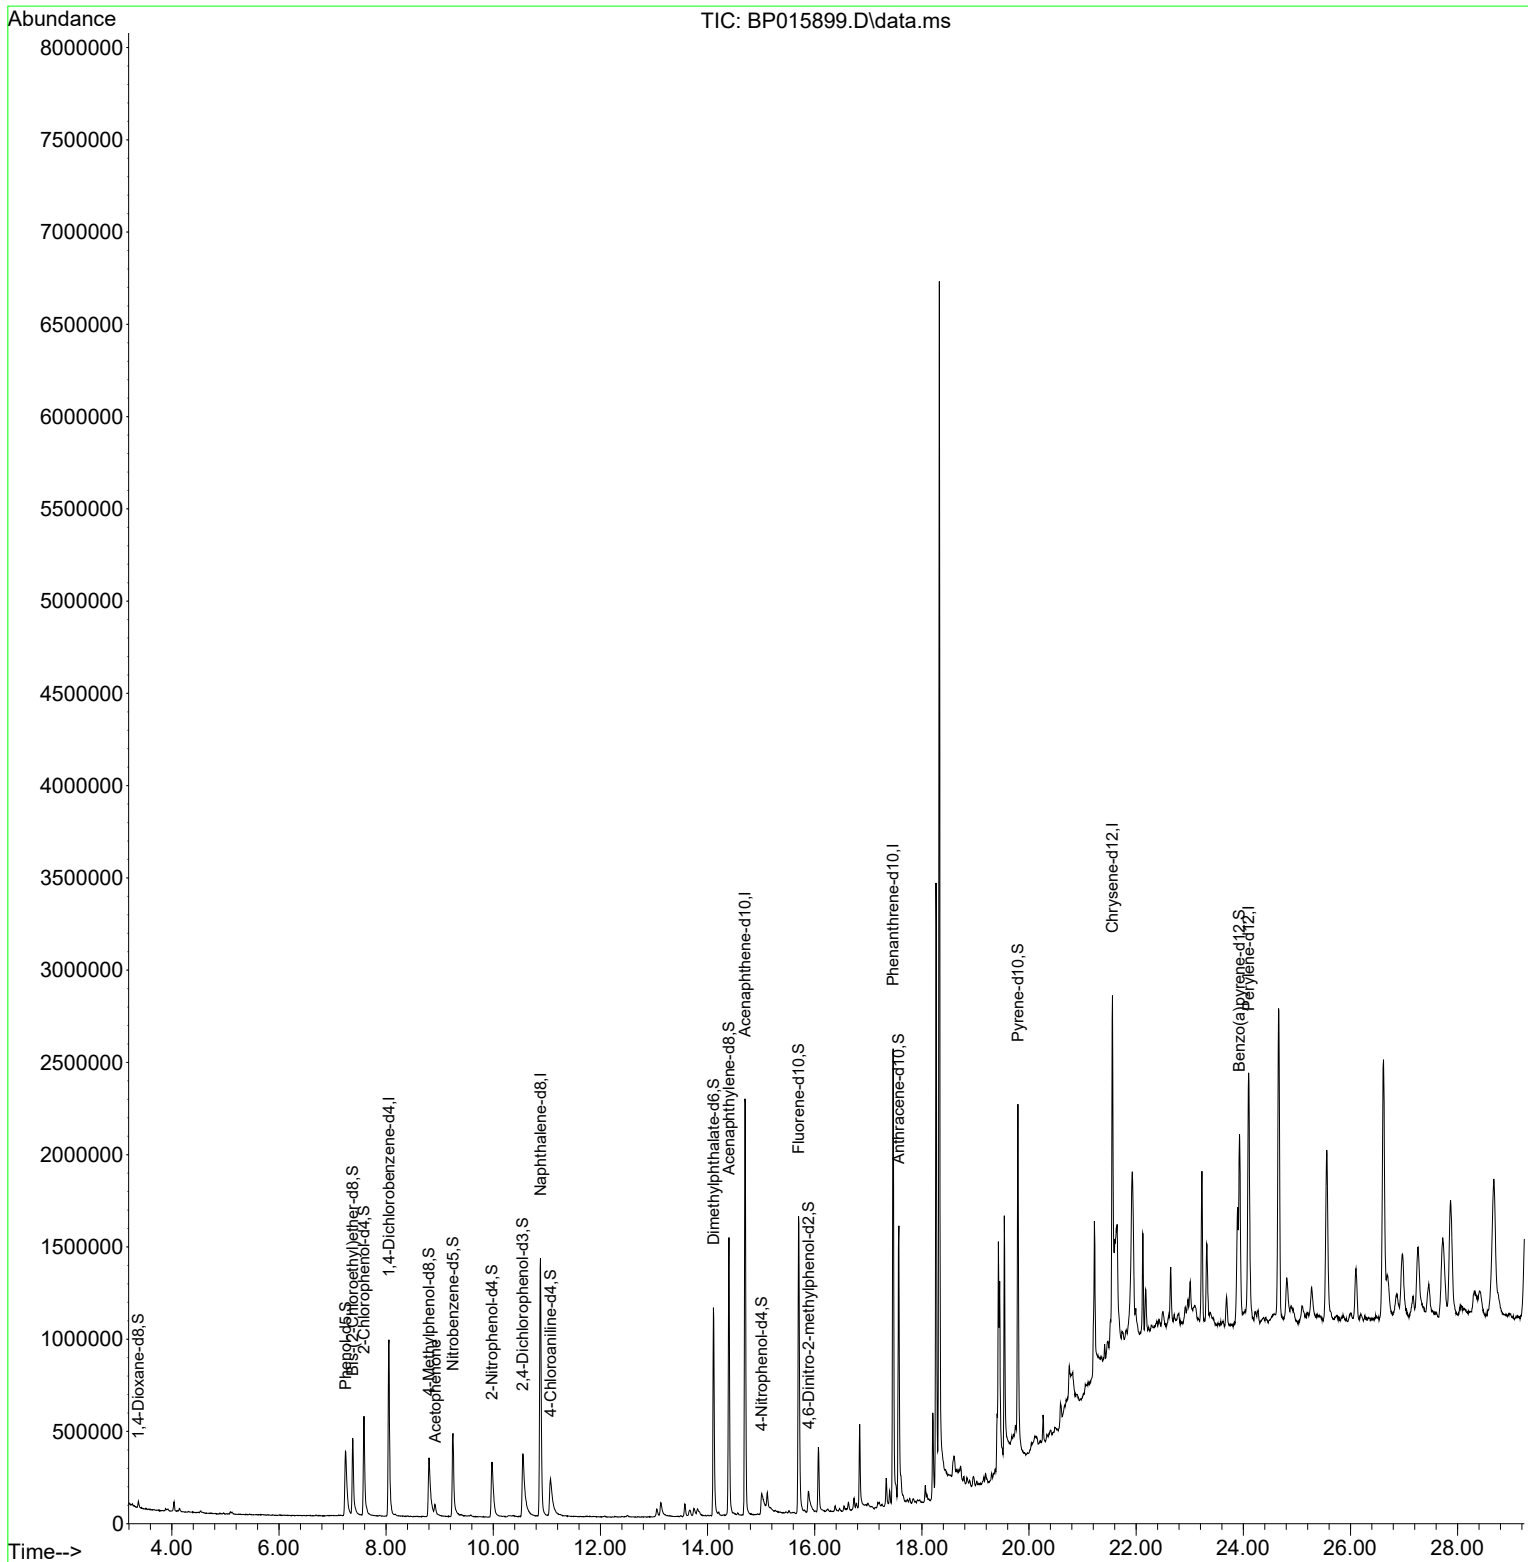

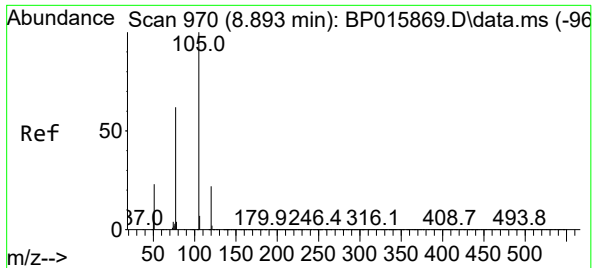

#16
 Acetophenone
 Concen: 1.097 ng/ul
 RT: 8.916 min Scan# 91
 Delta R.T. 0.023 min
 Lab File: BP015899.D
 Acq: 01 Jul 2023 23:53

Instrument :
 BNA_P
 ClientSampleId :
 DCGC2

Tgt Ion: 105 Resp: 36712

Ion	Ratio	Lower	Upper
105	100		
77	84.1	65.0	97.4
51	31.5	25.1	37.7

