

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015901.D
 Acq On : 02 Jul 2023 01:01
 Operator : MA/JU
 Sample : 03242-20
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC1

Quant Time: Jul 02 02:48:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 02:29:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	252922	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1117423	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	650971	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1265790	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.557	240	756708	20.000	ng/ul	# 0.00
88) Perylene-d12	24.098	264	866150	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	34282	4.877	ng/uL	0.00
4) Pyridine-d5	3.828	84	221933	12.524	ng/ul	0.01
7) Phenol-d5	7.234	99	686856	31.740	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.375	67	443964	33.160	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	536046	32.814	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	532703	31.160	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	268190	31.405	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	298581	29.957	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	518388	29.187	ng/ul	0.01
31) 4-Chloroaniline-d4	11.051	131	499288	21.883	ng/ul	0.01
46) Dimethylphthalate-d6	14.110	166	1662287	33.038	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	1880392	33.245	ng/ul	0.00
54) 4-Nitrophenol-d4	14.992	143	158649	23.894	ng/ul	0.02
60) Fluorene-d10	15.698	176	1366090	32.974	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	128790	16.544	ng/ul	0.00
73) Anthracene-d10	17.563	188	1884003	32.585	ng/ul	0.00
81) Pyrene-d10	19.792	212	1876247	37.972	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	1538774	35.218	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.904	105	64617	2.299	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015901.D
Acq On : 02 Jul 2023 01:01
Operator : MA/JU
Sample : 03242-20
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGC1

Quant Time: Jul 02 02:48:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 02:29:46 2023
Response via : Initial Calibration

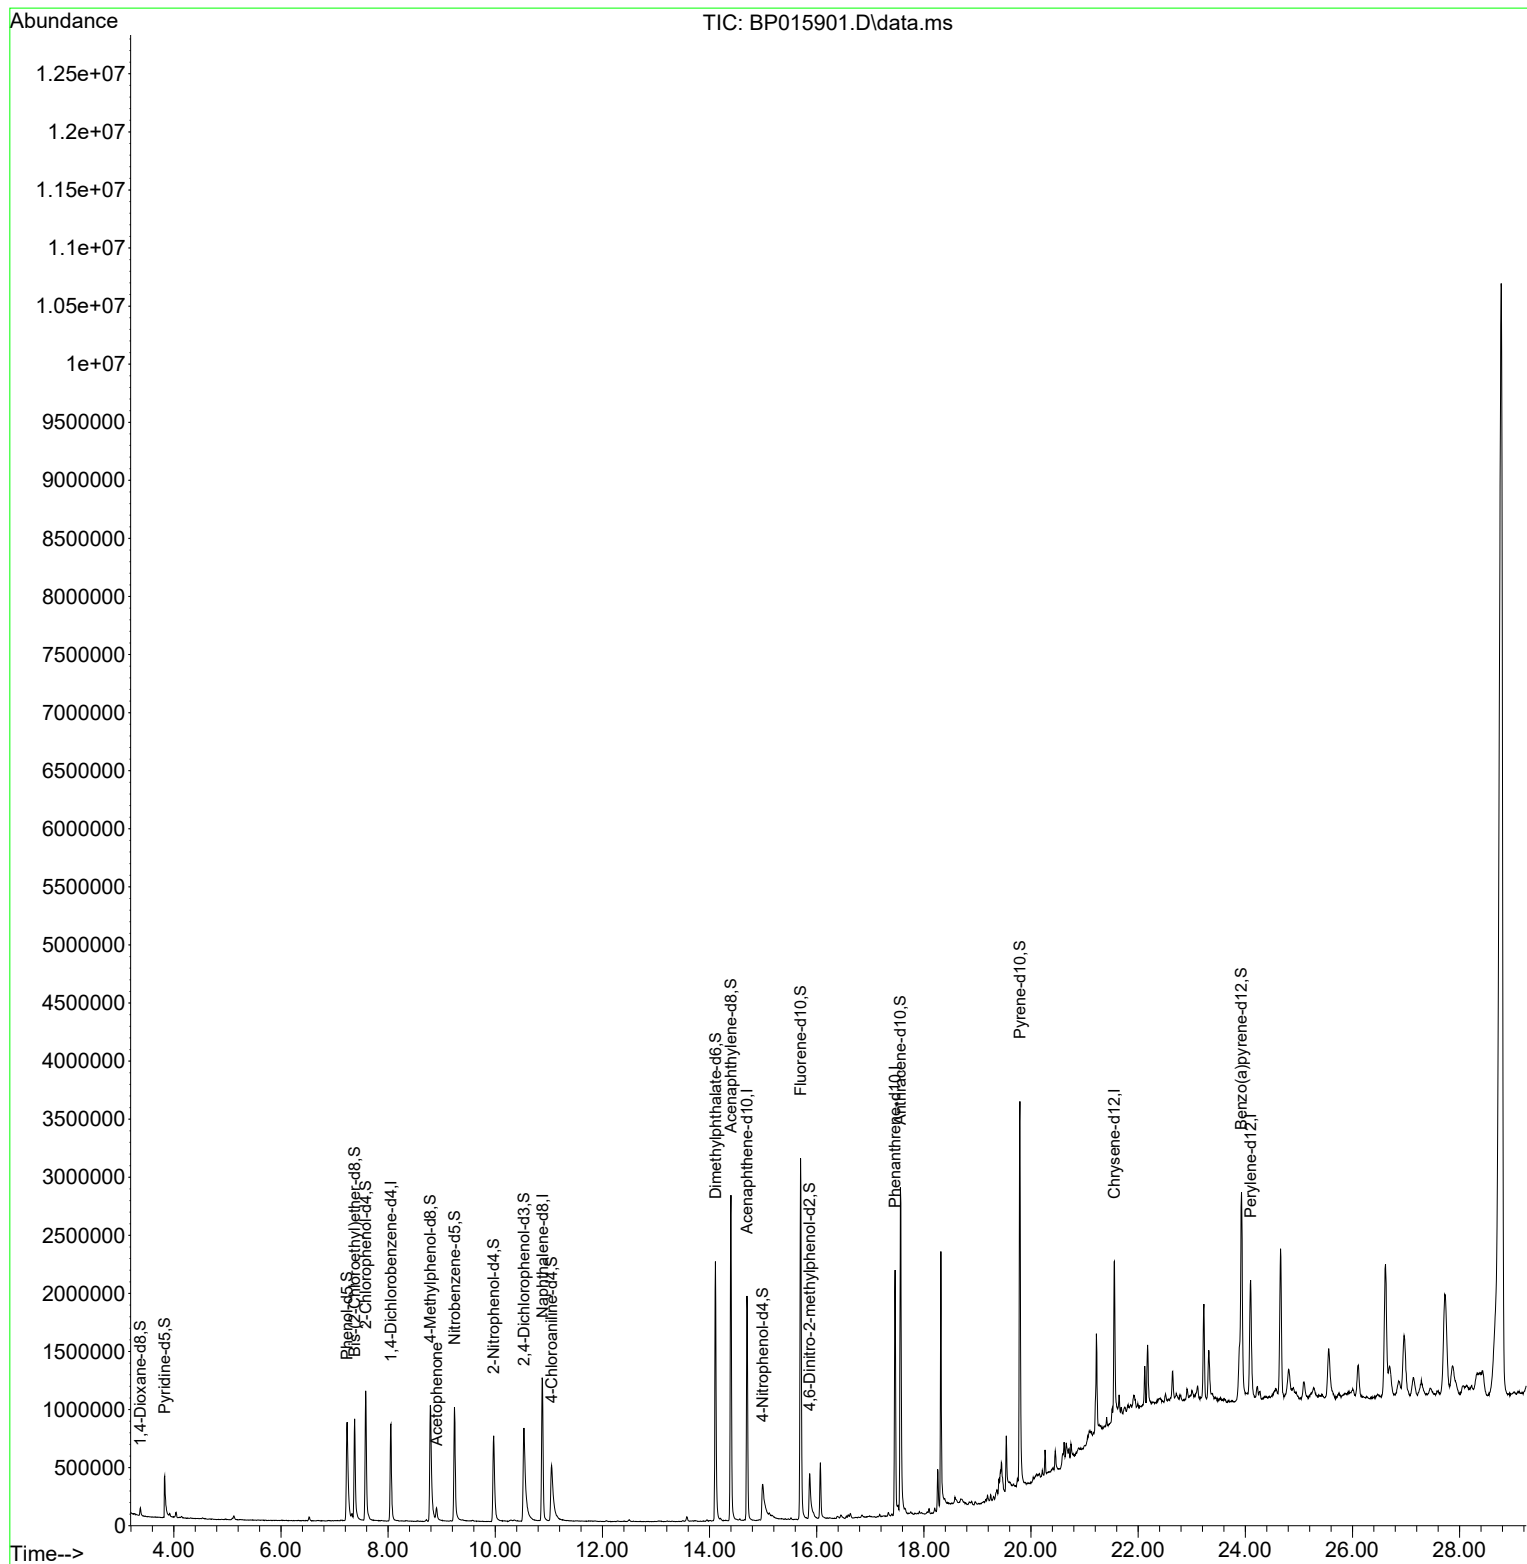

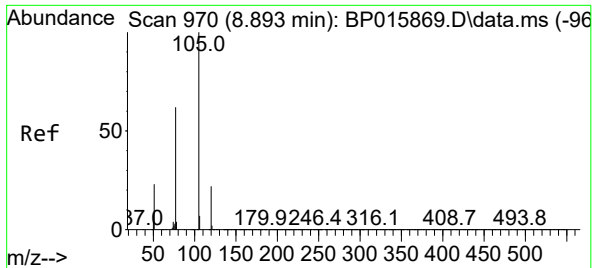

#16
 Acetophenone
 Concen: 2.299 ng/ul
 RT: 8.904 min Scan# 91
 Delta R.T. 0.011 min
 Lab File: BP015901.D
 Acq: 02 Jul 2023 01:01

Instrument :
 BNA_P
 ClientSampleId :
 DCGC1

Tgt Ion:	105	Resp:	64617
Ion Ratio	Lower	Upper	
105	100		
77	85.0	65.0	97.4
51	32.1	25.1	37.7

