

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015903.D
 Acq On : 02 Jul 2023 02:09
 Operator : MA/JU
 Sample : 03243-05
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC5

Quant Time: Jul 02 02:48:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 02:29:46 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	295853	20.000	ng/ul	0.00
20) Naphthalene-d8	10.881	136	1319324	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	764725	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1413352	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	863891	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	1013999	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	23555	2.865	ng/uL	0.00
4) Pyridine-d5	3.828	84	213944	10.321	ng/ul	0.01
7) Phenol-d5	7.240	99	424845	16.783	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.375	67	299891	19.149	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	365456	19.125	ng/ul	0.00
15) 4-Methylphenol-d8	8.799	113	239070	11.955	ng/ul	0.01
21) Nitrobenzene-d5	9.246	128	181101	17.961	ng/ul	0.01
24) 2-Nitrophenol-d4	9.975	143	195900	16.647	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.546	165	313108	14.931	ng/ul	0.02
31) 4-Chloroaniline-d4	11.069	131	213475	7.925	ng/ul	0.03
46) Dimethylphthalate-d6	14.110	166	1071700	18.131	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	1201659	18.085	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	154	0.020	ng/ul	-0.02
60) Fluorene-d10	15.698	176	874400	17.966	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	68953	7.933	ng/ul	0.02
73) Anthracene-d10	17.569	188	1090339	16.889	ng/ul	0.00
81) Pyrene-d10	19.792	212	1070023	18.969	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	916919	17.926	ng/ul	-0.01
Target Compounds						
10) Bis(2-Chloroethyl)ether	7.457	93	48591	2.325	ng/ul#	Qvalue 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015903.D
Acq On : 02 Jul 2023 02:09
Operator : MA/JU
Sample : 03243-05
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGC5

Quant Time: Jul 02 02:48:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 02:29:46 2023
Response via : Initial Calibration

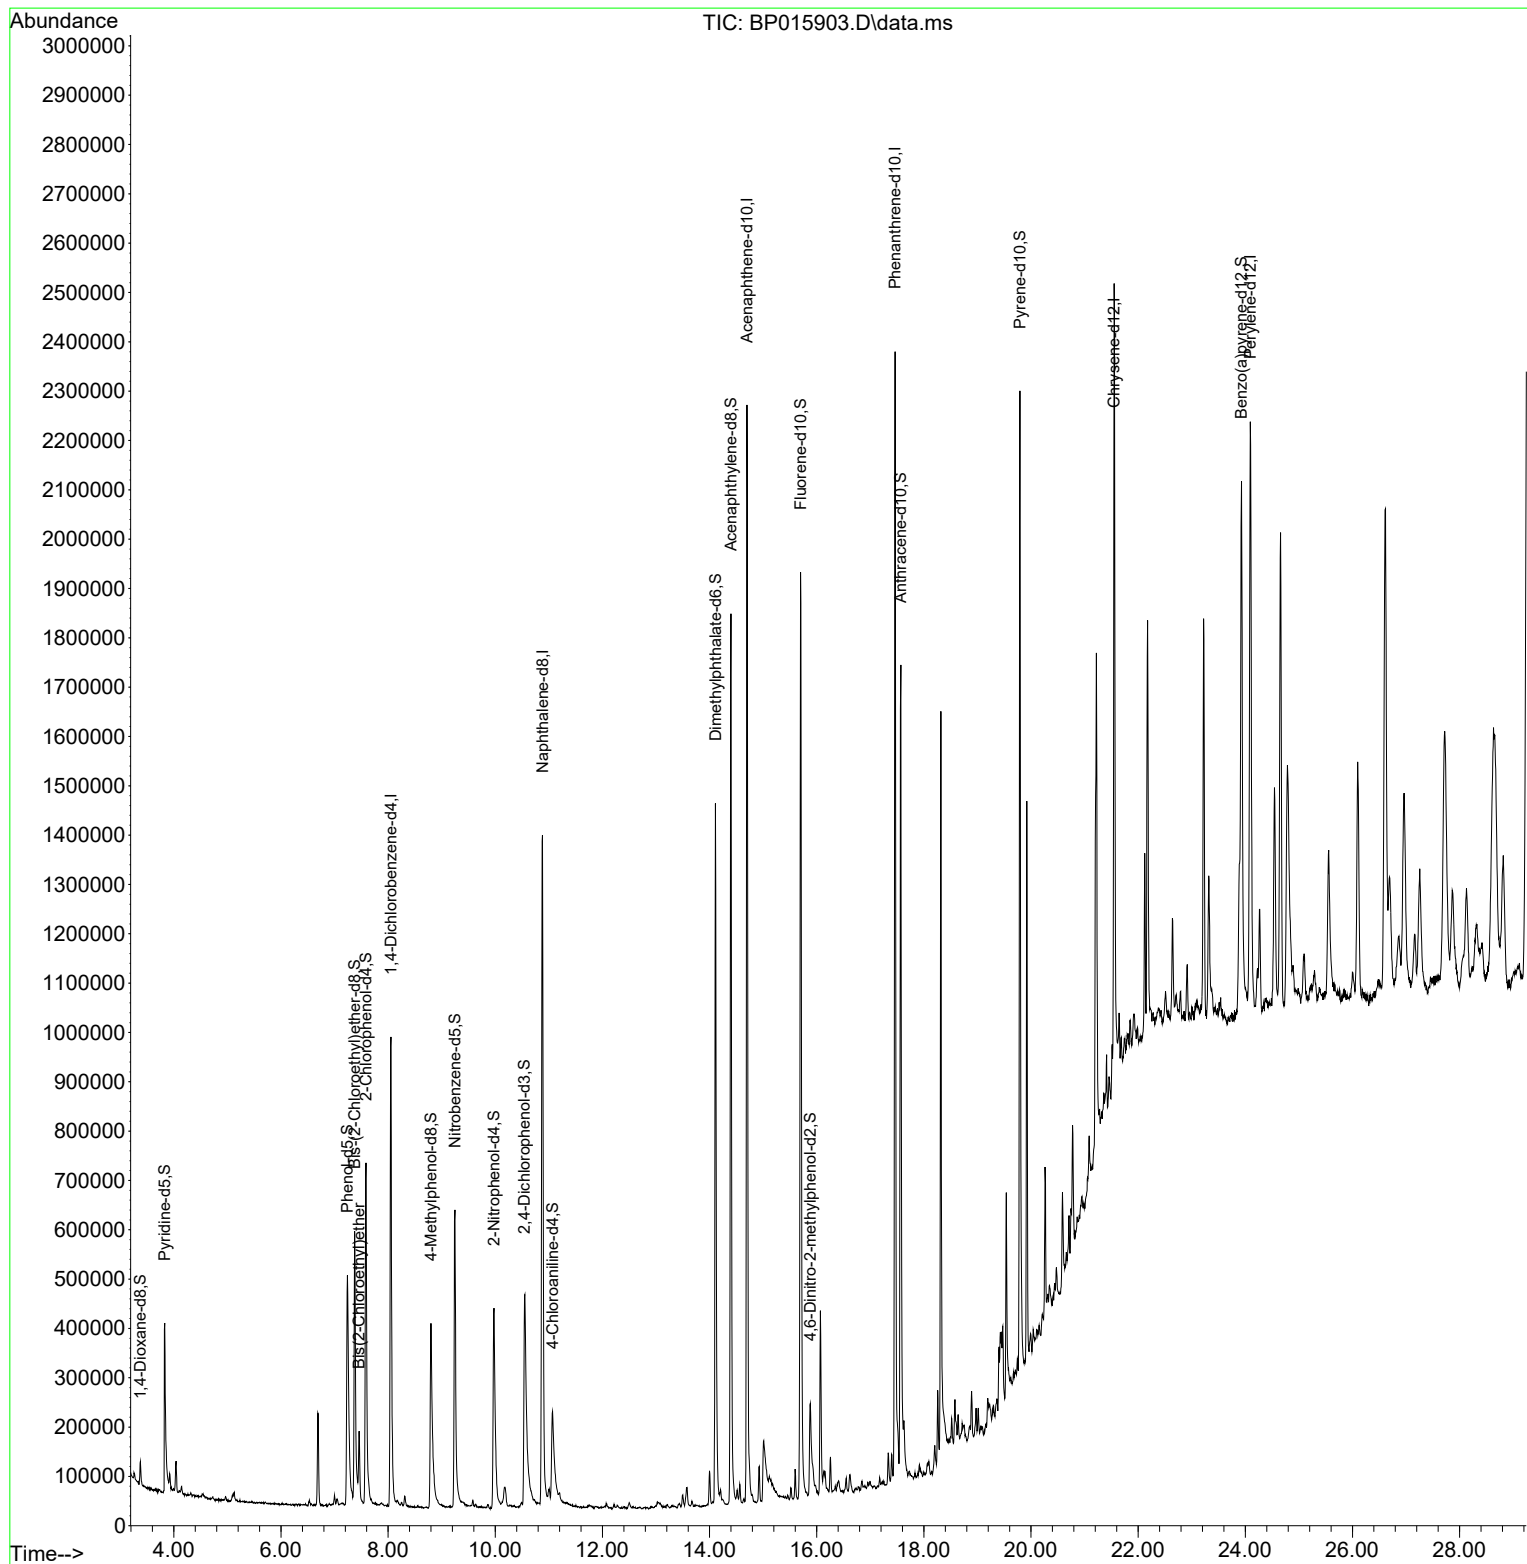

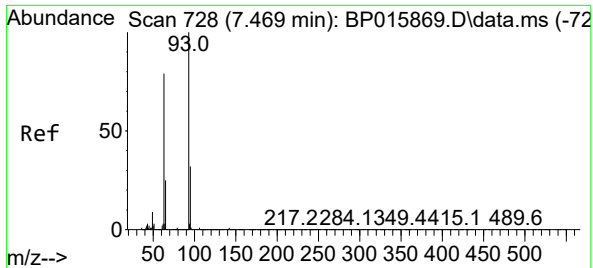

#10
Bis(2-Chloroethyl)ether
Concen: 2.325 ng/ul
RT: 7.457 min Scan# 71
Delta R.T. -0.012 min
Lab File: BP015903.D
Acq: 02 Jul 2023 02:09

Instrument :
BNA_P
ClientSampleId :
DCGC5

Tgt Ion:	93	Resp:	48591
Ion	Ratio	Lower	Upper
93	100		
63	3.1	62.8	94.2#
95	3.6	25.6	38.4#

