

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015847.D
 Acq On : 30 Jun 2023 16:48
 Operator : MA/JU
 Sample : 03161-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFW0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

Quant Time: Jun 30 23:38:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 30 22:30:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	204282	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	832785	20.000	ng/ul	# 0.01
38) Acenaphthene-d10	14.710	164	474937	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1010329	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.557	240	950933	20.000	ng/ul	# 0.00
88) Perylene-d12	24.098	264	1111844	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	13227	2.330	ng/uL	0.00
4) Pyridine-d5	3.864	84	29672m	2.073	ng/ul	0.04
7) Phenol-d5	7.246	99	190258	10.885	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.381	67	157464	14.562	ng/ul	0.00
11) 2-Chlorophenol-d4	7.593	132	176063	13.344	ng/ul	0.01
15) 4-Methylphenol-d8	8.816	113	106239	7.694	ng/ul	0.04
21) Nitrobenzene-d5	9.263	128	77673	12.204	ng/ul	0.02
24) 2-Nitrophenol-d4	9.993	143	80875	10.888	ng/ul	0.03
28) 2,4-Dichlorophenol-d3	10.575	165	127467m	9.630	ng/ul	0.06
31) 4-Chloroaniline-d4	11.104	131	95557m	5.620	ng/ul	0.07
46) Dimethylphthalate-d6	14.122	166	492376	13.413	ng/ul	0.01
49) Acenaphthylene-d8	14.404	160	569625	13.804	ng/ul	0.00
54) 4-Nitrophenol-d4	15.051	143	28104m	5.801	ng/ul	0.10
60) Fluorene-d10	15.710	176	430004	14.226	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.898	200	31900	5.134	ng/ul	0.04
73) Anthracene-d10	17.575	188	609525	13.208	ng/ul	0.01
81) Pyrene-d10	19.792	212	819591	13.199	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	788053	14.051	ng/ul	0.00
Target Compounds						
80) Fluoranthene	19.474	202	117711	1.525	ng/ul#	94
82) Pyrene	19.827	202	98905	1.256	ng/ul#	86
85) Benzo(a)anthracene	21.539	228	70500	1.054	ng/ul	96
87) Chrysene	21.598	228	72116	1.136	ng/ul	93
90) Benzo(b)fluoranthene	23.321	252	111192	1.556	ng/ul#	42
93) Benzo(a)pyrene	23.986	252	71670	1.148	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015847.D
Acq On : 30 Jun 2023 16:48
Operator : MA/JU
Sample : 03161-04
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
DCFW0

Quant Time: Jun 30 23:38:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 30 22:30:25 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

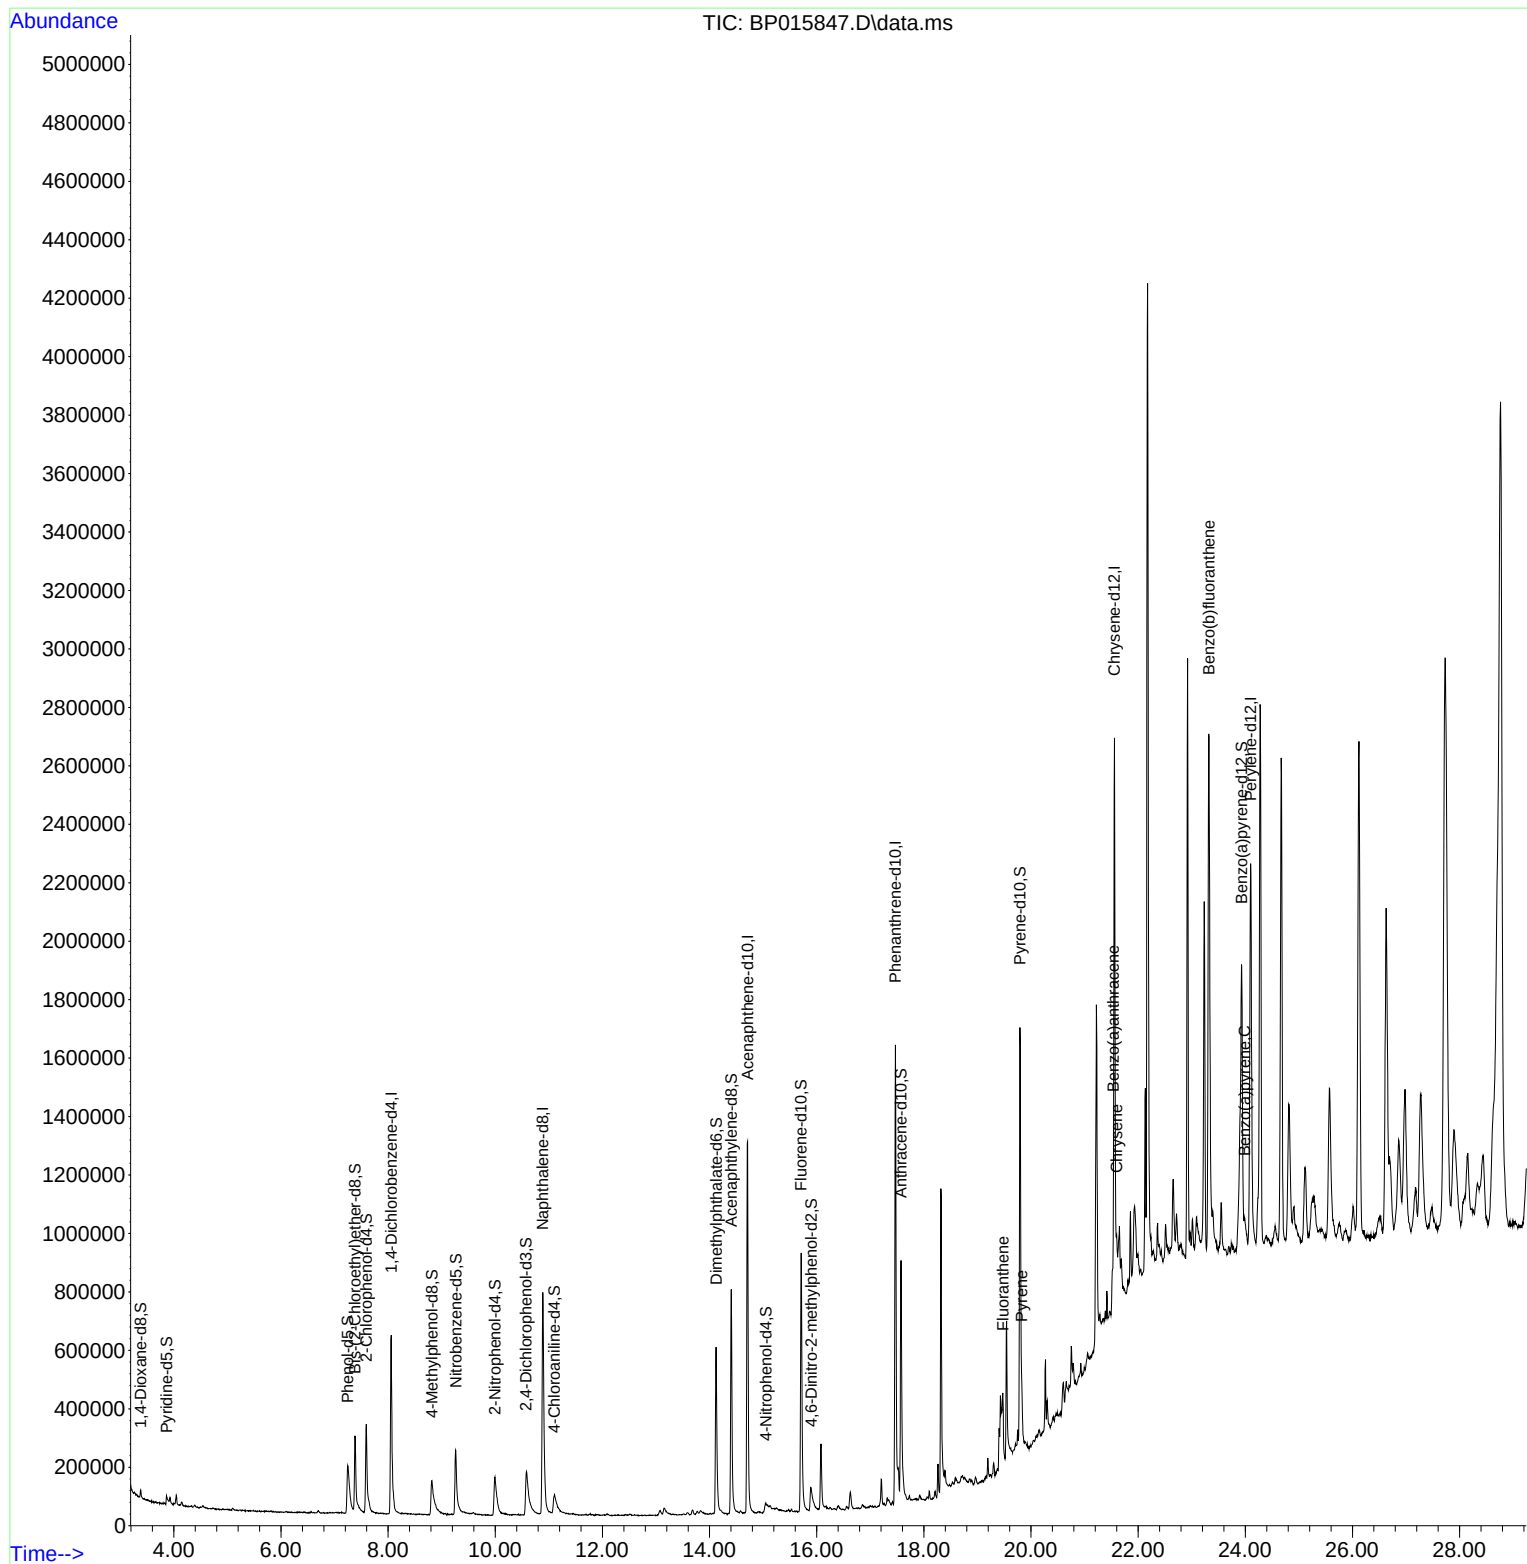

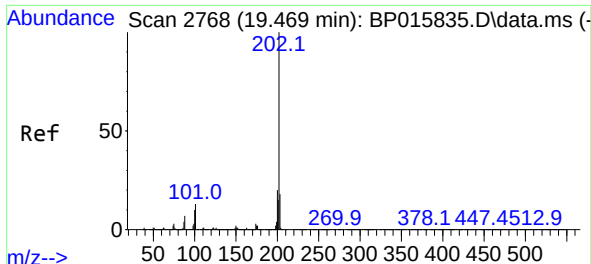





#80
Fluoranthene
Concen: 1.525 ng/u1
RT: 19.474 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48

Instrument :
BNA_P
ClientSampleId :
DCFV0

Tgt Ion:202 Resp: 11771
Ion Ratio Lower Upper
202 100
101 13.4 8.3 12.5
100 9.7 6.6 9.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

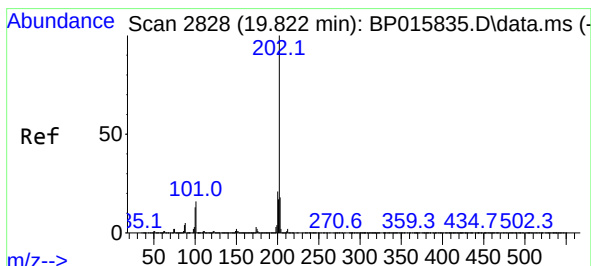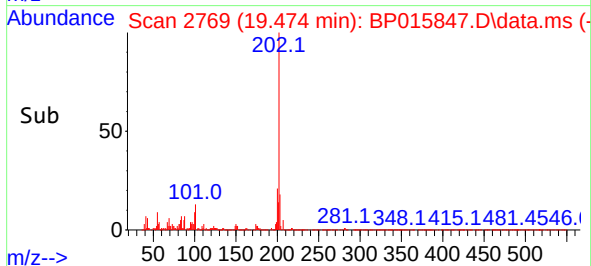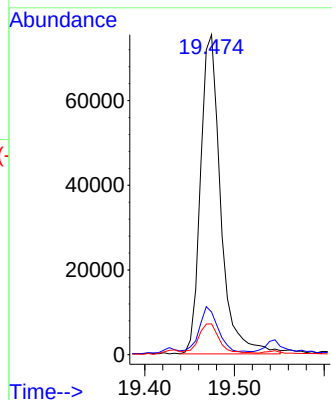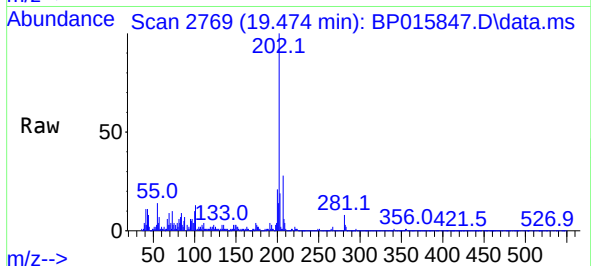

#82
Pyrene
Concen: 1.256 ng/u1
RT: 19.827 min Scan# 2829
Delta R.T. 0.006 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48


Tgt Ion:202 Resp: 98905
Ion Ratio Lower Upper
202 100
101 17.4 9.3 13.9#
100 13.9 7.6 11.4#

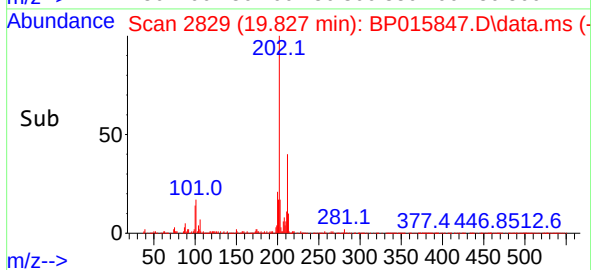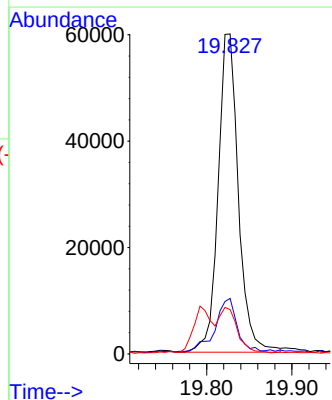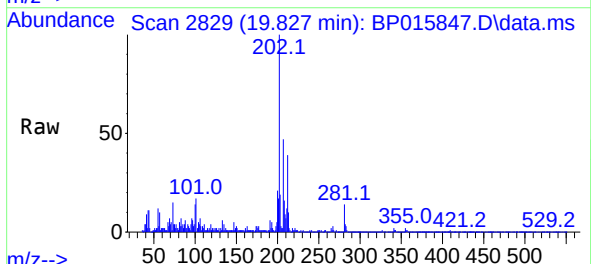

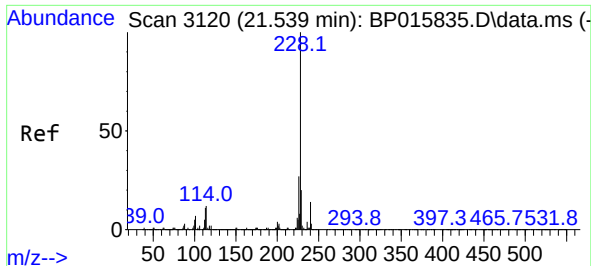

#85
Benzo(a)anthracene
Concen: 1.054 ng/u1
RT: 21.539 min Scan# 3120
Delta R.T. -0.000 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48




Instrument :
BNA_P
ClientSampleId :
DCFW0

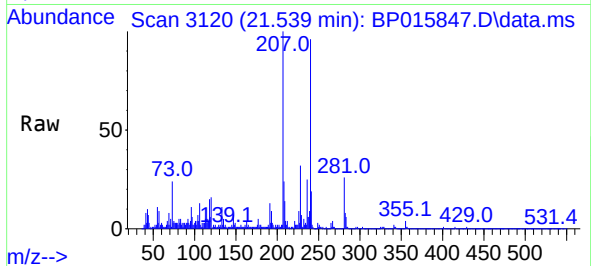


Tgt Ion:228 Resp: 70500
Ion Ratio Lower Upper
228 100
229 22.7 15.3 22.9
226 27.7 21.4 32.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

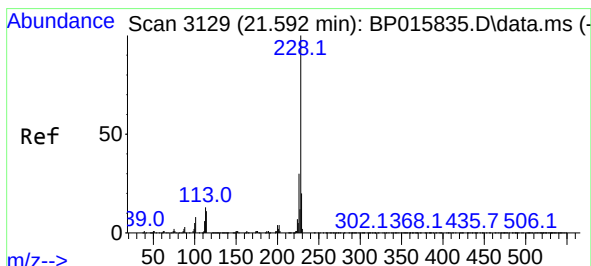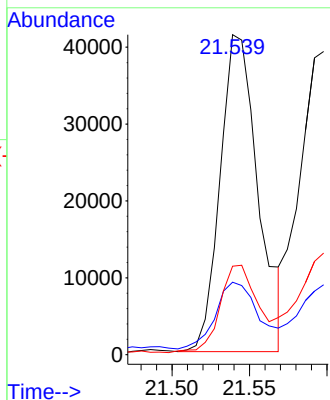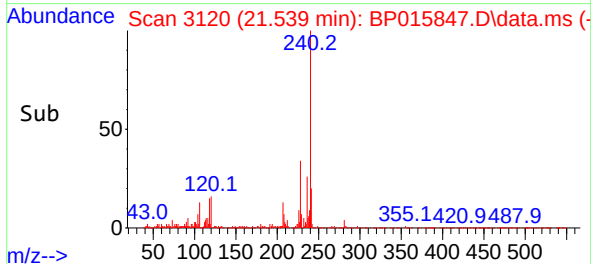


#87
Chrysene
Concen: 1.136 ng/u1
RT: 21.598 min Scan# 3130
Delta R.T. 0.006 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48

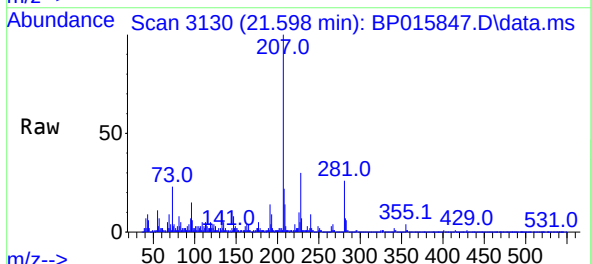

Tgt Ion:228 Resp: 72116
Ion Ratio Lower Upper
228 100
226 33.5 24.3 36.5
229 23.1 15.5 23.3

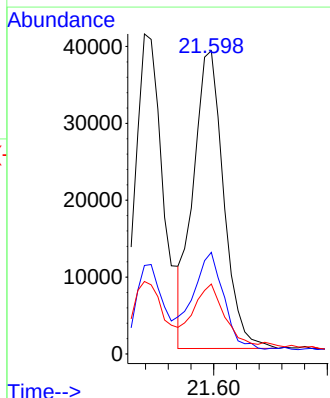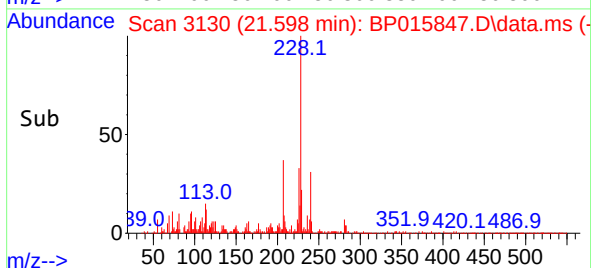

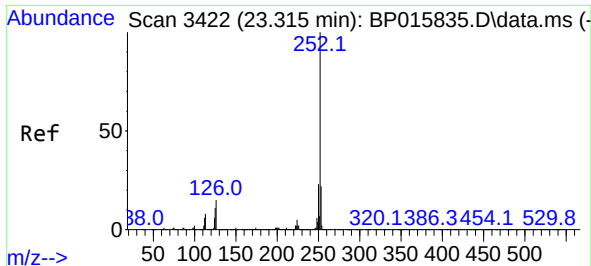





#90
Benzo(b)fluoranthene
Concen: 1.556 ng/u1
RT: 23.321 min Scan# 3422
Delta R.T. 0.006 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48

Instrument :
BNA_P
ClientSampleId :
DCFV0

Tgt Ion:252 Resp: 111192
Ion Ratio Lower Upper
252 100
253 24.0 17.3 25.9
125 74.6 7.5 11.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

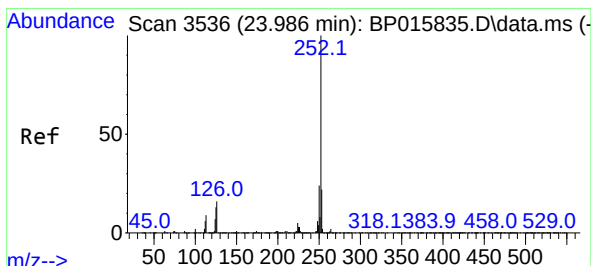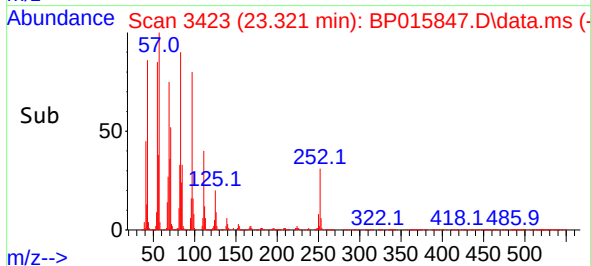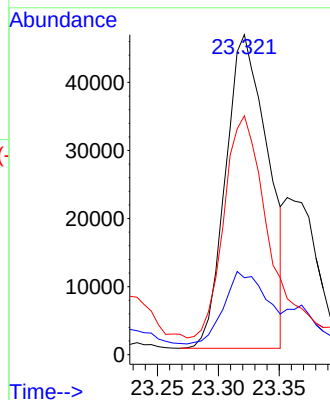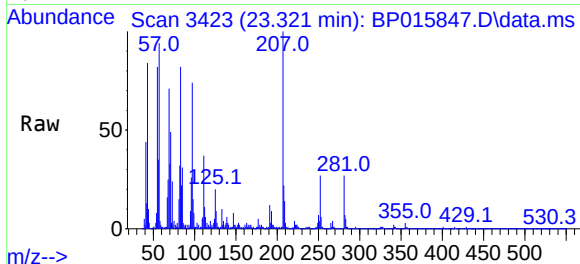

#93
Benzo(a)pyrene
Concen: 1.148 ng/u1
RT: 23.986 min Scan# 3536
Delta R.T. -0.000 min
Lab File: BP015847.D
Acq: 30 Jun 2023 16:48

Tgt Ion:252 Resp: 71670
Ion Ratio Lower Upper
252 100
253 29.3 17.7 26.5#
125 18.2 8.2 12.2#

