

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015836.D
 Acq On : 30 Jun 2023 10:34
 Operator : MA/JU
 Sample : PB153635BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	28	32	38	rVB	66443	89037	1.39%	0.133%
2	3.822	105	108	132	rBV	769347	1498460	23.44%	2.242%
3	6.652	586	589	595	rVB8	3842	6724	0.11%	0.010%
4	7.228	680	687	706	rBV	746374	1817267	28.43%	2.718%
5	7.381	706	713	727	rVV	772218	1433392	22.42%	2.144%
6	7.581	740	747	776	rVB	980299	1924042	30.10%	2.878%
7	8.052	820	827	844	rBV	708981	1424700	22.29%	2.131%
8	8.787	945	952	974	rBV	1038568	2364887	37.00%	3.538%
9	9.240	1020	1029	1051	rBV	913720	1910118	29.88%	2.857%
10	9.969	1146	1153	1175	rBV	704886	1577238	24.67%	2.359%
11	10.528	1240	1248	1278	rBV	684821	2300766	35.99%	3.442%
12	10.881	1301	1308	1324	rBV	1217955	2184882	34.18%	3.268%
13	11.046	1328	1336	1371	rBV	751057	2409786	37.70%	3.605%
14	12.516	1580	1586	1590	rBV3	16668	29721	0.46%	0.044%
15	14.116	1851	1858	1882	rBV	2059000	3614877	56.55%	5.407%
16	14.398	1899	1906	1930	rBV	2672133	4458995	69.76%	6.670%
17	14.704	1950	1958	1972	rVV	1907269	2976875	46.57%	4.453%
18	14.981	1997	2005	2041	rBV	264266	1310880	20.51%	1.961%
19	15.704	2121	2128	2149	rBV	2951466	5366533	83.96%	8.028%
20	15.863	2150	2155	2183	rVB	439221	1199526	18.77%	1.794%
21	16.486	2257	2261	2265	rBV7	5112	9210	0.14%	0.014%
22	17.139	2369	2372	2377	rVB7	6014	8648	0.14%	0.013%
23	17.463	2421	2427	2438	rBV	2334160	3514888	54.99%	5.258%
24	17.569	2438	2445	2470	rVB2	3100496	5845358	91.45%	8.744%
25	19.375	2748	2752	2756	rBV3	43995	60080	0.94%	0.090%
26	19.445	2761	2764	2770	rVV2	35689	54816	0.86%	0.082%
27	19.792	2818	2823	2844	rBV	3643420	6392151	100.00%	9.562%
28	21.563	3119	3124	3137	rBV2	1676836	2916907	45.63%	4.363%
29	23.933	3519	3527	3544	rVB2	2029690	5227698	81.78%	7.820%
30	24.104	3550	3556	3574	rVB	1104330	2920979	45.70%	4.369%




Sum of corrected areas: 66849441

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015836.D
Acq On : 30 Jun 2023 10:34
Operator : MA/JU
Sample : PB153635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

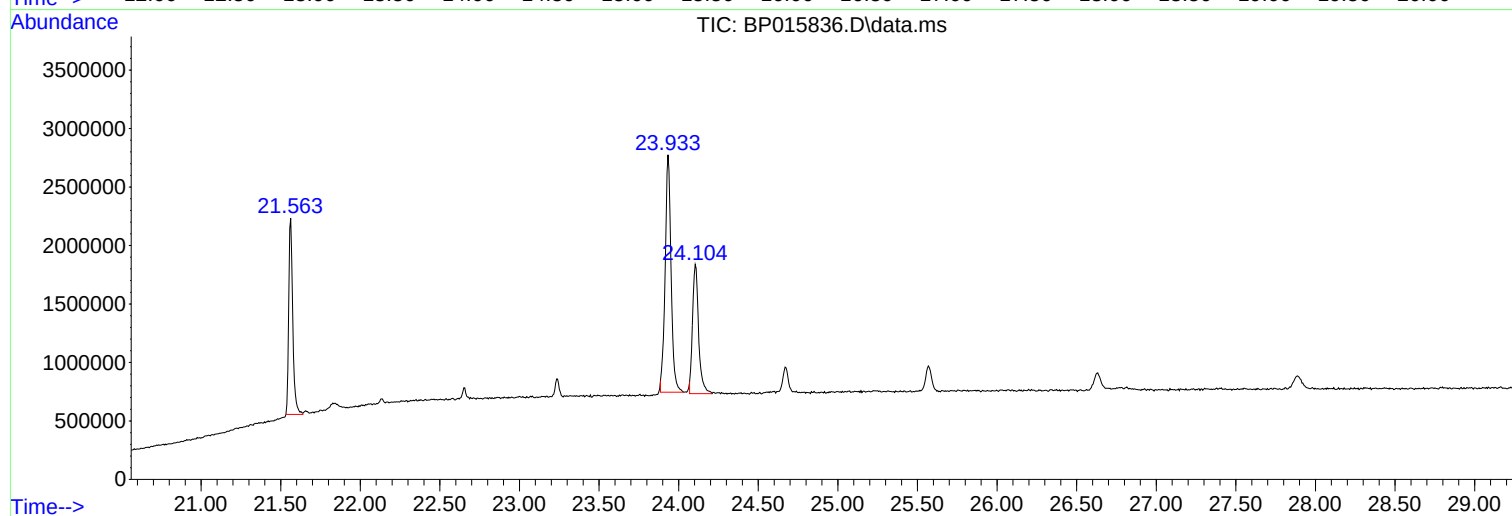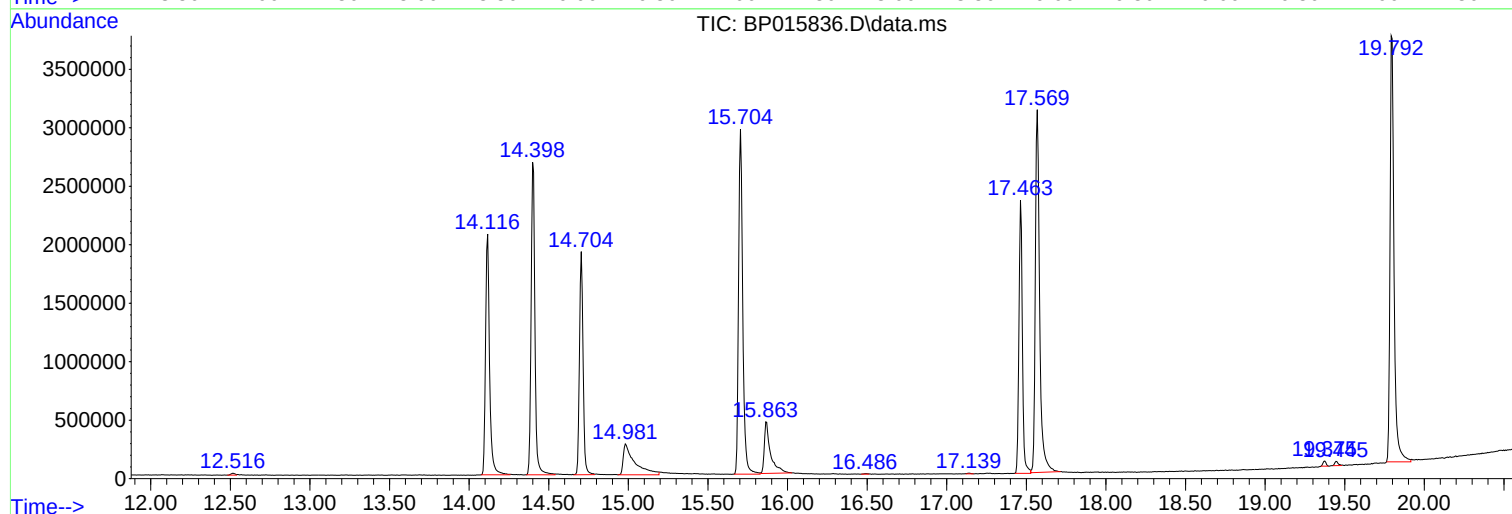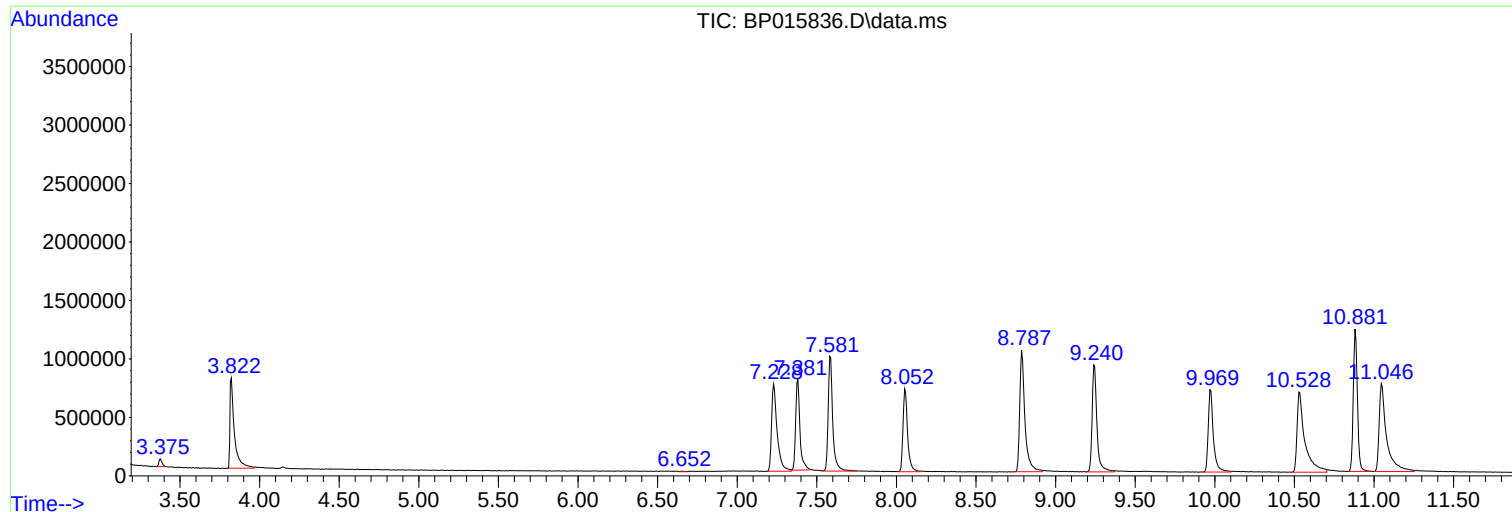

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015836.D
Acq On : 30 Jun 2023 10:34
Operator : MA/JU
Sample : PB153635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015836.D
Acq On : 30 Jun 2023 10:34
Operator : MA/JU
Sample : PB153635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------