

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015851.D
 Acq On : 30 Jun 2023 19:05
 Operator : MA/JU
 Sample : PB153574BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.066	328	331	333	rBV	1723855	1110118	21.71%	1.911%
2	3.007	486	491	502	rVV	156526	265073	5.18%	0.456%
3	3.090	502	505	513	rVB	73631	94056	1.84%	0.162%
4	3.378	550	554	563	rVB	63066	94579	1.85%	0.163%
5	3.819	626	629	652	rBV	754993	1341295	26.24%	2.309%
6	7.231	1202	1209	1228	rBV	723671	1751404	34.26%	3.015%
7	7.378	1228	1234	1259	rVV	735184	1454110	28.44%	2.503%
8	7.584	1262	1269	1295	rVB	960724	1811634	35.44%	3.119%
9	8.054	1342	1349	1366	rBV	631969	1263446	24.71%	2.175%
10	8.790	1464	1474	1500	rBV	976141	2278887	44.58%	3.923%
11	9.242	1544	1551	1576	rBV	860189	1769194	34.61%	3.045%
12	9.972	1667	1675	1697	rBV	573665	1303360	25.49%	2.244%
13	10.536	1763	1771	1807	rBV	611728	2119147	41.45%	3.648%
14	10.884	1822	1830	1845	rBV	1050628	1913511	37.43%	3.294%
15	11.048	1851	1858	1885	rBV	680207	2174149	42.53%	3.743%
16	13.583	2282	2289	2296	rBV3	18915	38797	0.76%	0.067%
17	14.113	2373	2379	2401	rBV	1776853	3221182	63.01%	5.545%
18	14.401	2421	2428	2445	rBV	2448044	3921676	76.71%	6.751%
19	14.707	2473	2480	2497	rBV	1518919	2455814	48.04%	4.227%
20	14.989	2521	2528	2566	rBV2	200506	1099135	21.50%	1.892%
21	15.707	2642	2650	2665	rBV	2411868	4658370	91.12%	8.019%
22	15.871	2672	2678	2699	rBV	238693	705572	13.80%	1.215%
23	17.466	2941	2949	2960	rBV	1777350	2746735	53.73%	4.728%
24	17.571	2960	2967	2992	rVB2	2451330	4849643	94.86%	8.348%
25	19.371	3270	3273	3279	rBV3	35883	48118	0.94%	0.083%
26	19.448	3283	3286	3294	rVV	28031	47825	0.94%	0.082%
27	19.795	3339	3345	3364	rBV	2984452	5112326	100.00%	8.800%
28	21.559	3641	3645	3659	rBV	1190376	2145947	41.98%	3.694%
29	23.936	4043	4049	4064	rVB2	1659337	4006944	78.38%	6.898%
30	24.100	4071	4077	4096	rVB	832732	2290294	44.80%	3.943%




Sum of corrected areas: 58092341

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015851.D
Acq On : 30 Jun 2023 19:05
Operator : MA/JU
Sample : PB153574BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

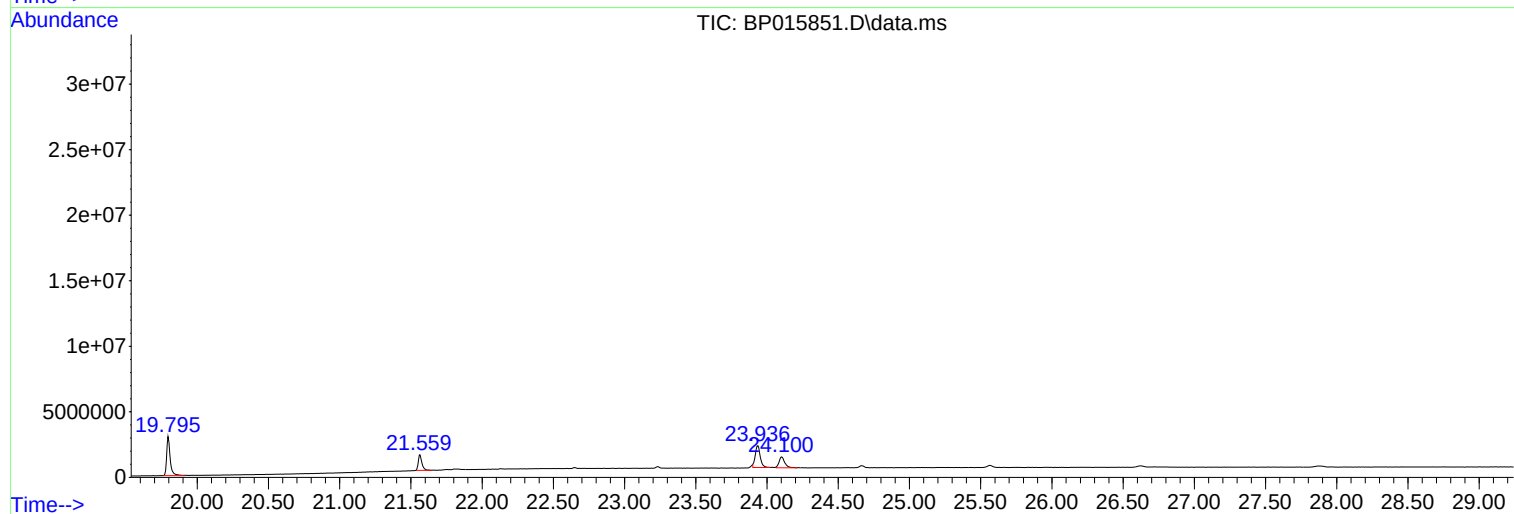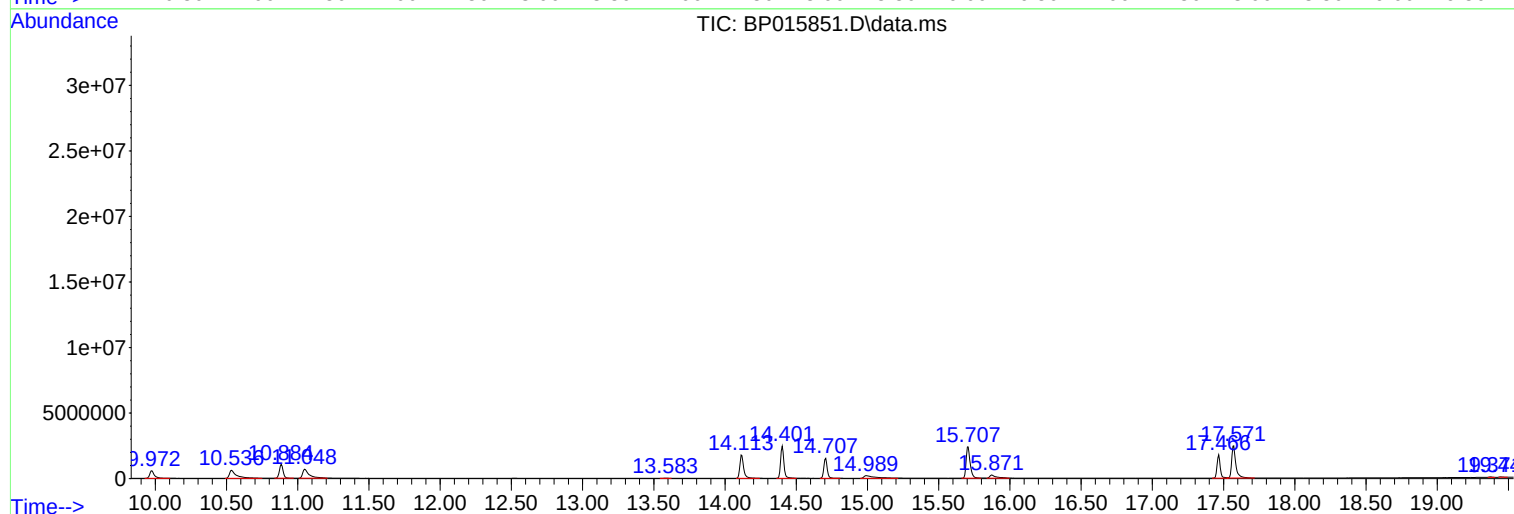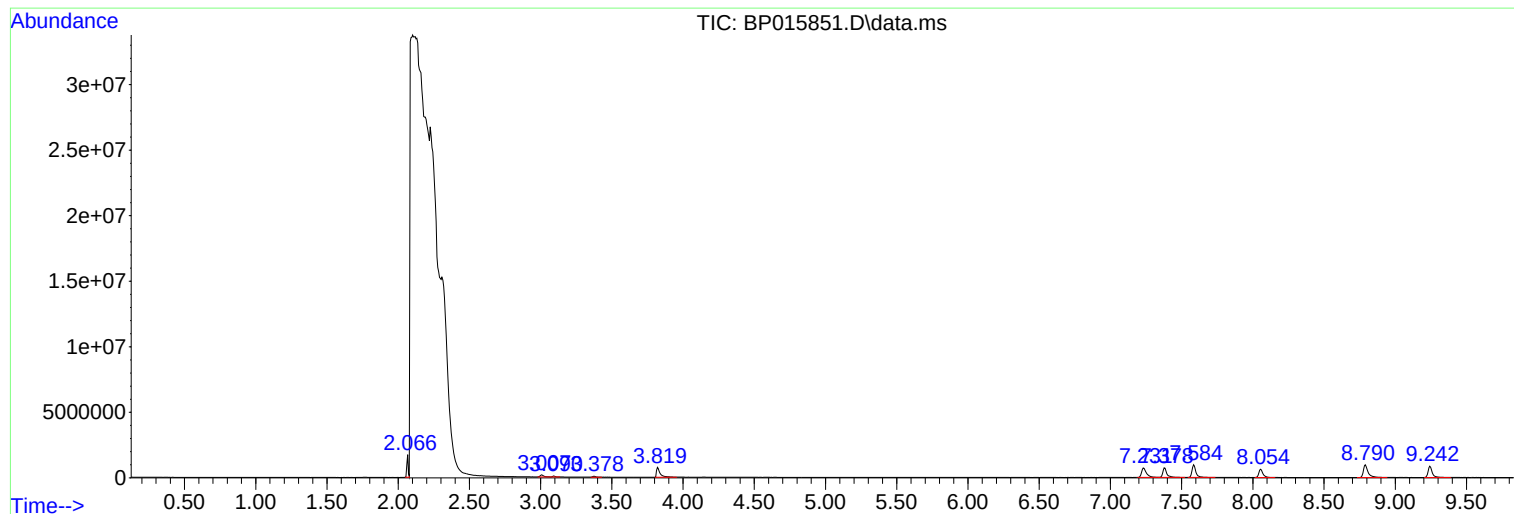

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015851.D
Acq On : 30 Jun 2023 19:05
Operator : MA/JU
Sample : PB153574BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.066	17.57 ng/ul	1110120	1,4-Dichlorobenzene-d4	8.054

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetone			58	C3H6O	000067-64-1	72
2	Acetone			58	C3H6O	000067-64-1	72
3	Acetone			58	C3H6O	000067-64-1	72
4	Acetone			58	C3H6O	000067-64-1	56
5	Acetone			58	C3H6O	000067-64-1	50

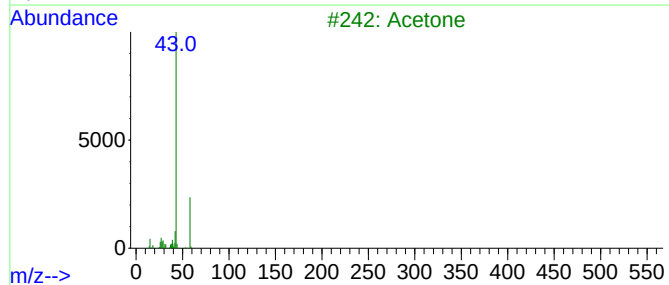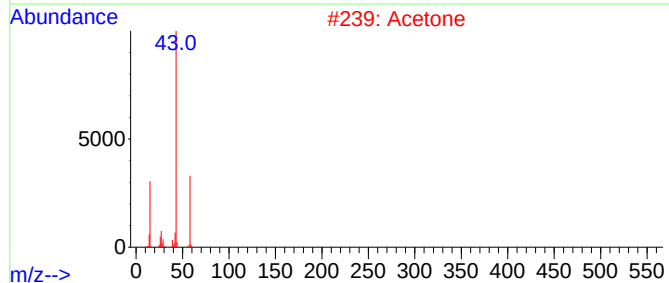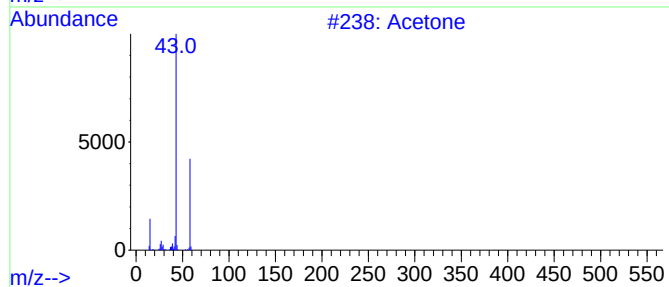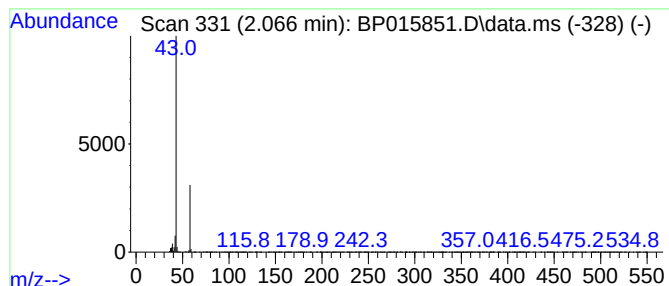

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015851.D
Acq On : 30 Jun 2023 19:05
Operator : MA/JU
Sample : PB153574BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic3.007 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.007	4.20 ng/ul	265073	1,4-Dichlorobenzene-d4	8.054

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	91
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclopentane, methyl-	84	C6H12	000096-37-7	83
5			Cyclohexane	84	C6H12	000110-82-7	80

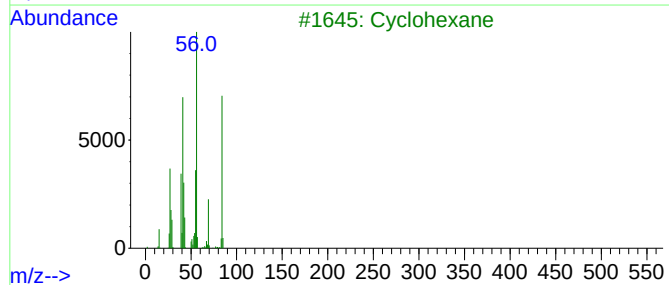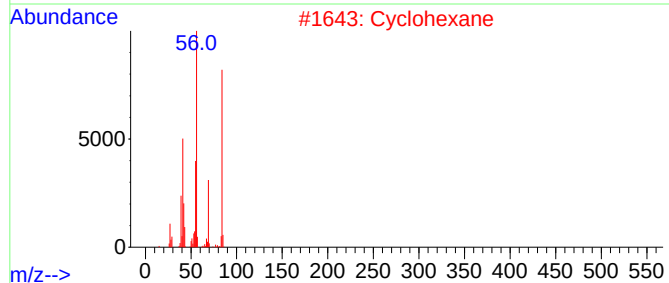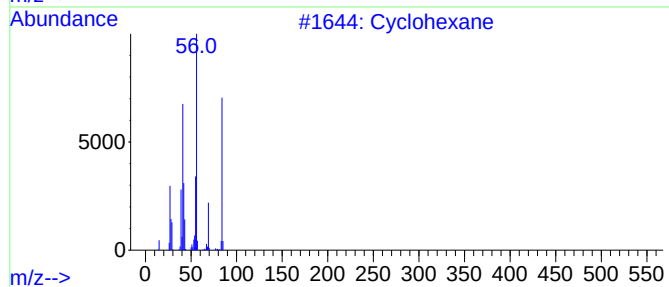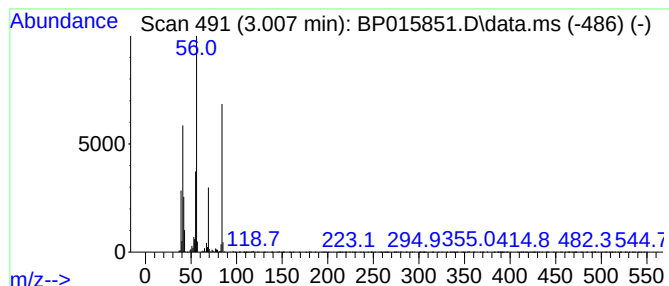

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015851.D
Acq On : 30 Jun 2023 19:05
Operator : MA/JU
Sample : PB153574BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetone	2.066	17.6	ng/ul	1110120	1	8.054	1263450	20.0
(DEL) Alkane: C...	3.007	4.2	ng/ul	265073	1	8.054	1263450	20.0