

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
 Data File : BP015887.D
 Acq On : 01 Jul 2023 17:05
 Operator : MA/JU
 Sample : PB153707BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK707

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	29	32	39	rVB	98398	124786	1.72%	0.166%
2	3.816	105	107	129	rBV	1000754	1738154	23.97%	2.319%
3	4.146	160	163	167	rVB2	13830	17841	0.25%	0.024%
4	7.228	680	687	705	rBV	865432	2077725	28.65%	2.772%
5	7.375	706	712	729	rVB	956048	1685547	23.24%	2.249%
6	7.581	740	747	763	rBV	1191864	2189073	30.18%	2.920%
7	8.046	819	826	842	rBV	903803	1748959	24.11%	2.333%
8	8.787	944	952	972	rBV2	1117415	2560628	35.31%	3.416%
9	9.240	1020	1029	1052	rBV	989813	2072274	28.57%	2.764%
10	9.969	1145	1153	1187	rBV	759370	1745454	24.07%	2.328%
11	10.534	1240	1249	1281	rBV	671464	2460608	33.93%	3.283%
12	10.881	1300	1308	1324	rBV	1312468	2454063	33.84%	3.274%
13	11.045	1327	1336	1366	rBV	764081	2458191	33.89%	3.279%
14	12.504	1577	1584	1596	rBV2	16585	42708	0.59%	0.057%
15	13.581	1759	1767	1773	rBV	24192	47097	0.65%	0.063%
16	14.063	1840	1849	1850	rBV9	3679	8244	0.11%	0.011%
17	14.110	1850	1857	1878	rBV	2043486	3591359	49.52%	4.791%
18	14.398	1897	1906	1929	rBV2	2707581	4457463	61.46%	5.946%
19	14.704	1950	1958	1976	rBV	1895554	3139049	43.28%	4.188%
20	14.986	1999	2006	2024	rBV2	331531	1326005	18.28%	1.769%
21	15.616	2108	2113	2118	rVB9	3988	7731	0.11%	0.010%
22	15.698	2120	2127	2144	rBV	2826758	5316336	73.30%	7.092%
23	15.869	2150	2156	2184	rVB	475262	1269075	17.50%	1.693%
24	17.133	2368	2371	2373	rBV4	6356	7764	0.11%	0.010%
25	17.251	2387	2391	2394	rBV5	6833	11114	0.15%	0.015%
26	17.463	2420	2427	2438	rBV	2452187	3751672	51.73%	5.005%
27	17.569	2438	2445	2472	rVB2	3151562	5998679	82.71%	8.002%
28	19.369	2747	2751	2756	rBV	54670	77479	1.07%	0.103%
29	19.439	2760	2763	2769	rVV	41329	66284	0.91%	0.088%
30	19.792	2817	2823	2839	rBV	4392712	7117502	98.13%	9.495%
31	21.557	3118	3123	3134	rBV2	2302097	3836824	52.90%	5.118%
32	23.927	3519	3526	3542	rVB2	2929016	7252865	100.00%	9.675%
33	24.098	3548	3555	3572	rVB	1658140	4302835	59.33%	5.740%




Sum of corrected areas: 74961388

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015887.D
Acq On : 01 Jul 2023 17:05
Operator : MA/JU
Sample : PB153707BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK707

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

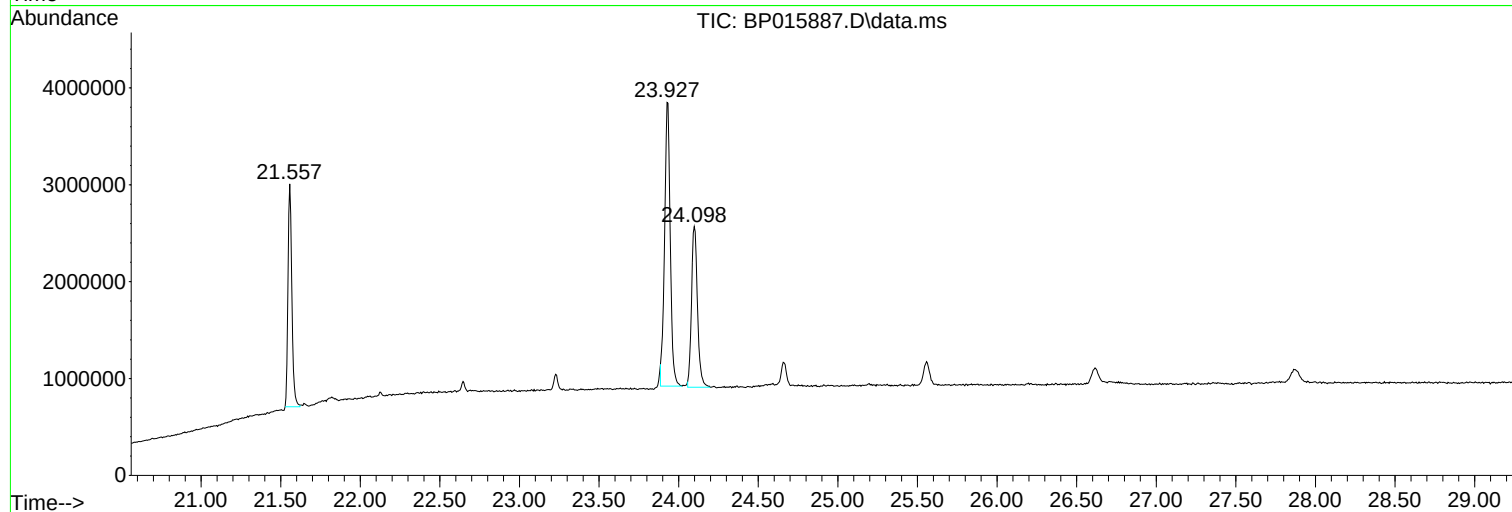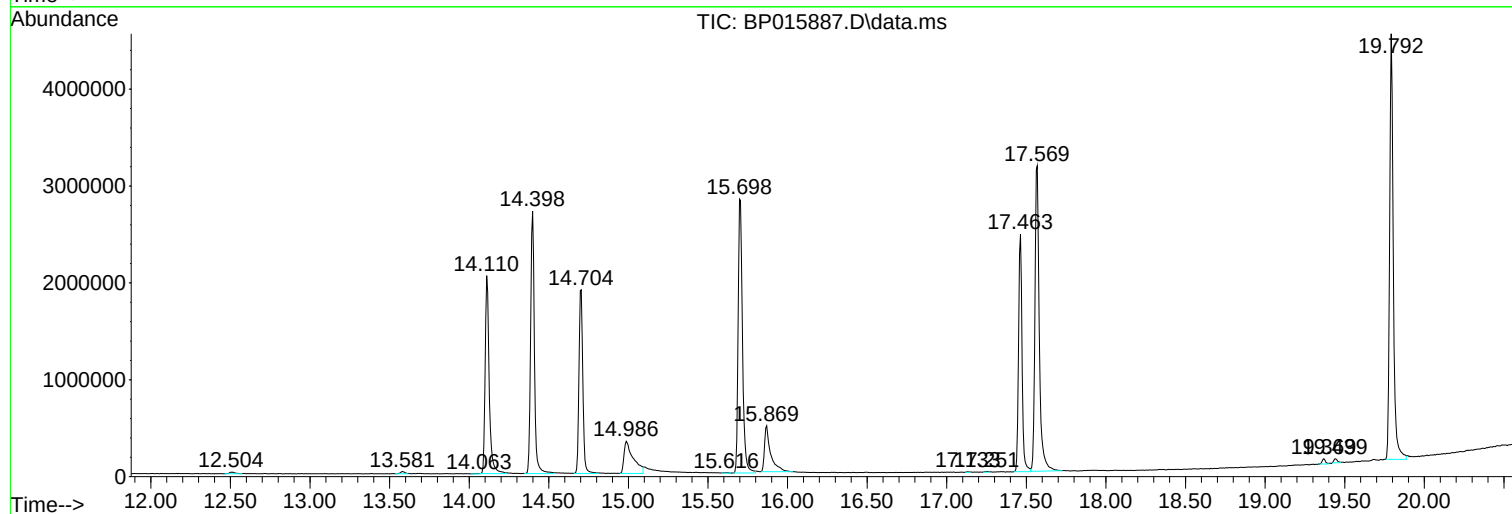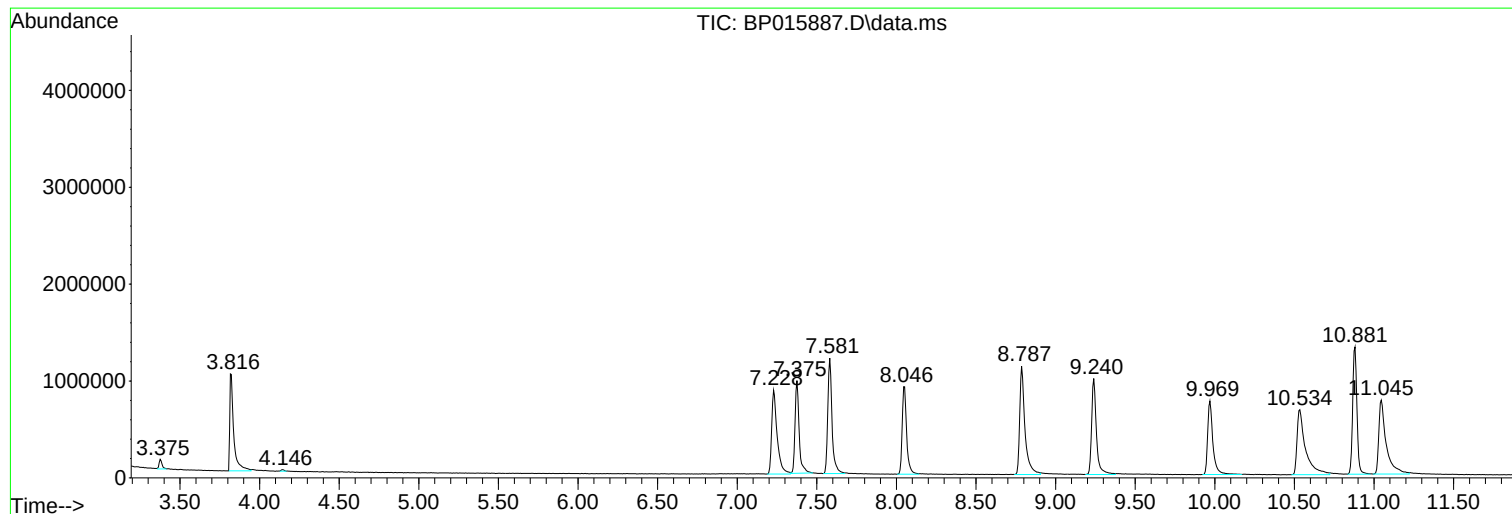

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015887.D
Acq On : 01 Jul 2023 17:05
Operator : MA/JU
Sample : PB153707BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK707

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP063023\
Data File : BP015887.D
Acq On : 01 Jul 2023 17:05
Operator : MA/JU
Sample : PB153707BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK707

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------