




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015916.D
 Acq On : 02 Jul 2023 10:03
 Operator : MA/JU
 Sample : 03243-06
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 13:08:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :mohammad ahmed 07/03/2023

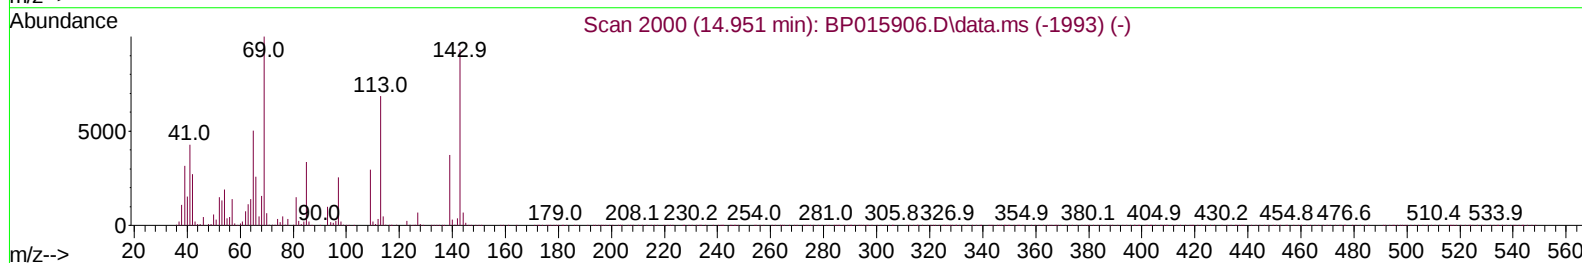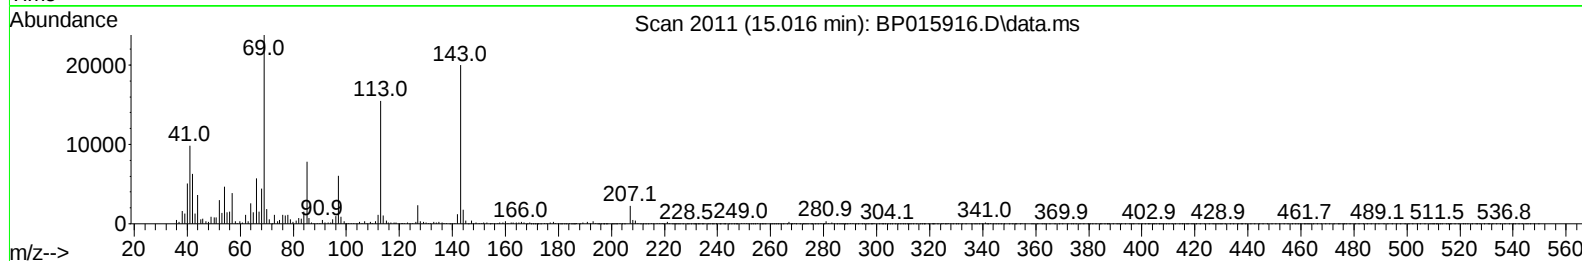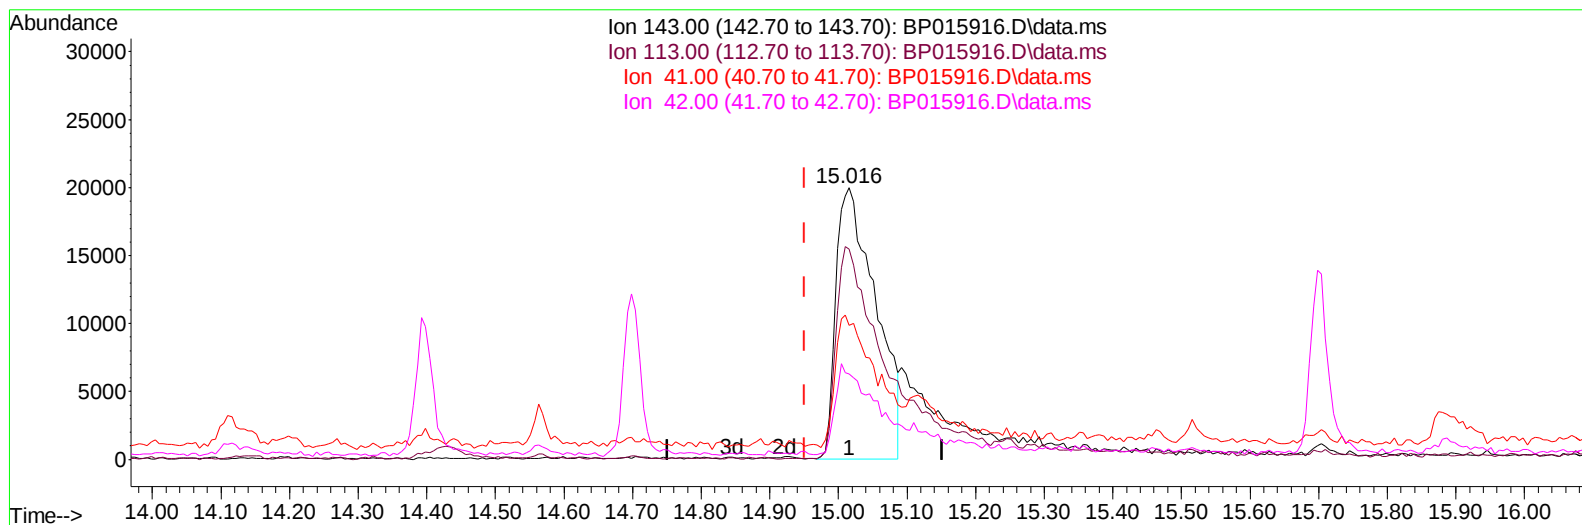

TIC: BP015916.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.016min (+ 0.065) 14.73 ng/u1

response 80580

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	77.40
41.00	45.70	49.36
42.00	31.20	31.40




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015916.D
 Acq On : 02 Jul 2023 10:03
 Operator : MA/JU
 Sample : 03243-06
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 13:08:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :mohammad ahmed 07/03/2023

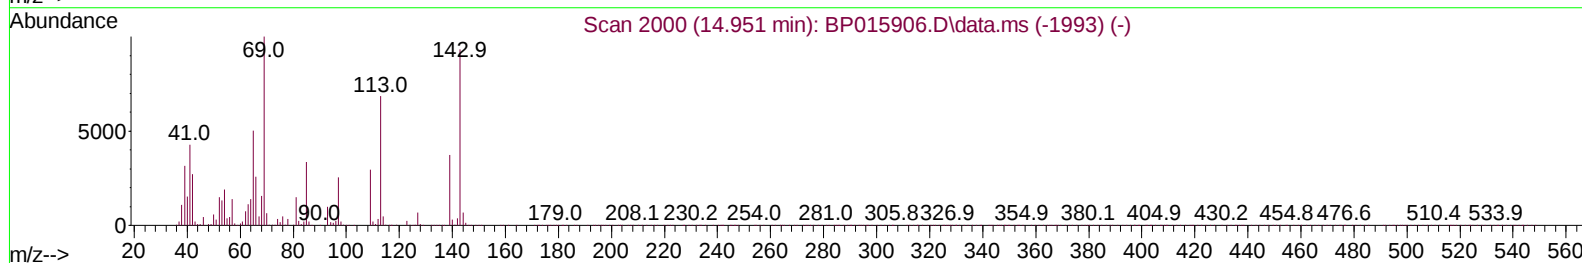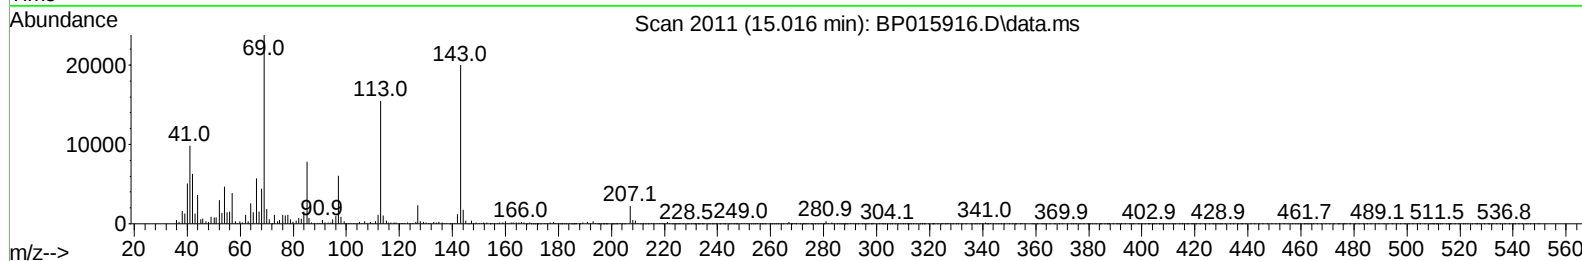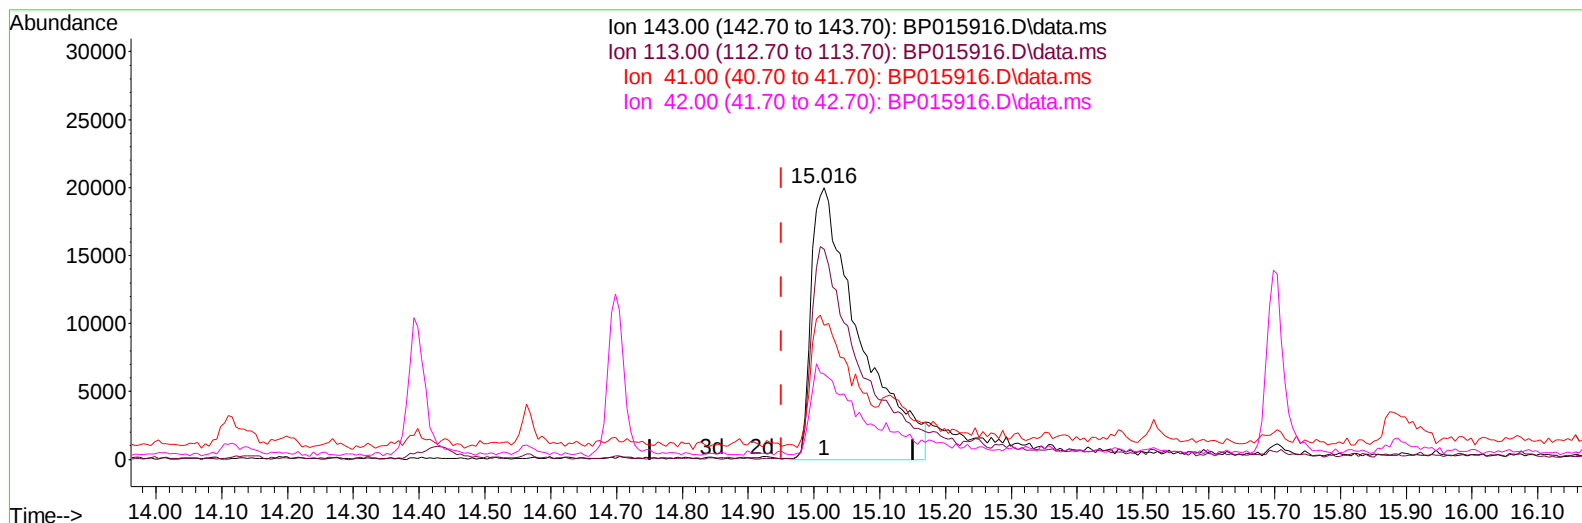

TIC: BP015916.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.016min (+ 0.065) 18.55 ng/ul m

response 101471

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	77.40
41.00	45.70	49.36
42.00	31.20	31.40

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015916.D
 Acq On : 02 Jul 2023 10:03
 Operator : MA/JU
 Sample : 03243-06
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGC6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :mohammad ahmed 07/03/2023

Quant Time: Jul 02 13:09:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	250198	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	1026814	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	536341	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	967462	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	871885	20.000	ng/ul	# 0.00
88) Perylene-d12	24.098	264	1026219	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	28298	4.069	ng/uL	0.00
4) Pyridine-d5	3.822	84	288254	16.444	ng/ul	0.00
7) Phenol-d5	7.234	99	492182	22.991	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.375	67	344371	26.002	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	403591	24.975	ng/ul	0.00
15) 4-Methylphenol-d8	8.793	113	373413	22.080	ng/ul	0.01
21) Nitrobenzene-d5	9.240	128	187838	23.937	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	206328	22.528	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.546	165	325739	19.958	ng/ul	0.04
31) 4-Chloroaniline-d4	11.057	131	351772	16.778	ng/ul	0.03
46) Dimethylphthalate-d6	14.110	166	1021108	24.632	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	1144796	24.566	ng/ul	0.00
54) 4-Nitrophenol-d4	15.016	143	101471m	18.548	ng/ul	0.06
60) Fluorene-d10	15.698	176	794913	23.288	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	62358	10.481	ng/ul	0.02
73) Anthracene-d10	17.563	188	1106823	25.046	ng/ul	0.00
81) Pyrene-d10	19.792	212	1370385	24.070	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	1411493	27.266	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015916.D
Acq On : 02 Jul 2023 10:03
Operator : MA/JU
Sample : 03243-06
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGC6

Manual IntegrationsAPPROVED

Quant Time: Jul 02 13:09:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
Supervised By :mohammad ahmed 07/03/2023

