




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015924.D
 Acq On : 02 Jul 2023 15:09
 Operator : MA/JU
 Sample : PB153766BL
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK766

Manual IntegrationsAPPROVED

Quant Time: Jul 03 04:19:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :mohammad ahmed 07/03/2023

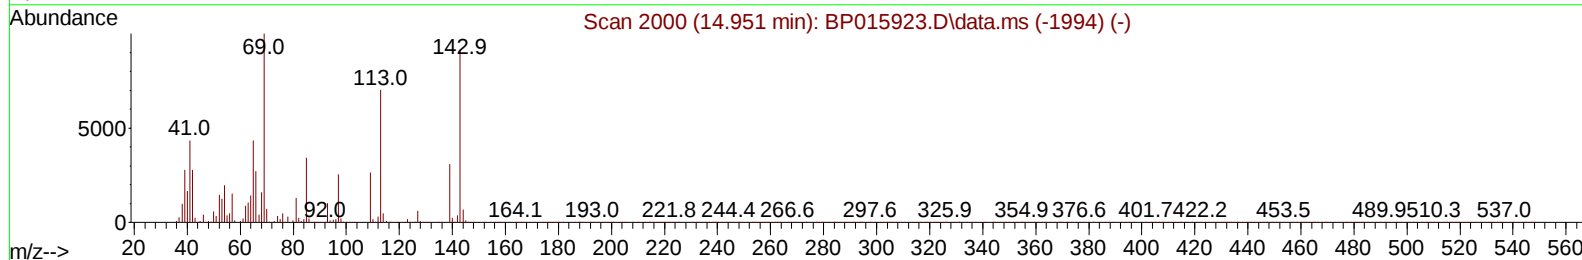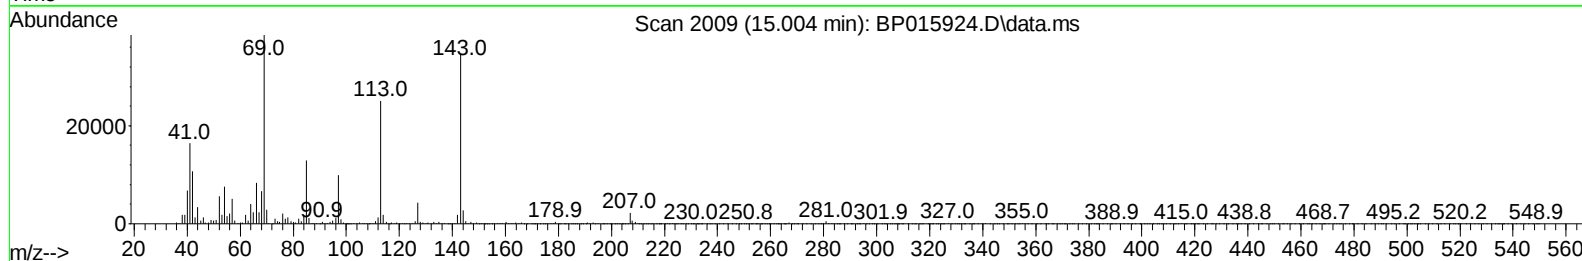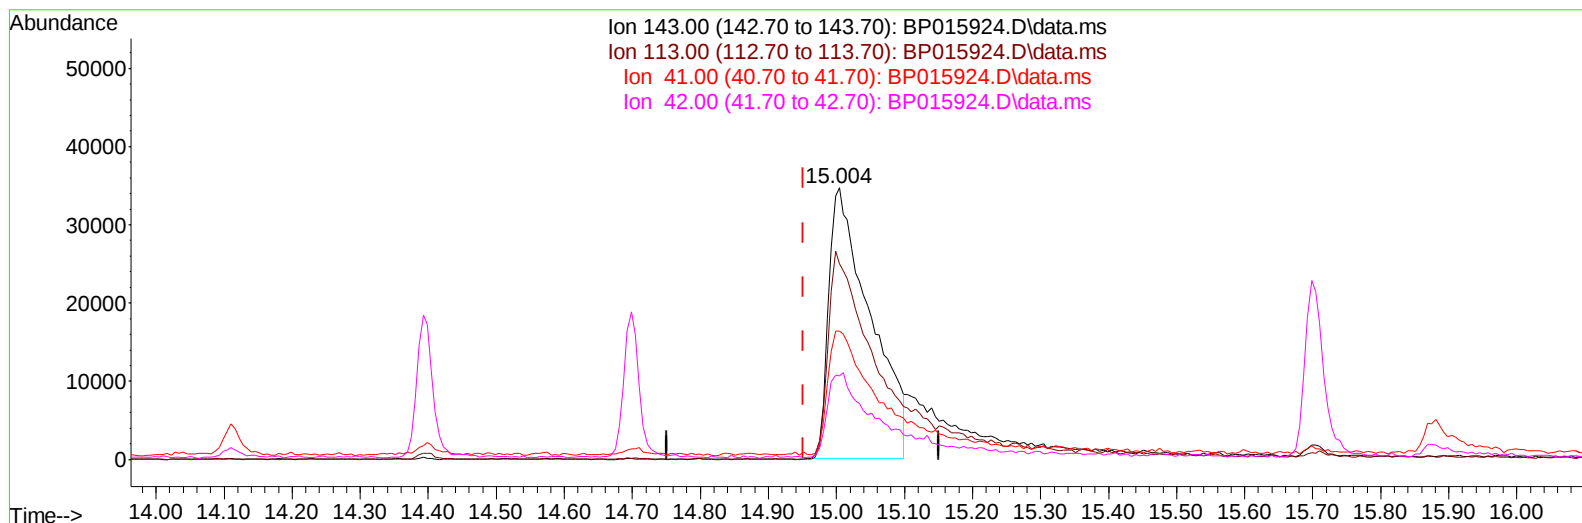

TIC: BP015924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.053) 18.25 ng/u1

response 146353

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	72.12#
41.00	45.70	47.37
42.00	31.20	30.82




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Manual IntegrationsAPPROVED

Quant Time: Jul 03 04:19:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
Supervised By :mohammad ahmed 07/03/2023

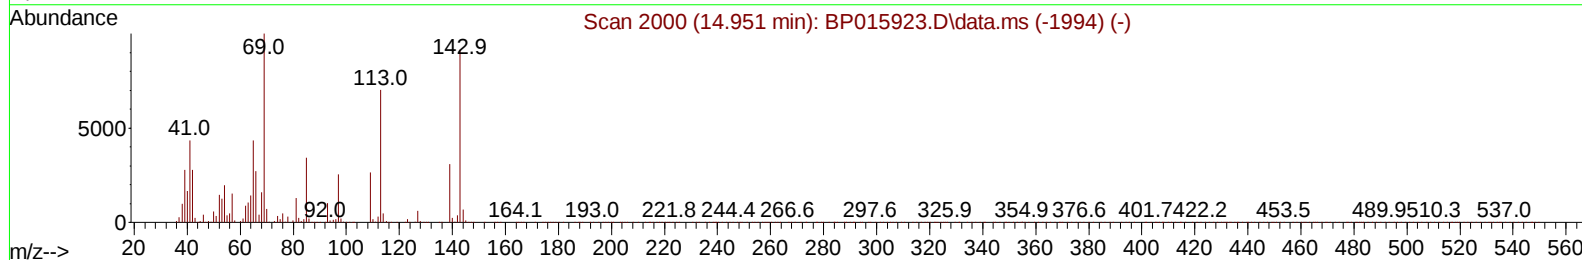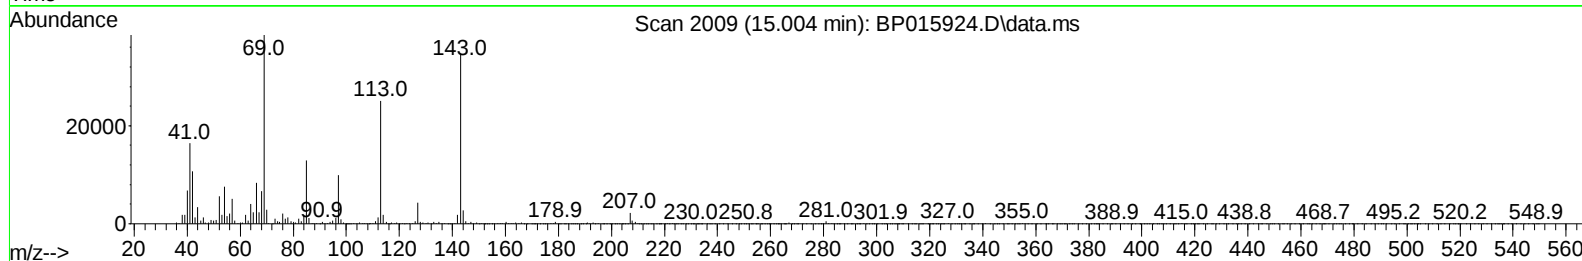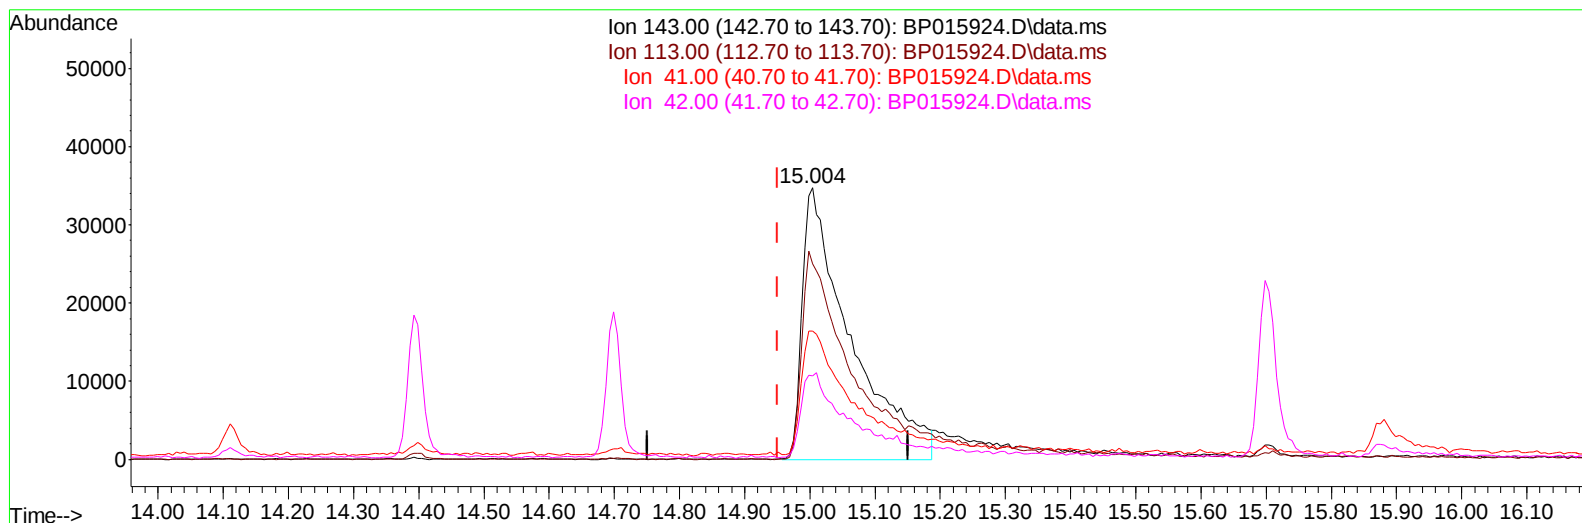

TIC: BP015924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.053) 22.17 ng/ul m

response 177784

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	72.12#
41.00	45.70	47.37
42.00	31.20	30.82

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015924.D
 Acq On : 02 Jul 2023 15:09
 Operator : MA/JU
 Sample : PB153766BL
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK766

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :mohammad ahmed 07/03/2023

Quant Time: Jul 03 04:25:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	337830	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	1446071	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	786030	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1339525	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.563	240	1064925	20.000	ng/ul	0.01
88) Perylene-d12	24.104	264	1258919	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	46822	4.987	ng/uL	0.00
4) Pyridine-d5	3.817	84	644114	27.213	ng/ul	0.00
7) Phenol-d5	7.228	99	839841	29.055	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	572694	32.024	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	671322	30.767	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	685668	30.027	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	330434	29.900	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	365236	28.316	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	577652	25.132	ng/ul	0.02
31) 4-Chloroaniline-d4	11.046	131	840448	28.465	ng/ul	0.02
46) Dimethylphthalate-d6	14.110	166	1822576	29.999	ng/ul	0.00
49) Acenaphthylene-d8	14.393	160	2015608	29.513	ng/ul	0.00
54) 4-Nitrophenol-d4	15.004	143	177784m	22.175	ng/ul	0.05
60) Fluorene-d10	15.698	176	1396258	27.911	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	125137	15.190	ng/ul	0.02
73) Anthracene-d10	17.569	188	1895167	30.973	ng/ul	0.01
81) Pyrene-d10	19.792	212	1923090	27.656	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	1941025	30.565	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Manual IntegrationsAPPROVED

Quant Time: Jul 03 04:25:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2023
Supervised By :mohammad ahmed 07/03/2023

