

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015907.D
 Acq On : 02 Jul 2023 04:58
 Operator : MA/JU
 Sample : PB153764BL
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK764

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	28	31	39	rVB	59958	87821	1.32%	0.130%
2	3.817	105	107	129	rBV	749806	1425076	21.38%	2.110%
3	4.140	159	162	169	rVB4	12461	20654	0.31%	0.031%
4	7.228	679	687	706	rBV	700314	1780544	26.71%	2.636%
5	7.375	706	712	733	rVB	748901	1412708	21.19%	2.091%
6	7.581	740	747	768	rVB	966277	1828048	27.42%	2.706%
7	8.046	817	826	845	rBV	668710	1365717	20.49%	2.022%
8	8.787	944	952	976	rBV	971392	2376495	35.65%	3.518%
9	9.240	1021	1029	1049	rBV	907199	1886922	28.31%	2.793%
10	9.969	1145	1153	1180	rBV2	661325	1589531	23.85%	2.353%
11	10.534	1241	1249	1272	rBV	650466	2275122	34.13%	3.368%
12	10.875	1300	1307	1324	rVB	1142151	2166945	32.51%	3.208%
13	11.046	1328	1336	1376	rBV	727509	2428021	36.42%	3.595%
14	12.510	1579	1585	1593	rBV2	14215	29669	0.45%	0.044%
15	13.575	1762	1766	1776	rVB2	22088	42326	0.63%	0.063%
16	14.110	1850	1857	1883	rVV	2032242	3653099	54.80%	5.408%
17	14.393	1898	1905	1930	rBV	2772273	4536807	68.06%	6.717%
18	14.698	1950	1957	1976	rBV	1950950	3069095	46.04%	4.544%
19	14.993	2000	2007	2039	rBV	285247	1424684	21.37%	2.109%
20	15.698	2120	2127	2144	rBV	3001278	5502098	82.54%	8.146%
21	15.869	2150	2156	2183	rBV2	380853	1119868	16.80%	1.658%
22	16.292	2223	2228	2231	rVB7	3978	7071	0.11%	0.010%
23	17.457	2420	2426	2438	rBV	2454658	3739535	56.10%	5.536%
24	17.563	2438	2444	2466	rVB2	3330126	6155991	92.35%	9.114%
25	19.369	2747	2751	2755	rBV3	50922	67595	1.01%	0.100%
26	19.445	2760	2764	2768	rBV	42544	66054	0.99%	0.098%
27	19.792	2817	2823	2842	rBV	3970837	6665889	100.00%	9.869%
28	21.557	3118	3123	3133	rBV2	1804857	3040966	45.62%	4.502%
29	23.927	3520	3526	3540	rVB2	2033655	4736403	71.05%	7.012%
30	24.098	3549	3555	3571	rVB	1134090	3046215	45.70%	4.510%




Sum of corrected areas: 67546969

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015907.D
Acq On : 02 Jul 2023 04:58
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

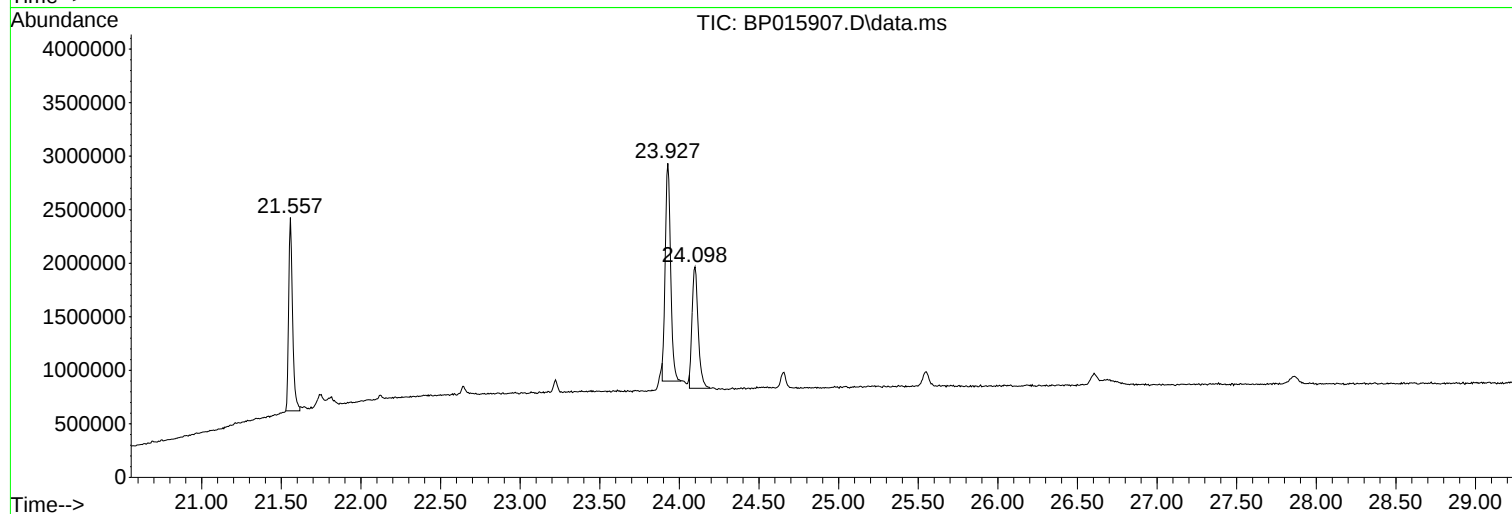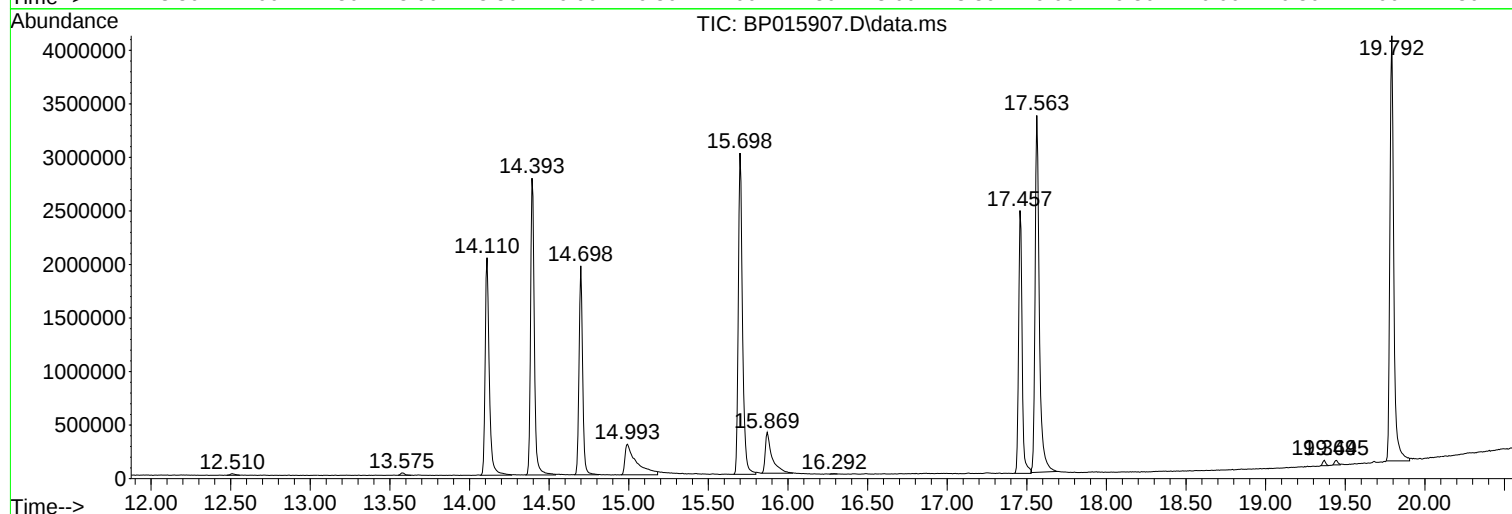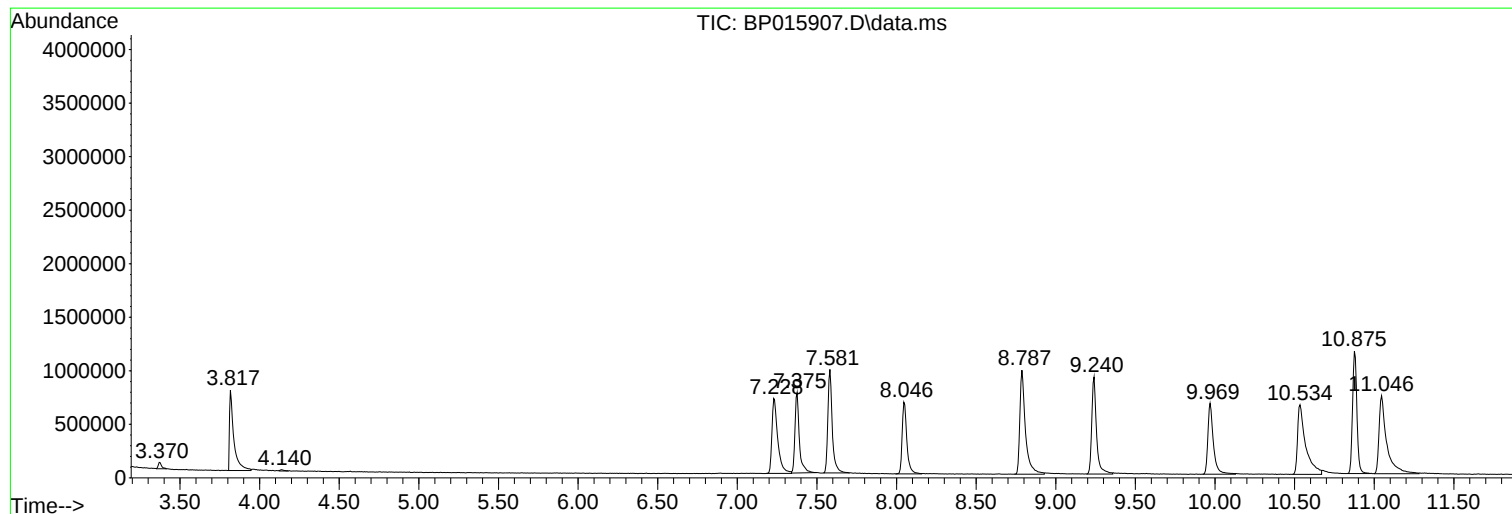

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015907.D
Acq On : 02 Jul 2023 04:58
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015907.D
Acq On : 02 Jul 2023 04:58
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------