

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
 Data File : BP015924.D
 Acq On : 02 Jul 2023 15:09
 Operator : MA/JU
 Sample : PB153766BL
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK766

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	28	31	40	rVB	94295	127053	2.34%	0.174%
2	3.817	104	107	139	rBV	1151865	1935834	35.64%	2.649%
3	4.140	159	162	169	rVB	25287	40361	0.74%	0.055%
4	6.911	631	633	637	rBV5	4118	5709	0.11%	0.008%
5	7.228	680	687	705	rBV	993632	2401051	44.21%	3.285%
6	7.369	705	711	726	rVB	1061726	1931426	35.56%	2.643%
7	7.581	739	747	772	rVB	1354537	2521147	46.42%	3.449%
8	8.046	819	826	844	rBV	1126473	2119969	39.04%	2.901%
9	8.787	944	952	974	rBV	1308958	3085140	56.81%	4.221%
10	9.234	1020	1028	1049	rBV	1220027	2487063	45.79%	3.403%
11	9.963	1145	1152	1173	rBV	886654	2069512	38.11%	2.831%
12	10.534	1238	1249	1282	rBV	811727	2935006	54.04%	4.016%
13	10.875	1299	1307	1327	rVB	1685708	3106911	57.21%	4.251%
14	11.046	1327	1336	1366	rBV	922860	2935003	54.04%	4.016%
15	12.510	1578	1585	1593	rVV2	19294	42811	0.79%	0.059%
16	13.581	1761	1767	1781	rBV2	35707	73142	1.35%	0.100%
17	13.681	1781	1784	1788	rBV6	3494	6961	0.13%	0.010%
18	14.110	1849	1857	1882	rVV	2294723	4056674	74.70%	5.550%
19	14.393	1898	1905	1924	rBV	2930762	4818138	88.72%	6.592%
20	14.698	1950	1957	1979	rBV	2359681	3637561	66.98%	4.977%
21	15.004	2002	2009	2043	rBV2	236033	1293230	23.81%	1.769%
22	15.428	2079	2081	2085	rVB4	5381	6154	0.11%	0.008%
23	15.604	2109	2111	2115	rBV5	3968	5921	0.11%	0.008%
24	15.704	2120	2128	2145	rBV	2802221	5430920	100.00%	7.430%
25	15.875	2151	2157	2185	rVB	295081	956461	17.61%	1.309%
26	17.134	2369	2371	2374	rVB4	5872	6398	0.12%	0.009%
27	17.251	2388	2391	2398	rVB8	7036	14405	0.27%	0.020%
28	17.463	2420	2427	2438	rBV	2116457	3411248	62.81%	4.667%
29	17.569	2438	2445	2471	rVB2	2411886	5043091	92.86%	6.900%
30	19.369	2748	2751	2756	rBV2	36287	49457	0.91%	0.068%
31	19.445	2761	2764	2772	rVV	37289	58131	1.07%	0.080%
32	19.792	2818	2823	2840	rBV	2966436	5157433	94.96%	7.056%
33	21.563	3119	3124	3137	rBV	1749720	3011545	55.45%	4.120%
34	23.933	3521	3527	3540	rVB2	1995968	4848955	89.28%	6.634%
35	24.104	3549	3556	3571	rVB	1342084	3459838	63.71%	4.734%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 73089659

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

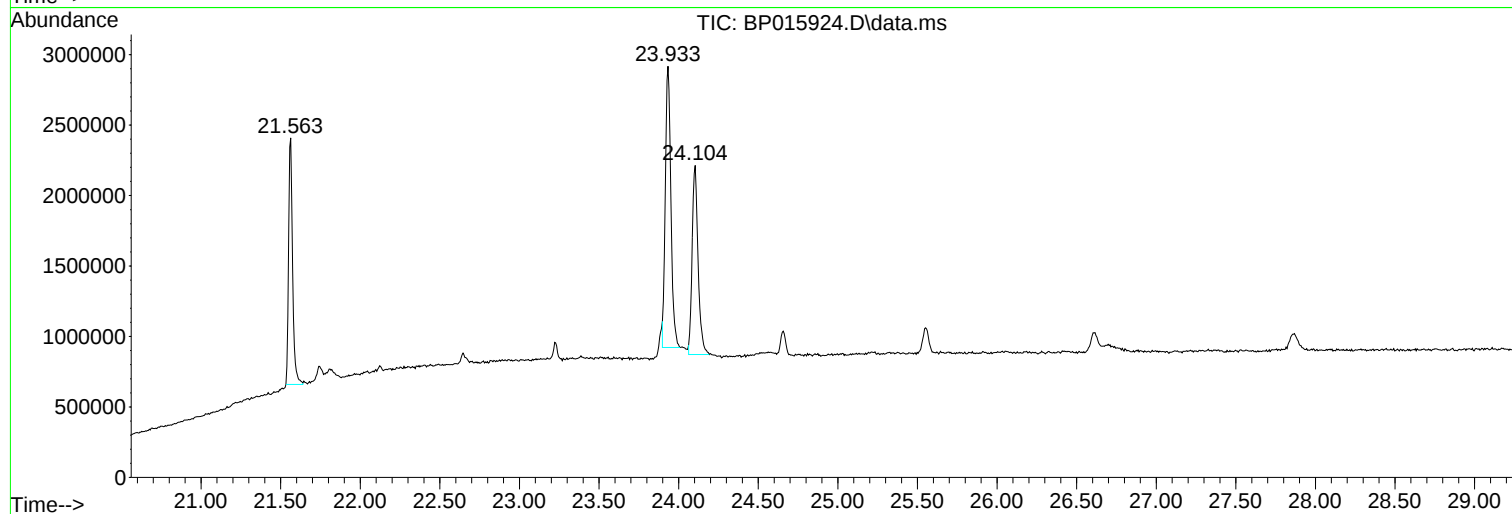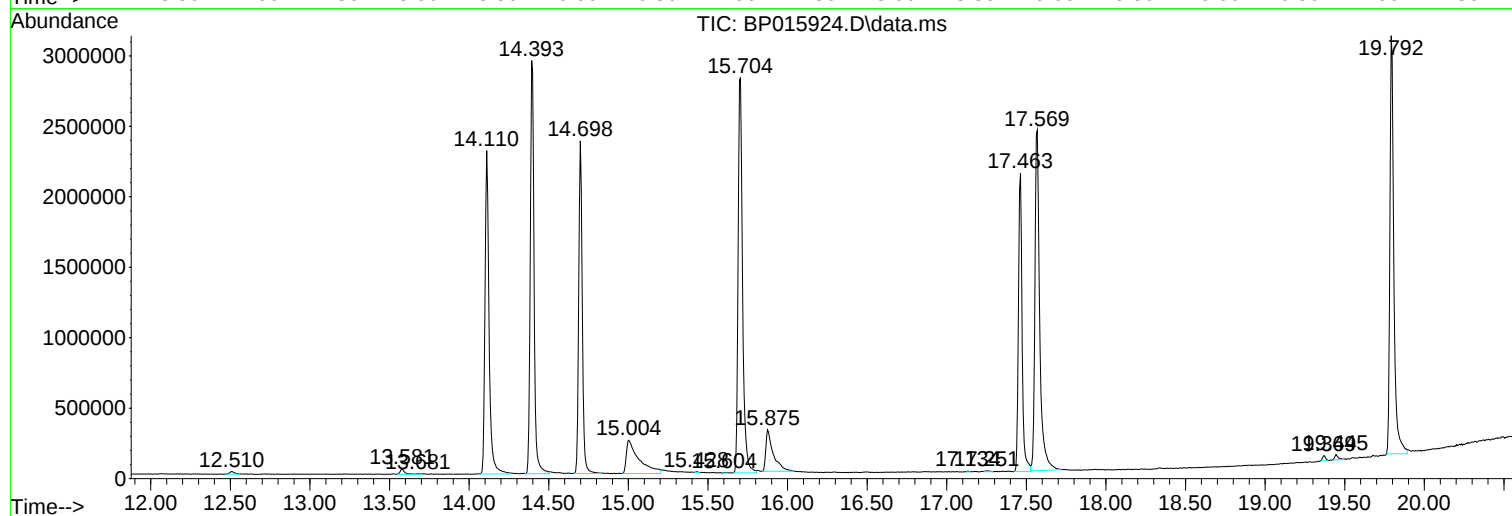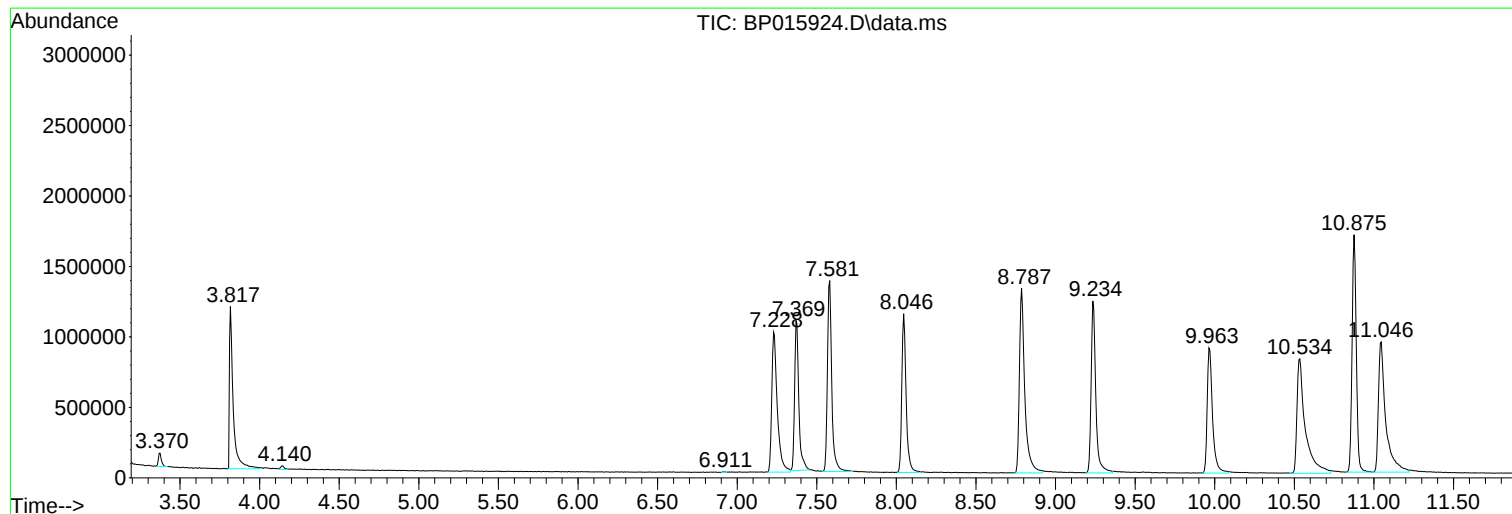

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070223\
Data File : BP015924.D
Acq On : 02 Jul 2023 15:09
Operator : MA/JU
Sample : PB153766BL
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK766

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------