




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015943.D
 Acq On : 03 Jul 2023 10:31
 Operator : MA/JU
 Sample : 03245-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGH0

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:07:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :Yogesh Patel 07/04/2023

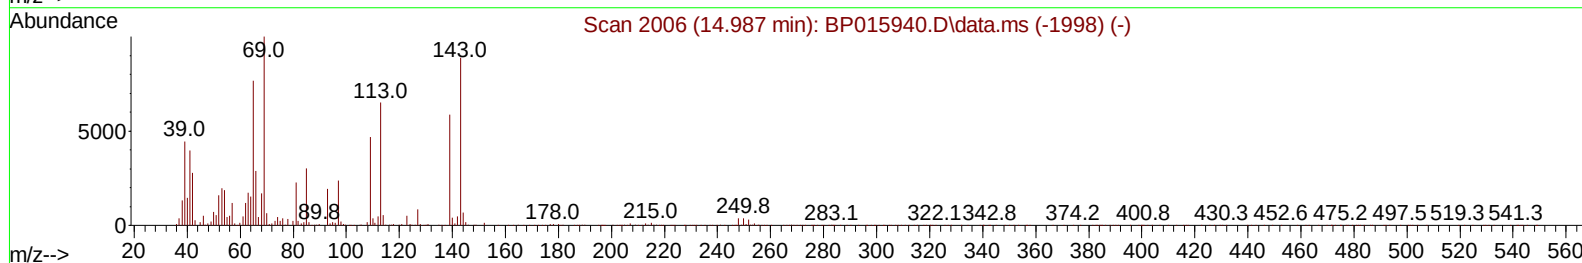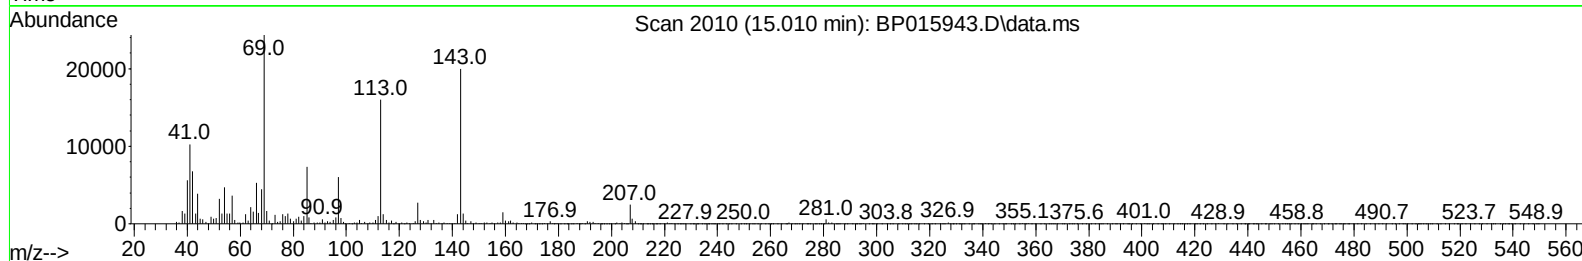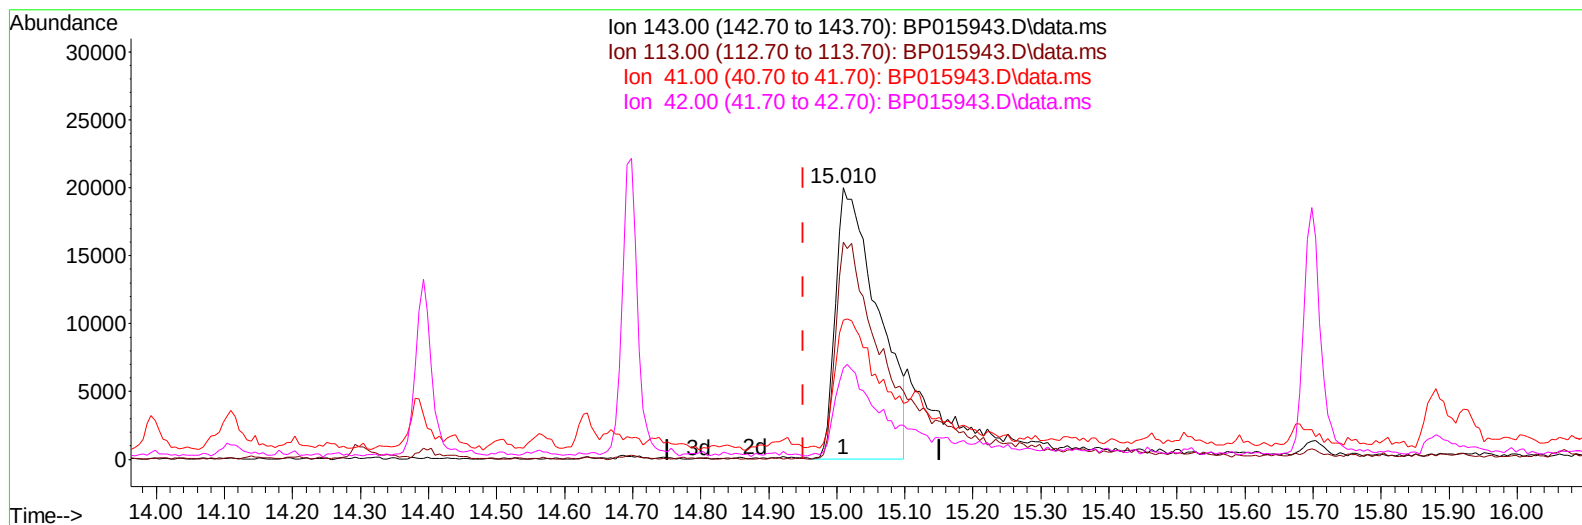

TIC: BP015943.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.010min (+ 0.059) 9.34 ng/ul

response 85455

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	79.97
41.00	45.70	51.38
42.00	31.20	33.68




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015943.D
Acq On : 03 Jul 2023 10:31
Operator : MA/JU
Sample : 03245-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGH0

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:07:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :Yogesh Patel 07/04/2023

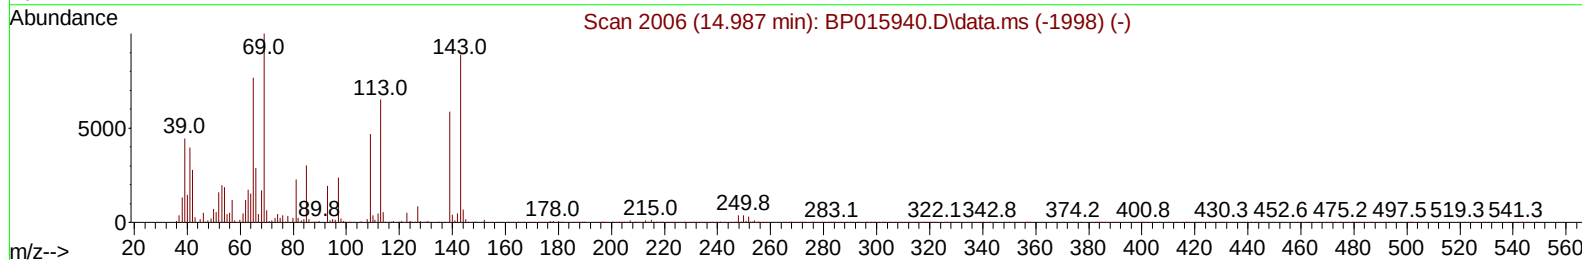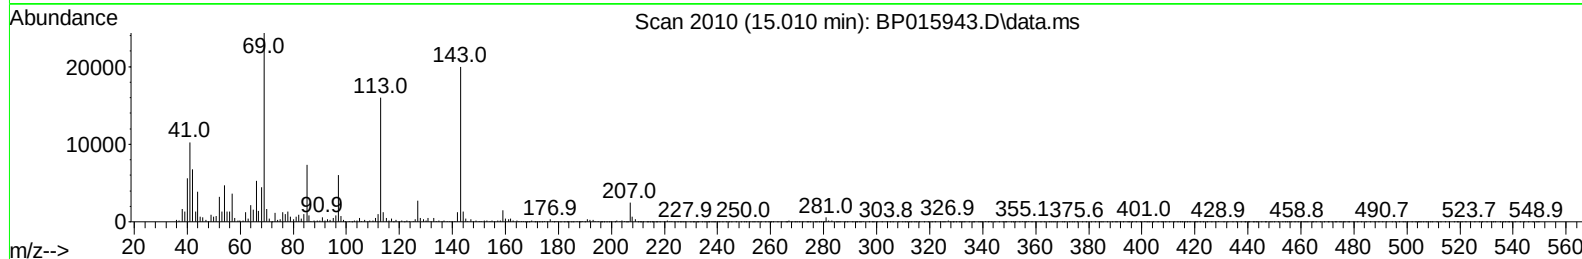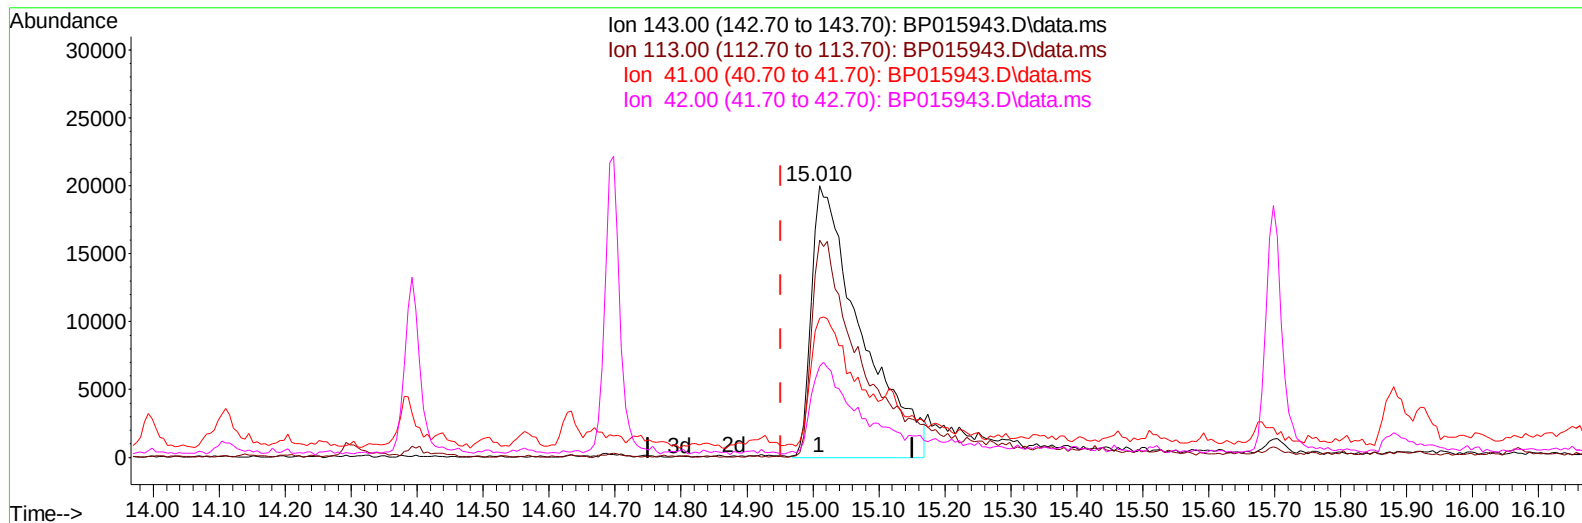

TIC: BP015943.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.010min (+ 0.059) 11.29 ng/ul m

response 103243

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	79.97
41.00	45.70	51.38
42.00	31.20	33.68

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015943.D
 Acq On : 03 Jul 2023 10:31
 Operator : MA/JU
 Sample : 03245-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGH0

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :Yogesh Patel 07/04/2023

Quant Time: Jul 03 22:23:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.045	152	371722	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	1574263	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	896795	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1767860	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	1380711	20.000	ng/ul	# 0.00
88) Perylene-d12	24.097	264	1565335	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	30718	2.973	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.234	99	525533	16.524	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.369	67	383312	19.480	ng/ul	0.00
11) 2-Chlorophenol-d4	7.581	132	451674	18.813	ng/ul	0.00
15) 4-Methylphenol-d8	8.792	113	322761	12.846	ng/ul	0.01
21) Nitrobenzene-d5	9.239	128	216308	17.979	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	222632	15.855	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.545	165	375045	14.988	ng/ul	0.04
31) 4-Chloroaniline-d4	11.069	131	272395	8.474	ng/ul	0.04
46) Dimethylphthalate-d6	14.110	166	1222048	17.630	ng/ul	0.00
49) Acenaphthylene-d8	14.392	160	1379135	17.699	ng/ul	0.00
54) 4-Nitrophenol-d4	15.010	143	103243m	11.287	ng/ul	0.06
60) Fluorene-d10	15.698	176	1002102	17.558	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.880	200	108806	10.008	ng/ul	0.02
73) Anthracene-d10	17.563	188	1362998	16.879	ng/ul	0.00
81) Pyrene-d10	19.792	212	1641397	18.206	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	1431113	18.124	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015943.D
Acq On : 03 Jul 2023 10:31
Operator : MA/JU
Sample : 03245-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGH0

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :Yogesh Patel 07/04/2023

Quant Time: Jul 03 22:23:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

