




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015952.D
 Acq On : 03 Jul 2023 15:38
 Operator : MA/JU
 Sample : 03239-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:09:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

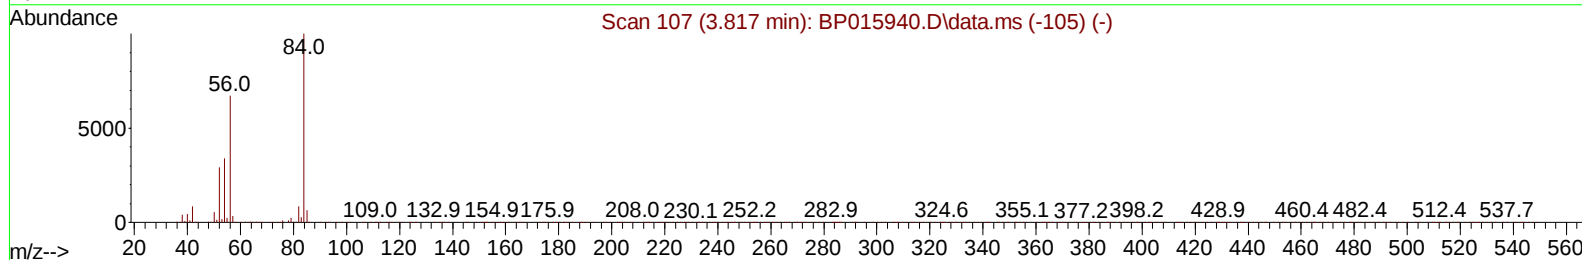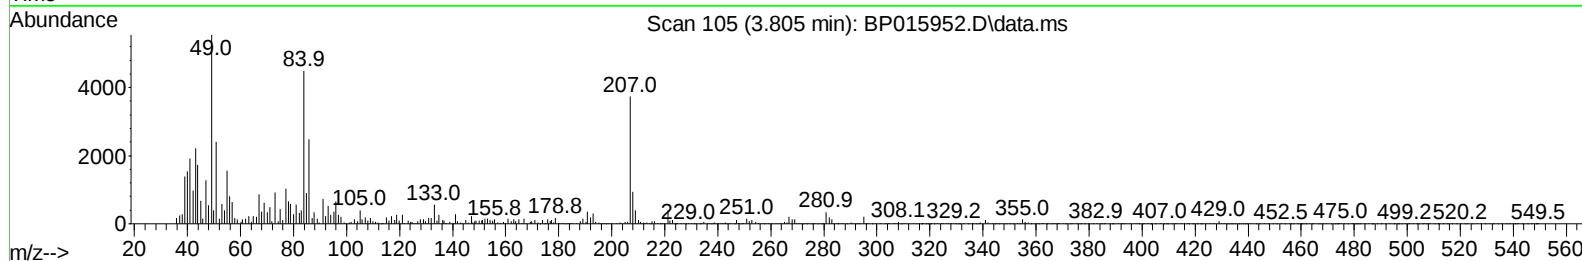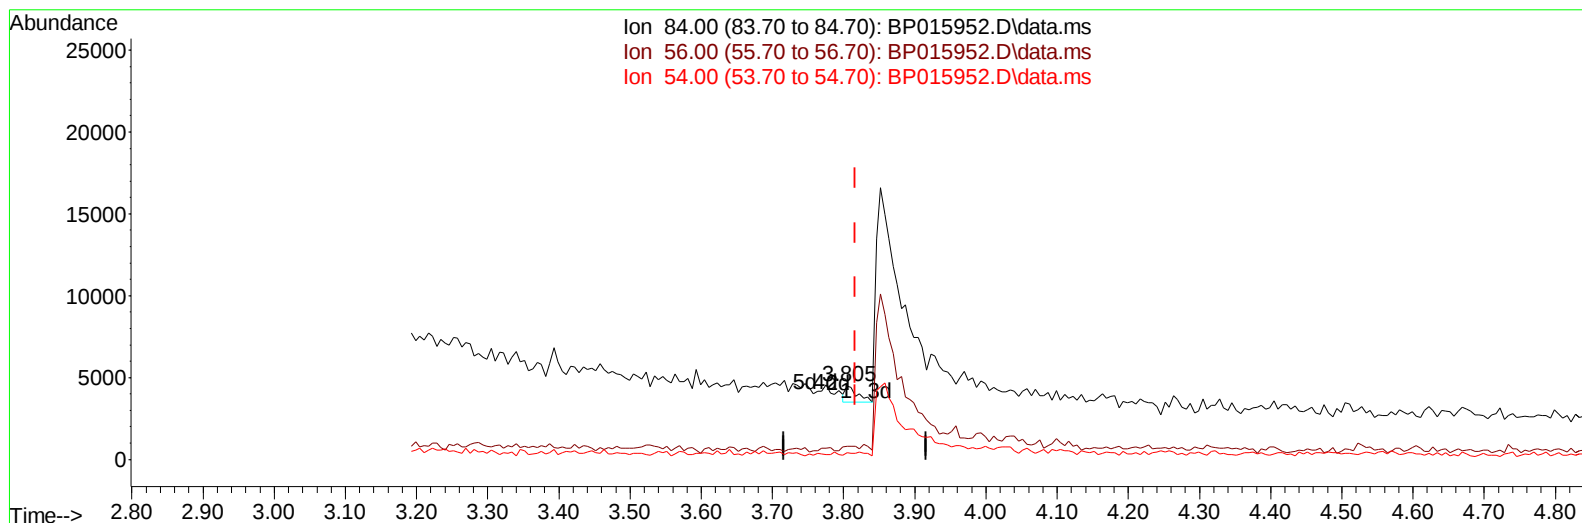

TIC: BP015952.D\data.ms

(4) Pyridine-d5 (S)

3.805min (-0.012) 0.07 ng/u1

response 1165

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.10	18.02#
54.00	34.20	8.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015952.D
Acq On : 03 Jul 2023 15:38
Operator : MA/JU
Sample : 03239-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

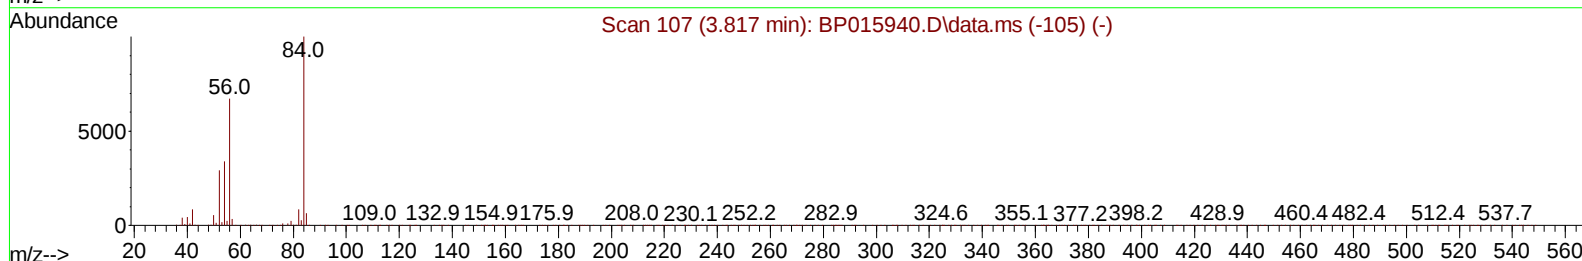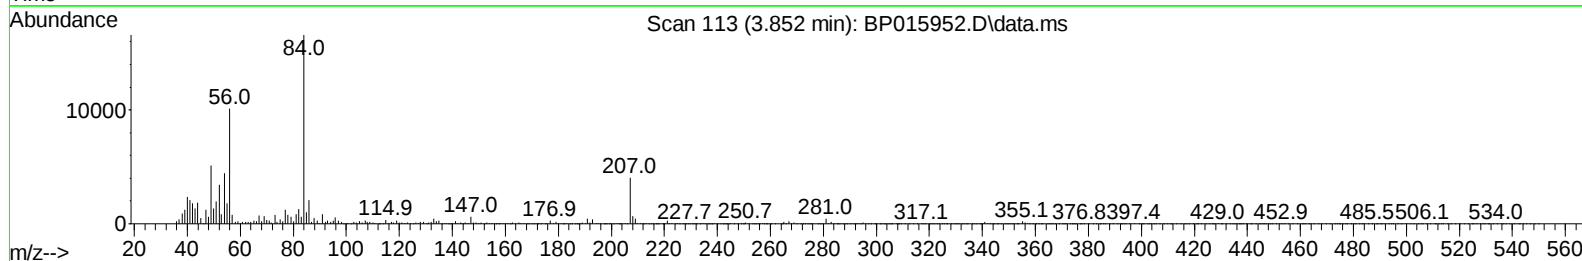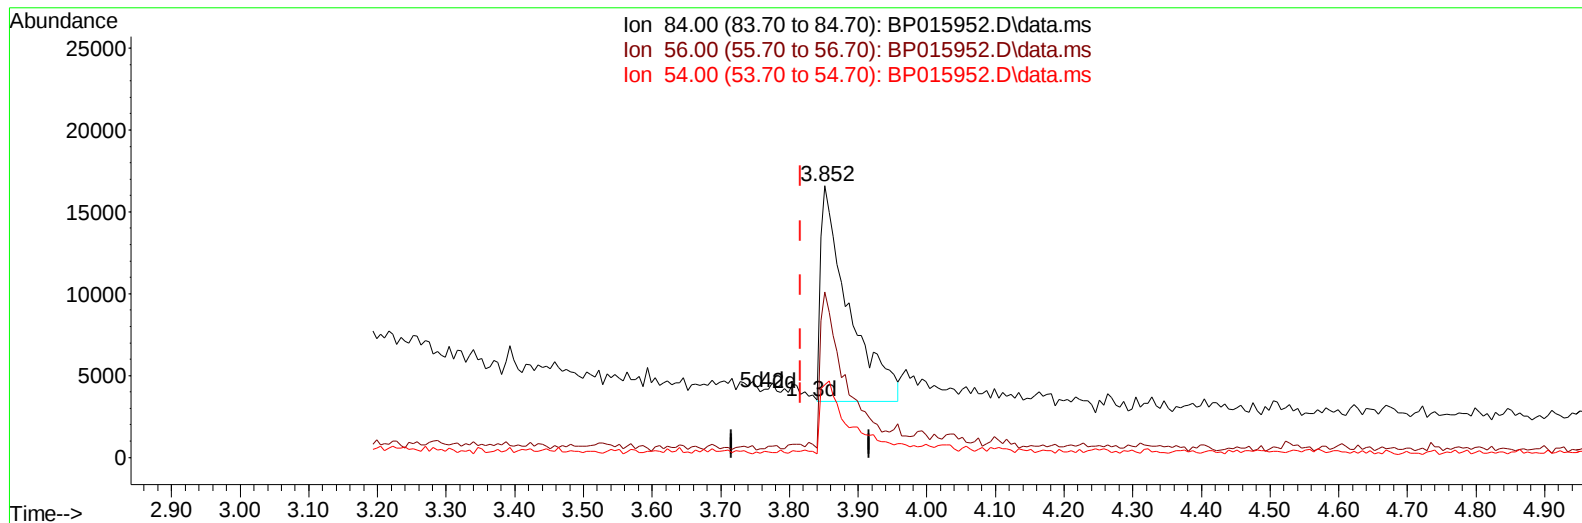

TIC: BP015952.D\data.ms

(4) Pyridine-d5 (S)

3.852min (+ 0.035) 2.19 ng/u1 m

response 37250

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.10	60.97
54.00	34.20	26.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015952.D
Acq On : 03 Jul 2023 15:38
Operator : MA/JU
Sample : 03239-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

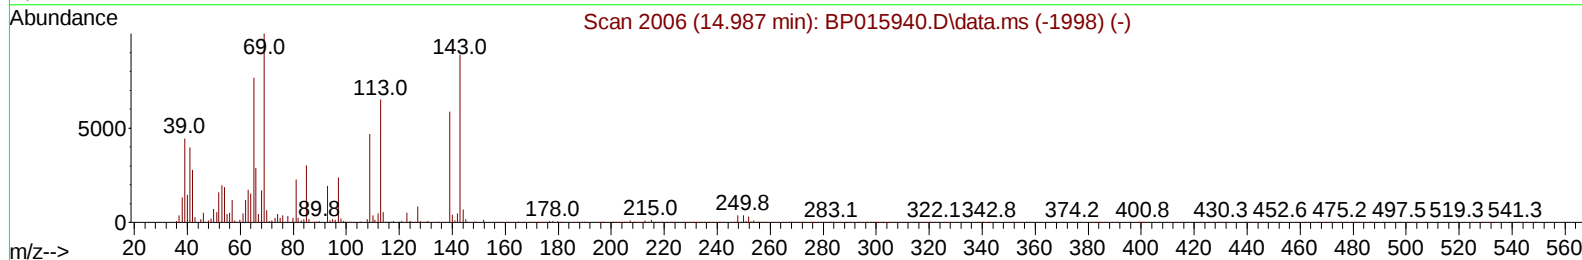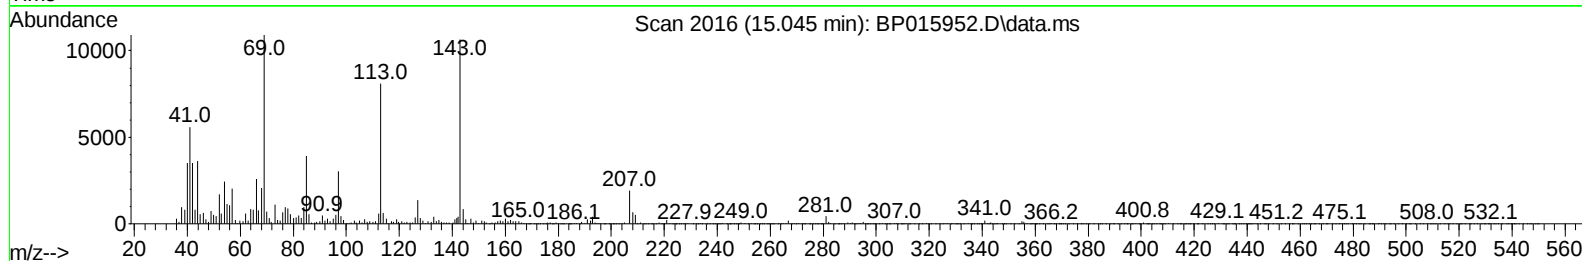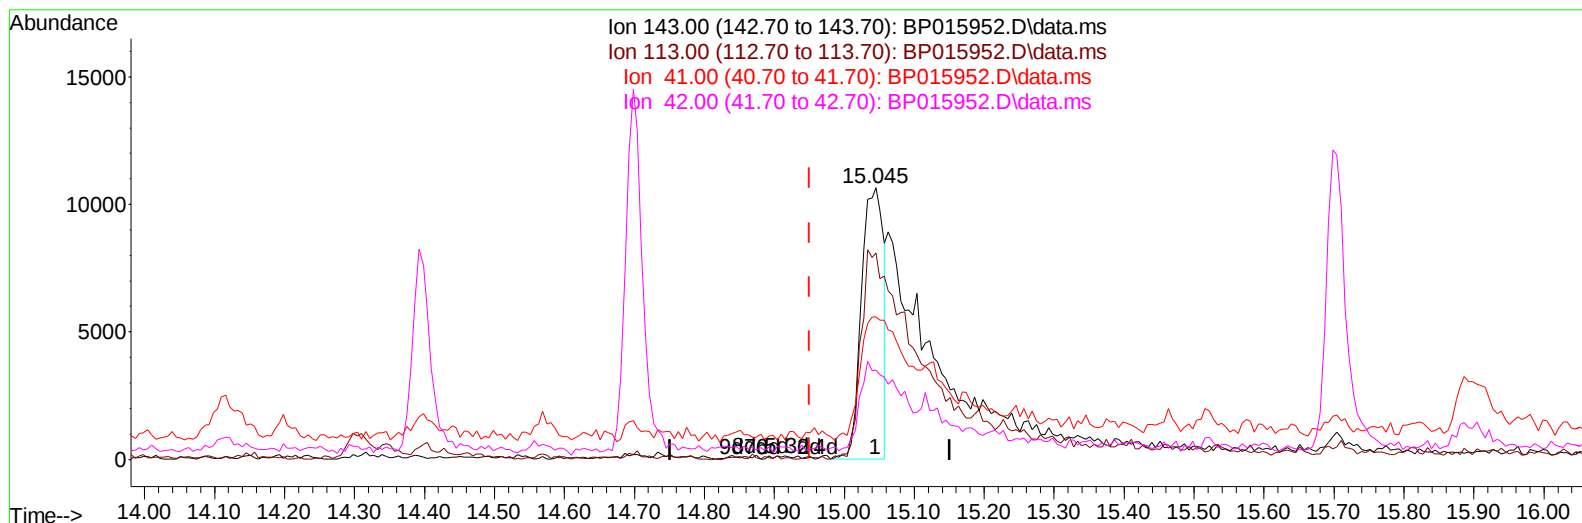

TIC: BP015952.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.045min (+ 0.094) 3.59 ng/u1

response 23163

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	75.95
41.00	45.70	52.57
42.00	31.20	32.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015952.D
Acq On : 03 Jul 2023 15:38
Operator : MA/JU
Sample : 03239-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 22:09:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

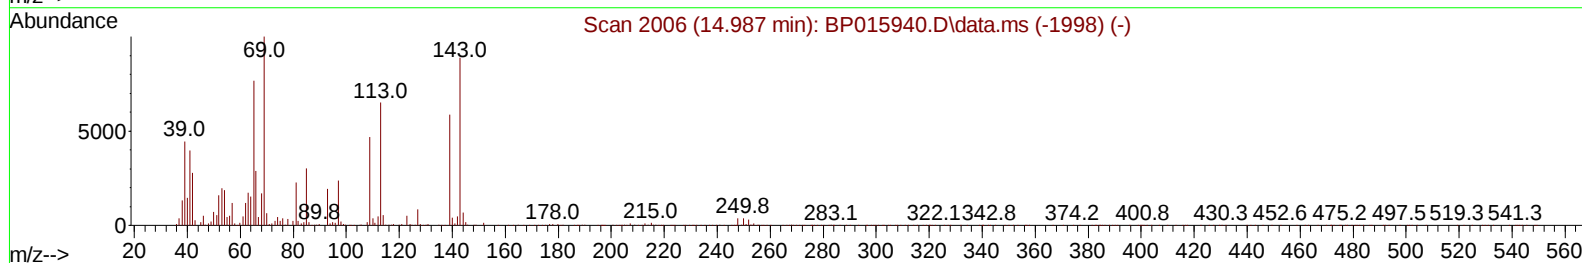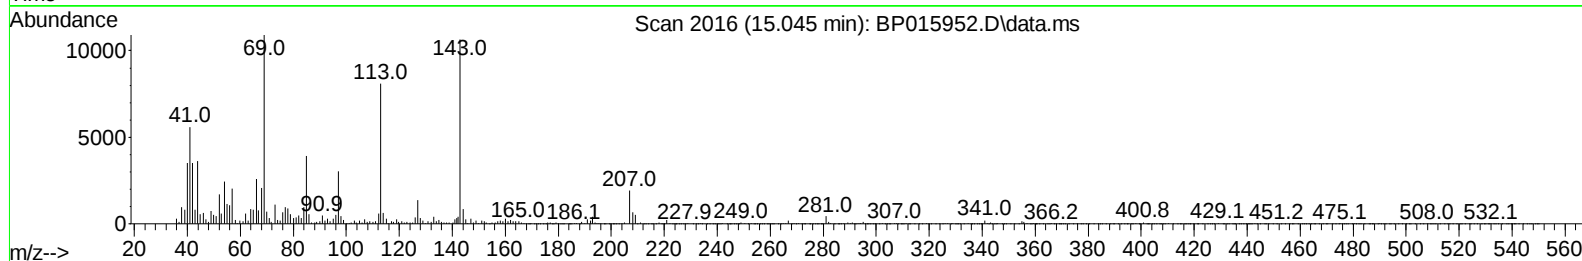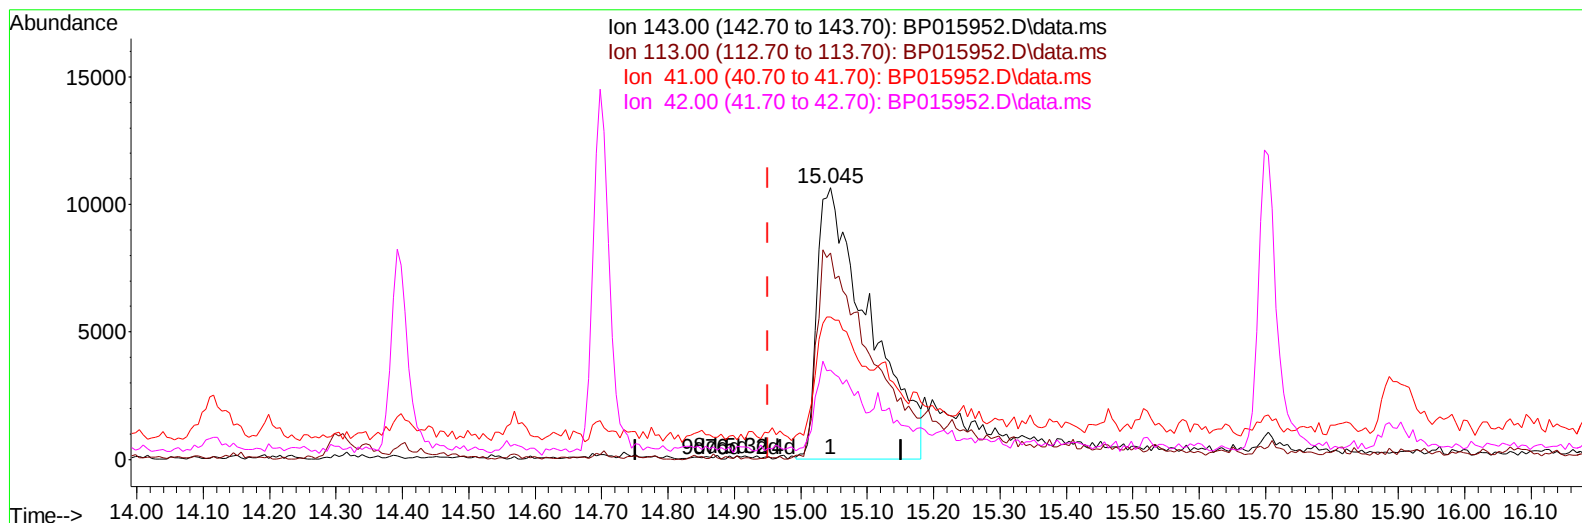

TIC: BP015952.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.045min (+ 0.094) 8.90 ng/ul m

response 57436

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	75.95
41.00	45.70	52.57
42.00	31.20	32.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015952.D
 Acq On : 03 Jul 2023 15:38
 Operator : MA/JU
 Sample : 03239-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 23:34:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

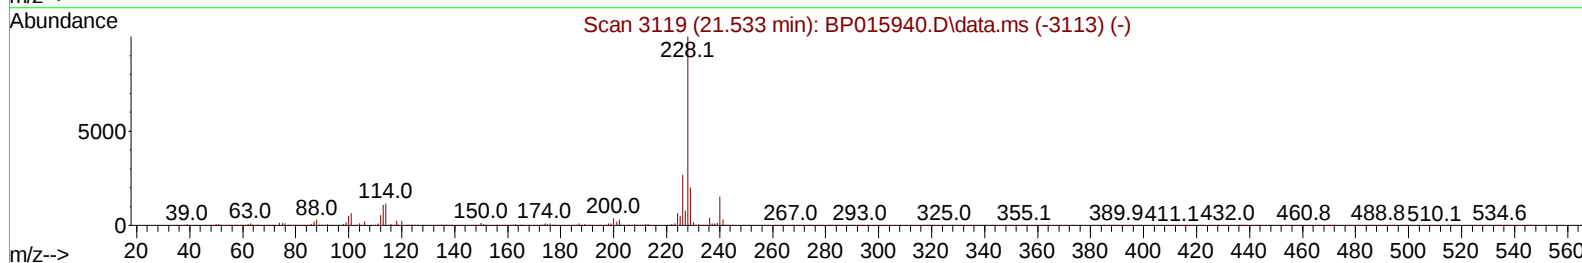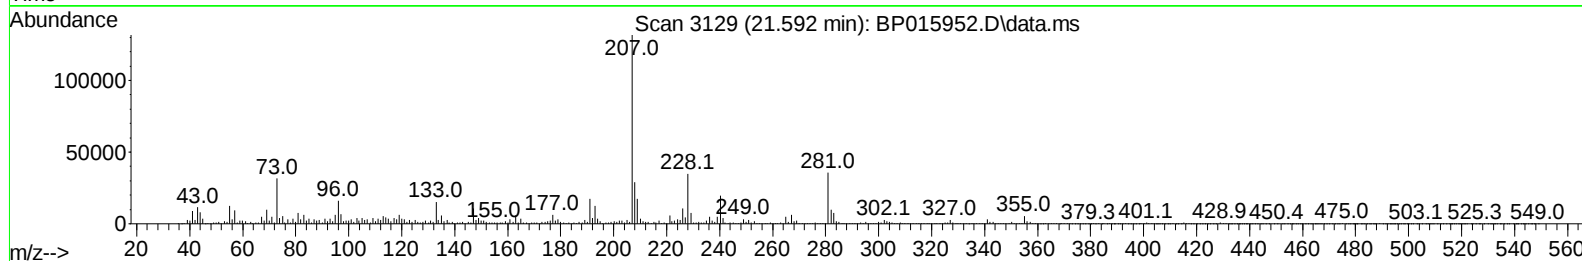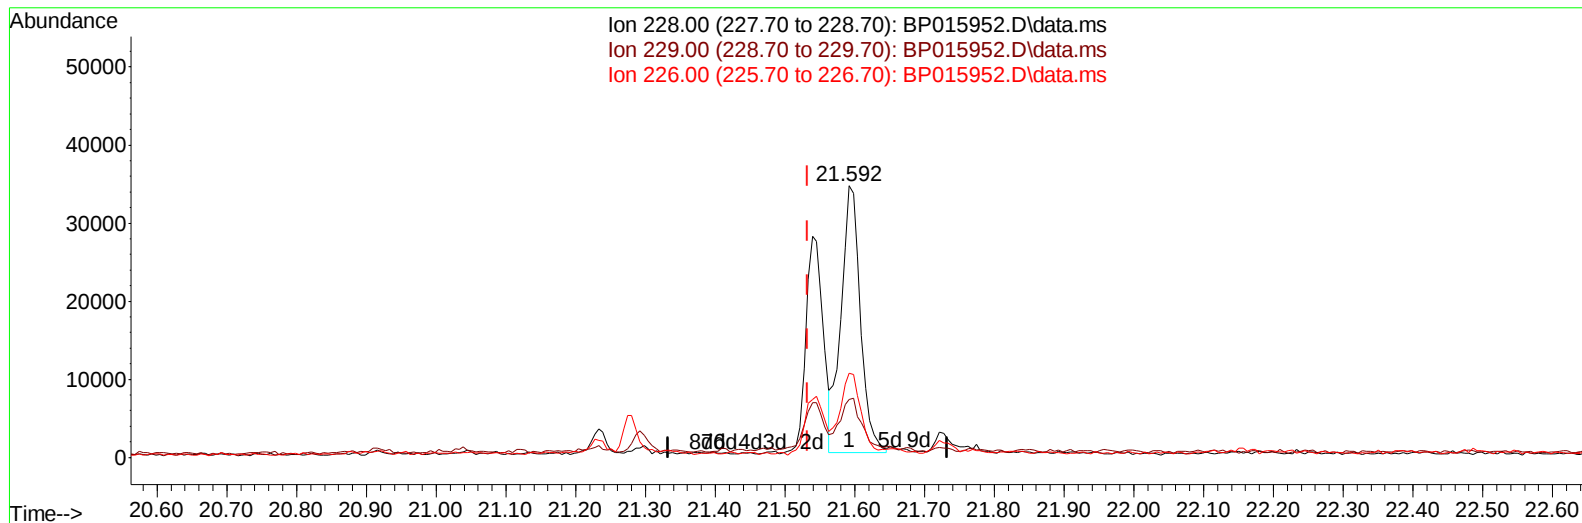

TIC: BP015952.D\data.ms

(85) Benzo(a)anthracene

21.592min (+ 0.059) 1.03 ng/u1

response 66138

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.10	21.38
226.00	26.70	30.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015952.D
 Acq On : 03 Jul 2023 15:38
 Operator : MA/JU
 Sample : 03239-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFZ3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 23:34:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

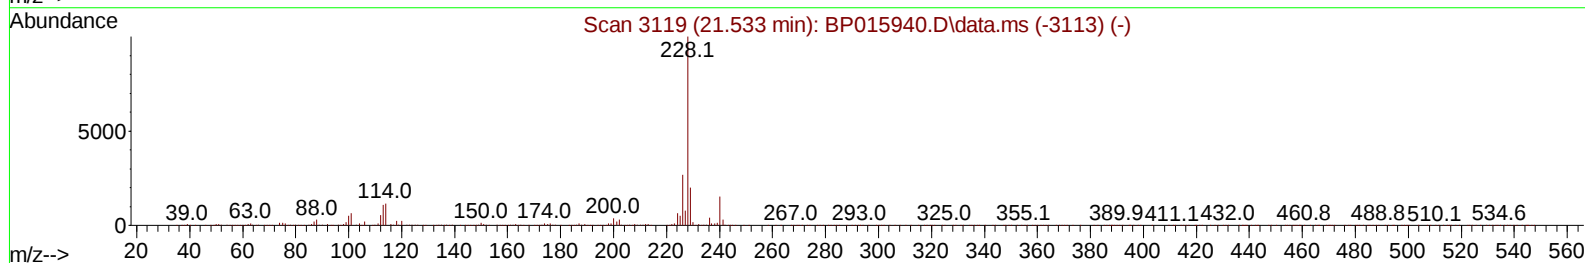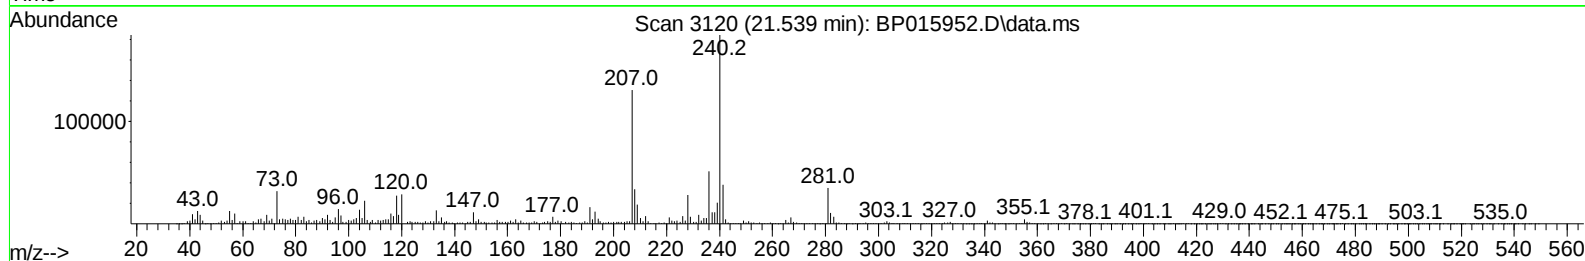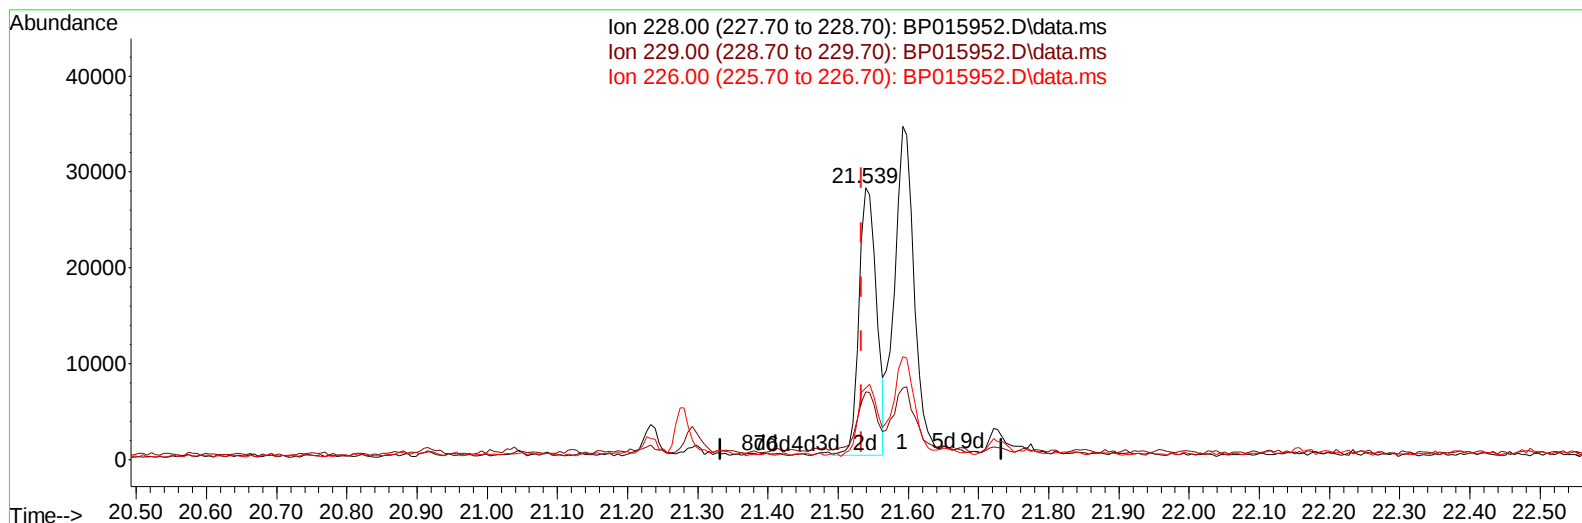

TIC: BP015952.D\data.ms

(85) Benzo(a)anthracene

21.539min (+ 0.006) 0.75 ng/ul m

response 48179

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.10	24.89#
226.00	26.70	26.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015952.D
 Acq On : 03 Jul 2023 15:38
 Operator : MA/JU
 Sample : 03239-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCFZ3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
 Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 03 23:34:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	243319	20.000	ng/ul	0.00
20) Naphthalene-d8	10.875	136	1035815	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.698	164	632965	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1293734	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	913033	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	1004276	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	18424	2.724	ng/uL	0.00
4) Pyridine-d5	3.852	84	37250m	2.185	ng/ul	0.04
7) Phenol-d5	7.246	99	296873	14.260	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.375	67	230413	17.889	ng/ul	0.00
11) 2-Chlorophenol-d4	7.587	132	259451	16.509	ng/ul	0.01
15) 4-Methylphenol-d8	8.810	113	198371	12.062	ng/ul	0.03
21) Nitrobenzene-d5	9.251	128	127427	16.097	ng/ul	0.02
24) 2-Nitrophenol-d4	9.987	143	137706	14.905	ng/ul	0.03
28) 2,4-Dichlorophenol-d3	10.569	165	207618	12.610	ng/ul	0.06
31) 4-Chloroaniline-d4	11.087	131	144749	6.844	ng/ul	0.06
46) Dimethylphthalate-d6	14.116	166	824591	16.855	ng/ul	0.01
49) Acenaphthylene-d8	14.398	160	937820	17.052	ng/ul	0.00
54) 4-Nitrophenol-d4	15.045	143	57436m	8.896	ng/ul	0.09
60) Fluorene-d10	15.704	176	706889	17.548	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.886	200	65041	8.175	ng/ul	0.03
73) Anthracene-d10	17.569	188	1029590	17.423	ng/ul	0.01
81) Pyrene-d10	19.792	212	1167181	19.577	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.927	264	901314	17.791	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.469	202	98571	1.330	ng/ul#	90
82) Pyrene	19.821	202	89125	1.179	ng/ul#	82
87) Chrysene	21.592	228	64523	1.059	ng/ul	98
90) Benzo(b)fluoranthene	23.315	252	97416	1.510	ng/ul#	83
93) Benzo(a)pyrene	23.980	252	64758	1.149	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015952.D
Acq On : 03 Jul 2023 15:38
Operator : MA/JU
Sample : 03239-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCFZ3

Manual IntegrationsAPPROVED

Reviewed By :Sohil Jodhani 07/04/2023
Supervised By :mohammad ahmed 07/04/2023

Quant Time: Jul 03 23:34:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

