

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015957.D
 Acq On : 03 Jul 2023 18:52
 Operator : MA/JU
 Sample : PB153766BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS766

Quant Time: Jul 03 22:10:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	266136	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	1185893	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.698	164	734240	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1617218	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.556	240	1190230	20.000	ng/u1	0.00
88) Perylene-d12	24.109	264	1164380	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	39203	5.300	ng/uL	0.00
4) Pyridine-d5	3.810	84	570867	30.615	ng/u1	0.00
7) Phenol-d5	7.222	99	772517	33.926	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.369	67	489782	34.766	ng/u1	0.00
11) 2-Chlorophenol-d4	7.575	132	600669	34.945	ng/u1	0.00
15) 4-Methylphenol-d8	8.781	113	609820	33.900	ng/u1	0.00
21) Nitrobenzene-d5	9.228	128	302501	33.378	ng/u1	0.00
24) 2-Nitrophenol-d4	9.957	143	336686	31.830	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	590601	31.333	ng/u1	0.00
31) 4-Chloroaniline-d4	11.028	131	813800	33.609	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	1756902	30.958	ng/u1	0.00
49) Acenaphthylene-d8	14.392	160	2063084	32.339	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	226154	30.198	ng/u1	0.01
60) Fluorene-d10	15.692	176	1494331	31.979	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	270107	27.158	ng/u1	0.00
73) Anthracene-d10	17.563	188	2327331	31.505	ng/u1	0.00
81) Pyrene-d10	19.792	212	2573090	33.107	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	1970230	33.544	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.404	88	83743	10.520	ng/uL	96
5) Pyridine	3.834	79	584475	29.963	ng/u1	95
6) Benzaldehyde	7.187	77	473720	51.456	ng/u1	96
8) Phenol	7.251	94	855818	36.217	ng/u1	90
10) Bis(2-Chloroethyl)ether	7.463	93	662882	35.258	ng/u1	99
12) 2-Chlorophenol	7.610	128	629985	34.497	ng/u1	99
13) 2-Methylphenol	8.510	108	631097	35.373	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.575	45	979273	38.135	ng/u1	98
16) Acetophenone	8.886	105	1019554	34.478	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.863	70	553304	33.689	ng/u1	99
18) 4-Methylphenol	8.845	108	683783	35.671	ng/u1	99
19) Hexachloroethane	9.122	117	261186	30.967	ng/u1	93
22) Nitrobenzene	9.275	77	830785	32.643	ng/u1	96
23) Isophorone	9.798	82	1571435	32.265	ng/u1	99
25) 2-Nitrophenol	9.992	139	371030	33.051	ng/u1	94
26) 2,4-Dimethylphenol	10.051	107	626580	25.390	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.275	93	942943	34.296	ng/u1	98
29) 2,4-Dichlorophenol	10.539	162	616392	32.892	ng/u1	100
30) Naphthalene	10.922	128	2055168	31.879	ng/u1	99
32) 4-Chloroaniline	11.057	127	742194	29.502	ng/u1	99
33) Hexachlorobutadiene	11.186	225	371331	26.239	ng/u1	100
34) Caprolactam	11.869	113	223285	38.953	ng/u1	92
35) 4-Chloro-3-methylphenol	12.192	107	718406	32.751	ng/u1	97
36) 2-Methylnaphthalene	12.527	142	1372845	32.349	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015957.D
 Acq On : 03 Jul 2023 18:52
 Operator : MA/JU
 Sample : PB153766BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS766

Quant Time: Jul 03 22:10:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.745	142	1367414	31.585	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.898	216	725819	29.998	ng/ul	99
40) Hexachlorocyclopentadiene	12.851	237	75495	10.430	ng/ul	98
41) 2,4,6-Trichlorophenol	13.151	196	483613	31.627	ng/ul	98
42) 2,4,5-Trichlorophenol	13.239	196	549781	33.897	ng/ul	99
43) 1,1'-Biphenyl	13.527	154	1821805	31.326	ng/ul	97
44) 2-Chloronaphthalene	13.580	162	1442822	31.493	ng/ul	98
45) 2-Nitroaniline	13.810	65	525628	36.463	ng/ul	94
47) Dimethylphthalate	14.157	163	1827183	31.110	ng/ul	99
48) 2,6-Dinitrotoluene	14.298	165	400769	33.640	ng/ul	96
50) Acenaphthylene	14.422	152	2281523	32.457	ng/ul	99
51) 3-Nitroaniline	14.645	138	417780	44.718	ng/ul	98
52) Acenaphthene	14.763	153	1554555	31.892	ng/ul	99
53) 2,4-Dinitrophenol	14.880	184	163318	25.839	ng/ul	86
55) 4-Nitrophenol	14.974	109	188143	24.243	ng/ul#	77
56) Dibenzofuran	15.098	168	2162516	31.958	ng/ul	97
57) 2,4-Dinitrotoluene	15.104	165	564221	34.753	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.345	232	438833	31.500	ng/ul	98
59) Diethylphthalate	15.510	149	1876493	31.572	ng/ul	99
61) Fluorene	15.751	166	1780496	32.440	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.733	204	858712	30.576	ng/ul	97
63) 4-Nitroaniline	15.816	138	389706	60.947	ng/ul	85
66) 4,6-Dinitro-2-methylph...	15.874	198	276069	27.434	ng/ul	99
67) N-Nitrosodiphenylamine	15.957	169	1512686	31.245	ng/ul	99
68) 4-Bromophenyl-phenylether	16.633	248	545600	29.544	ng/ul	93
69) Hexachlorobenzene	16.763	284	632533	29.028	ng/ul	97
70) Atrazine	16.916	200	445298	24.028	ng/ul	99
71) Pentachlorophenol	17.127	266	303469	29.017	ng/ul	97
72) Phenanthrene	17.504	178	2837588	32.298	ng/ul	100
74) Anthracene	17.598	178	2841127	32.183	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.504	216	744351	28.286	ng/uL	98
76) Pentachlorobenzene	15.021	250	1656510	62.371	ng/uL	100
77) Carbazole	17.880	167	2662067	35.777	ng/ul	99
78) Di-n-butylphthalate	18.392	149	3439520	34.868	ng/ul	99
80) Fluoranthene	19.468	202	3241769	33.562	ng/ul#	94
82) Pyrene	19.821	202	3257185	33.058	ng/ul#	89
83) Butylbenzylphthalate	20.668	149	1580146	39.310	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.468	252	903619	33.584	ng/ul	100
85) Benzo(a)anthracene	21.539	228	2750014	32.845	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.415	149	2262815	40.961	ng/ul	99
87) Chrysene	21.592	228	2592353	32.634	ng/ul	99
89) Di-n-octyl phthalate	22.374	149	3728082	43.811	ng/ul	100
90) Benzo(b)fluoranthene	23.315	252	2477500	33.114	ng/ul	98
91) Benzo(k)fluoranthene	23.368	252	2544349	33.659	ng/ul#	97
93) Benzo(a)pyrene	23.992	252	2197008	33.607	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	26.809	276	2829805	31.886	ng/ul#	92
95) Dibenzo(a,h)anthracene	26.809	278	2347197	32.200	ng/ul#	95
96) Benzo(g,h,i)perylene	27.650	276	2306821	31.596	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015957.D
Acq On : 03 Jul 2023 18:52
Operator : MA/JU
Sample : PB153766BS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS766

Quant Time: Jul 03 22:10:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration




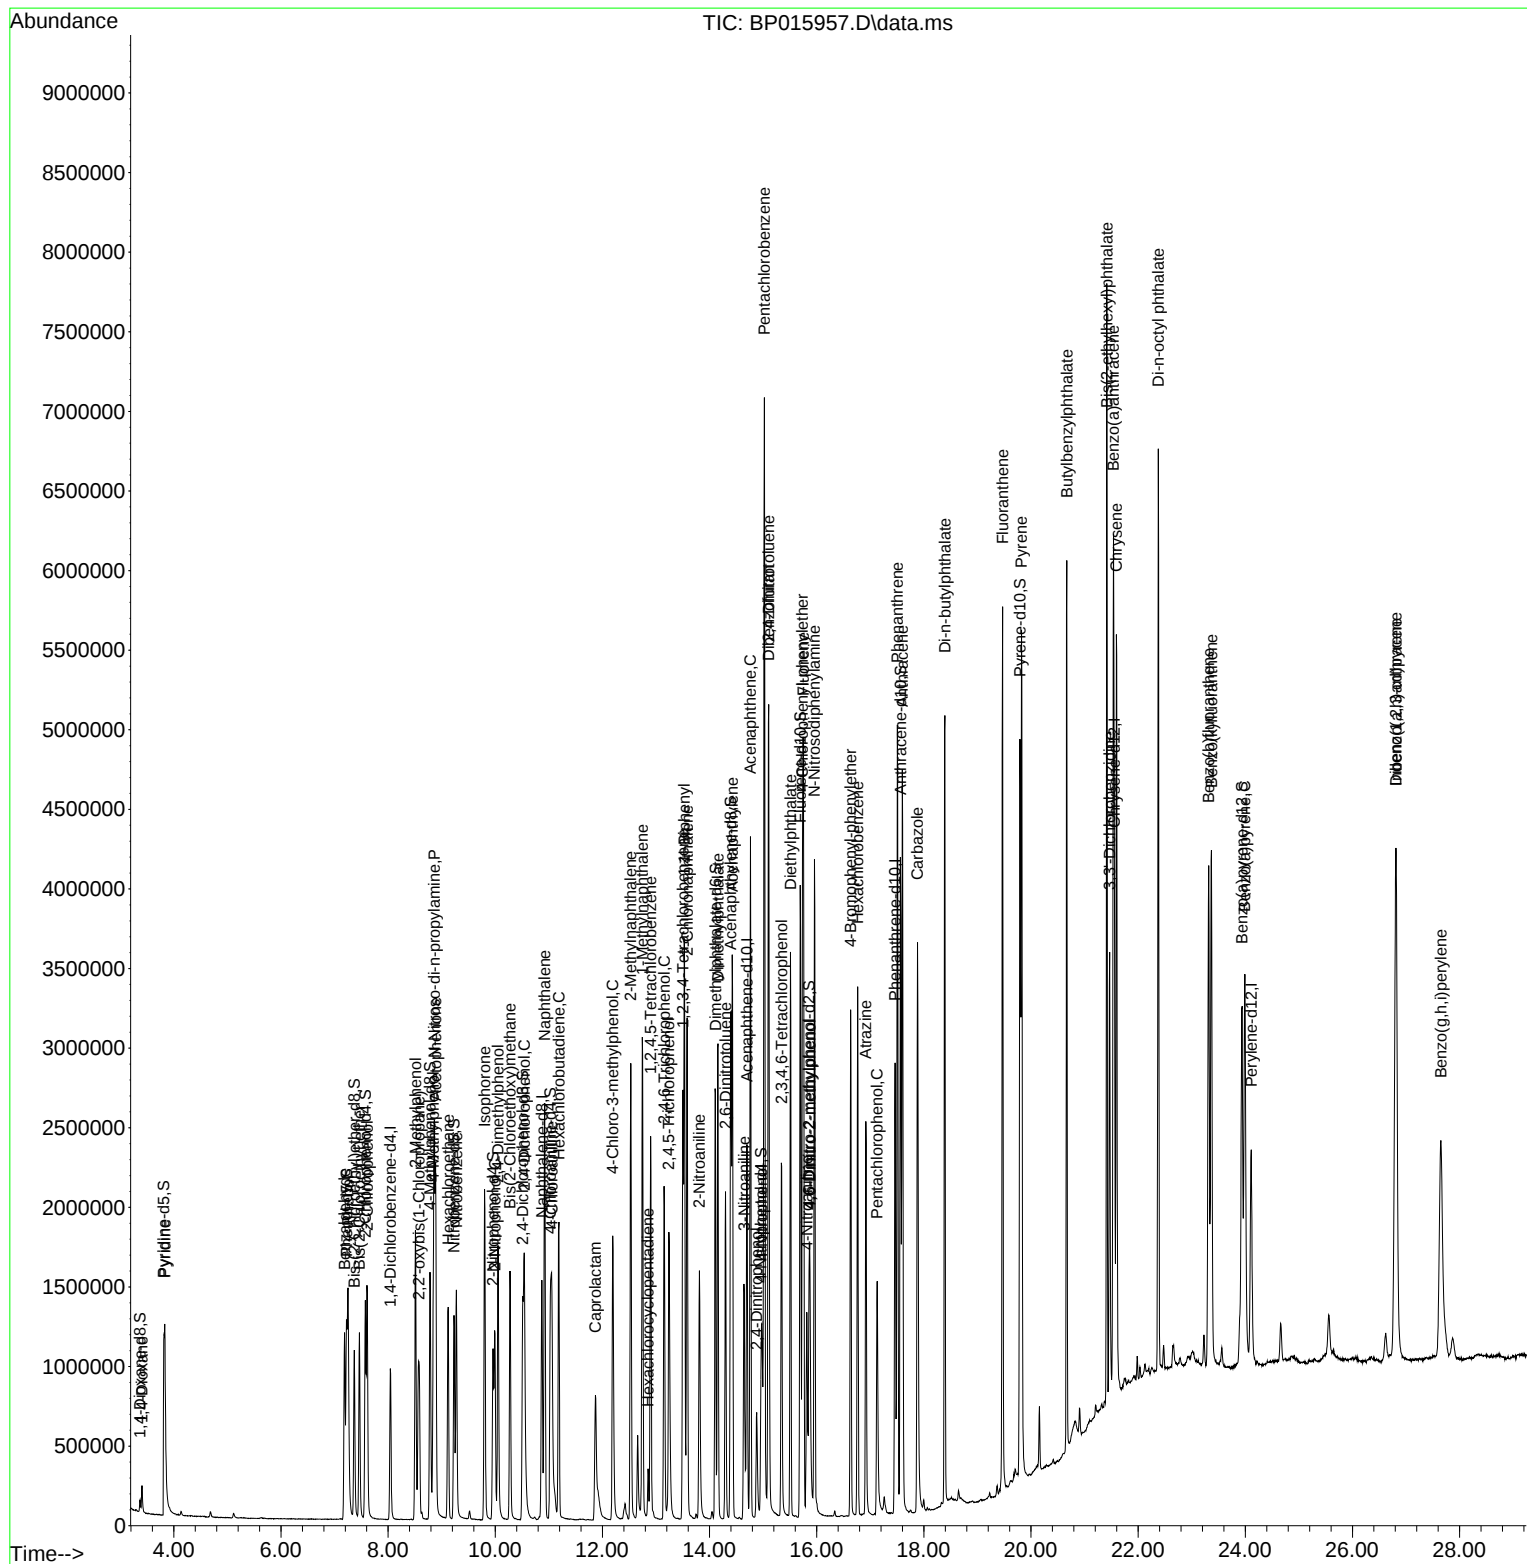




#2
1,4-Dioxane
Concen: 10.520 ng/uL
RT: 3.404 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion: 88 Resp: 83743
Ion Ratio Lower Upper
88 100
43 32.7 27.4 41.2
58 78.7 59.8 89.8

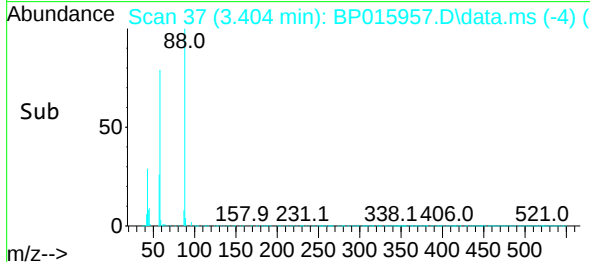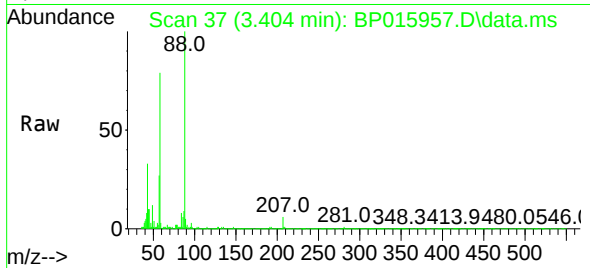

#5
Pyridine
Concen: 29.963 ng/uL
RT: 3.834 min Scan# 110
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion: 79 Resp: 584475
Ion Ratio Lower Upper
79 100
52 77.0 65.5 98.3
51 37.0 31.8 47.8


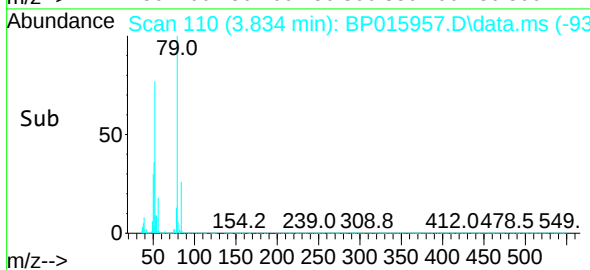






#6
Benzaldehyde
Concen: 51.456 ng/ul
RT: 7.187 min Scan# 681
Delta R.T. -0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion: 77 Resp: 473720
Ion Ratio Lower Upper
77 100
105 94.0 73.4 110.0
106 88.2 66.6 100.0



#8
Phenol
Concen: 36.217 ng/ul
RT: 7.251 min Scan# 691
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion: 94 Resp: 855818
Ion Ratio Lower Upper
94 100
65 29.2 26.4 39.6
66 38.4 37.3 55.9

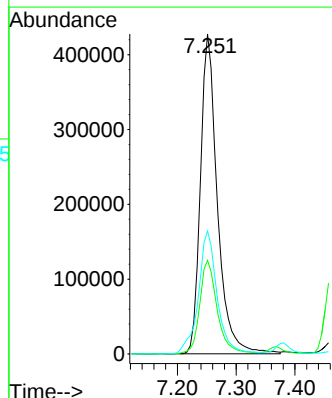







#10
 Bis(2-Chloroethyl)ether
 Concen: 35.258 ng/ul
 RT: 7.463 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52

Instrument :
 BNA_P
 ClientSampleId :
 SLCS766

Tgt Ion: 93 Resp: 662882




Ion	Ratio	Lower	Upper
93	100		
63	78.2	62.8	94.2
95	32.5	25.6	38.4




#12
 2-Chlorophenol
 Concen: 34.497 ng/ul
 RT: 7.610 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52

Tgt Ion: 128 Resp: 629985

Ion	Ratio	Lower	Upper
128	100		
64	52.4	41.2	61.8
130	32.7	26.0	39.0









#13
2-Methylphenol
Concen: 35.373 ng/ul
RT: 8.510 min Scan# 905
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:108 Resp: 631097
Ion Ratio Lower Upper
108 100
107 90.0 73.8 110.6

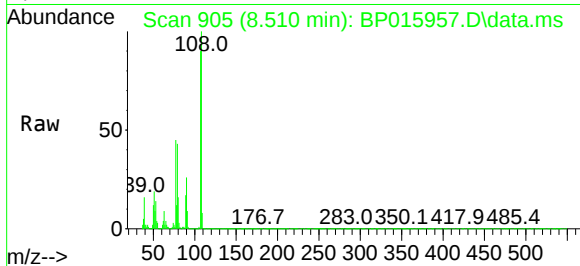

#14
2,2'-oxybis(1-Chloropropane)
Concen: 38.135 ng/ul
RT: 8.575 min Scan# 916
Delta R.T. -0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion: 45 Resp: 979273
Ion Ratio Lower Upper
45 100
77 14.2 12.4 18.6
79 11.1 9.3 13.9




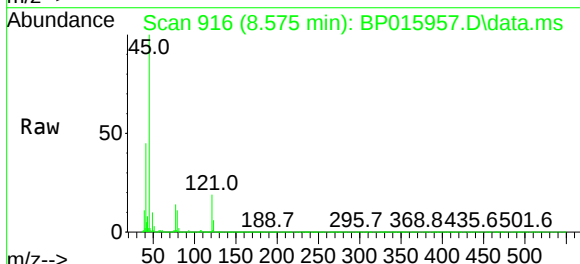




#16
Acetophenone
Concen: 34.478 ng/ul
RT: 8.886 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:105 Resp: 1019554
Ion Ratio Lower Upper
105 100
77 83.3 65.0 97.4
51 30.5 25.1 37.7



#17
N-Nitroso-di-n-propylamine
Concen: 33.689 ng/ul
RT: 8.863 min Scan# 965
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52


Tgt Ion: 70 Resp: 553304
Ion Ratio Lower Upper
70 100
42 59.7 48.2 72.2
101 9.3 7.6 11.4
130 18.3 13.9 20.9

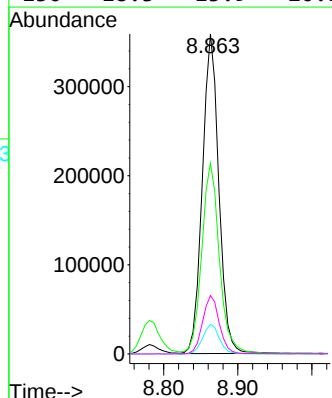






#18
4-Methylphenol
Concen: 35.671 ng/ul
RT: 8.845 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Instrument :
BNA_P
ClientSampleId :
SLCS766







Tgt Ion:108 Resp: 683783
Ion Ratio Lower Upper
108 100
107 112.7 91.3 136.9



#19
Hexachloroethane
Concen: 30.967 ng/ul
RT: 9.122 min Scan# 1009
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:117 Resp: 261186
Ion Ratio Lower Upper
117 100
201 96.6 84.2 126.2
199 60.2 51.8 77.8









#22
Nitrobenzene
Concen: 32.643 ng/ul
RT: 9.275 min Scan# 1035
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion: 77 Resp: 830785
Ion Ratio Lower Upper
77 100
123 41.2 31.0 46.4
65 13.3 11.3 16.9



#23
Isophorone
Concen: 32.265 ng/ul
RT: 9.798 min Scan# 1124
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion: 82 Resp: 1571435
Ion Ratio Lower Upper
82 100
95 6.9 6.3 9.5
138 15.5 12.3 18.5



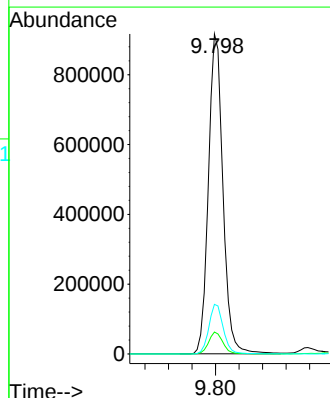





#25
2-Nitrophenol
Concen: 33.051 ng/ul
RT: 9.992 min Scan# 1157
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:139 Resp: 371030
Ion Ratio Lower Upper
139 100
65 59.0 50.2 75.2
109 33.7 31.3 46.9



#26
2,4-Dimethylphenol
Concen: 25.390 ng/ul
RT: 10.051 min Scan# 1167
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:107 Resp: 626580
Ion Ratio Lower Upper
107 100
121 49.0 38.2 57.2
122 81.3 62.1 93.1









#27
 Bis(2-Chloroethoxy)methane
 Concen: 34.296 ng/ul
 RT: 10.275 min Scan# 1205
 Delta R.T. -0.000 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52




Instrument :
 BNA_P
 ClientSampleId :
 SLCS766


Tgt Ion: 93 Resp: 942943
 Ion Ratio Lower Upper
 93 100
 95 31.9 26.6 39.8
 123 10.6 8.6 13.0

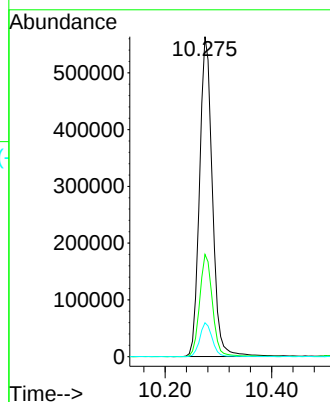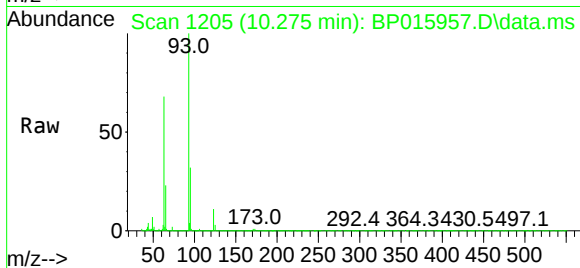

#29
 2,4-Dichlorophenol
 Concen: 32.892 ng/ul
 RT: 10.539 min Scan# 1250
 Delta R.T. -0.000 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52

Tgt Ion: 162 Resp: 616392
 Ion Ratio Lower Upper
 162 100
 164 66.1 53.0 79.6
 98 39.5 31.3 46.9


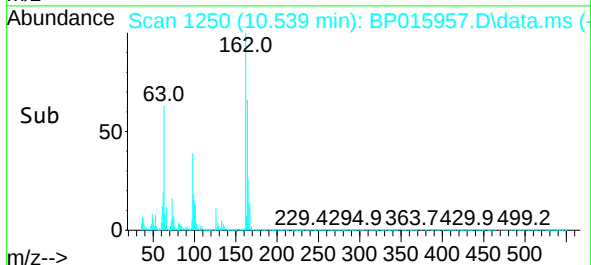

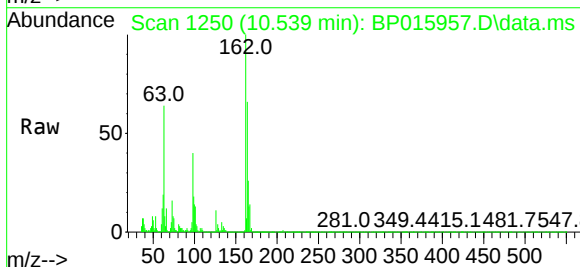




#30
Naphthalene
Concen: 31.879 ng/ul
RT: 10.922 min Scan# 1315
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:128 Resp: 2055168
Ion Ratio Lower Upper
128 100
129 10.9 8.6 12.8
127 13.2 10.3 15.5

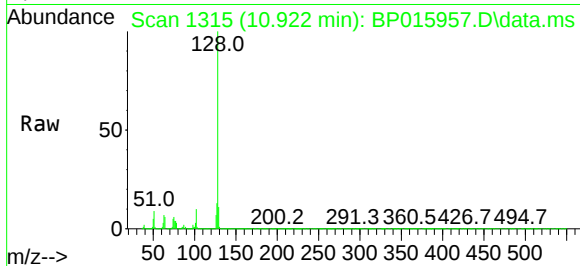

#32
4-Chloroaniline
Concen: 29.502 ng/ul
RT: 11.057 min Scan# 1338
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:127 Resp: 742194
Ion Ratio Lower Upper
127 100
129 31.6 24.7 37.1




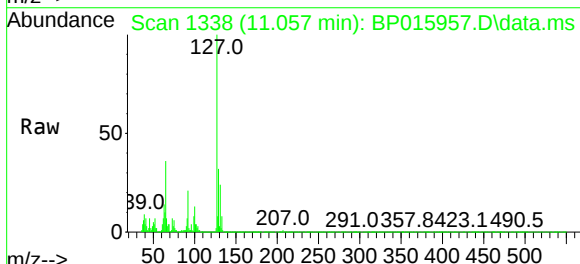




#33
Hexachlorobutadiene
Concen: 26.239 ng/ul
RT: 11.186 min Scan# 1359
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:225 Resp: 371331
Ion Ratio Lower Upper
225 100
223 63.0 50.4 75.6
227 64.2 51.0 76.4

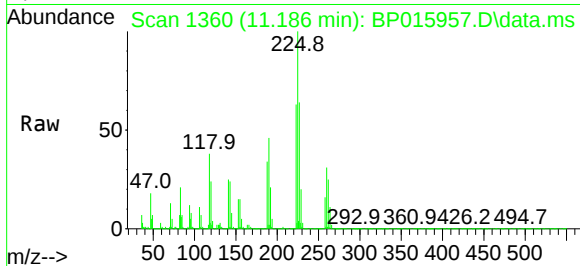

#34
Caprolactam
Concen: 38.953 ng/ul
RT: 11.869 min Scan# 1476
Delta R.T. 0.012 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:113 Resp: 223285
Ion Ratio Lower Upper
113 100
55 187.6 142.8 214.2
56 134.7 116.9 175.3




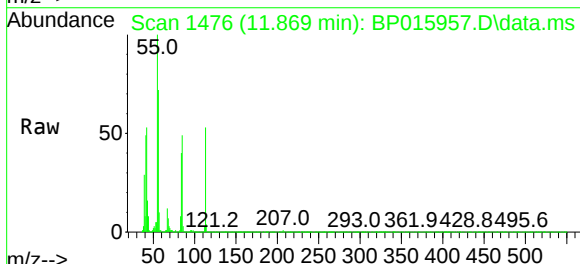




#35
4-Chloro-3-methylphenol
Concen: 32.751 ng/ul
RT: 12.192 min Scan# 1531
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:107 Resp: 718406
Ion Ratio Lower Upper
107 100
144 24.5 18.4 27.6
142 75.9 58.6 87.8

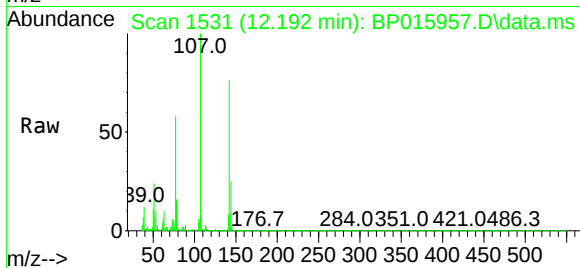

#36
2-Methylnaphthalene
Concen: 32.349 ng/ul
RT: 12.527 min Scan# 1588
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:142 Resp: 1372845
Ion Ratio Lower Upper
142 100
141 87.8 73.2 109.8

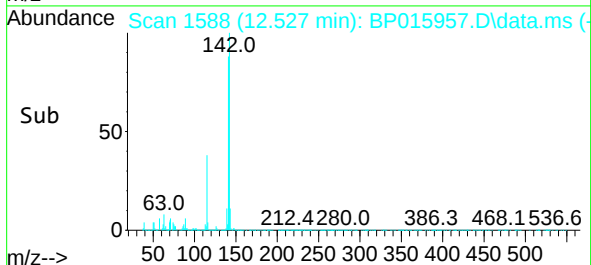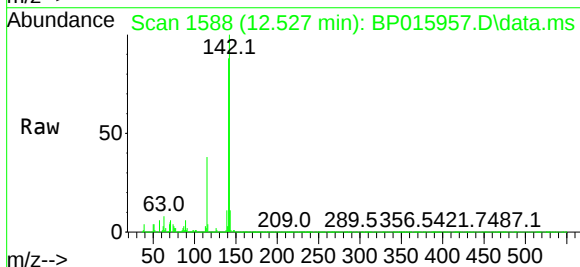



#37

1-Methylnaphthalene

Concen: 31.585 ng/ul

RT: 12.745 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:142 Resp: 1367414

Ion Ratio Lower Upper

142 100

141 92.4 73.1 109.7

116 4.3 4.0 6.0

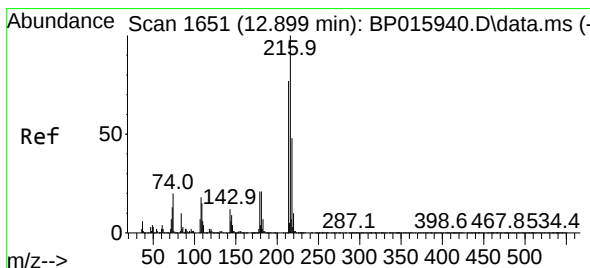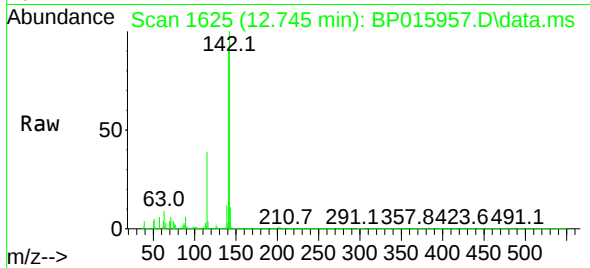

#39

1,2,4,5-Tetrachlorobenzene

Concen: 29.998 ng/ul

RT: 12.898 min Scan# 1651

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Tgt Ion:216 Resp: 725819




Ion Ratio Lower Upper


216 100

214 79.1 62.4 93.6

179 21.9 17.6 26.4

108 19.9 15.5 23.3


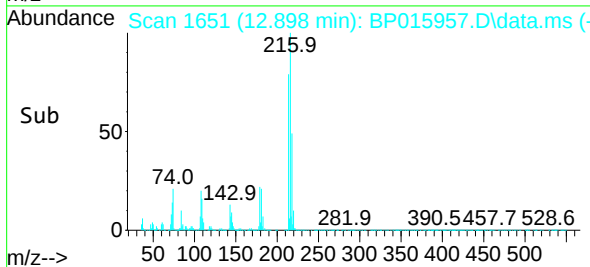
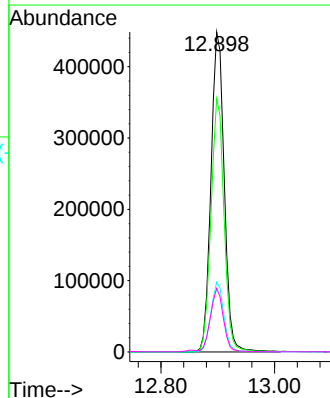
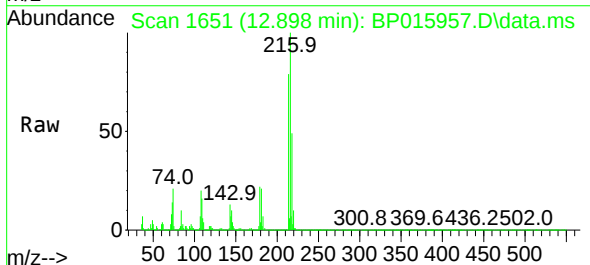




#40
Hexachlorocyclopentadiene
Concen: 10.430 ng/ul
RT: 12.851 min Scan# 1643
Delta R.T. -0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:237 Resp: 75495
Ion Ratio Lower Upper
237 100
235 62.2 48.6 73.0
272 12.7 10.5 15.7

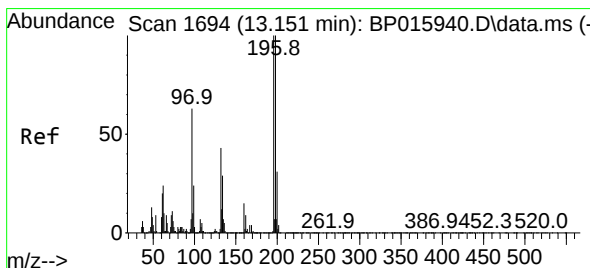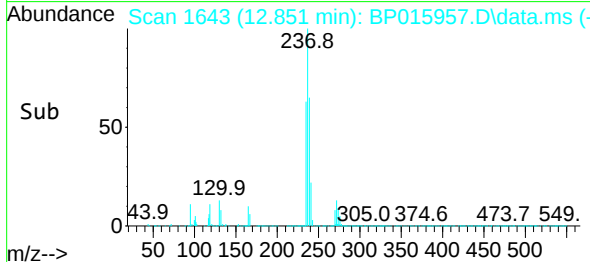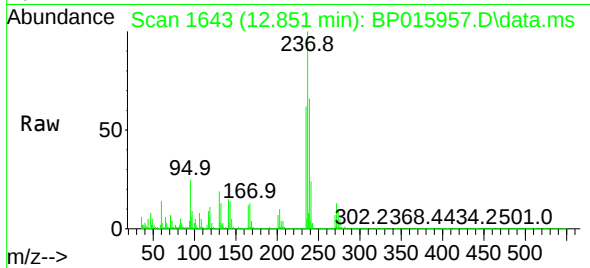

#41
2,4,6-Trichlorophenol
Concen: 31.627 ng/ul
RT: 13.151 min Scan# 1694
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:196 Resp: 483613
Ion Ratio Lower Upper
196 100
198 96.7 75.4 113.2
200 30.8 23.6 35.4


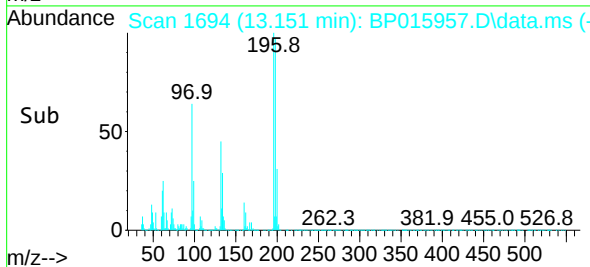

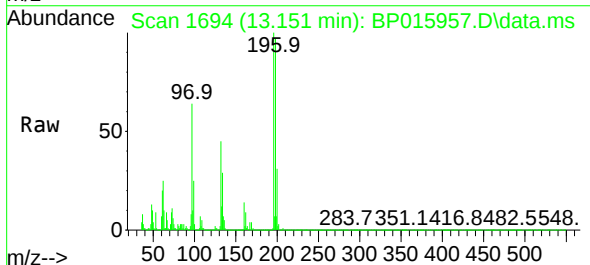




#42
2,4,5-Trichlorophenol
Concen: 33.897 ng/ul
RT: 13.239 min Scan# 1710
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:196 Resp: 549781
Ion Ratio Lower Upper
196 100
198 94.7 74.9 112.3
200 30.1 24.3 36.5



#43
1,1'-Biphenyl
Concen: 31.326 ng/ul
RT: 13.527 min Scan# 1758
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:154 Resp: 1821805
Ion Ratio Lower Upper
154 100
153 40.2 32.8 49.2
76 16.0 10.7 16.1

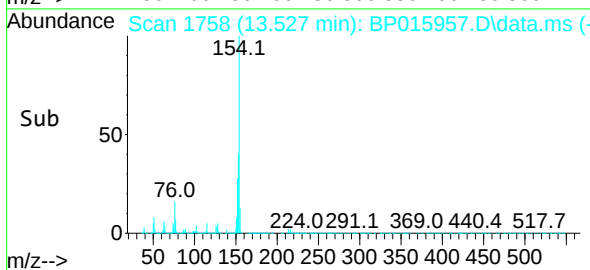



#44

2-Chloronaphthalene

Concen: 31.493 ng/ul

RT: 13.580 min Scan# 11

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:162 Resp: 1442822

Ion Ratio Lower Upper

162 100

164 33.2 26.1 39.1

127 39.9 33.4 50.0

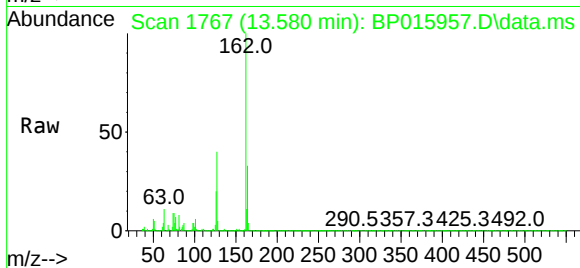

#45

2-Nitroaniline

Concen: 36.463 ng/ul

RT: 13.810 min Scan# 1806

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion: 65 Resp: 525628


Ion Ratio Lower Upper

65 100

92 66.3 49.5 74.3

138 94.6 71.4 107.2

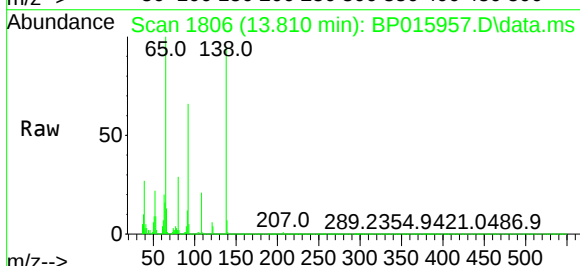



#47

Dimethylphthalate

Concen: 31.110 ng/ul

RT: 14.157 min Scan# 1865

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:163 Resp: 1827183

Ion Ratio Lower Upper

163 100

194 3.8 3.1 4.7

164 9.9 7.7 11.5



#48

2,6-Dinitrotoluene

Concen: 33.640 ng/ul

RT: 14.298 min Scan# 1889

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:165 Resp: 400769


Ion Ratio Lower Upper

165 100

89 63.4 54.1 81.1

121 21.8 18.2 27.2





#50

Acenaphthylene

Concen: 32.457 ng/ul

RT: 14.422 min Scan# 1910

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:152 Resp: 2281523

Ion Ratio Lower Upper

152 100

151 19.7 16.2 24.2

153 13.1 10.5 15.7

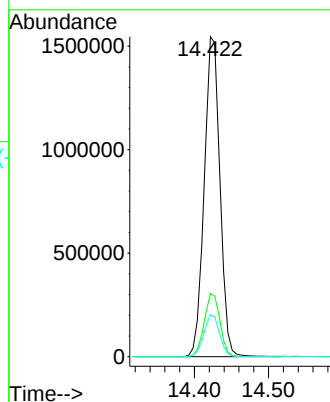

#51

3-Nitroaniline

Concen: 44.718 ng/ul

RT: 14.645 min Scan# 1948

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:138 Resp: 417780


Ion Ratio Lower Upper

138 100

108 10.9 9.1 13.7

92 123.4 96.8 145.2


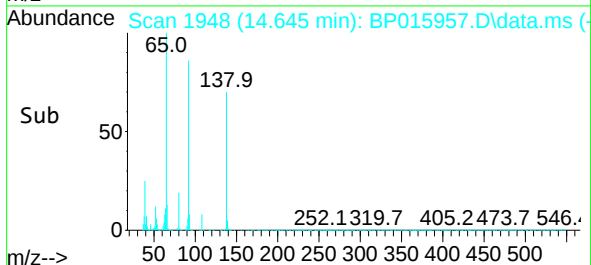

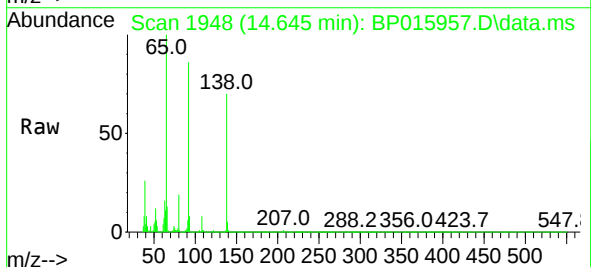




#52
Acenaphthene
Concen: 31.892 ng/ul
RT: 14.763 min Scan# 1967
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:153 Resp: 1554555
Ion Ratio Lower Upper
153 100
152 48.3 39.4 59.2
154 88.1 71.4 107.2



#53
2,4-Dinitrophenol
Concen: 25.839 ng/ul
RT: 14.880 min Scan# 1988
Delta R.T. 0.012 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:184 Resp: 163318
Ion Ratio Lower Upper
184 100
63 76.0 71.4 107.0
154 64.0 61.1 91.7









#55
4-Nitrophenol
Concen: 24.243 ng/ul
RT: 14.974 min Scan# 2010
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:109 Resp: 188143
Ion Ratio Lower Upper
109 100
139 126.5 81.3 121.9#
65 149.9 99.9 149.9



#56
Dibenzofuran
Concen: 31.958 ng/ul
RT: 15.098 min Scan# 2025
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:168 Resp: 2162516
Ion Ratio Lower Upper
168 100
139 38.7 32.2 48.4









#57
2,4-Dinitrotoluene
Concen: 34.753 ng/ul
RT: 15.104 min Scan# 2026
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:165 Resp: 564221
Ion Ratio Lower Upper
165 100
63 71.9 56.8 85.2
182 2.8 2.0 3.0



#58
2,3,4,6-Tetrachlorophenol
Concen: 31.500 ng/ul
RT: 15.345 min Scan# 2067
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:232 Resp: 438833
Ion Ratio Lower Upper
232 100
131 45.8 38.2 57.2
130 2.5 2.2 3.2
166 31.4 25.6 38.4


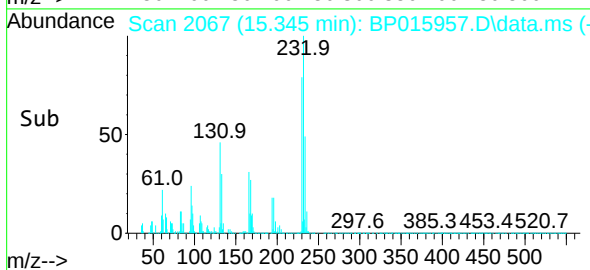






#59
Diethylphthalate
Concen: 31.572 ng/ul
RT: 15.510 min Scan# 2095
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:149 Resp: 1876493
Ion Ratio Lower Upper
149 100
177 21.4 16.8 25.2
150 12.6 10.3 15.5

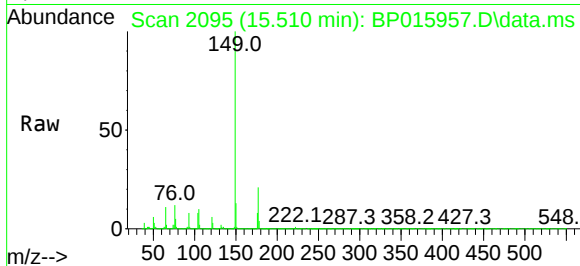

#61
Fluorene
Concen: 32.440 ng/ul
RT: 15.751 min Scan# 2136
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:166 Resp: 1780496
Ion Ratio Lower Upper
166 100
165 97.6 78.7 118.1
167 13.3 10.5 15.7




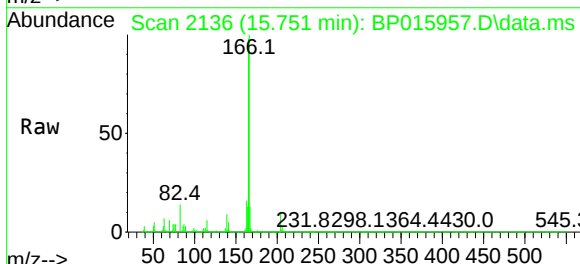




#62
4-Chlorophenyl-phenylether
Concen: 30.576 ng/ul
RT: 15.733 min Scan# 2133
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:204 Resp: 858712
Ion Ratio Lower Upper
204 100
206 32.7 26.0 39.0
141 61.1 51.8 77.8



#63
4-Nitroaniline
Concen: 60.947 ng/ul
RT: 15.816 min Scan# 2147
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:138 Resp: 389706
Ion Ratio Lower Upper
138 100
92 56.4 50.1 75.1
108 87.8 85.5 128.3









#66
4,6-Dinitro-2-methylphenol
Concen: 27.434 ng/ul
RT: 15.874 min Scan# 2157
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:198 Resp: 276069
Ion Ratio Lower Upper
198 100
182 4.5 3.4 5.2
77 30.1 24.4 36.6



#67
N-Nitrosodiphenylamine
Concen: 31.245 ng/ul
RT: 15.957 min Scan# 2171
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:169 Resp: 1512686
Ion Ratio Lower Upper
169 100
168 66.7 54.2 81.4
167 36.2 29.7 44.5


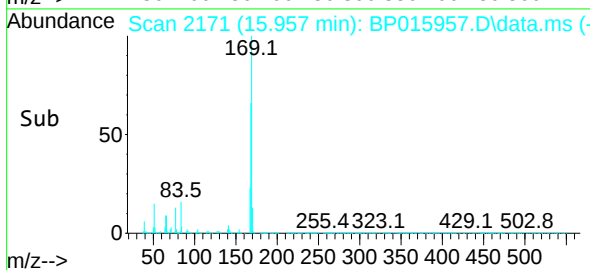




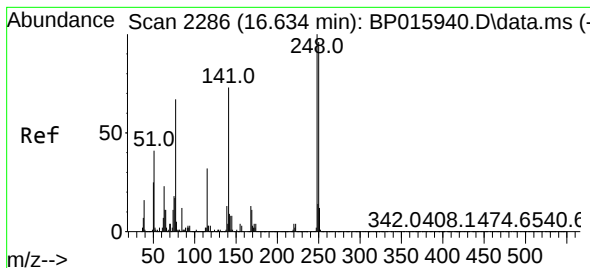

#68
4-Bromophenyl-phenylether
Concen: 29.544 ng/ul
RT: 16.633 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:248 Resp: 545600
Ion Ratio Lower Upper
248 100
250 97.9 84.6 126.8
141 78.9 67.8 101.6

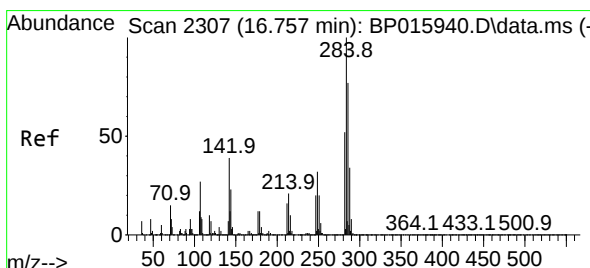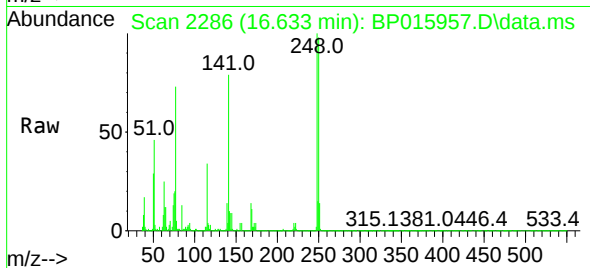

#69
Hexachlorobenzene
Concen: 29.028 ng/ul
RT: 16.763 min Scan# 2308
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:284 Resp: 632533
Ion Ratio Lower Upper
284 100
142 37.5 27.8 41.8
249 32.1 26.1 39.1

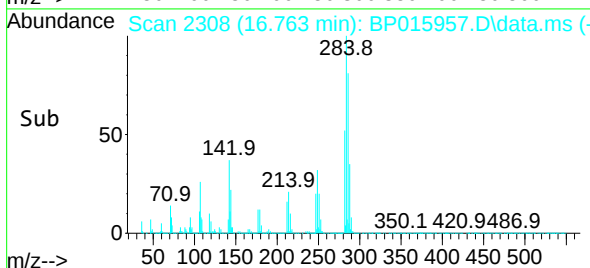



#70

Atrazine

Concen: 24.028 ng/ul

RT: 16.916 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:200 Resp: 445298

Ion Ratio Lower Upper

200 100

173 26.3 19.8 29.8

215 46.2 36.8 55.2

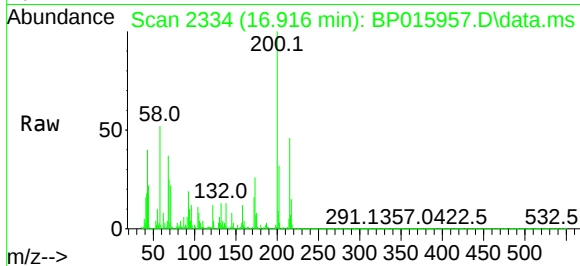

#71

Pentachlorophenol

Concen: 29.017 ng/ul

RT: 17.127 min Scan# 2370

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:266 Resp: 303469


Ion Ratio Lower Upper

266 100

264 63.2 53.4 80.2

268 64.6 51.4 77.2

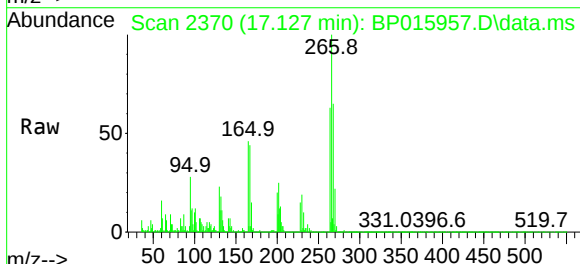



#72

Phenanthrene

Concen: 32.298 ng/ul

RT: 17.504 min Scan# 2433

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:178 Resp: 2837588

Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6

176 19.7 15.6 23.4

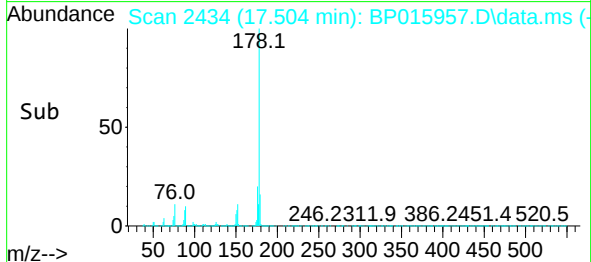

#74

Anthracene

Concen: 32.183 ng/ul

RT: 17.598 min Scan# 2450

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:178 Resp: 2841127


Ion Ratio Lower Upper

178 100

179 15.6 12.1 18.1

176 18.4 14.6 22.0

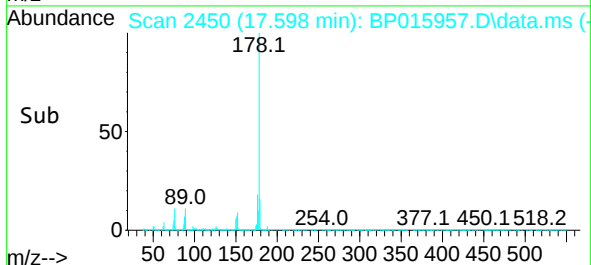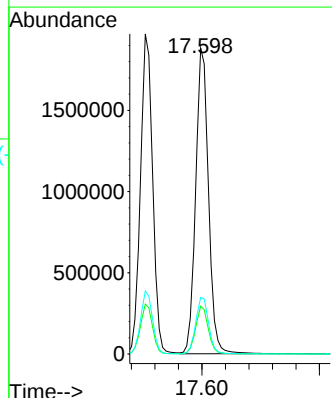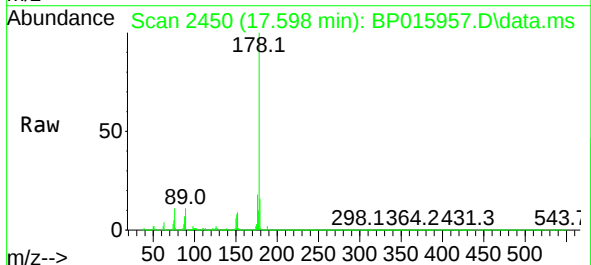



#75

1,2,3,4-Tetrachlorobenzene

Concen: 28.286 ng/uL

RT: 13.504 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:216 Resp: 744351

Ion Ratio Lower Upper

216 100

214 79.2 62.0 93.0

218 49.5 38.4 57.6

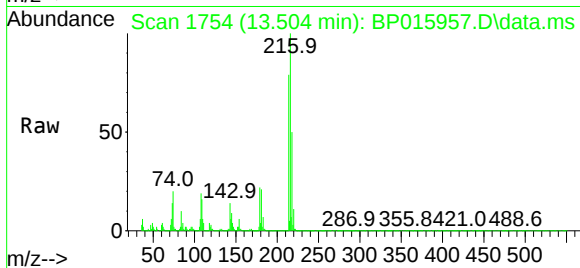

#76

Pentachlorobenzene

Concen: 62.371 ng/uL

RT: 15.021 min Scan# 2012

Delta R.T. -0.000 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:250 Resp: 1656510


Ion Ratio Lower Upper

250 100

248 63.9 50.7 76.1

252 63.8 51.2 76.8

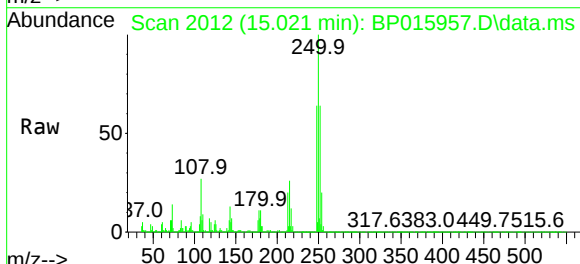



#77

Carbazole

Concen: 35.777 ng/ul

RT: 17.880 min Scan# 2498

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:167 Resp: 2662067

Ion Ratio Lower Upper

167 100

166 21.6 17.4 26.0

139 13.3 11.0 16.4

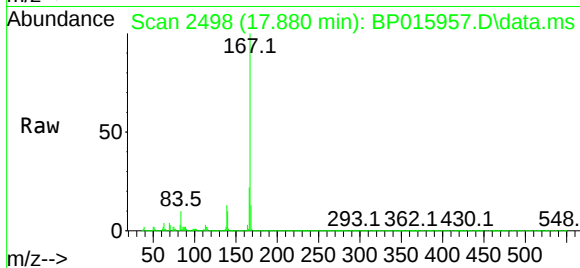

#78

Di-n-butylphthalate

Concen: 34.868 ng/ul

RT: 18.392 min Scan# 2585

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:149 Resp: 3439520


Ion Ratio Lower Upper

149 100

150 9.1 7.5 11.3

104 5.5 4.6 7.0


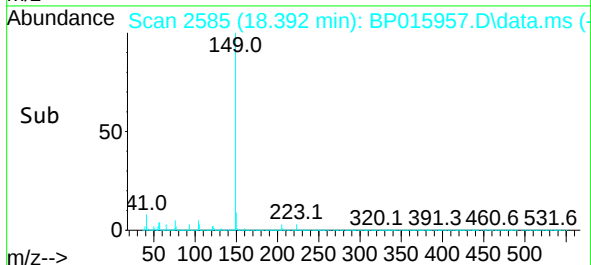
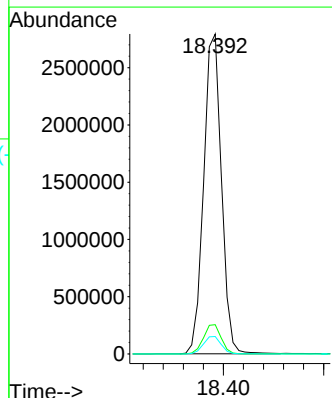
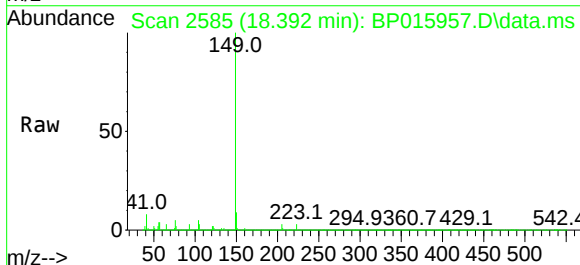




#80
Fluoranthene
Concen: 33.562 ng/u1
RT: 19.468 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:202 Resp: 3241769
Ion Ratio Lower Upper
202 100
101 12.9 8.3 12.5#
100 9.9 6.6 9.8#

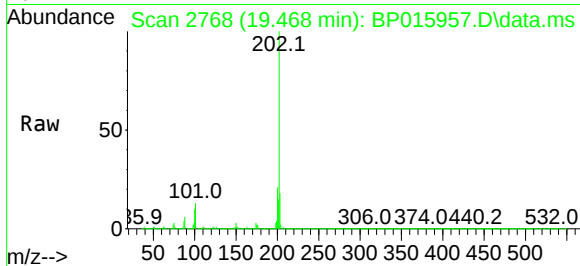

#82
Pyrene
Concen: 33.058 ng/u1
RT: 19.821 min Scan# 2828
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:202 Resp: 3257185
Ion Ratio Lower Upper
202 100
101 15.7 9.3 13.9#
100 13.3 7.6 11.4#

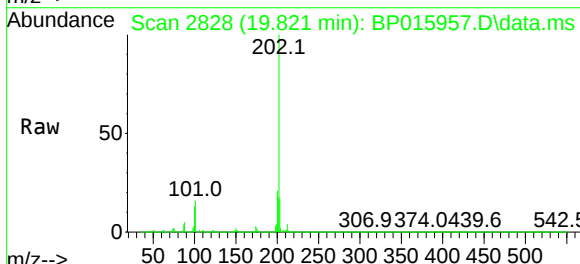



#83

Butylbenzylphthalate

Concen: 39.310 ng/ul

RT: 20.668 min Scan# 2971

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:149 Resp: 1580146

Ion Ratio Lower Upper

149 100

91 76.5 59.8 89.6

206 20.5 16.4 24.6

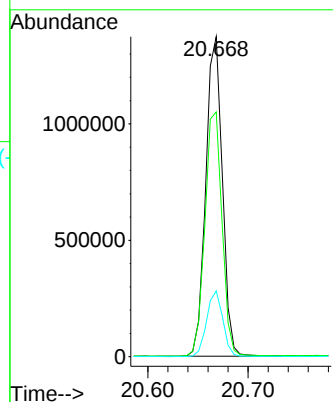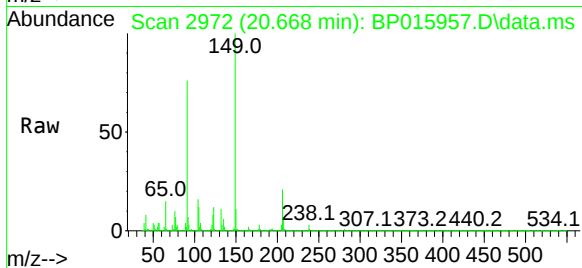

#84

3,3'-Dichlorobenzidine

Concen: 33.584 ng/ul

RT: 21.468 min Scan# 3108

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:252 Resp: 903619


Ion Ratio Lower Upper

252 100

254 63.8 51.0 76.6

126 11.9 8.6 13.0

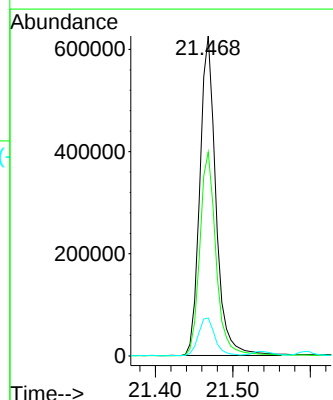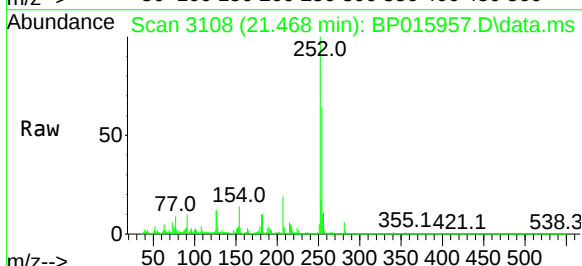



#85

Benzo(a)anthracene

Concen: 32.845 ng/ul

RT: 21.539 min Scan# 3119

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:228 Resp: 2750014

Ion Ratio Lower Upper

228 100

229 19.8 15.3 22.9

226 27.9 21.4 32.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 40.961 ng/ul

RT: 21.415 min Scan# 3099

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:149 Resp: 2262815


Ion Ratio Lower Upper

149 100

167 26.8 21.0 31.6

279 4.1 3.8 5.6





#87

Chrysene

Concen: 32.634 ng/ul

RT: 21.592 min Scan# 3129

Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:228 Resp: 2592353

Ion Ratio Lower Upper

228 100

226 30.2 24.3 36.5

229 19.8 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 43.811 ng/ul




RT: 22.374 min Scan# 3262


Delta R.T. 0.006 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Tgt Ion:149 Resp: 3728082



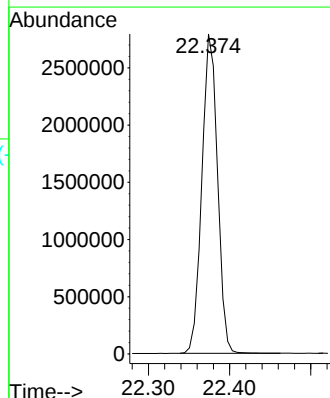





#90
Benzo(b)fluoranthene
Concen: 33.114 ng/ul
RT: 23.315 min Scan# 3422
Delta R.T. 0.006 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52




Instrument :
BNA_P
ClientSampleId :
SLCS766


Tgt Ion:252 Resp: 2477500
Ion Ratio Lower Upper
252 100
253 22.1 17.3 25.9
125 11.2 7.5 11.3



#91
Benzo(k)fluoranthene
Concen: 33.659 ng/ul
RT: 23.368 min Scan# 3431
Delta R.T. 0.012 min
Lab File: BP015957.D
Acq: 03 Jul 2023 18:52

Tgt Ion:252 Resp: 2544349
Ion Ratio Lower Upper
252 100
253 21.9 17.0 25.4
125 11.1 7.3 10.9#





#93

Benzo(a)pyrene

Concen: 33.607 ng/ul

RT: 23.992 min Scan# 3

Delta R.T. 0.012 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52

Instrument :

BNA_P

ClientSampleId :

SLCS766





Tgt Ion:252 Resp: 2197008

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 12.3 8.2 12.2#

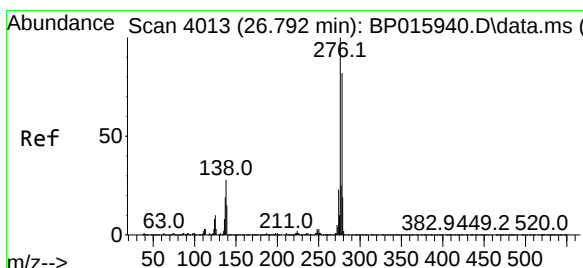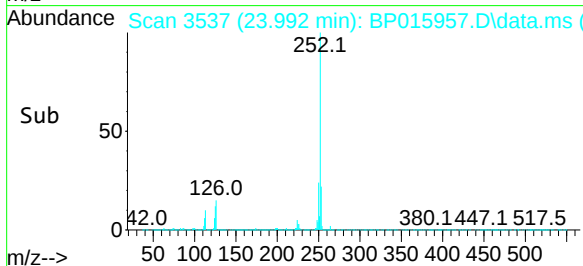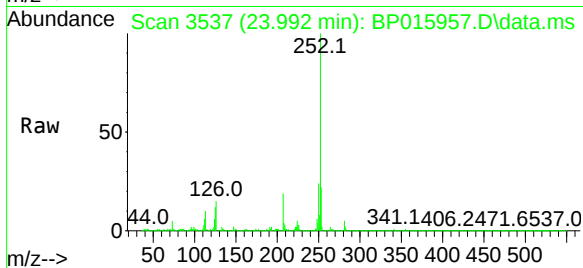

#94

Indeno(1,2,3-cd)pyrene

Concen: 31.886 ng/ul

RT: 26.809 min Scan# 4016

Delta R.T. 0.018 min

Lab File: BP015957.D

Acq: 03 Jul 2023 18:52




Tgt Ion:276 Resp: 2829805


Ion Ratio Lower Upper

276 100

138 27.2 15.7 23.5#

277 25.1 19.6 29.4


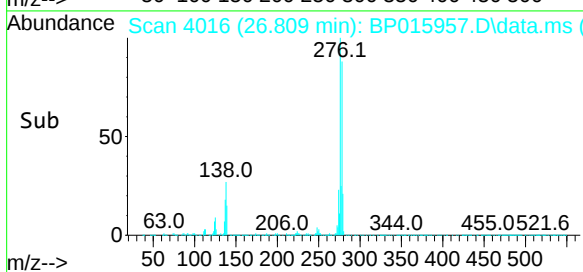

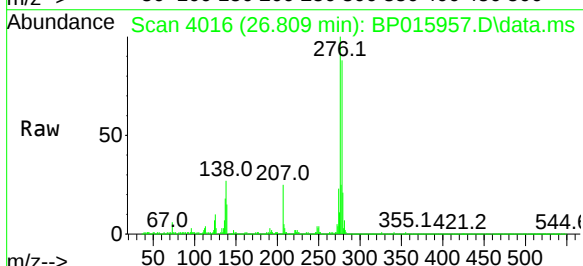




#95
 Dibenzo(a,h)anthracene
 Concen: 32.200 ng/ul
 RT: 26.809 min Scan# 4014
 Delta R.T. 0.012 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52

Instrument :
 BNA_P
 ClientSampleId :
 SLCS766

Tgt Ion:278 Resp: 2347197
 Ion Ratio Lower Upper
 278 100
 139 17.6 10.5 15.7#
 279 23.9 18.4 27.6



#96
 Benzo(g,h,i)perylene
 Concen: 31.596 ng/ul
 RT: 27.650 min Scan# 4159
 Delta R.T. 0.023 min
 Lab File: BP015957.D
 Acq: 03 Jul 2023 18:52

Tgt Ion:276 Resp: 2306821
 Ion Ratio Lower Upper
 276 100
 138 24.0 15.1 22.7#
 277 24.3 18.8 28.2

