

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
 Data File : BP015942.D
 Acq On : 03 Jul 2023 09:57
 Operator : MA/JU
 Sample : PB153768BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK768

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	42	rVB	68219	110828	2.05%	0.195%
2	3.816	105	107	133	rBV	757893	1463523	27.12%	2.572%
3	4.134	159	161	169	rVB3	14541	22547	0.42%	0.040%
4	7.234	681	688	706	rBV	630783	1702164	31.54%	2.991%
5	7.369	706	711	736	rVV	711843	1422331	26.36%	2.500%
6	7.581	740	747	766	rBV	893568	1788349	33.14%	3.143%
7	8.046	819	826	845	rBV	502166	1057046	19.59%	1.858%
8	8.793	945	953	982	rBV	826154	2256581	41.82%	3.966%
9	9.240	1021	1029	1050	rBV	796560	1792880	33.22%	3.151%
10	9.969	1144	1153	1176	rBV	566423	1484939	27.52%	2.610%
11	10.540	1243	1250	1285	rBV	553645	2158259	39.99%	3.793%
12	10.875	1299	1307	1326	rVB	844964	1661907	30.80%	2.921%
13	11.046	1328	1336	1373	rBV	608834	2177652	40.35%	3.827%
14	11.522	1414	1417	1422	rVB7	4095	7579	0.14%	0.013%
15	12.063	1507	1509	1515	rVB7	3898	6538	0.12%	0.011%
16	12.516	1579	1586	1592	rBV3	13144	29380	0.54%	0.052%
17	13.581	1762	1767	1772	rBV2	19420	35778	0.66%	0.063%
18	14.110	1850	1857	1881	rBV	1714072	3306686	61.28%	5.811%
19	14.392	1898	1905	1927	rBV	2411526	4002461	74.17%	7.034%
20	14.698	1950	1957	1976	rBV	1369715	2182128	40.44%	3.835%
21	15.010	2003	2010	2040	rBV3	186665	1068364	19.80%	1.877%
22	15.698	2120	2127	2145	rBV	2422878	4811513	89.16%	8.456%
23	15.881	2151	2158	2185	rBV2	249549	852886	15.80%	1.499%
24	17.133	2367	2371	2376	rBV7	5712	9302	0.17%	0.016%
25	17.457	2420	2426	2438	rBV	1464820	2426215	44.96%	4.264%
26	17.563	2438	2444	2474	rVB2	2479901	5092133	94.36%	8.949%
27	19.369	2748	2751	2755	rBV5	38363	50219	0.93%	0.088%
28	19.445	2761	2764	2769	rBV	35668	48702	0.90%	0.086%
29	19.792	2817	2823	2844	rBV	2981281	5396360	100.00%	9.483%
30	21.563	3119	3124	3134	rBV	1129468	2107220	39.05%	3.703%
31	23.933	3521	3527	3543	rVB2	1760960	4291033	79.52%	7.541%
32	24.104	3550	3556	3572	rVB	789636	2080388	38.55%	3.656%




Sum of corrected areas: 56903891

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015942.D
Acq On : 03 Jul 2023 09:57
Operator : MA/JU
Sample : PB153768BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK768

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

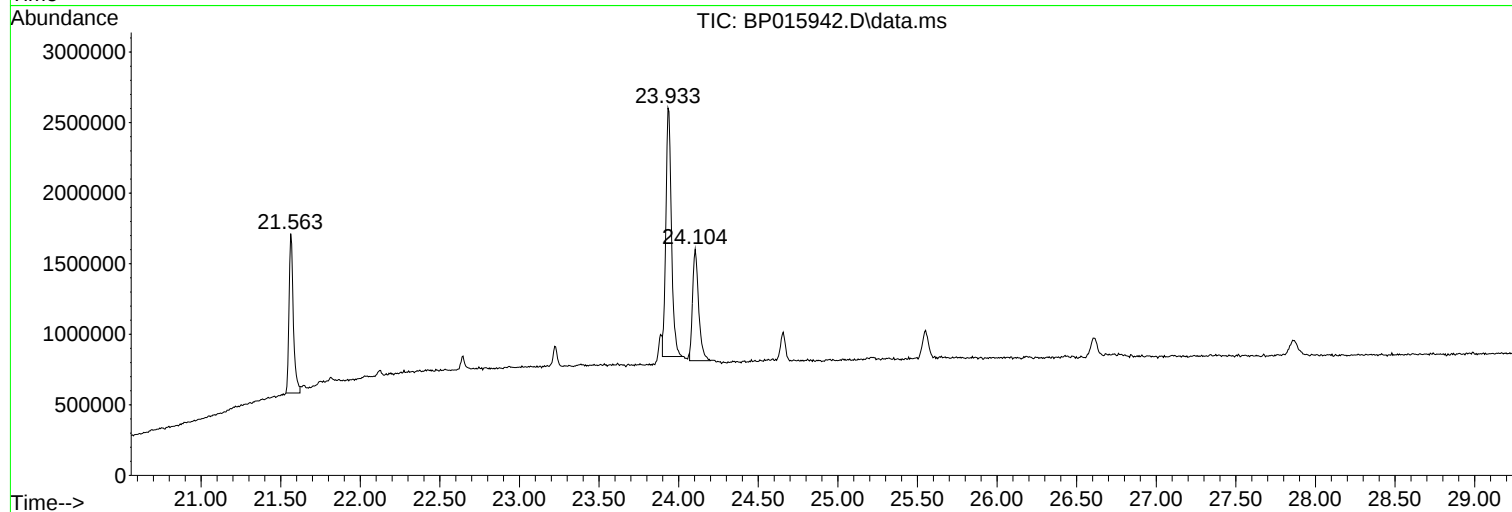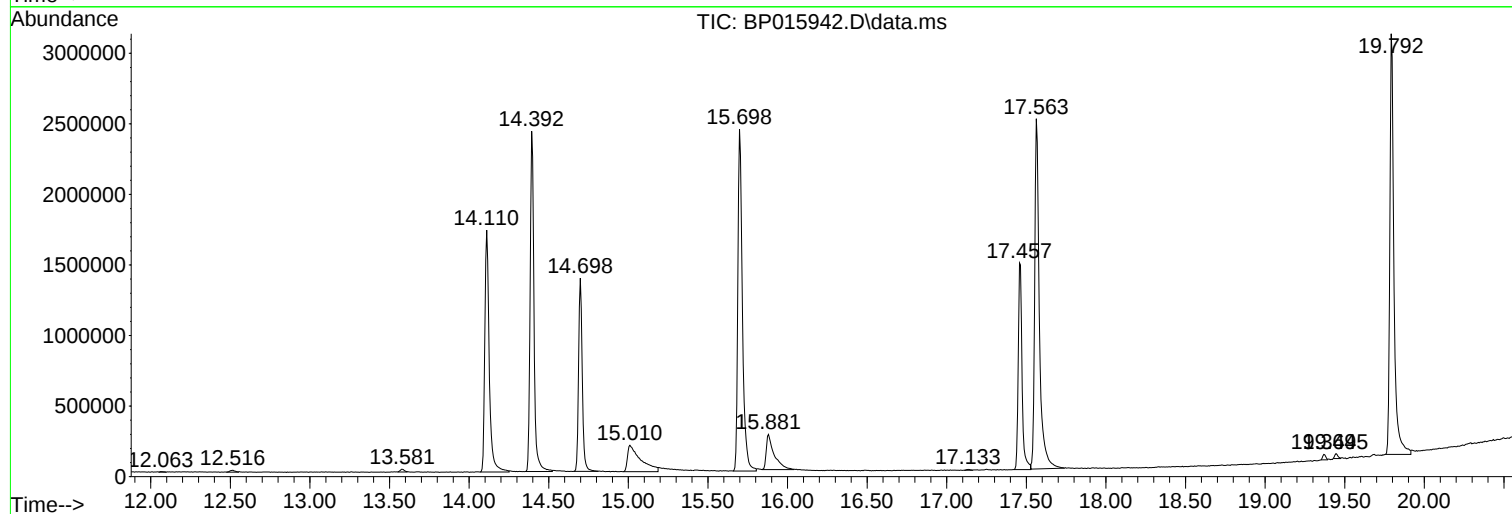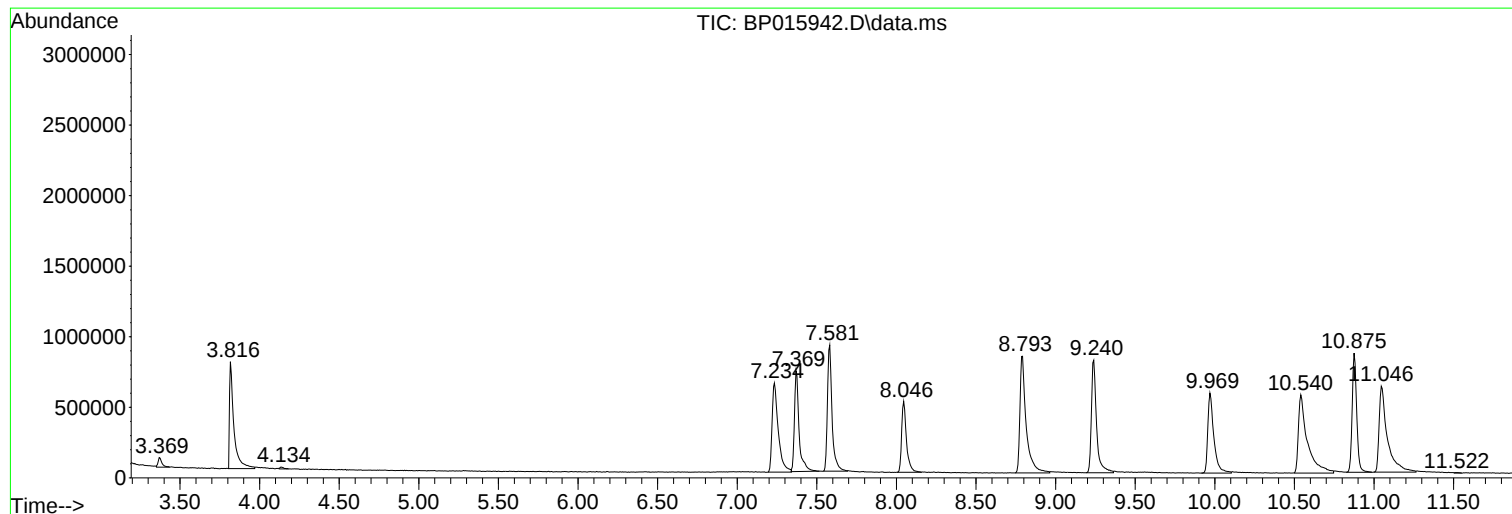

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015942.D
Acq On : 03 Jul 2023 09:57
Operator : MA/JU
Sample : PB153768BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK768

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070323\
Data File : BP015942.D
Acq On : 03 Jul 2023 09:57
Operator : MA/JU
Sample : PB153768BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK768

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc