
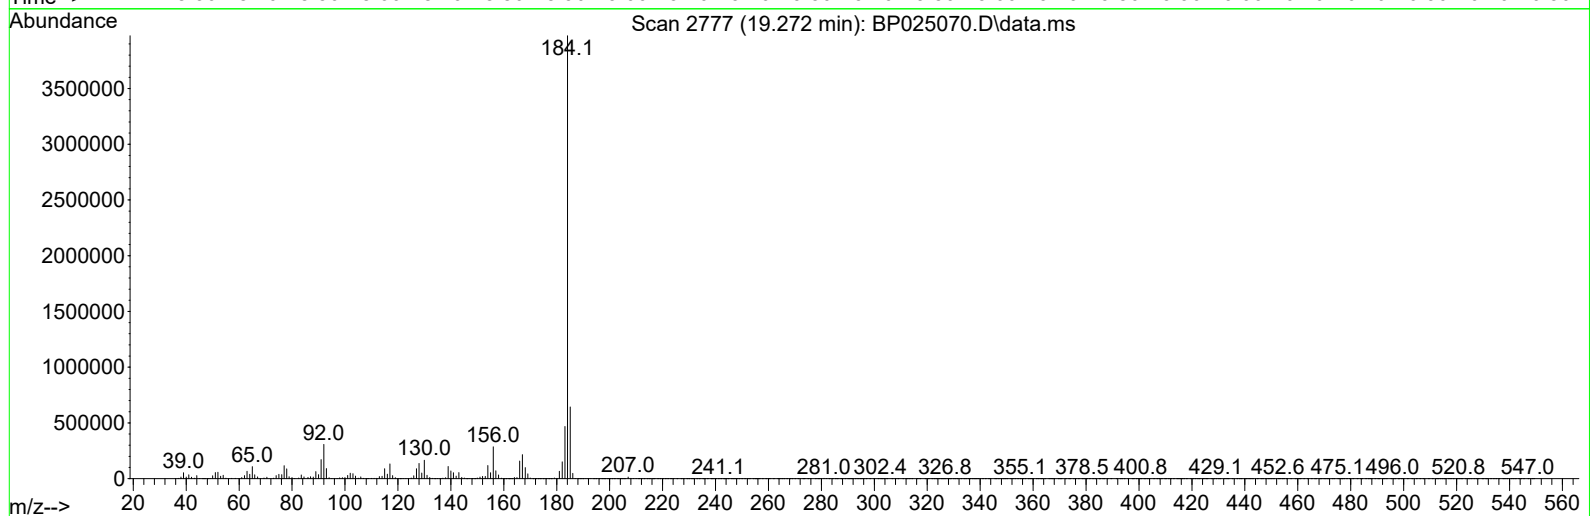


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070325\
Data File : BP025070.D
Acq On : 03 Jul 2025 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 16:24:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

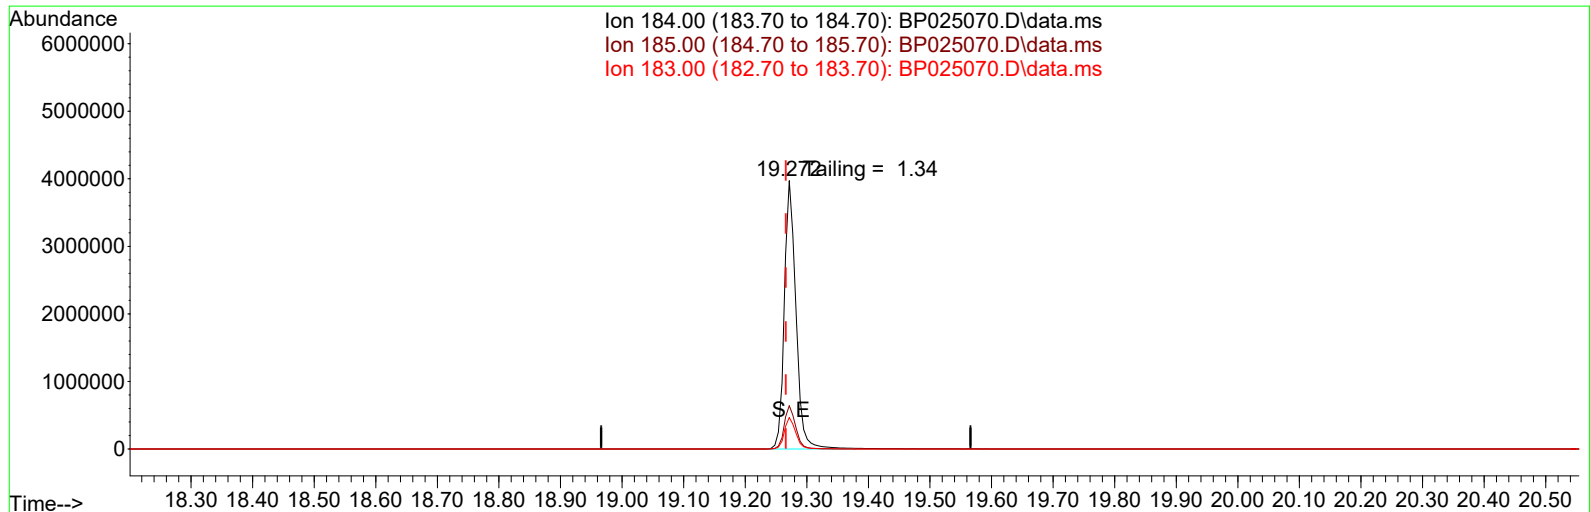



TIC: BP025070.D\data.ms

(77) Benzidine**19.272min (+ 0.006) 5891.13 ng****response 5273970**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.19
183.00	11.80	11.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070325\
Data File : BP025070.D
Acq On : 03 Jul 2025 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 16:24:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

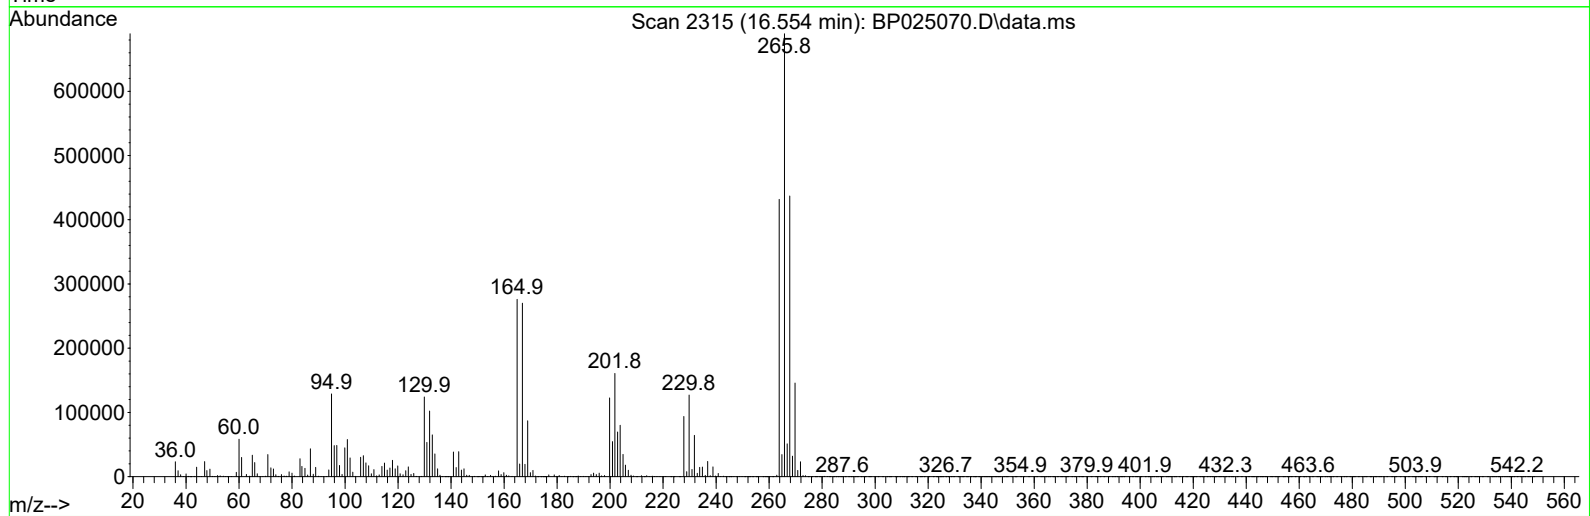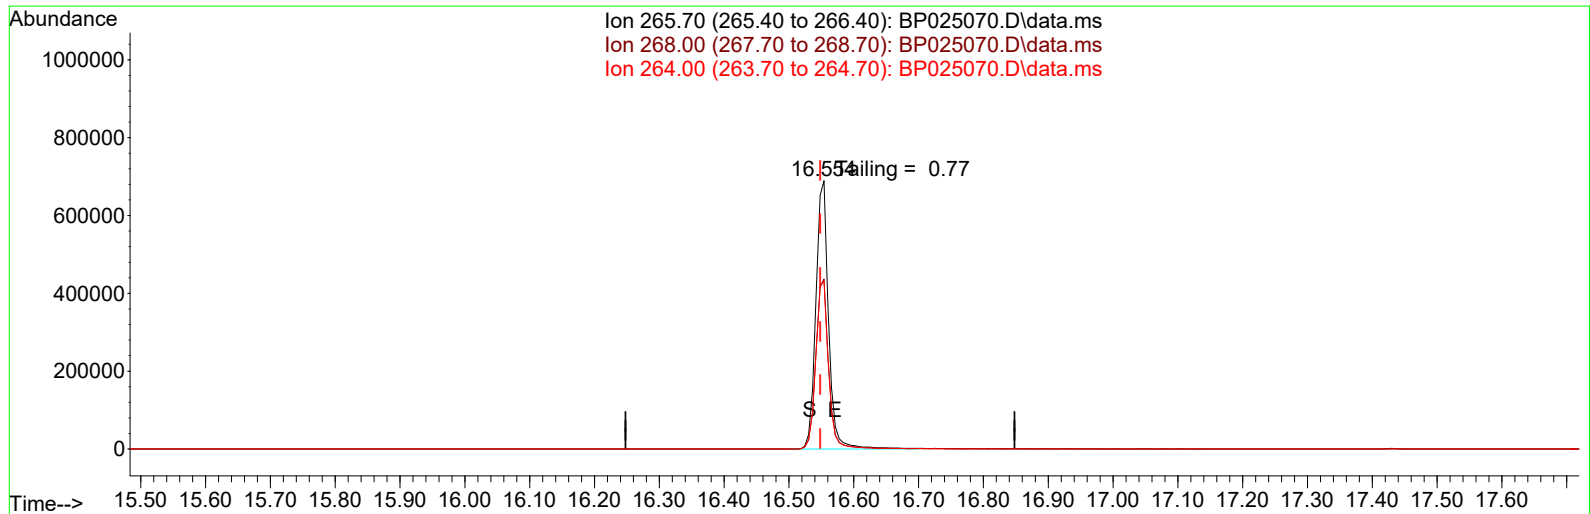

TIC: BP025070.D\data.ms

(70) Pentachlorophenol (C)

16.554min (+ 0.006) 170301.74 ng

response 942789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.35
264.00	62.70	62.60
0.00	0.00	0.00