

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015972.D
 Acq On : 04 Jul 2023 12:52
 Operator : MA/JU
 Sample : 03245-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGH9

Quant Time: Jul 04 21:56:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	729865	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	2954506	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.692	164	1546682	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	2683586	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	2169928	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	2489703	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	44598	2.198	ng/uL	0.00
4) Pyridine-d5	3.846	84	31014	0.606	ng/ul	0.03
7) Phenol-d5	7.228	99	771122	12.348	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	568511	14.715	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	655974	13.915	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	427382	8.663	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	325088	14.398	ng/ul	0.00
24) 2-Nitrophenol-d4	9.957	143	349230	13.252	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	537021	11.435	ng/ul	0.02
31) 4-Chloroaniline-d4	11.069	131	120112	1.991	ng/ul	0.04
46) Dimethylphthalate-d6	14.104	166	1723212	14.415	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1855608	13.808	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	401	0.025	ng/ul	-0.04
60) Fluorene-d10	15.692	176	1285491	13.059	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	123657	7.493	ng/ul	0.01
73) Anthracene-d10	17.557	188	1483708	12.104	ng/ul	0.00
81) Pyrene-d10	19.786	212	1839621	12.983	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1738291	13.841	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.446	93	383437	7.437	ng/ul#	22
16) Acetophenone	8.899	105	107959	1.331	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.404	149	135030	1.341	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015972.D
Acq On : 04 Jul 2023 12:52
Operator : MA/JU
Sample : 03245-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGH9

Quant Time: Jul 04 21:56:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration




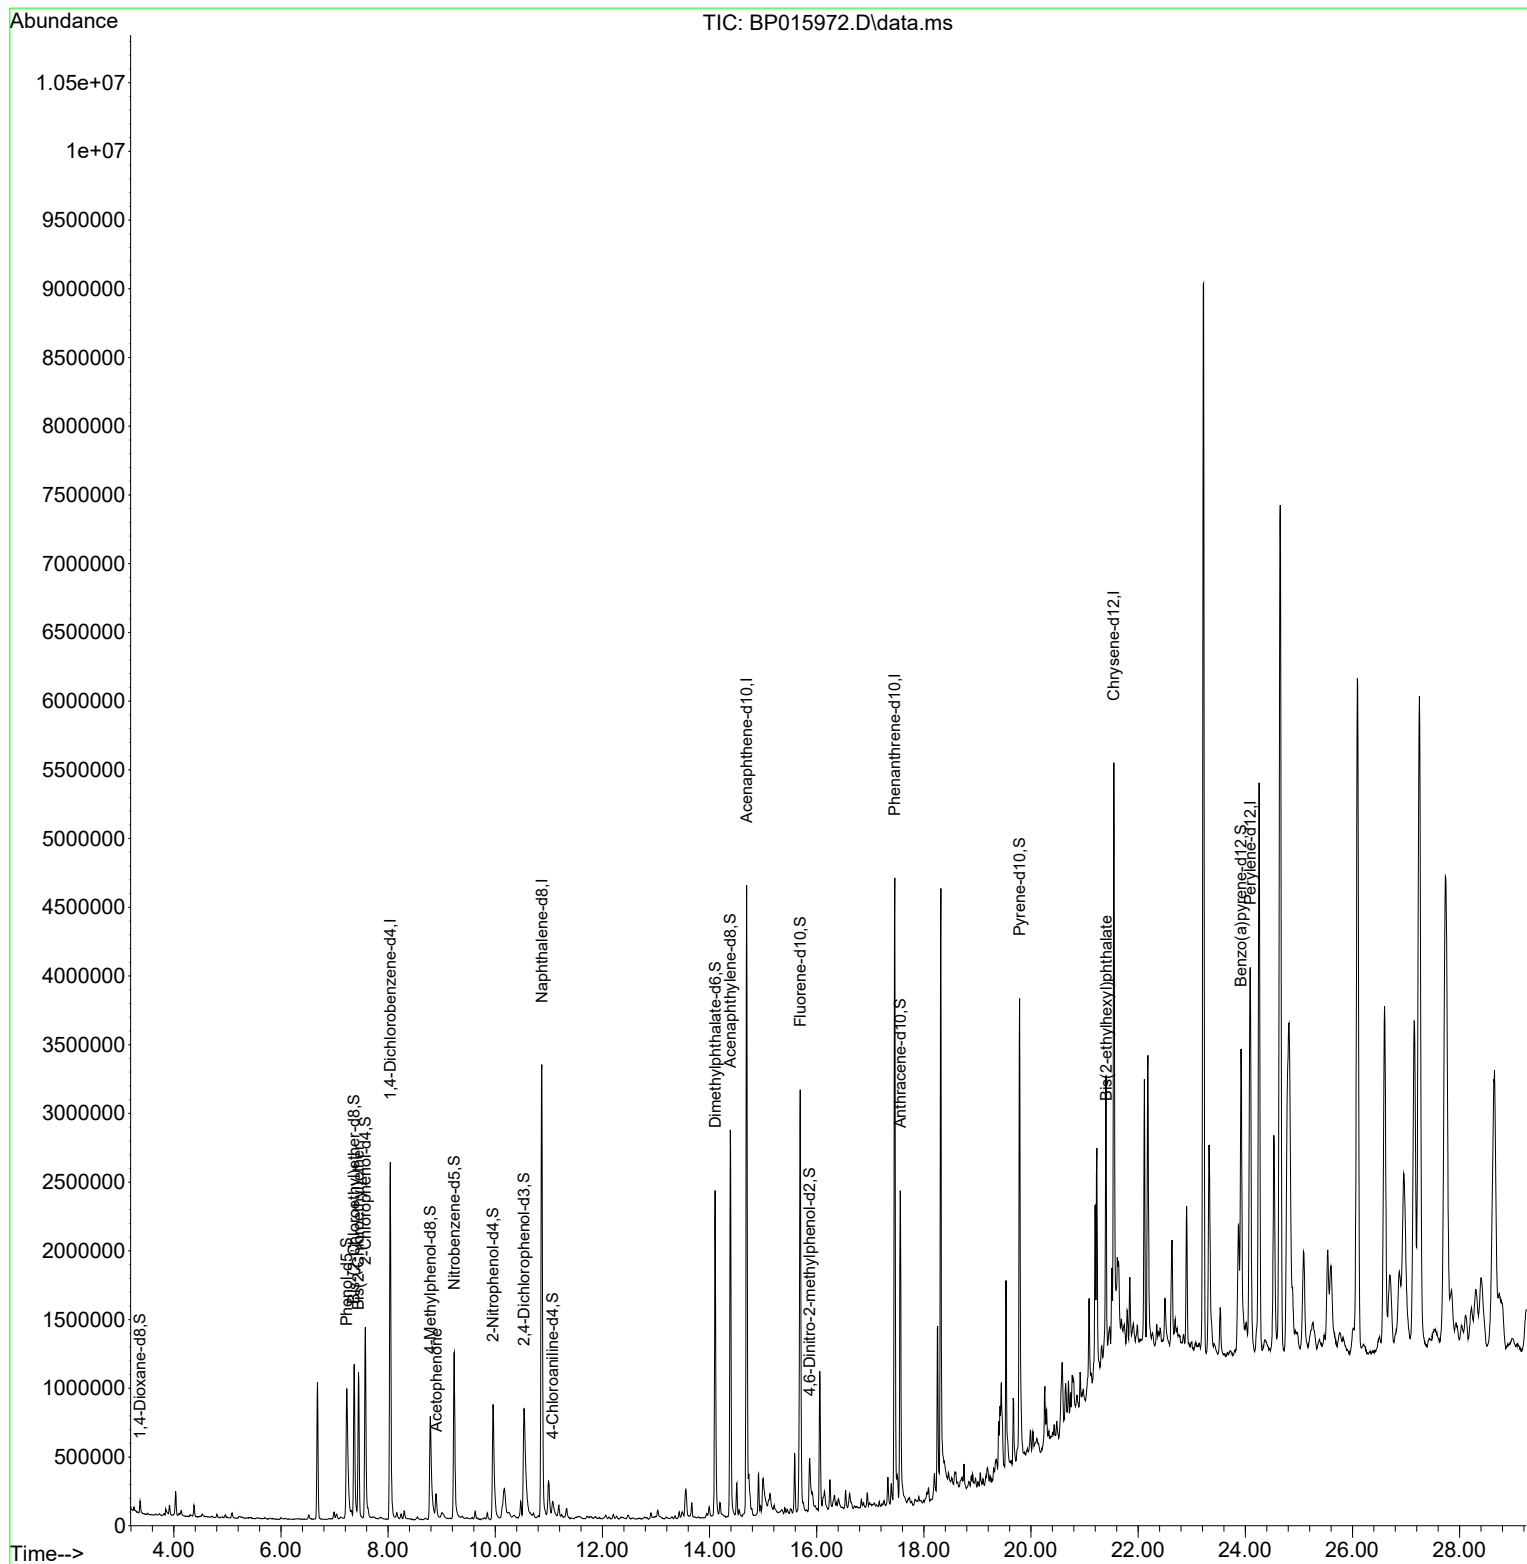


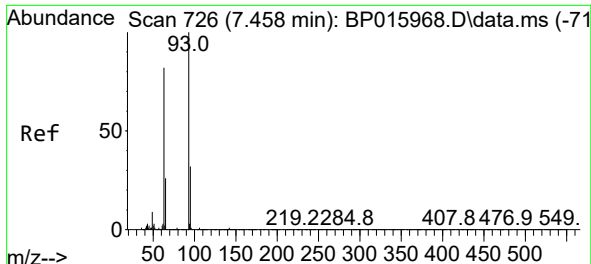

#10
Bis(2-Chloroethyl)ether
Concen: 7.437 ng/ul
RT: 7.446 min Scan# 71
Delta R.T. -0.017 min
Lab File: BP015972.D
Acq: 04 Jul 2023 12:52




Instrument :
BNA_P
ClientSampleId :
DCGH9


Tgt Ion: 93 Resp: 383437
Ion Ratio Lower Upper
93 100
63 2.1 62.8 94.2#
95 2.3 25.6 38.4#

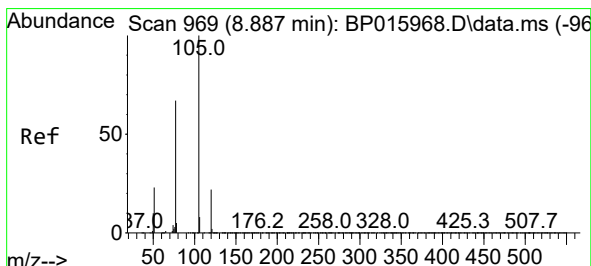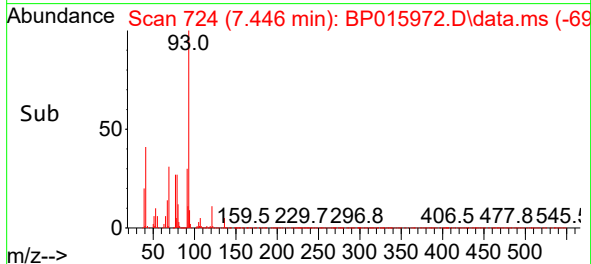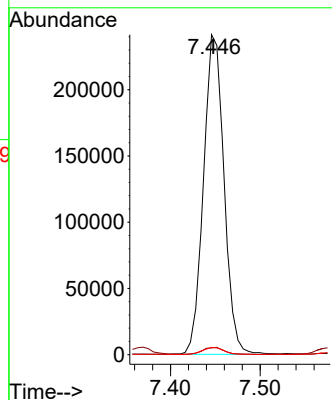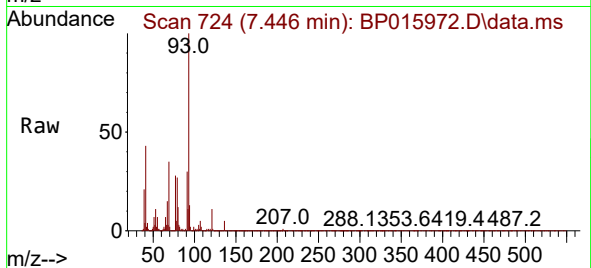

#16
Acetophenone
Concen: 1.331 ng/ul
RT: 8.899 min Scan# 971
Delta R.T. 0.012 min
Lab File: BP015972.D
Acq: 04 Jul 2023 12:52

Tgt Ion:105 Resp: 107959
Ion Ratio Lower Upper
105 100
77 78.3 65.0 97.4
51 29.2 25.1 37.7

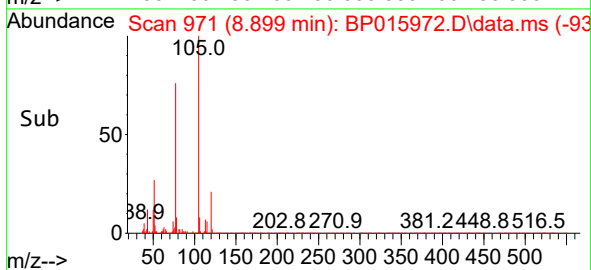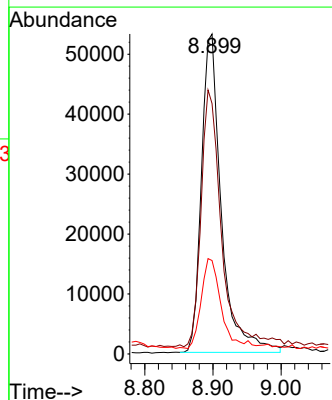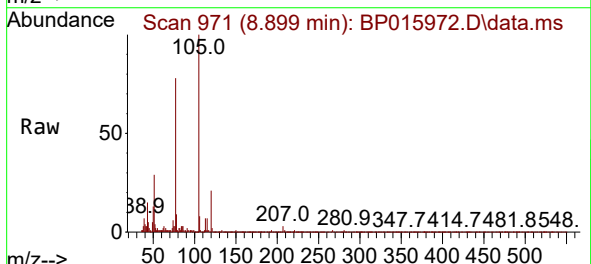

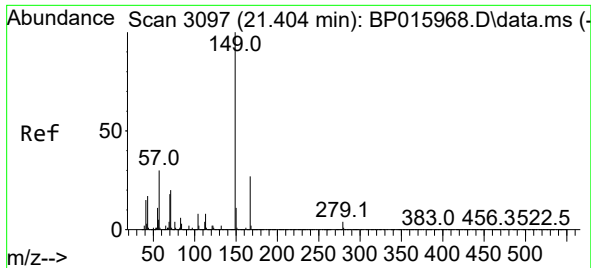

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.341 ng/ul
RT: 21.404 min Scan# 3097
Delta R.T. -0.006 min
Lab File: BP015972.D
Acq: 04 Jul 2023 12:52

Instrument :
BNA_P
ClientSampleId :
DCGH9

Tgt Ion	Ratio	Lower	Upper
149	100		
167	43.1	21.0	31.6#
279	4.0	3.8	5.6

