

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015980.D
 Acq On : 04 Jul 2023 17:24
 Operator : MA/JU
 Sample : 03244-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE9

Quant Time: Jul 04 21:57:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	303407	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	1293484	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.693	164	747090	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1453813	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.551	240	1106028	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	1262374	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	38220	4.532	ng/uL	0.00
4) Pyridine-d5	3.817	84	386086	18.162	ng/ul	0.00
7) Phenol-d5	7.234	99	715448	27.560	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.369	67	472418	29.414	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	558401	28.495	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	534924	26.084	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	277551	28.077	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	305450	26.475	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	535135	26.029	ng/ul	0.02
31) 4-Chloroaniline-d4	11.052	131	482217	18.258	ng/ul	0.02
46) Dimethylphthalate-d6	14.104	166	1865330	32.303	ng/ul	0.00
49) Acenaphthylene-d8	14.393	160	2023824	31.178	ng/ul	0.00
54) 4-Nitrophenol-d4	14.993	143	213247	27.984	ng/ul	0.04
60) Fluorene-d10	15.692	176	1518485	31.937	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	181595	20.311	ng/ul	0.01
73) Anthracene-d10	17.557	188	1954896	29.438	ng/ul	0.00
81) Pyrene-d10	19.786	212	2418996	33.494	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	2257421	35.450	ng/ul	0.00
Target Compounds						
					Qvalue	
90) Benzo(b)fluoranthene	23.310	252	81641	1.007	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015980.D
Acq On : 04 Jul 2023 17:24
Operator : MA/JU
Sample : 03244-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGE9

Quant Time: Jul 04 21:57:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

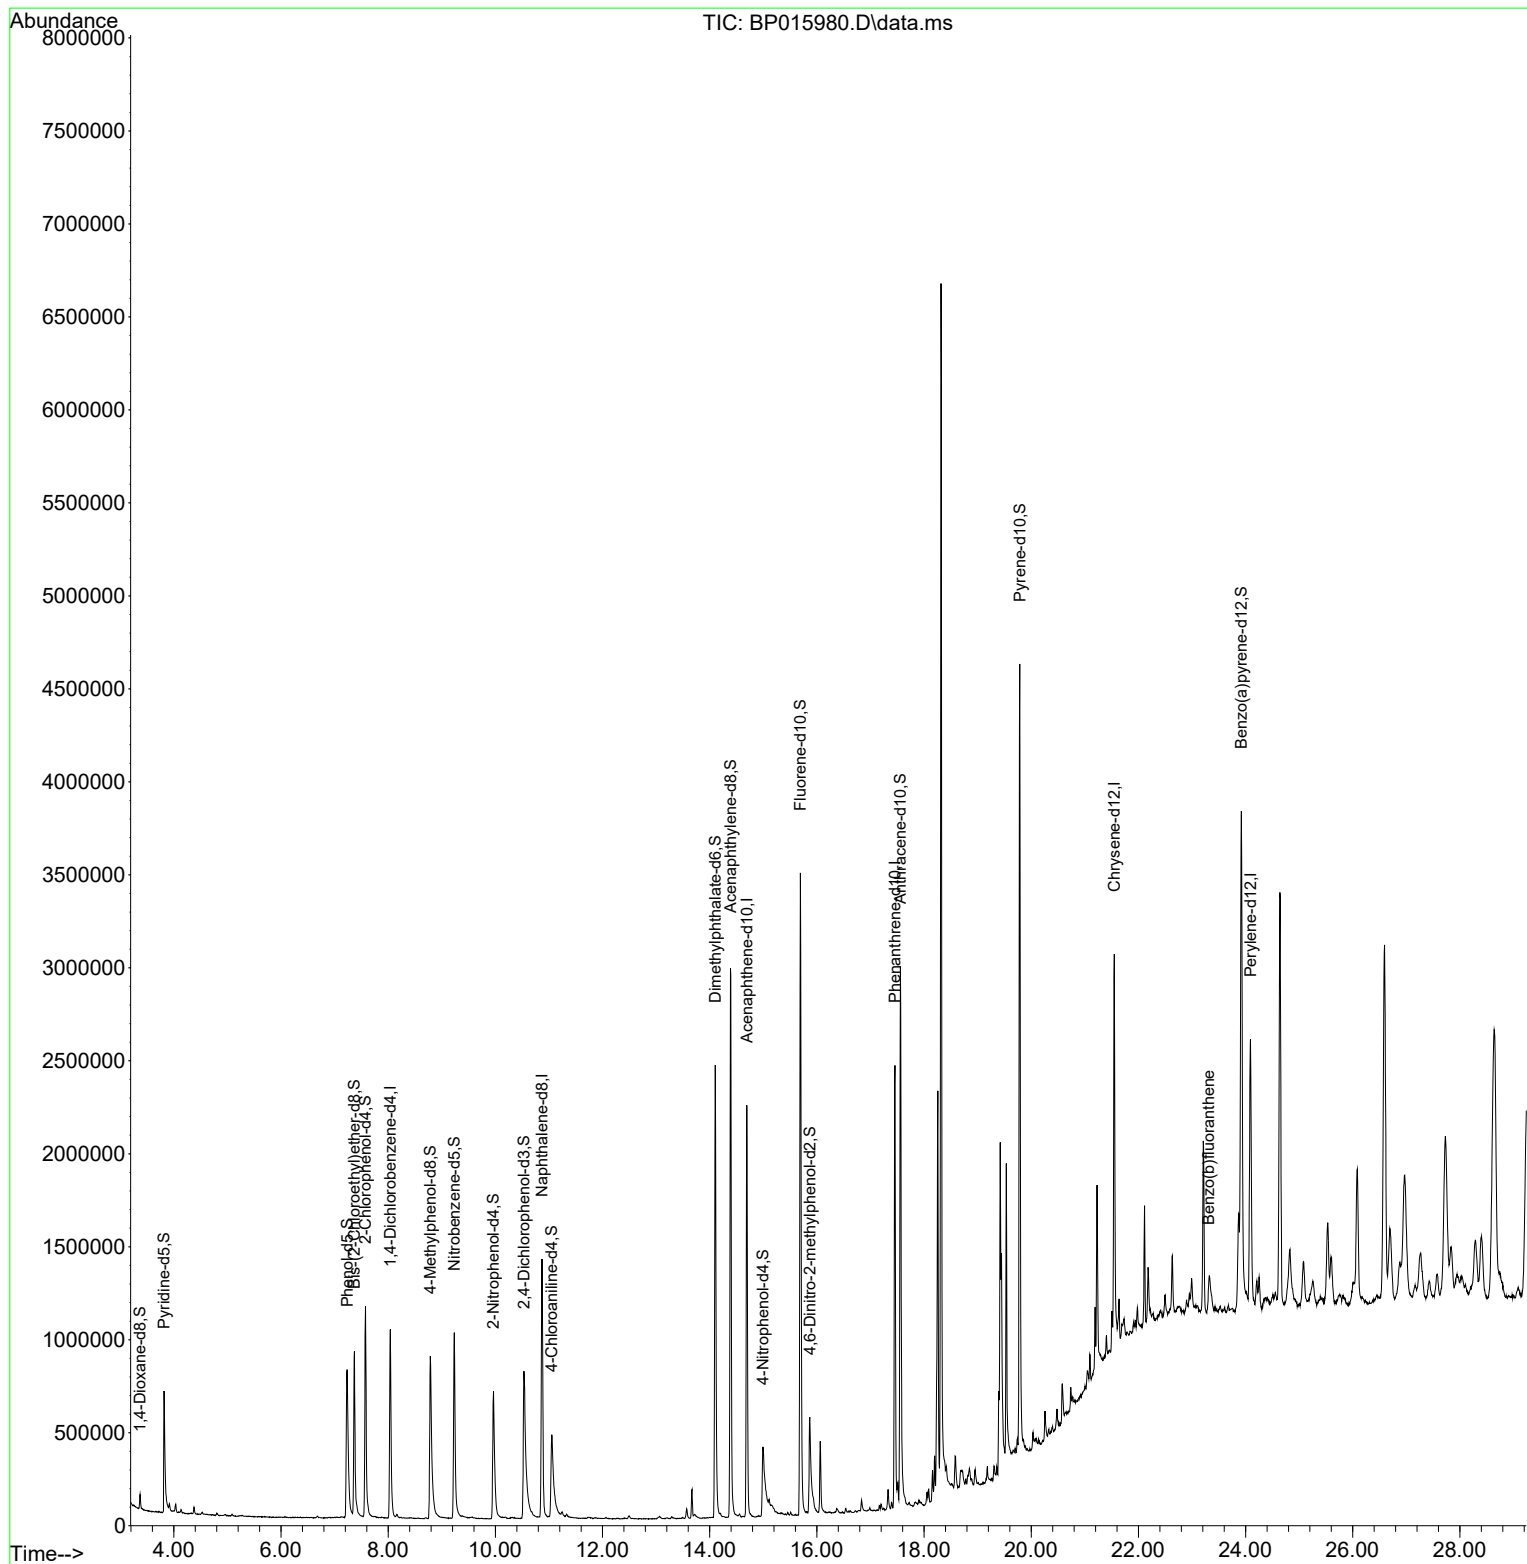

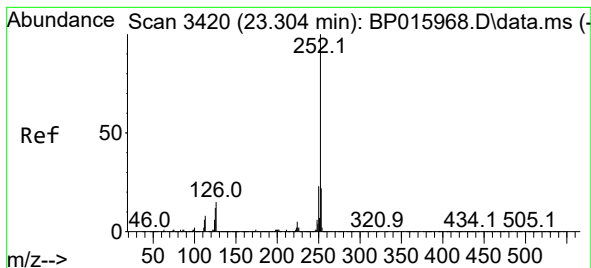

#90

Benzo(b)fluoranthene

Concen: 1.007 ng/ul

RT: 23.310 min Scan# 34

Delta R.T. 0.000 min

Lab File: BP015980.D


Acq: 04 Jul 2023 17:24

Instrument :

BNA_P

ClientSampleId :

DCGE9

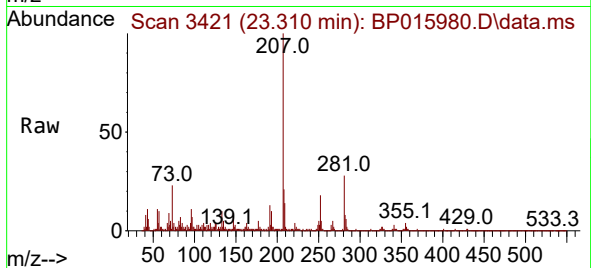

Tgt Ion:252 Resp: 81641

Ion Ratio Lower Upper

252 100

253 25.6 17.3 25.9

125 22.0 7.5 11.3#

