




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015989.D
 Acq On : 04 Jul 2023 23:03
 Operator : MA/JU
 Sample : PB153764BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK764

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:41:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :mohammad ahmed 07/05/2023

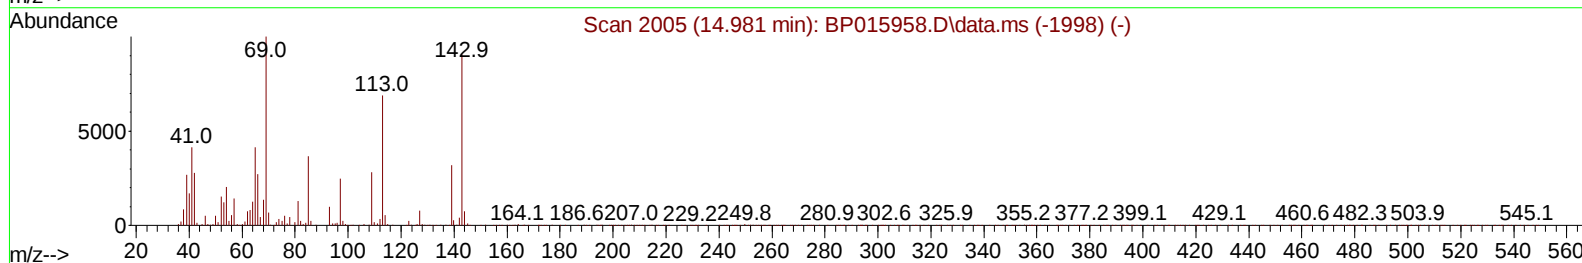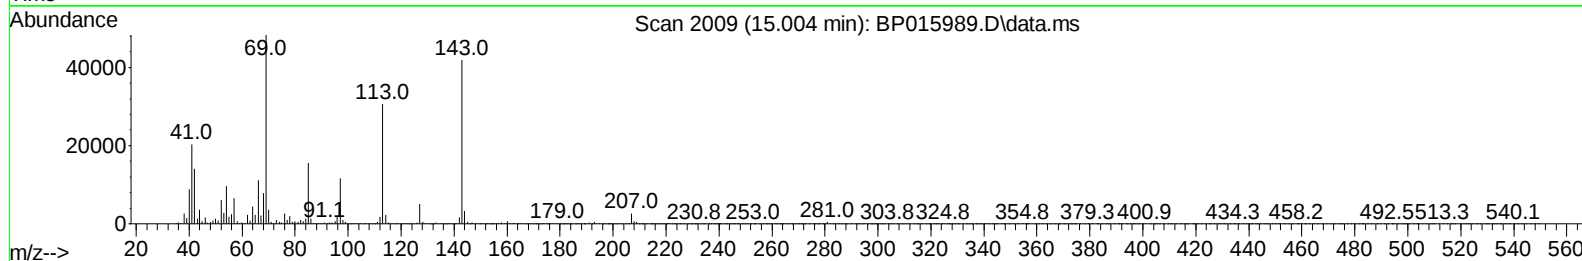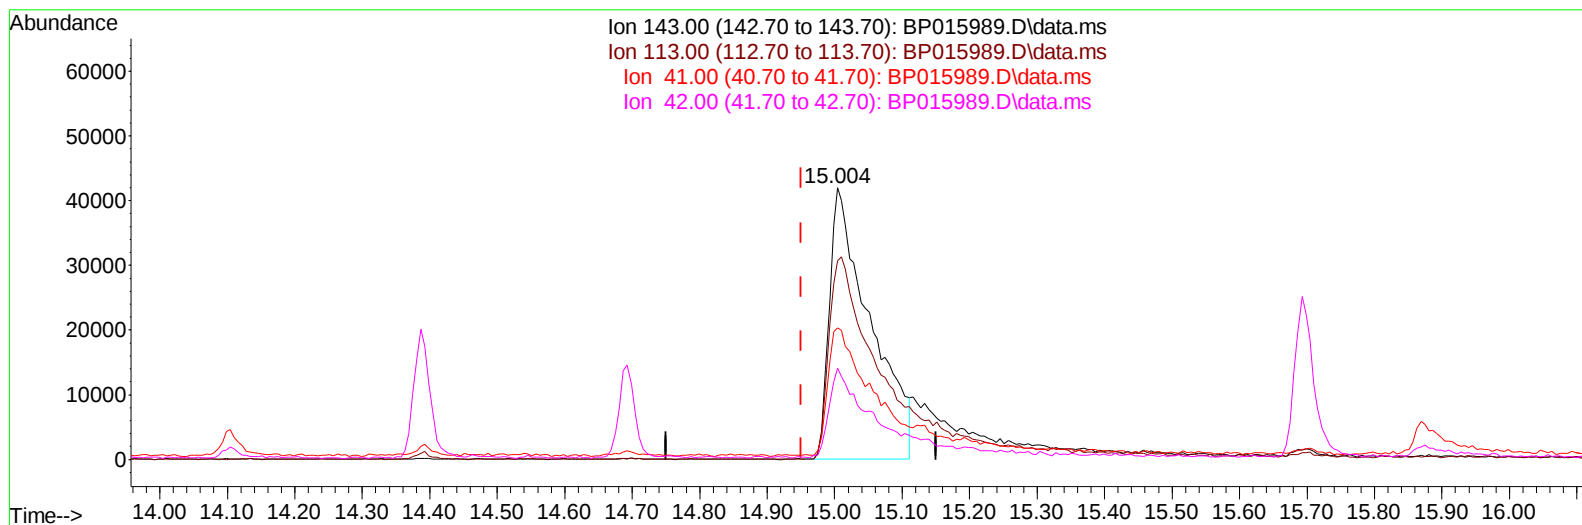

TIC: BP015989.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.053) 27.96 ng/u1

response 175628

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	73.14#
41.00	45.70	48.49
42.00	31.20	33.73




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015989.D
 Acq On : 04 Jul 2023 23:03
 Operator : MA/JU
 Sample : PB153764BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK764

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:41:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :mohammad ahmed 07/05/2023

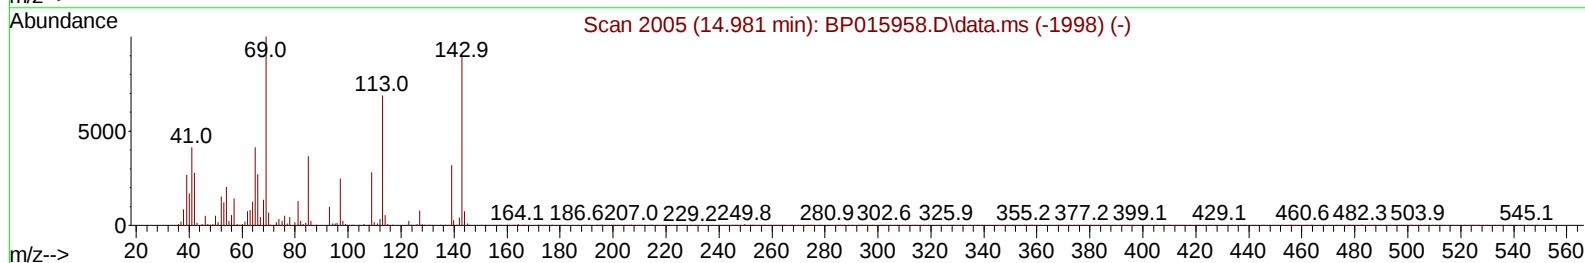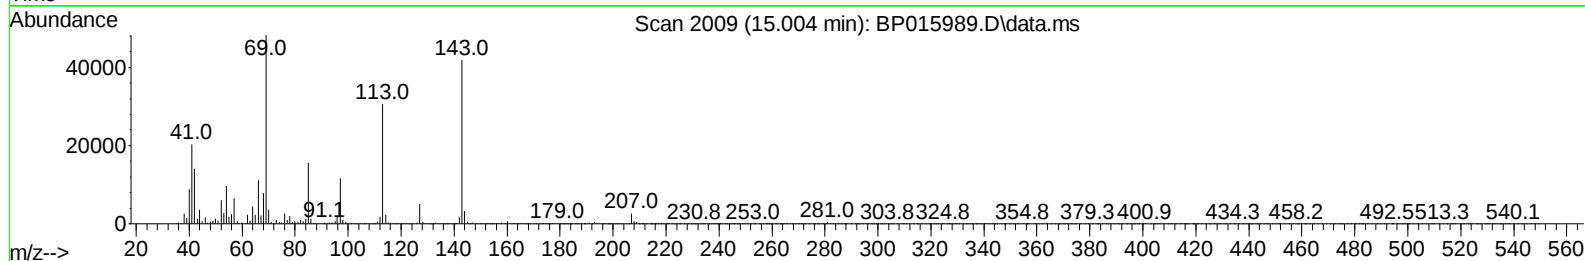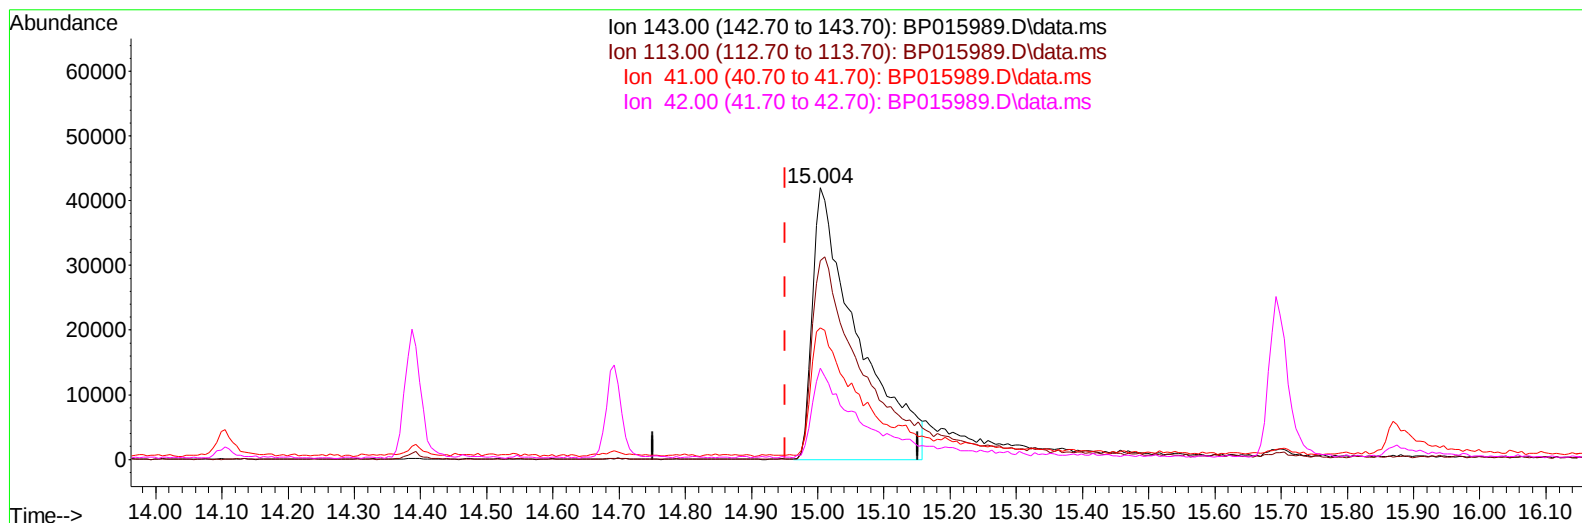

TIC: BP015989.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.053) 31.47 ng/ul m

response 197699

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	73.14#
41.00	45.70	48.49
42.00	31.20	33.73

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015989.D
 Acq On : 04 Jul 2023 23:03
 Operator : MA/JU
 Sample : PB153764BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK764

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :mohammad ahmed 07/05/2023

Quant Time: Jul 04 23:47:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	245116	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	1098123	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	615812	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1126870	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.557	240	838115	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	964507	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	47817	7.019	ng/uL	0.00
4) Pyridine-d5	3.811	84	666270	38.796	ng/ul	0.00
7) Phenol-d5	7.228	99	857548	40.889	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	595831	45.921	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	691061	43.651	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	710773	42.900	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	343275	40.904	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	379214	38.716	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	608589	34.868	ng/ul	0.02
31) 4-Chloroaniline-d4	11.040	131	888032	39.606	ng/ul	0.01
46) Dimethylphthalate-d6	14.104	166	1985382	41.712	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	2217749	41.449	ng/ul	0.00
54) 4-Nitrophenol-d4	15.004	143	197699m	31.475	ng/ul	0.05
60) Fluorene-d10	15.693	176	1559469	39.791	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	148409	21.415	ng/ul	0.02
73) Anthracene-d10	17.563	188	2223004	43.188	ng/ul	0.00
81) Pyrene-d10	19.786	212	2283715	41.729	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.922	264	2084311	42.839	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015989.D
Acq On : 04 Jul 2023 23:03
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023

