




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:58:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

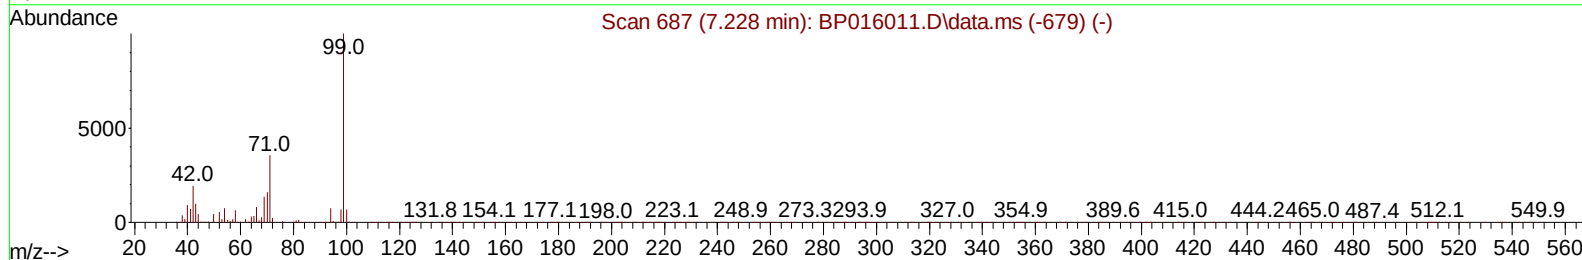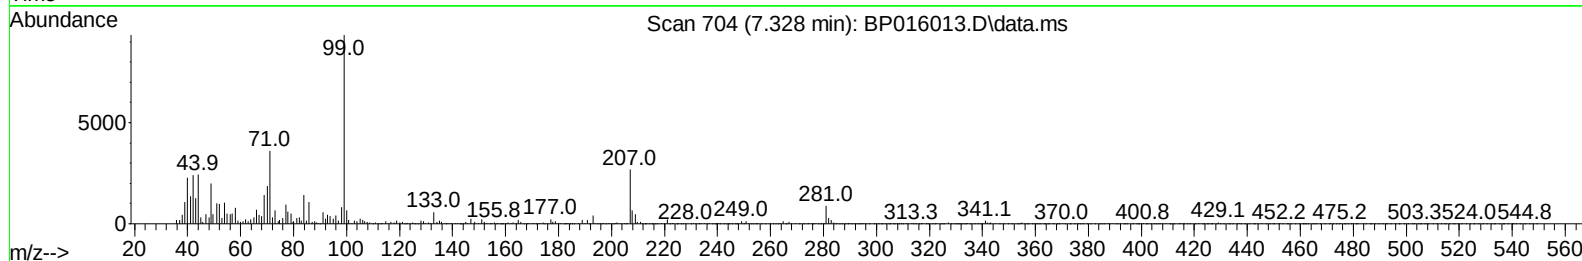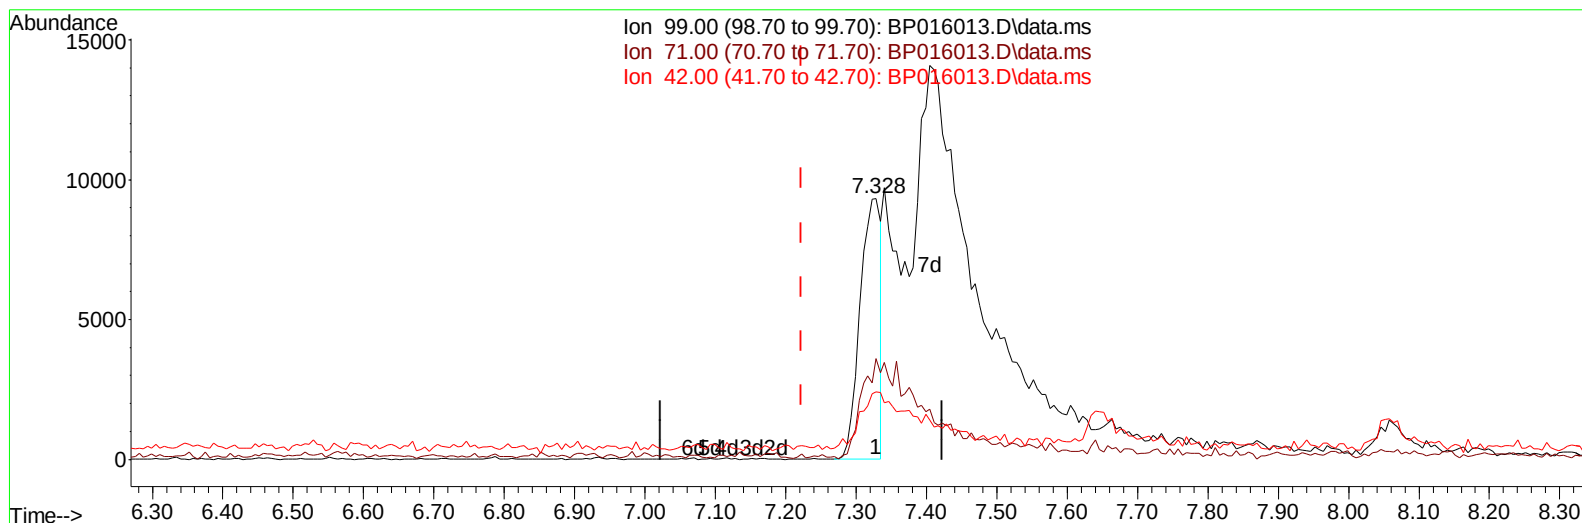

TIC: BP016013.D\data.ms

(7) Phenol-d5 (S)

7.328min (+ 0.106) 1.03 ng/ul

response 18788

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	38.53
42.00	21.90	25.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:58:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

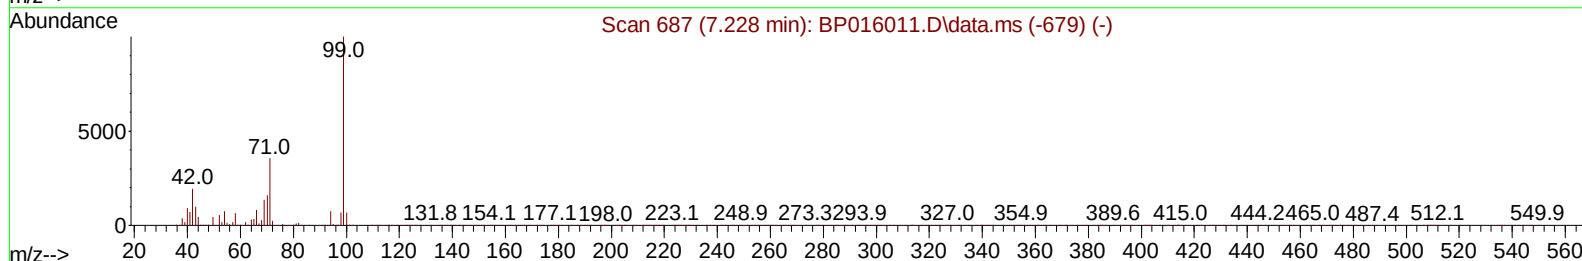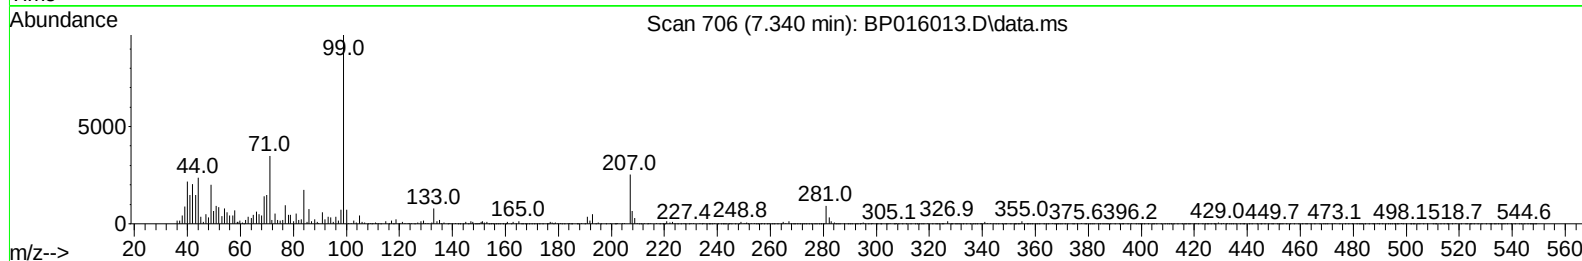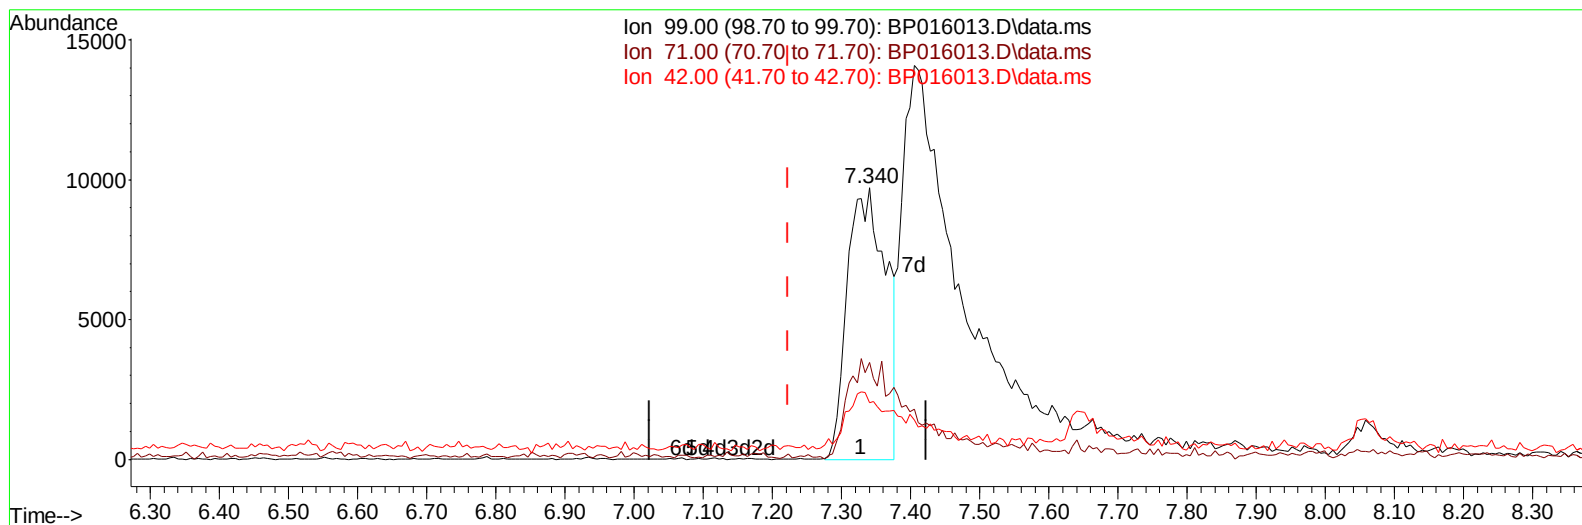

TIC: BP016013.D\data.ms

(7) Phenol-d5 (S)

7.340min (+ 0.118) 2.05 ng/ul m

response 37546

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	35.83
42.00	21.90	20.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:58:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

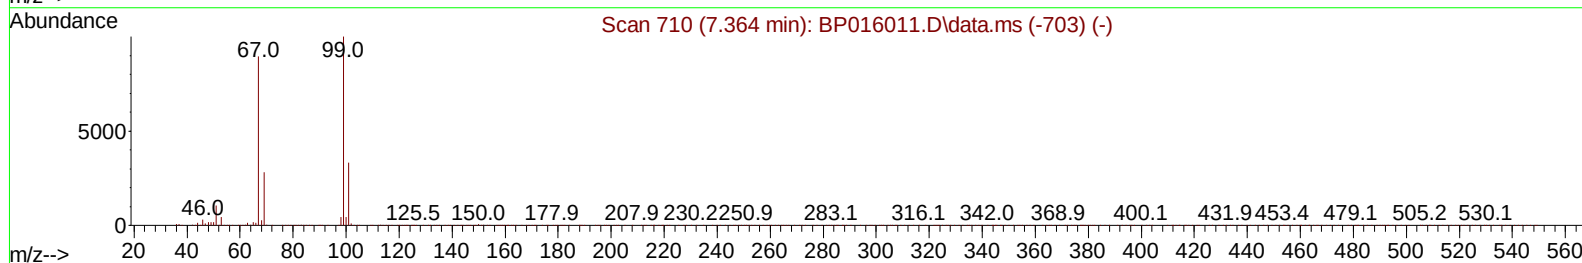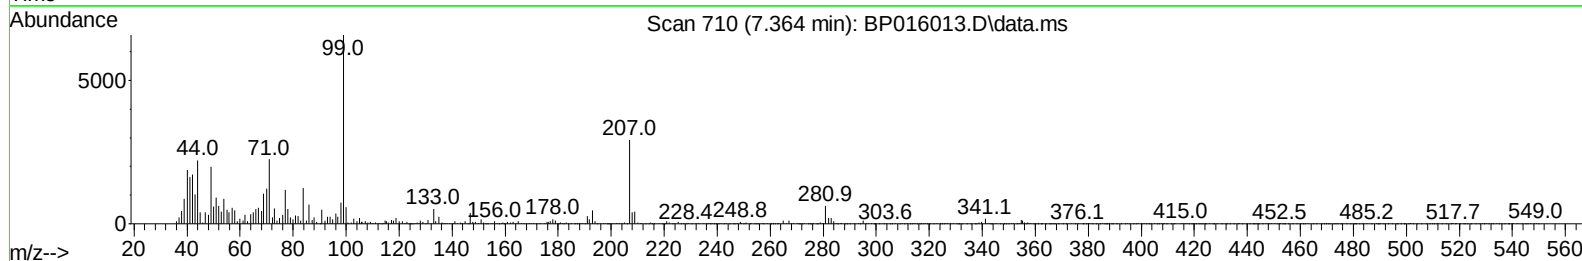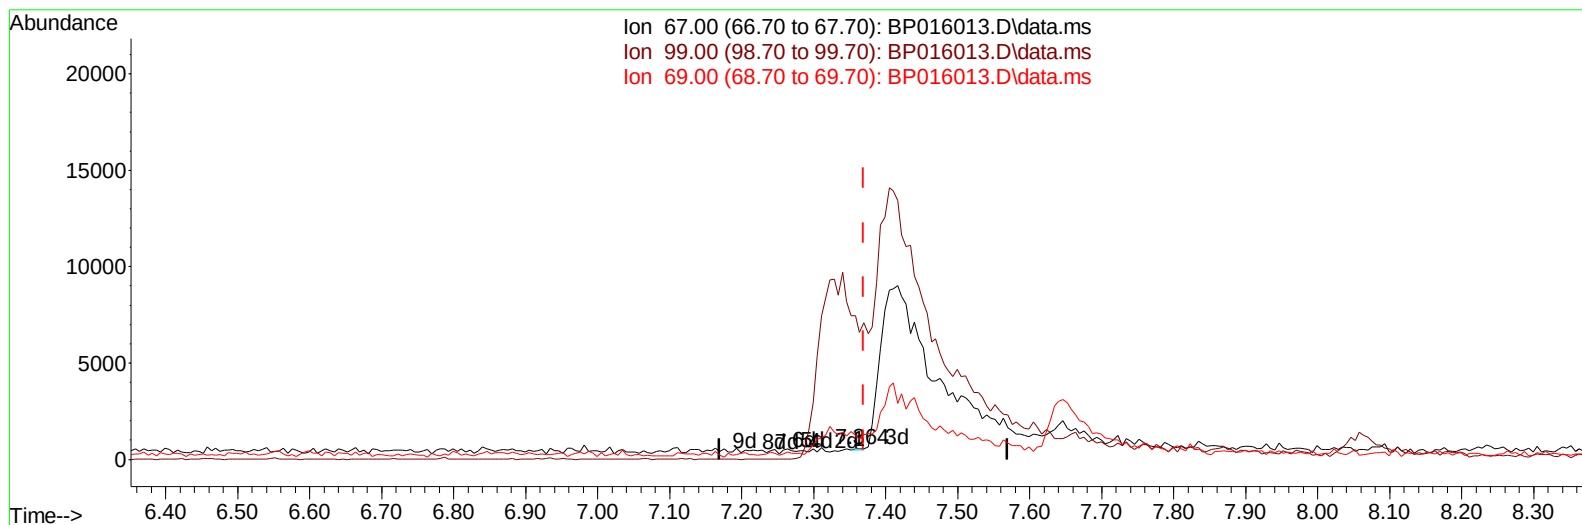

TIC: BP016013.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.364min (-0.005) 0.01 ng/u1

response 90

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	1165.84#
69.00	32.10	186.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:58:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

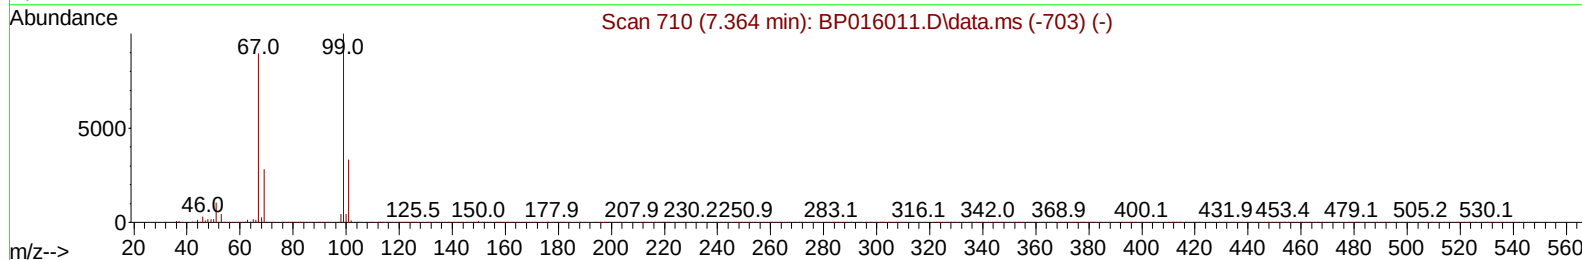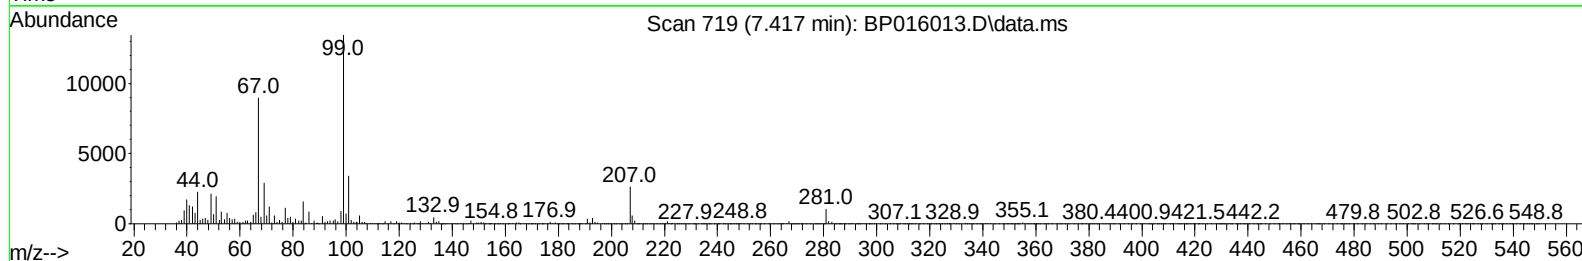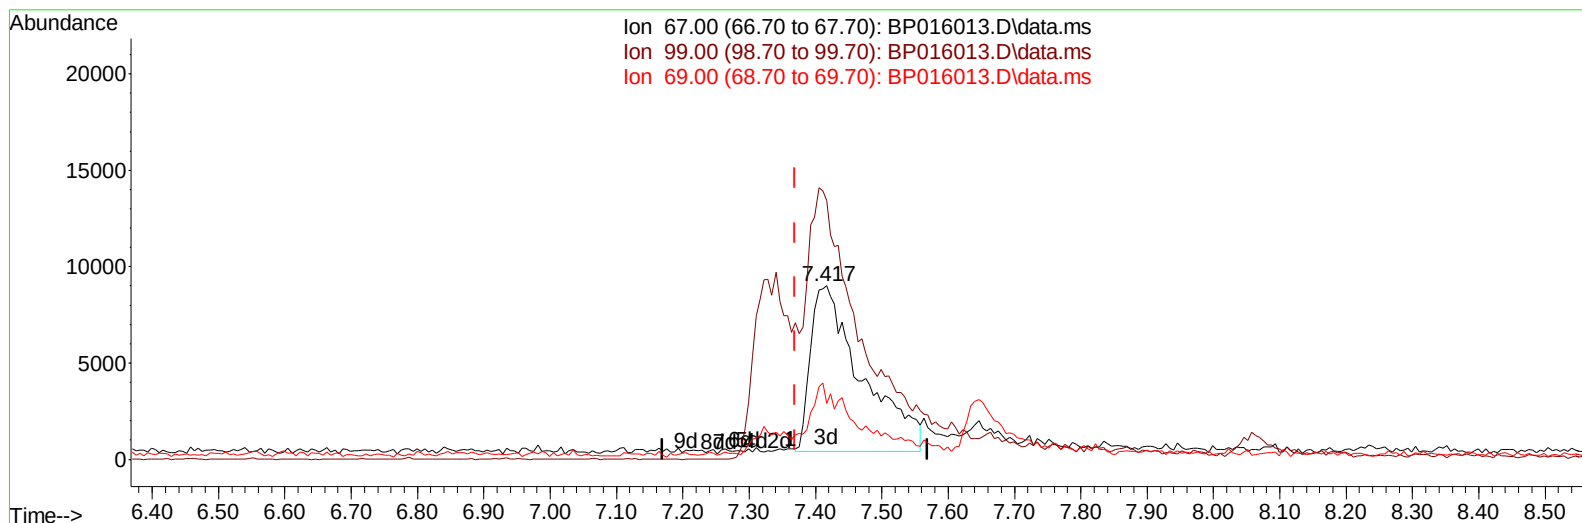

TIC: BP016013.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.417min (+ 0.048) 4.09 ng/ul m

response 46342

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	149.34#
69.00	32.10	32.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:59:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

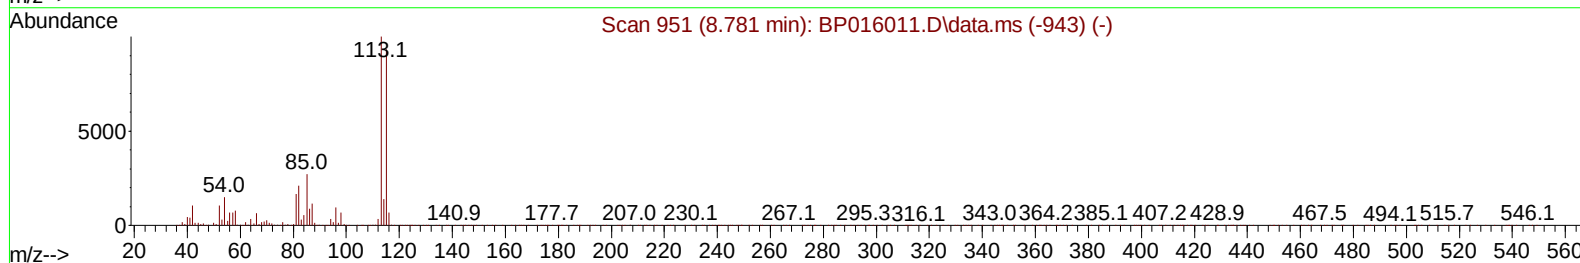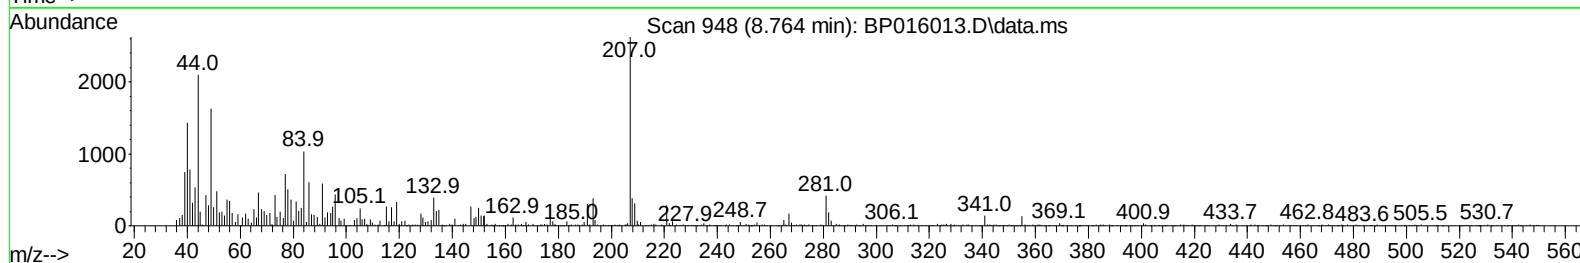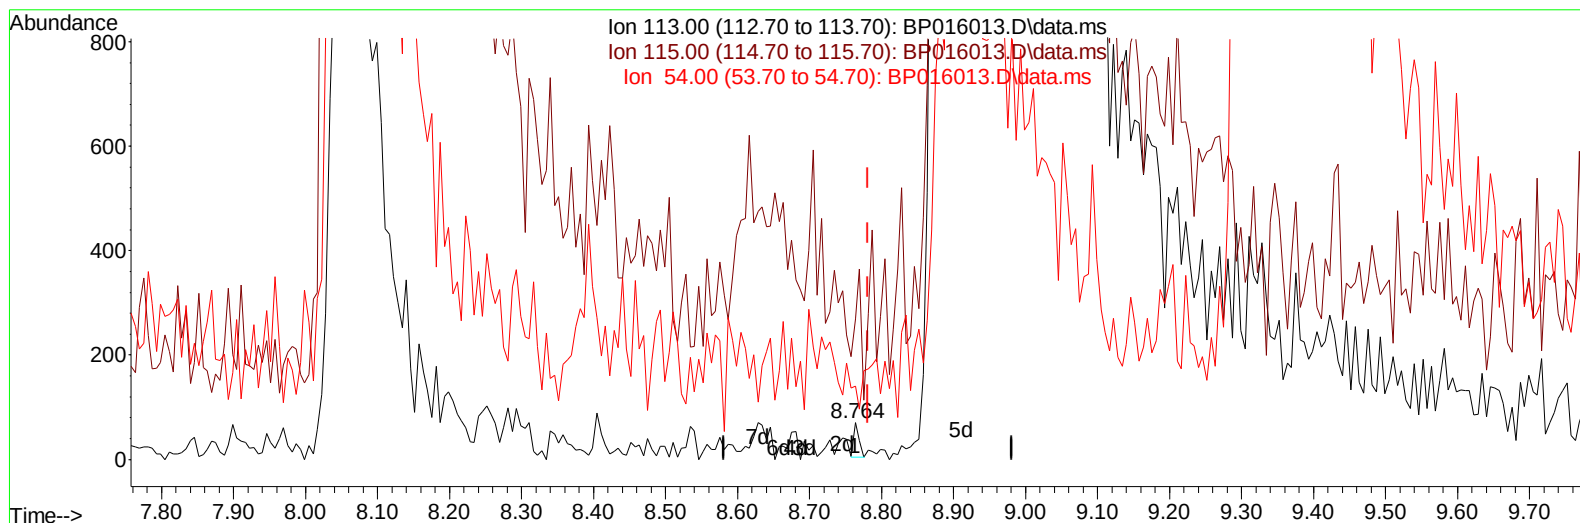

TIC: BP016013.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.764min (-0.017) 0.00 ng/u1

response 35

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	384.29#
54.00	16.10	200.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:59:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

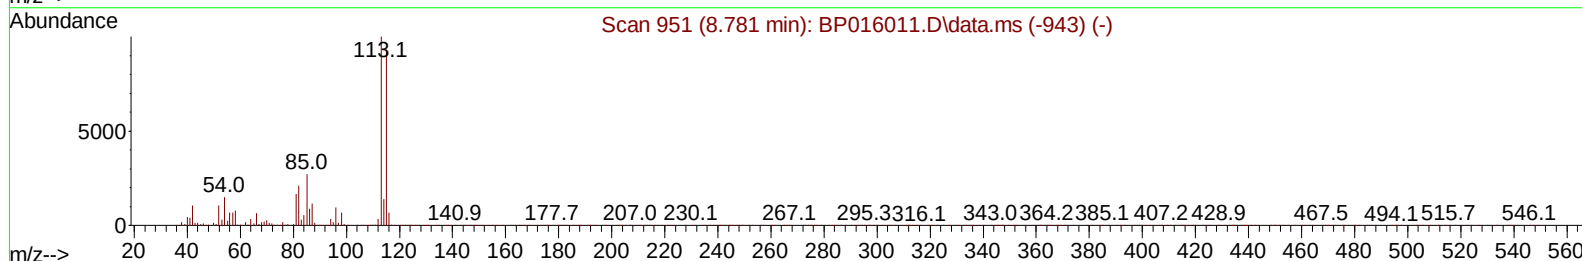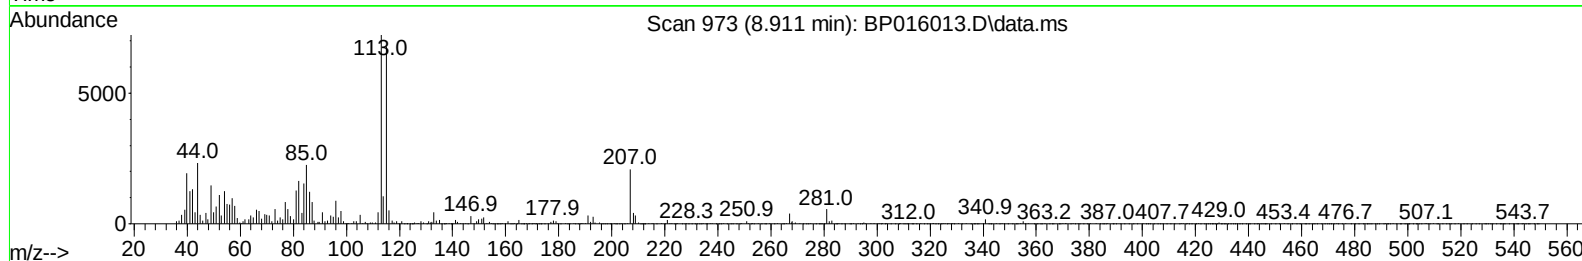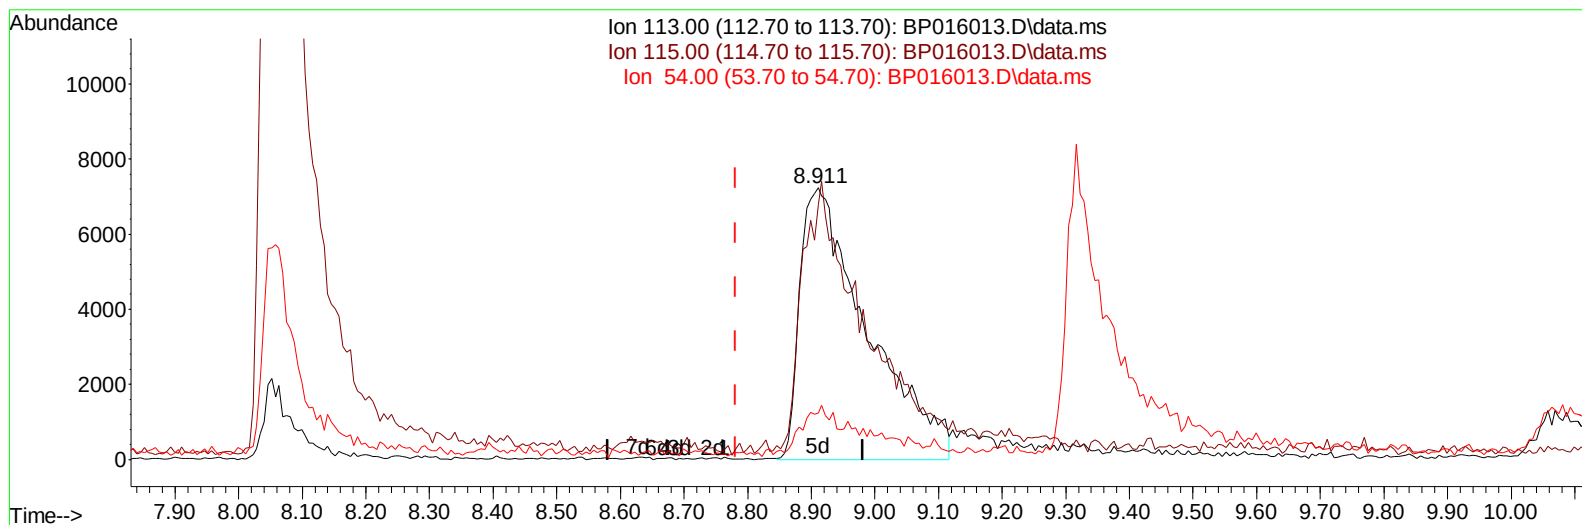

TIC: BP016013.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.911min (+ 0.130) 3.66 ng/ul m

response 52982

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	94.07
54.00	16.10	17.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:59:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

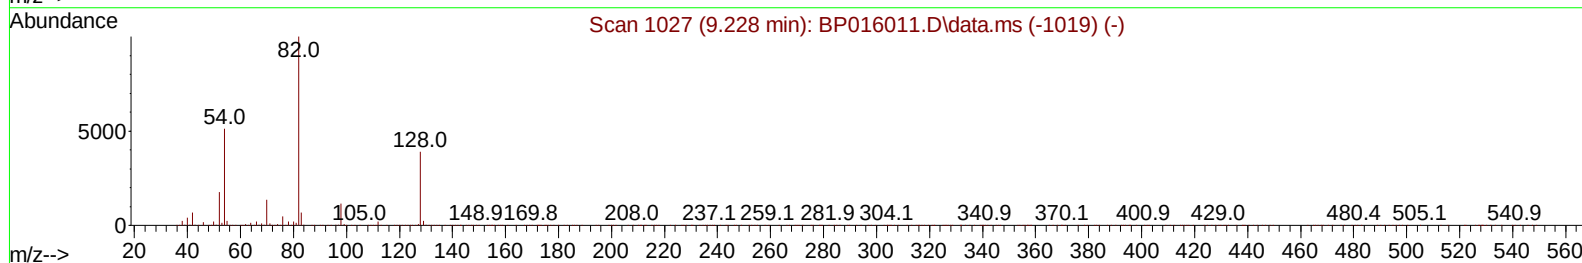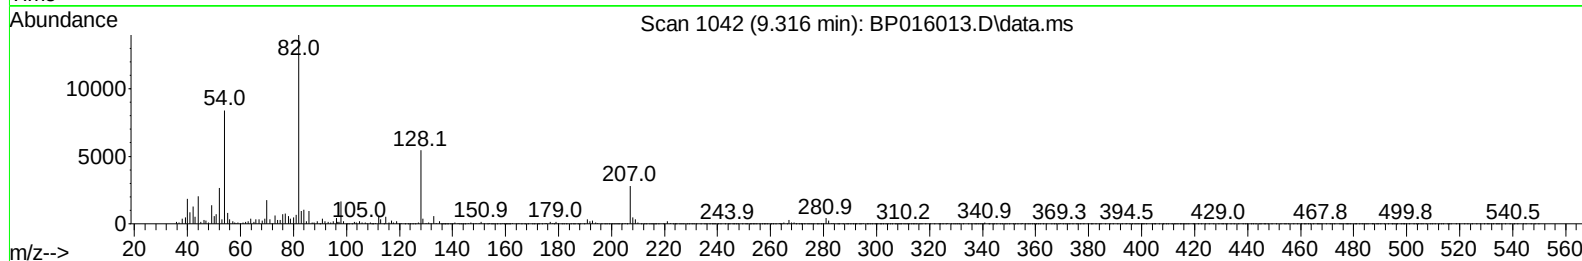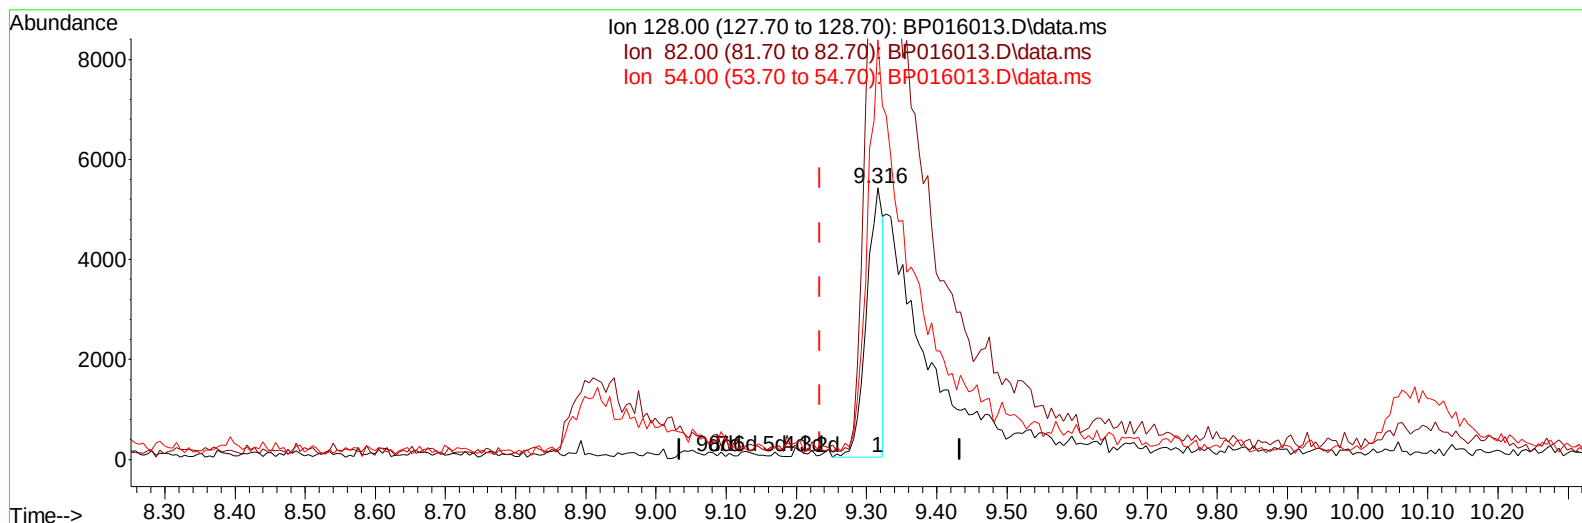

TIC: BP016013.D\data.ms

(21) Nitrobenzene-d5 (S)

9.316min (+ 0.083) 1.19 ng/uI

response 8642

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	257.56
54.00	141.60	154.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016013.D
Acq On : 05 Jul 2023 14:42
Operator : MA/JU
Sample : 03244-07DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 21:59:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

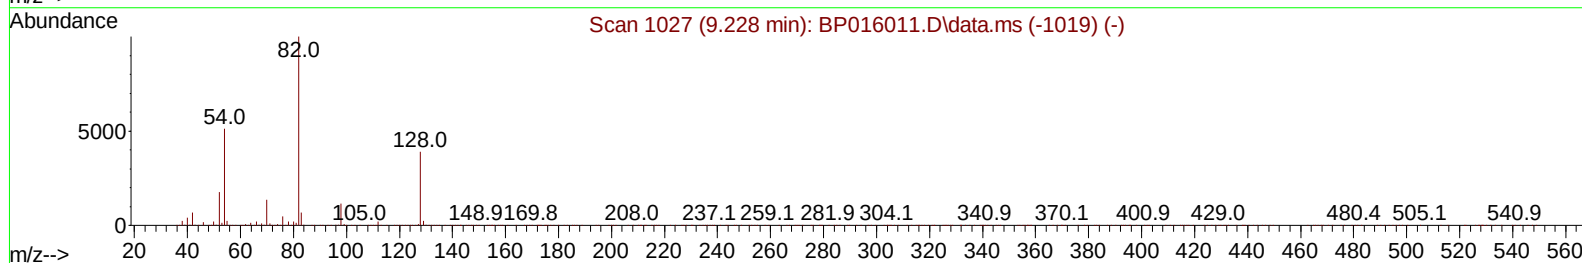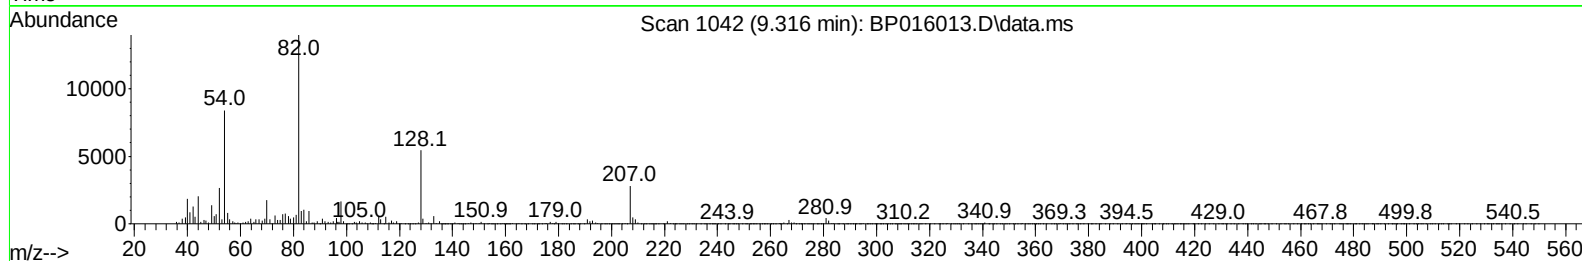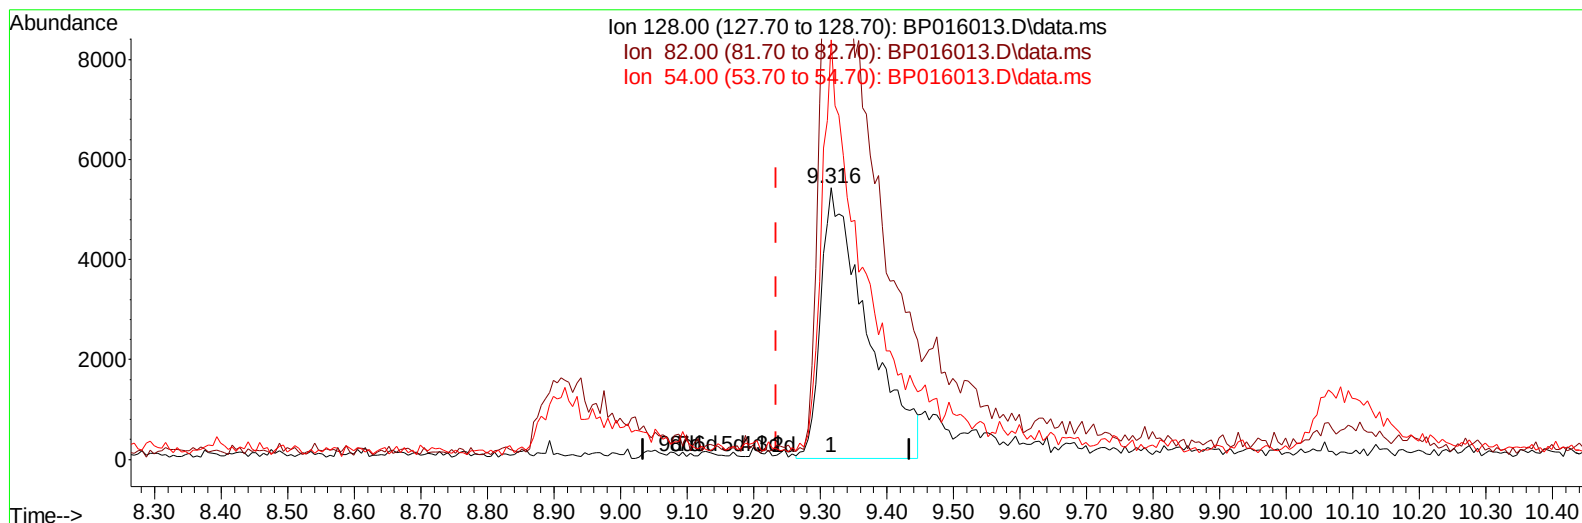

TIC: BP016013.D\data.ms

(21) Nitrobenzene-d5 (S)

9.316min (+ 0.083) 3.59 ng/ul m

response 25982

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	257.56
54.00	141.60	154.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:00:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

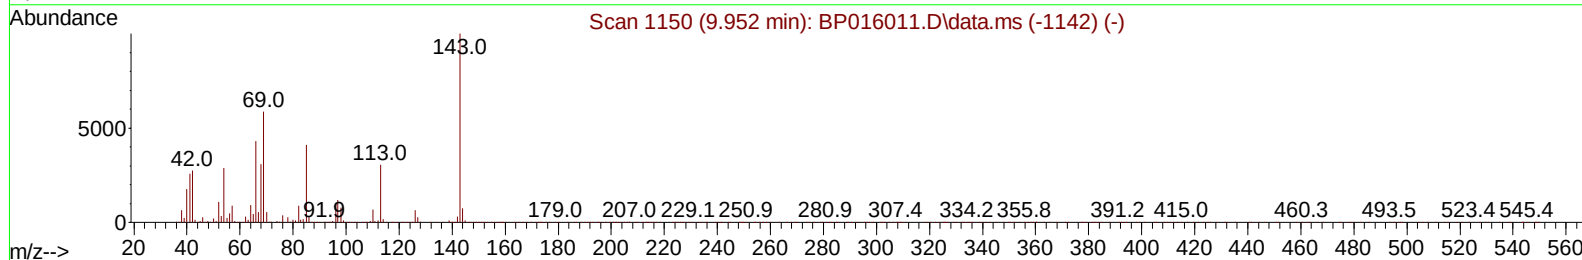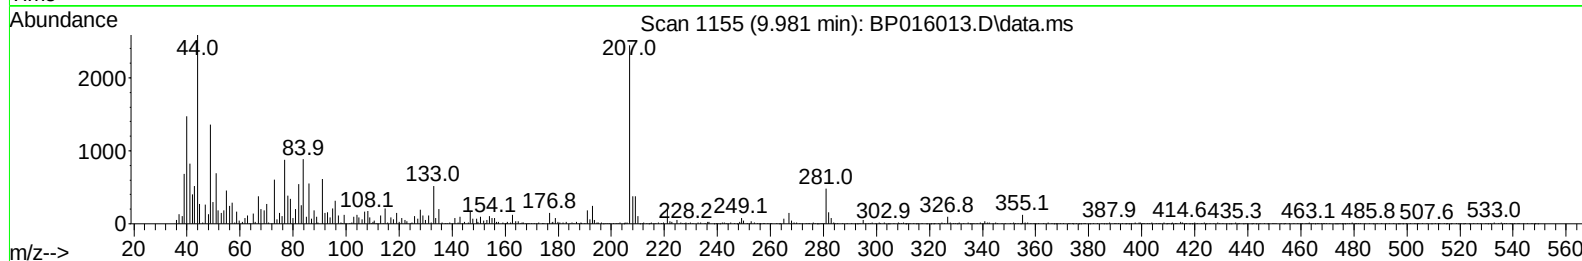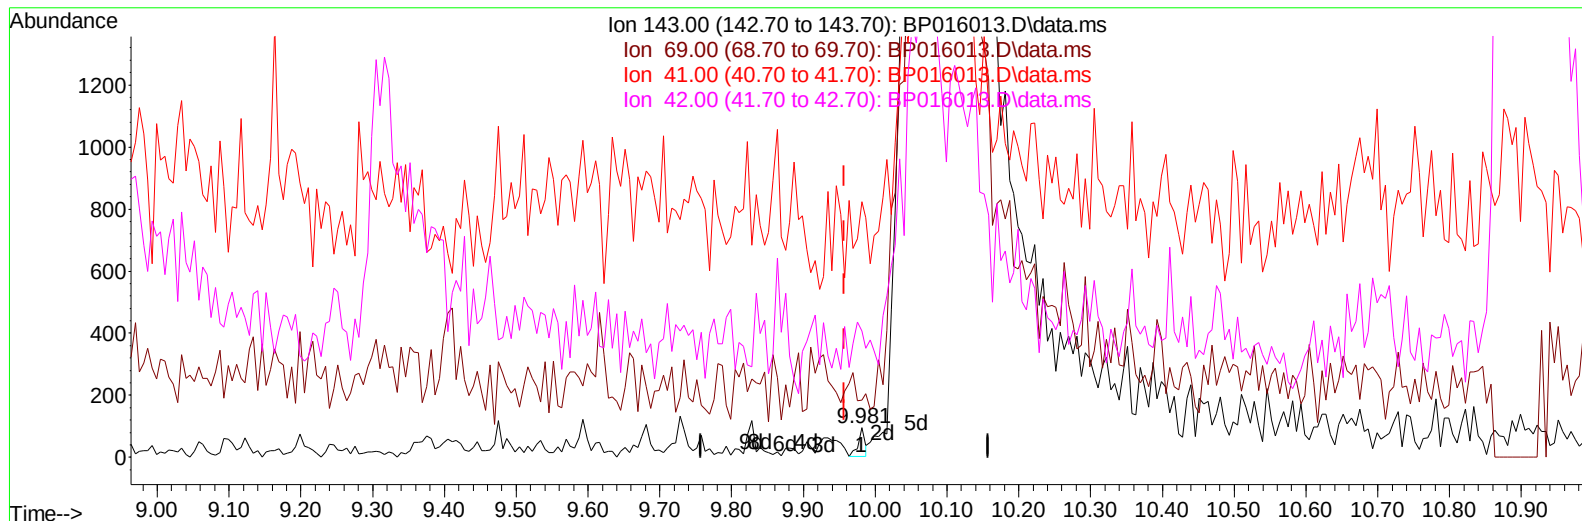

TIC: BP016013.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.981min (+ 0.024) 0.01 ng/ul

response 62

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	191.67#
41.00	26.80	857.29#
42.00	30.50	425.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:00:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

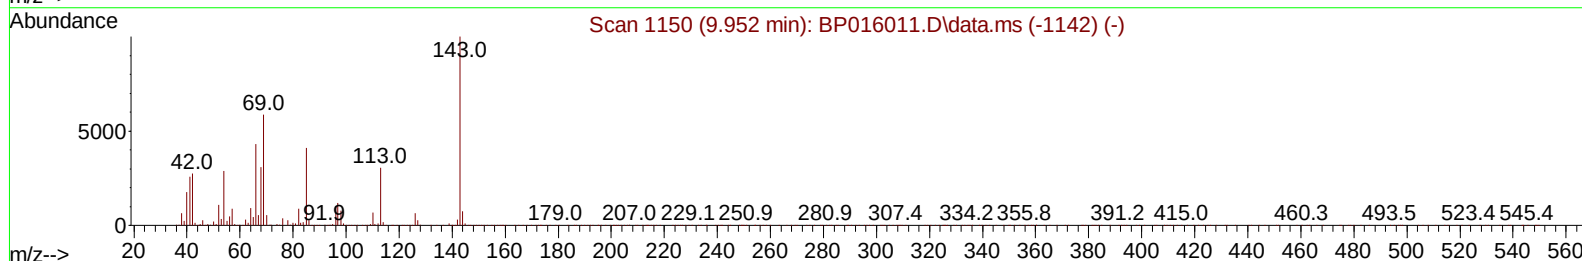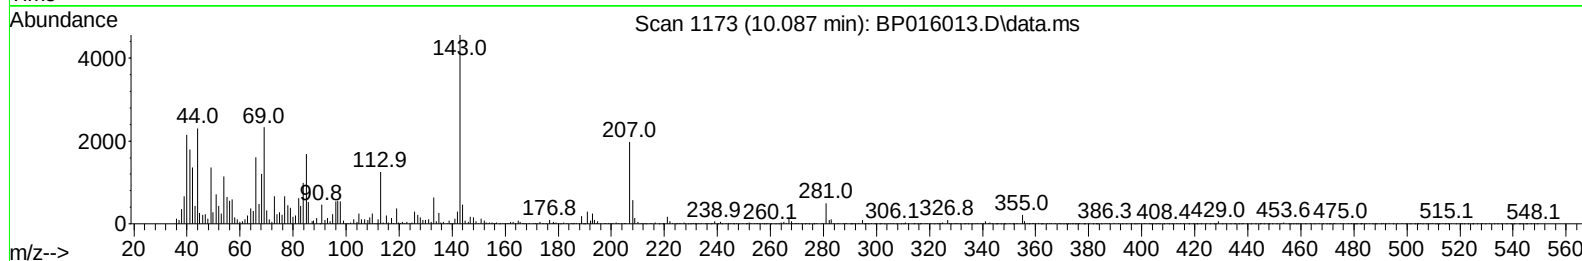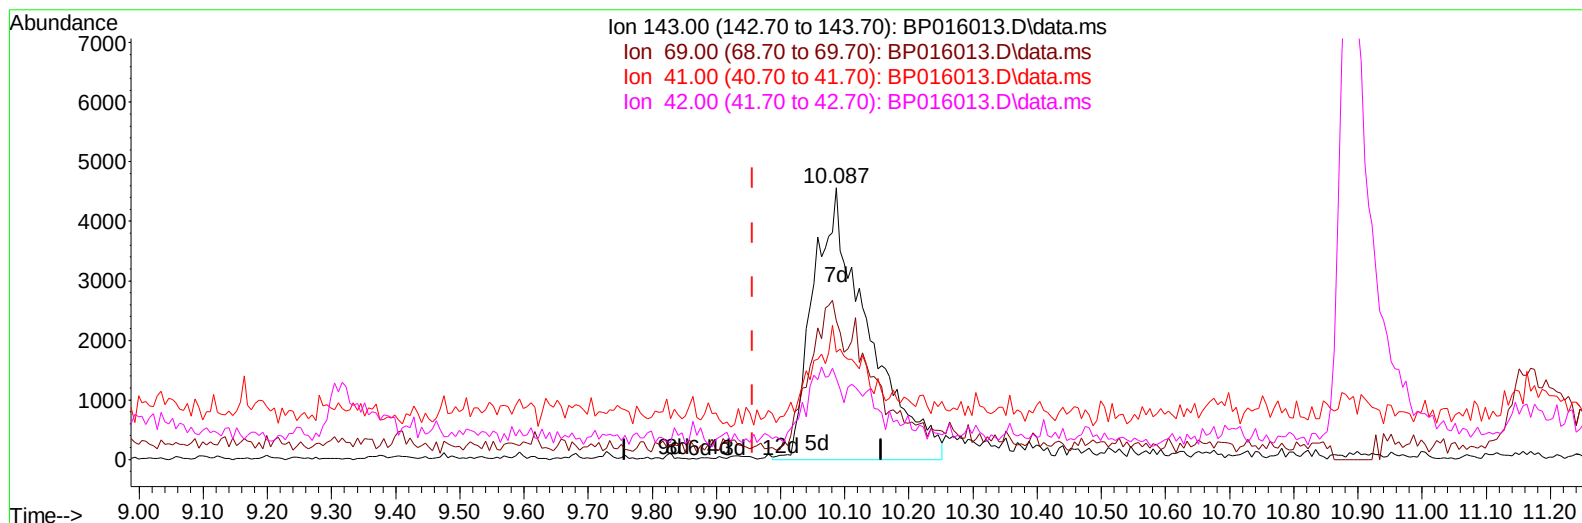

TIC: BP016013.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.087min (+ 0.130) 3.19 ng/ul m

response 26982

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	51.10
41.00	26.80	39.41#
42.00	30.50	29.78




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016013.D
Acq On : 05 Jul 2023 14:42
Operator : MA/JU
Sample : 03244-07DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:00:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

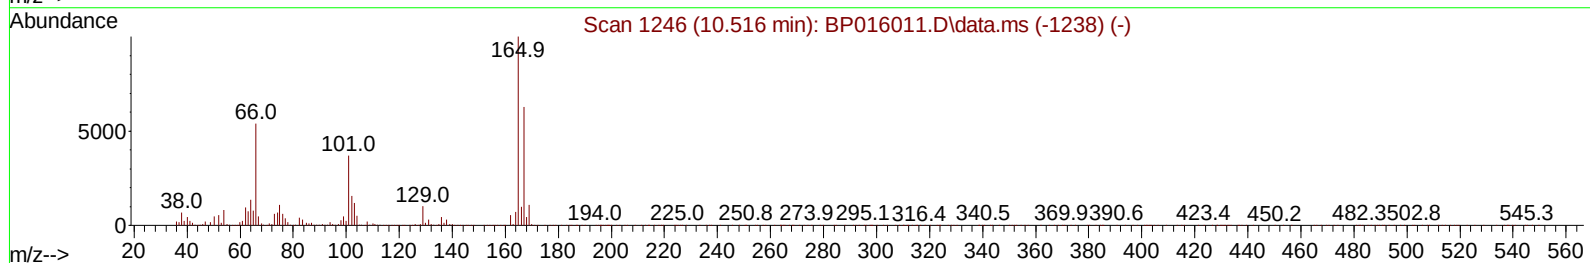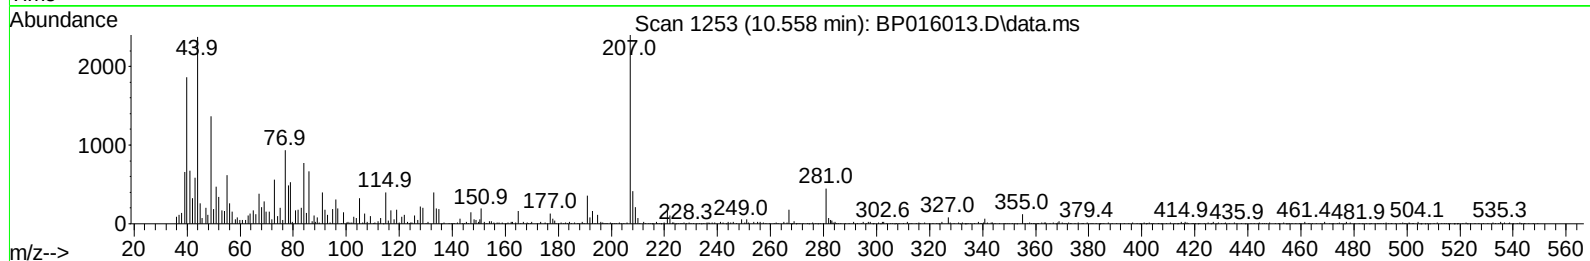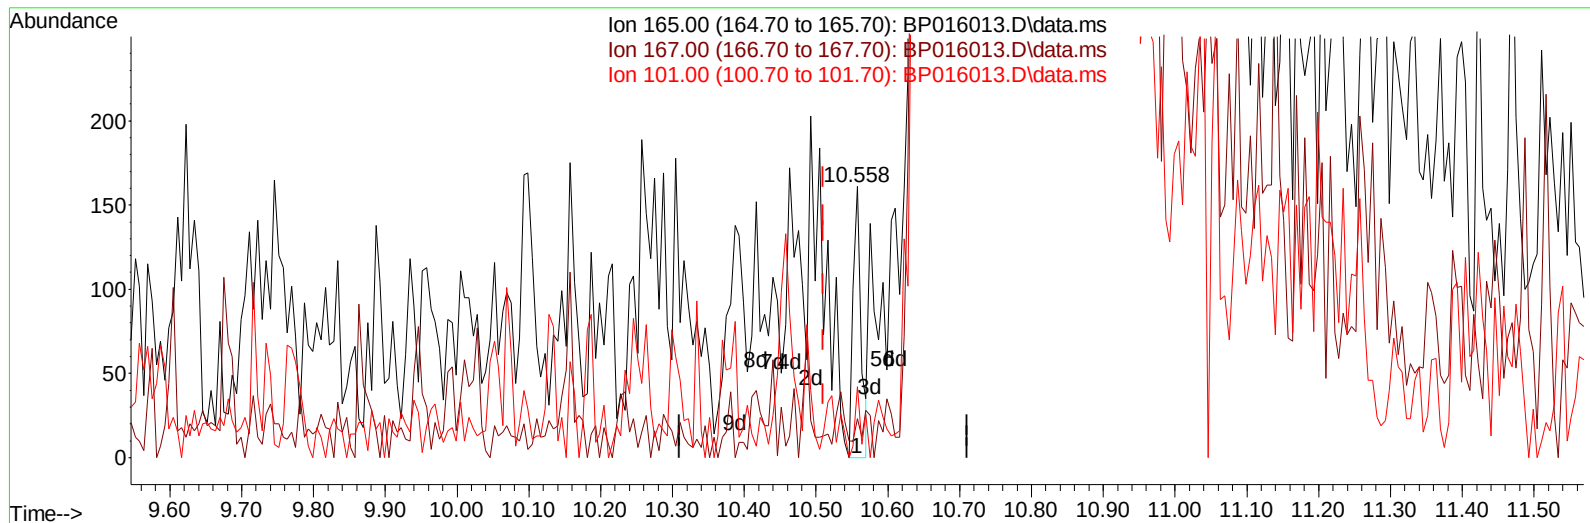

TIC: BP016013.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.558min (+ 0.048) 0.01 ng/ul

response 122

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	14.29#
101.00	37.30	26.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:00:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

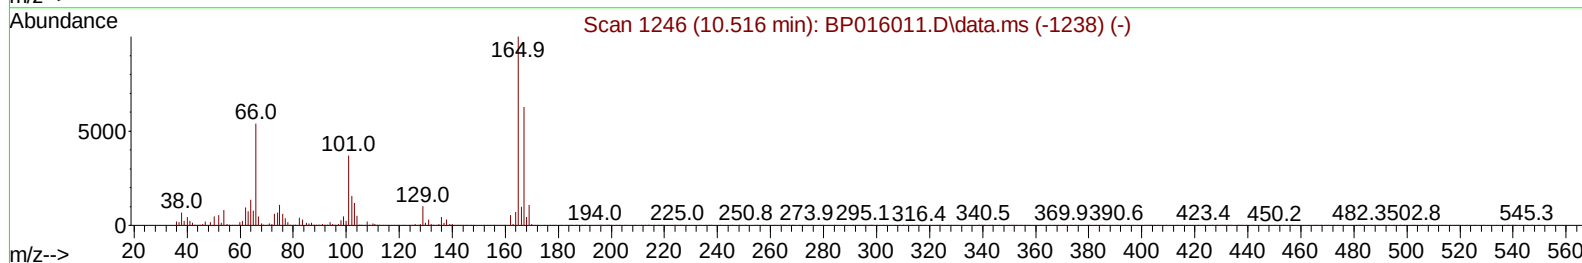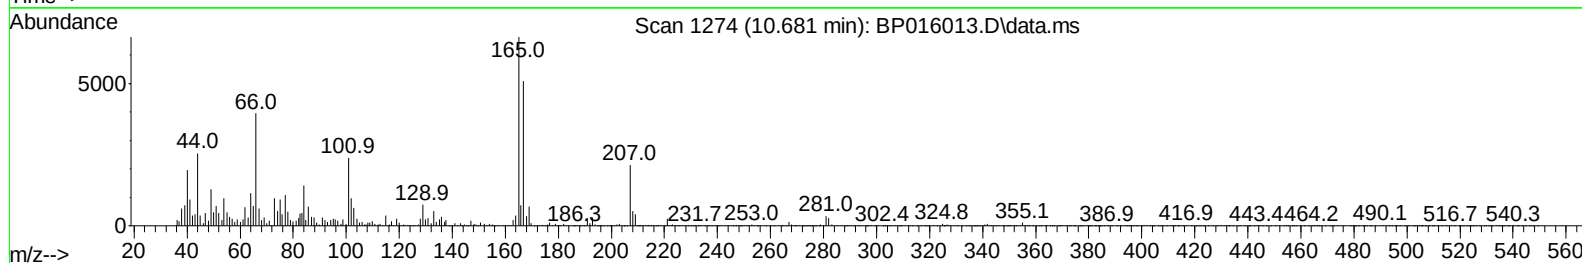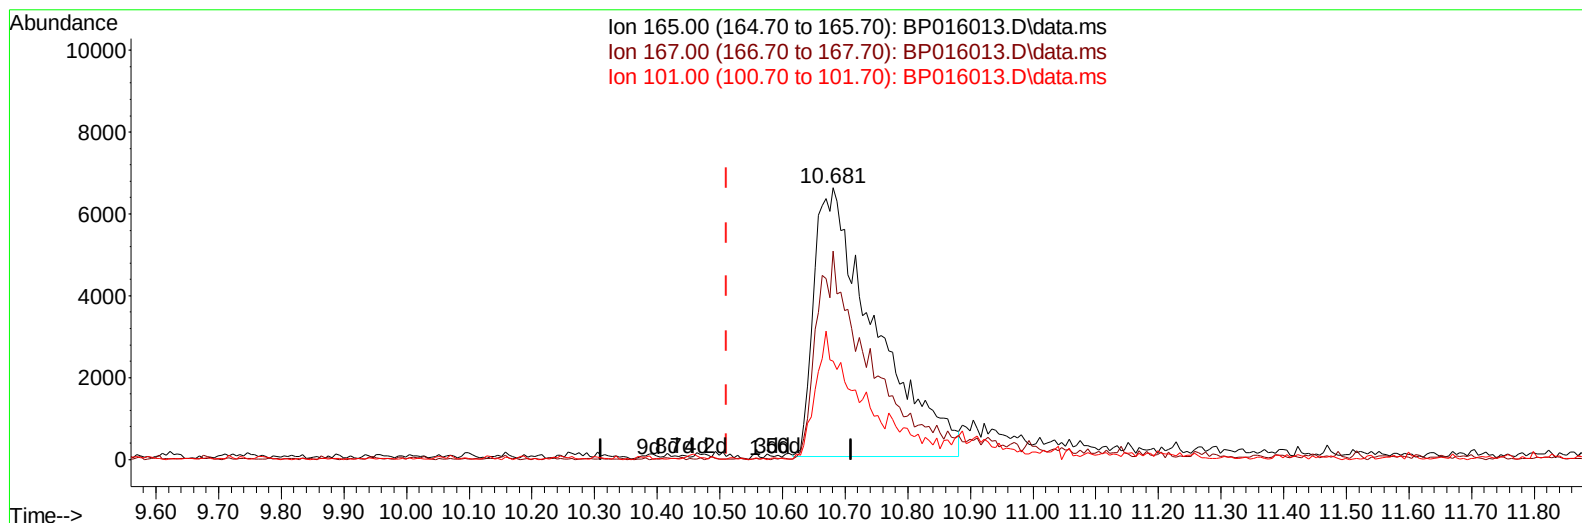

TIC: BP016013.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.681min (+ 0.171) 2.95 ng/ul m

response 44493

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	76.70
101.00	37.30	36.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:01:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

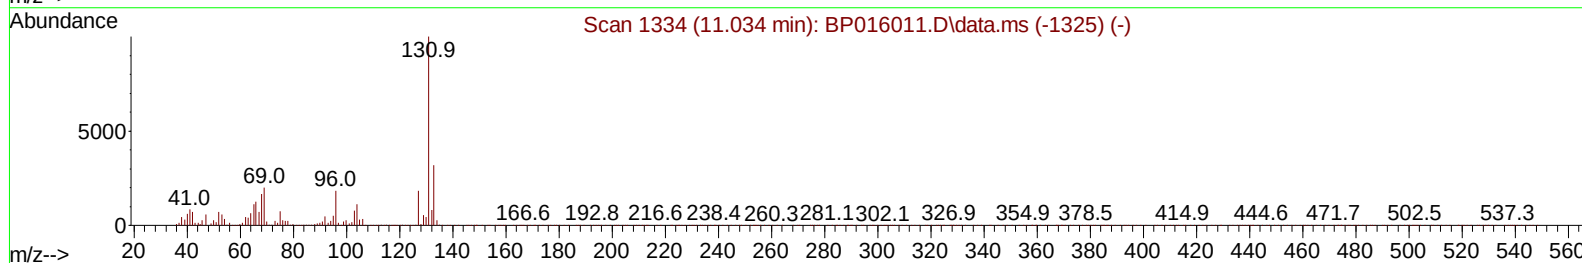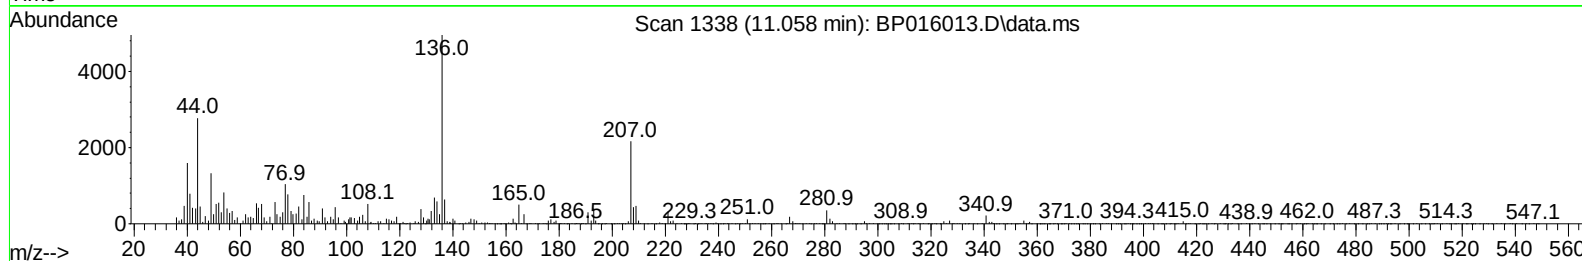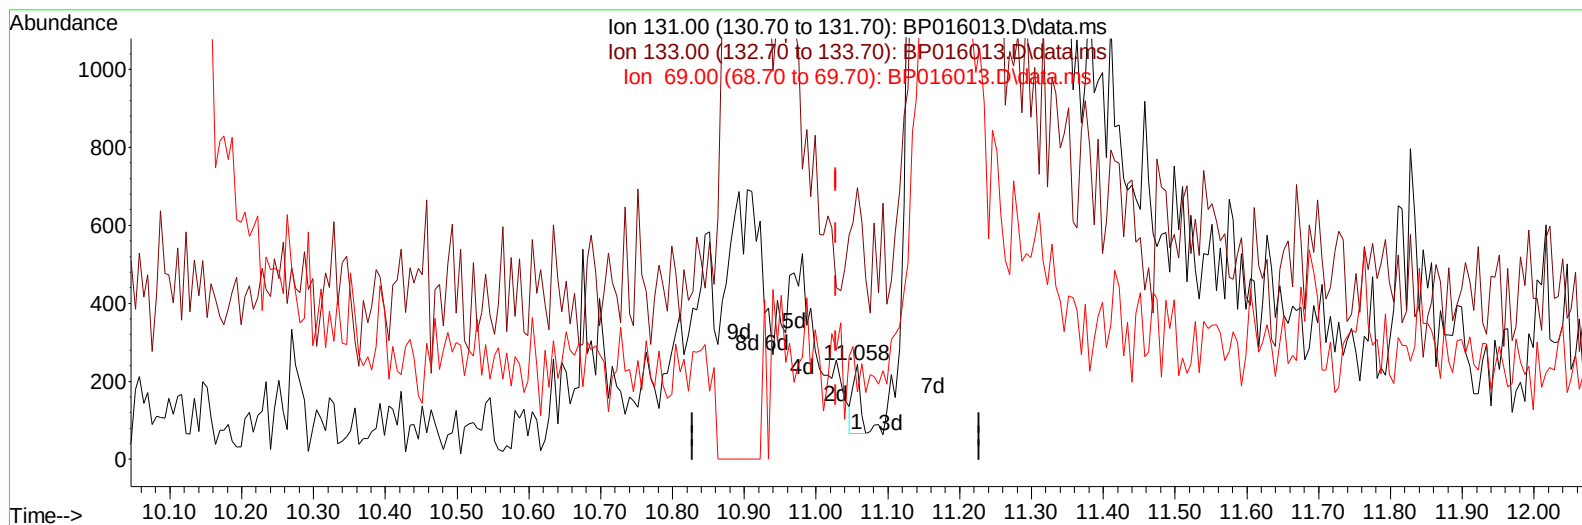

TIC: BP016013.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.058min (+ 0.030) 0.01 ng/ul

response 121

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	286.42#
69.00	22.20	71.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:01:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

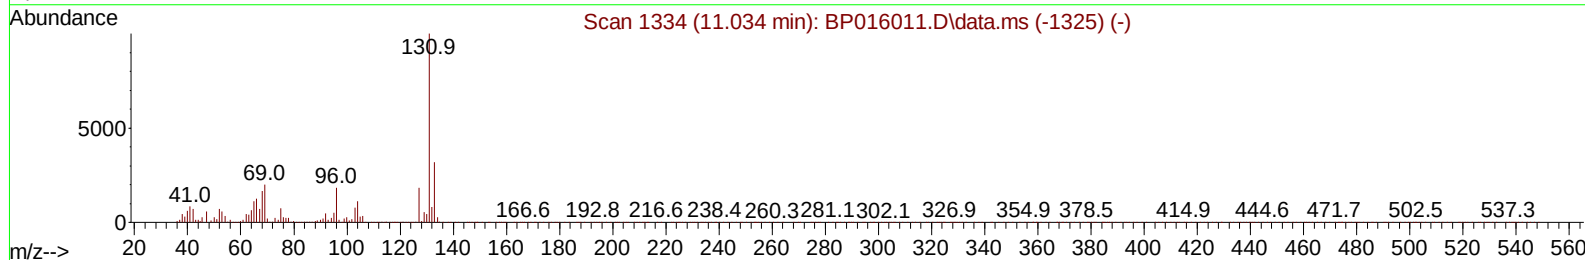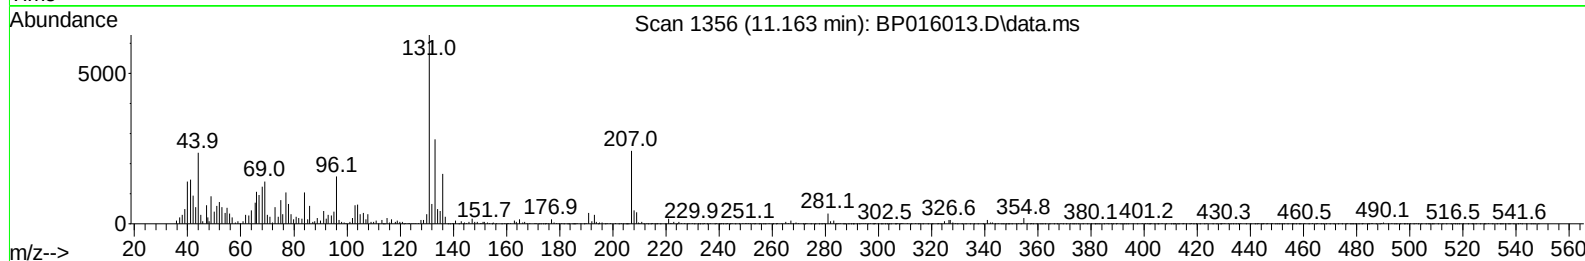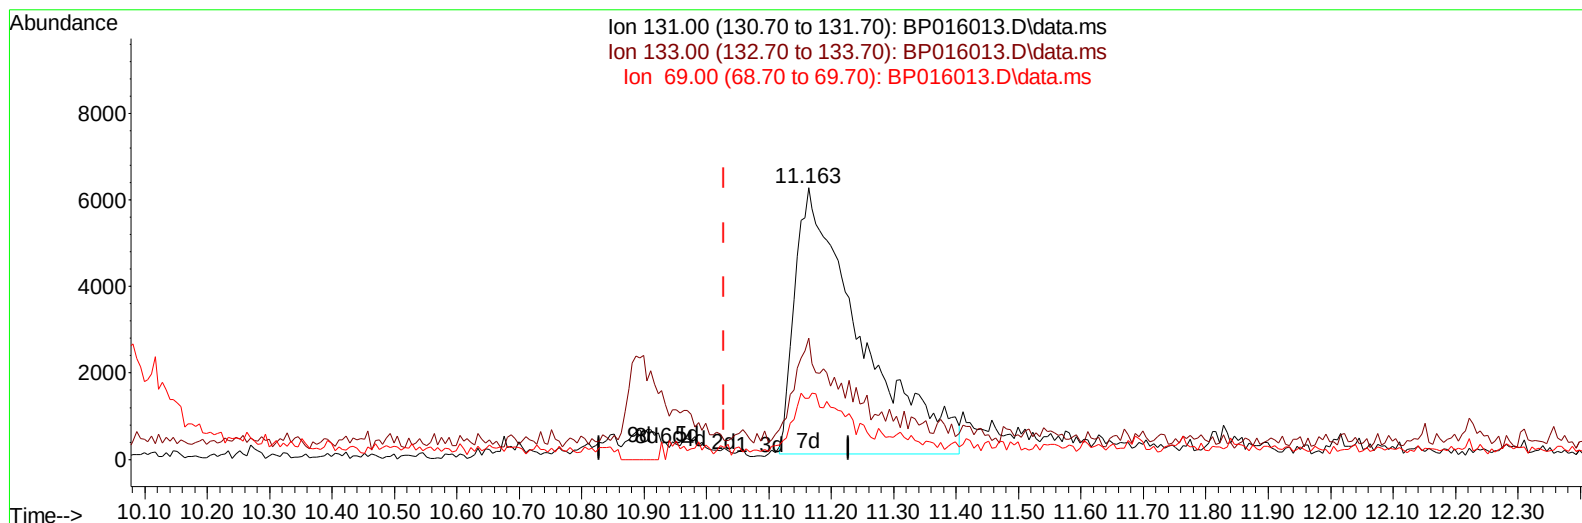

TIC: BP016013.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.163min (+ 0.136) 2.32 ng/ul m

response 44855

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	44.66#
69.00	22.20	22.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:02:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

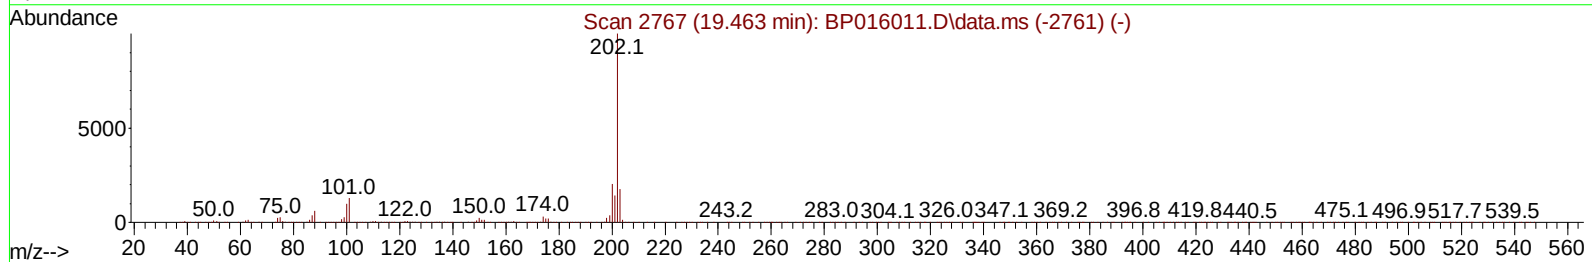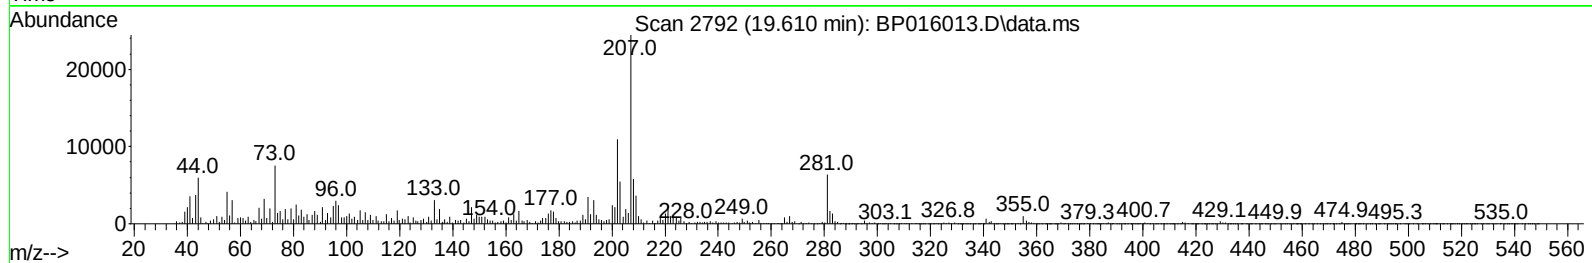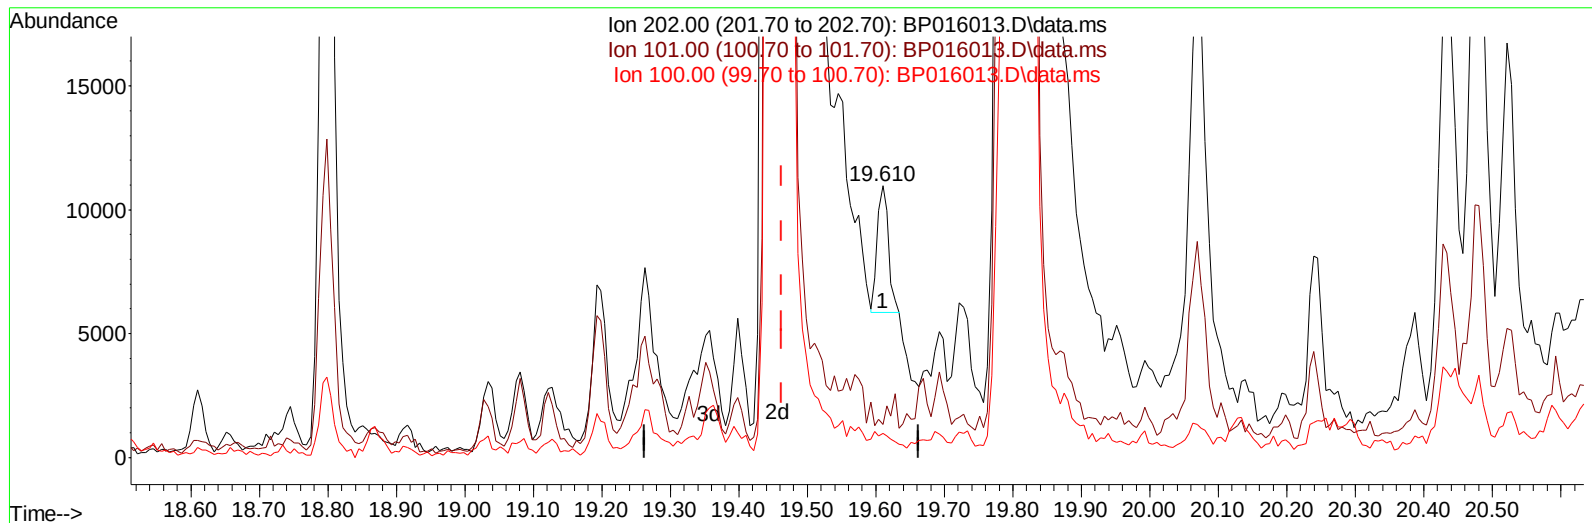

TIC: BP016013.D\data.ms

(80) Fluoranthene**19.610min (+ 0.148) 0.10 ng/u1****response 5776**

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	10.40	12.14
100.00	8.20	8.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:02:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

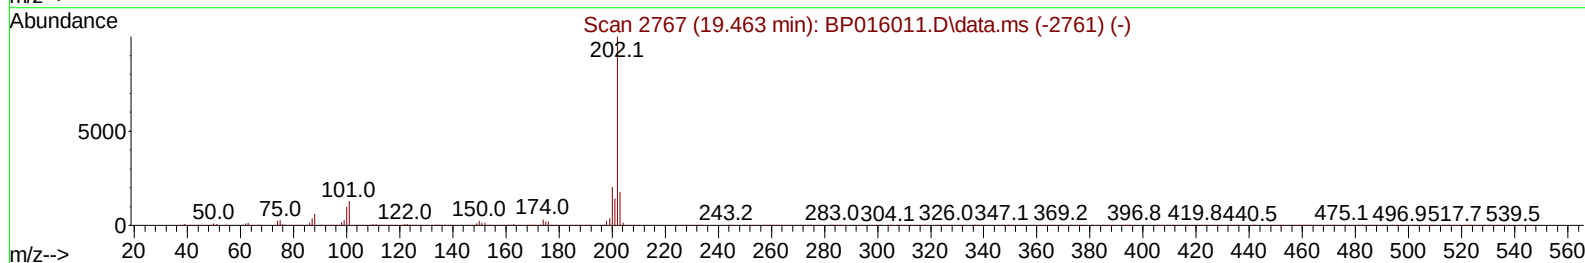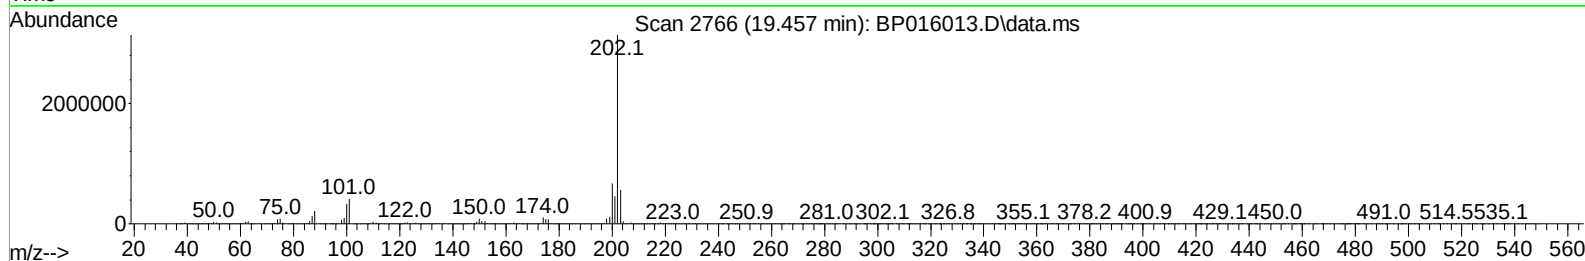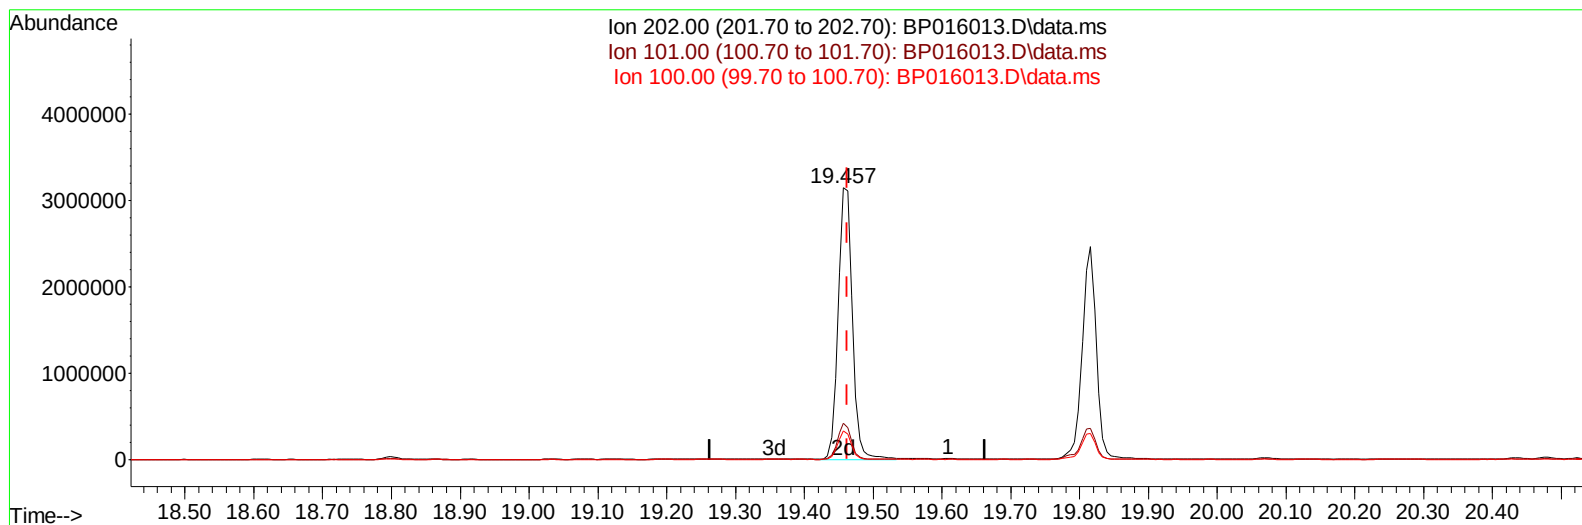

TIC: BP016013.D\data.ms

(80) Fluoranthene

19.457min (-0.005) 78.53 ng/ul m

response 4530268

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	10.40	13.30#
100.00	8.20	10.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016013.D
 Acq On : 05 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03244-07DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGE6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 05 22:03:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.058	152	213932	20.000	ng/ul	0.01
20) Naphthalene-d8	10.887	136	948081	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.698	164	547880	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	976157	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	710827	20.000	ng/ul	# 0.00
88) Perylene-d12	24.086	264	865921	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	4463	0.751	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.340	99	37546m	2.051	ng/ul	0.12
9) Bis-(2-Chloroethyl)eth...	7.417	67	46342m	4.092	ng/ul	0.05
11) 2-Chlorophenol-d4	7.640	132	51117	3.699	ng/ul	0.07
15) 4-Methylphenol-d8	8.911	113	52982m	3.664	ng/ul	0.13
21) Nitrobenzene-d5	9.316	128	25982m	3.586	ng/ul	0.08
24) 2-Nitrophenol-d4	10.087	143	26982m	3.191	ng/ul	0.13
28) 2,4-Dichlorophenol-d3	10.681	165	44493m	2.953	ng/ul	0.17
31) 4-Chloroaniline-d4	11.163	131	44855m	2.317	ng/ul	0.14
46) Dimethylphthalate-d6	14.134	166	194470	4.592	ng/ul	0.03
49) Acenaphthylene-d8	14.404	160	201356	4.230	ng/ul	0.01
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.710	176	158747	4.553	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.569	188	210264	4.716	ng/ul	0.01
81) Pyrene-d10	19.781	212	214393	4.619	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.922	264	216550	4.958	ng/ul	0.00
Target Compounds						
					Qvalue	
52) Acenaphthene	14.769	153	79372	2.182	ng/ul	97
61) Fluorene	15.763	166	83016	2.027	ng/ul	99
72) Phenanthrene	17.504	178	2004756	37.804	ng/ul	99
74) Anthracene	17.604	178	482851	9.061	ng/ul	98
80) Fluoranthene	19.457	202	4530268m	78.534	ng/ul	
82) Pyrene	19.816	202	3529090	59.974	ng/ul#	92
85) Benzo(a)anthracene	21.528	228	2103509	42.067	ng/ul	98
87) Chrysene	21.586	228	2212961	46.647	ng/ul	98
90) Benzo(b)fluoranthene	23.310	252	3030344	54.464	ng/ul#	98
91) Benzo(k)fluoranthene	23.351	252	994772	17.696	ng/ul#	96
93) Benzo(a)pyrene	23.980	252	1806953	37.167	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	26.786	276	1304590	19.767	ng/ul	97
95) Dibenzo(a,h)anthracene	26.786	278	384158	7.086	ng/ul#	81
96) Benzo(g,h,i)perylene	27.633	276	1141114	21.017	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016013.D
Acq On : 05 Jul 2023 14:42
Operator : MA/JU
Sample : 03244-07DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGE6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

Quant Time: Jul 05 22:03:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

