

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016002.D
 Acq On : 05 Jul 2023 06:22
 Operator : MA/JU
 Sample : 03244-17
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGF6

Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

Quant Time: Jul 05 08:25:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	457870	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.863	136	2061070	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.687	164	1266439	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.451	188	2745086	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1865159	20.000	ng/ul	0.00
88) Perylene-d12	24.086	264	2006424	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	36275	2.850	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.228	99	829678	21.178	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.363	67	570824	23.551	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	670146	22.661	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	574610	18.567	ng/ul	0.00
21) Nitrobenzene-d5	9.228	128	352655	22.389	ng/ul	0.00
24) 2-Nitrophenol-d4	9.957	143	388503	21.133	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	648966	19.810	ng/ul	0.01
31) 4-Chloroaniline-d4	11.040	131	566694	13.466	ng/ul	0.01
46) Dimethylphthalate-d6	14.098	166	2168471	22.153	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	2507251	22.785	ng/ul	0.00
54) 4-Nitrophenol-d4	14.987	143	242336	18.760	ng/ul	0.04
60) Fluorene-d10	15.686	176	1871433	23.219	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	172842	10.238	ng/ul	0.00
73) Anthracene-d10	17.557	188	2663123	21.239	ng/ul	0.00
81) Pyrene-d10	19.780	212	2995899	24.599	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	2399563	23.708	ng/ul	0.00
Target Compounds						
					Qvalue	
50) Acenaphthylene	14.416	152	141331	1.166	ng/ul	97
72) Phenanthrene	17.492	178	613837	4.116	ng/ul	99
80) Fluoranthene	19.457	202	1285990	8.496	ng/ul#	94
82) Pyrene	19.810	202	1012951	6.561	ng/ul#	91
85) Benzo(a)anthracene	21.527	228	532758	4.061	ng/ul	96
87) Chrysene	21.580	228	617584	4.961	ng/ul	97
90) Benzo(b)fluoranthene	23.304	252	832273	6.456	ng/ul#	96
91) Benzo(k)fluoranthene	23.351	252	247673m	1.901	ng/ul	
93) Benzo(a)pyrene	23.968	252	498503	4.425	ng/ul#	95
94) Indeno(1,2,3-cd)pyrene	26.792	276	387572	2.534	ng/ul#	90
96) Benzo(g,h,i)perylene	27.627	276	363039	2.886	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

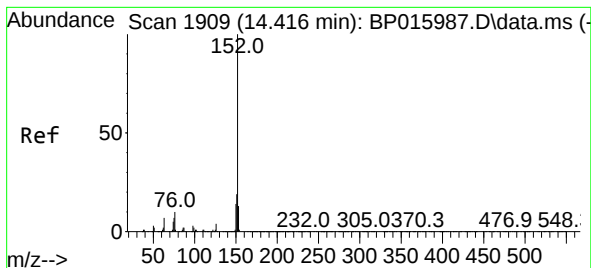

#50
Acenaphthylene
Concen: 1.166 ng/ul
RT: 14.416 min Scan# 1909
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22




Instrument :
BNA_P
ClientSampleId :
DCGF6

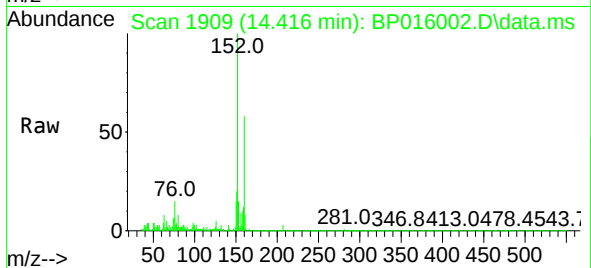


Tgt Ion:152 Resp: 14133
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.2
153 15.4 10.5 15.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

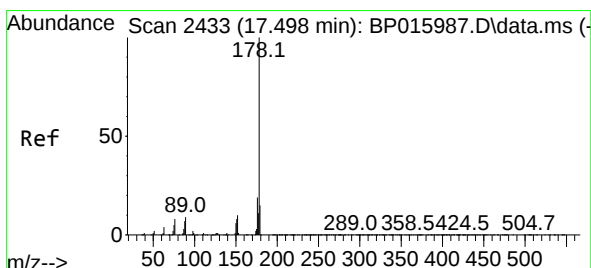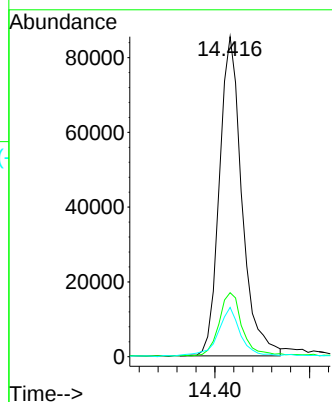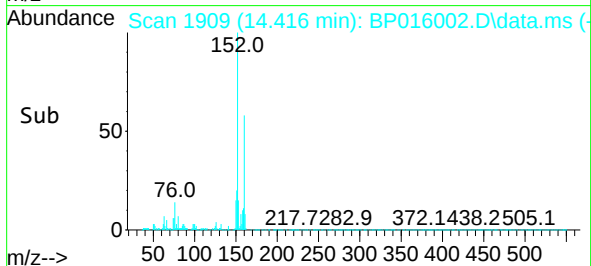


#72
Phenanthrene
Concen: 4.116 ng/ul
RT: 17.492 min Scan# 2432
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

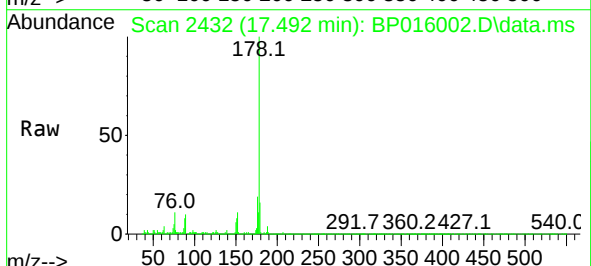


Tgt Ion:178 Resp: 613837
Ion Ratio Lower Upper
178 100
179 15.7 12.4 18.6
176 18.9 15.6 23.4

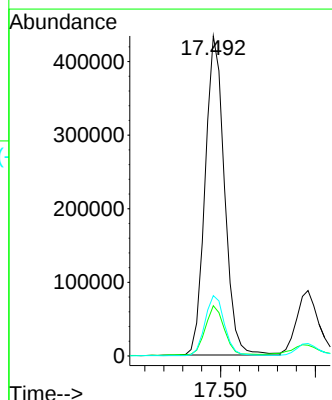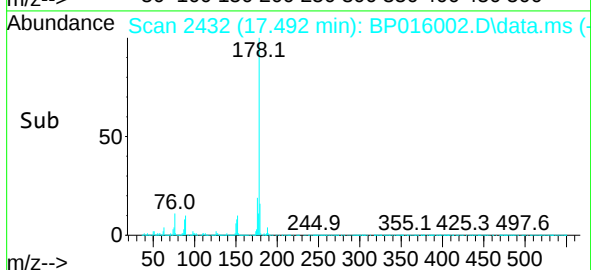

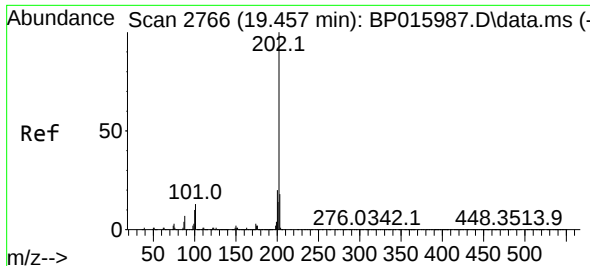

#80
Fluoranthene
Concen: 8.496 ng/u1
RT: 19.457 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22




Instrument :
BNA_P
ClientSampleId :
DCGF6

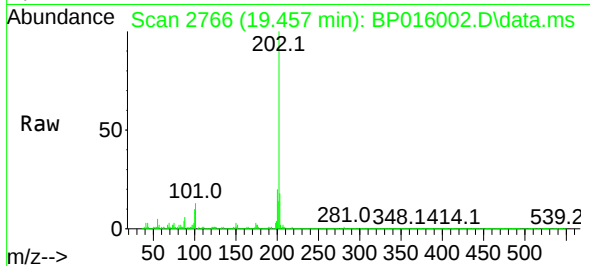


Tgt Ion:202 Resp: 1285990
Ion Ratio Lower Upper
202 100
101 12.9 8.3 12.5#
100 9.6 6.6 9.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

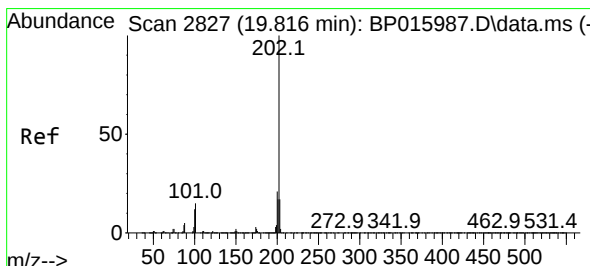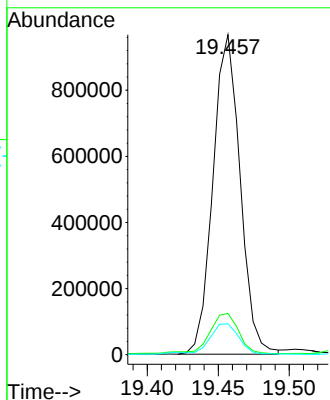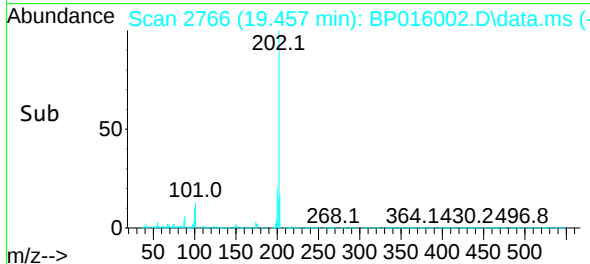


#82
Pyrene
Concen: 6.561 ng/u1
RT: 19.810 min Scan# 2826
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

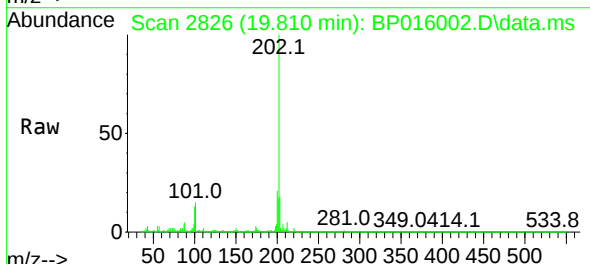


Tgt Ion:202 Resp: 1012951
Ion Ratio Lower Upper
202 100
101 15.0 9.3 13.9#
100 12.8 7.6 11.4#

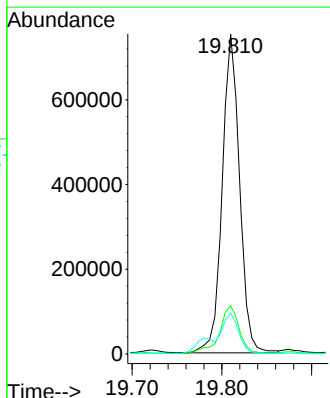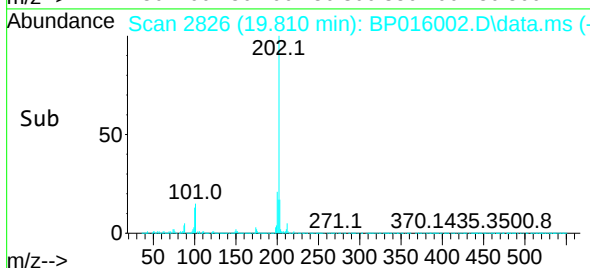

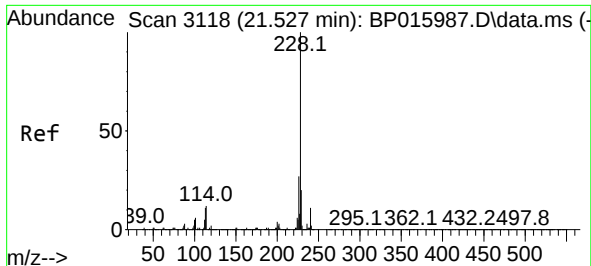

#85
Benzo(a)anthracene
Concen: 4.061 ng/ul
RT: 21.527 min Scan# 3118
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22




Instrument :
BNA_P
ClientSampleId :
DCGF6

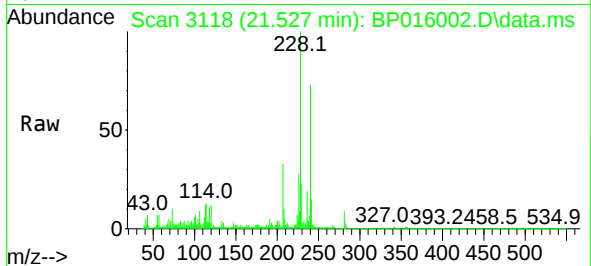


Tgt Ion:228 Resp: 532758
Ion Ratio Lower Upper
228 100
229 22.6 15.3 22.9
226 27.5 21.4 32.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

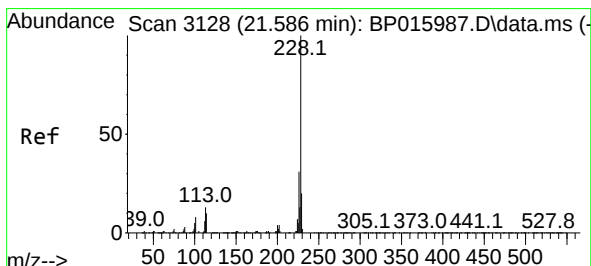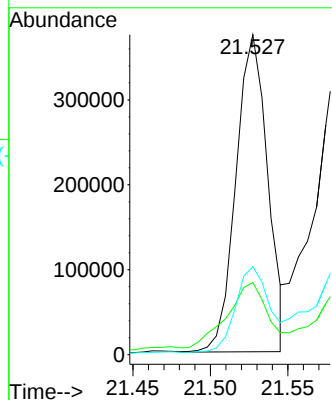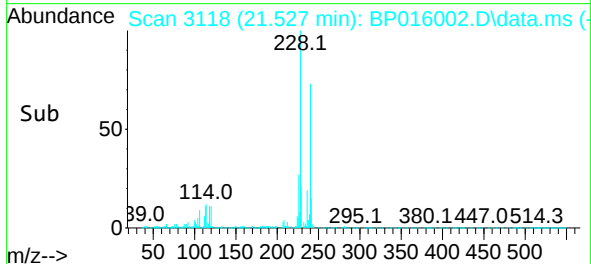


#87
Chrysene
Concen: 4.961 ng/ul
RT: 21.580 min Scan# 3127
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

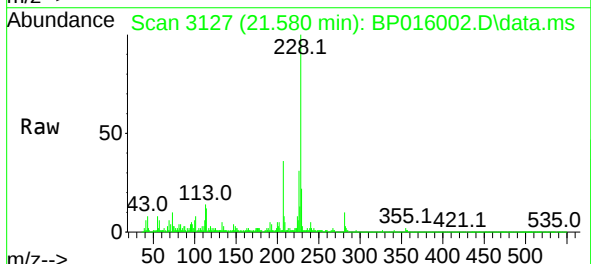

Tgt Ion:228 Resp: 617584
Ion Ratio Lower Upper
228 100
226 30.9 24.3 36.5
229 22.0 15.5 23.3

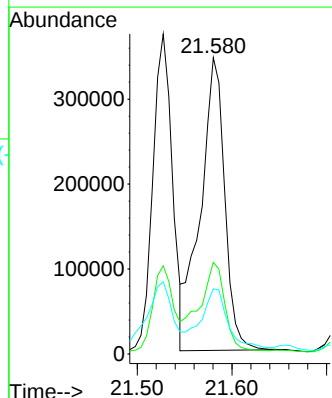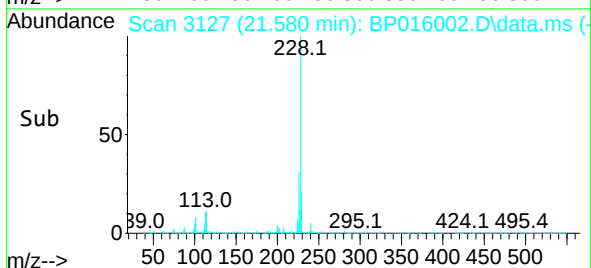

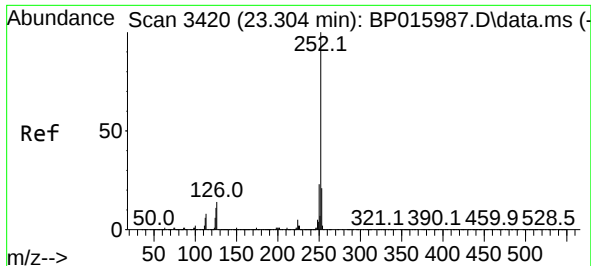


#90
Benzo(b)fluoranthene
Concen: 6.456 ng/ul
RT: 23.304 min Scan# 3420
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

Instrument :

BNA_P

ClientSampleId :

DCGF6



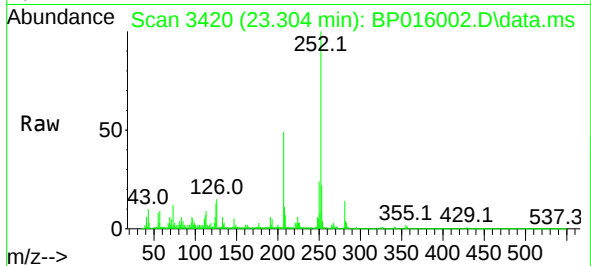


Tgt Ion:252 Resp: 832273
Ion Ratio Lower Upper
252 100
253 22.5 17.3 25.9
125 12.9 7.5 11.3


Manual Integrations

APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

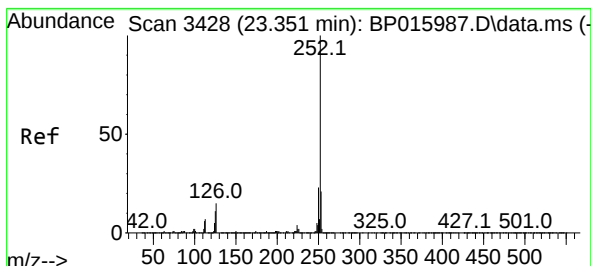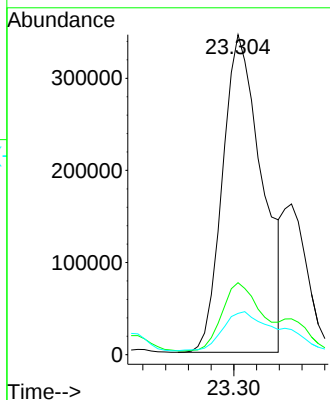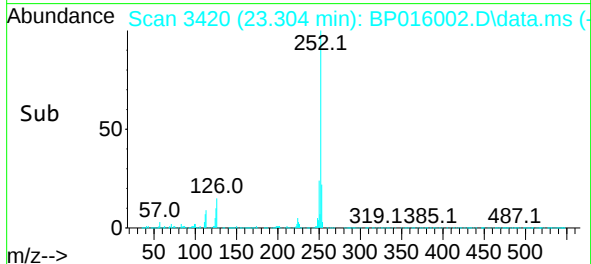


#91
Benzo(k)fluoranthene
Concen: 1.901 ng/ul m
RT: 23.351 min Scan# 3428
Delta R.T. -0.006 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

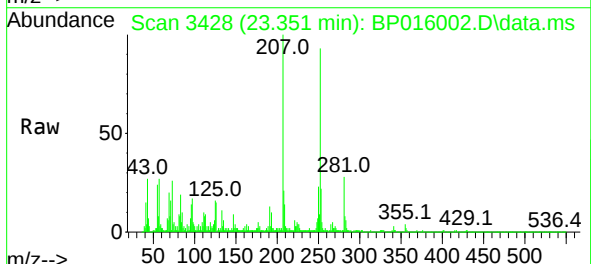


Tgt Ion:252 Resp: 247673
Ion Ratio Lower Upper
252 100
253 23.8 17.0 25.4
125 16.7 7.3 10.9

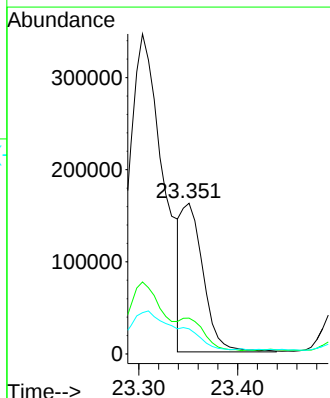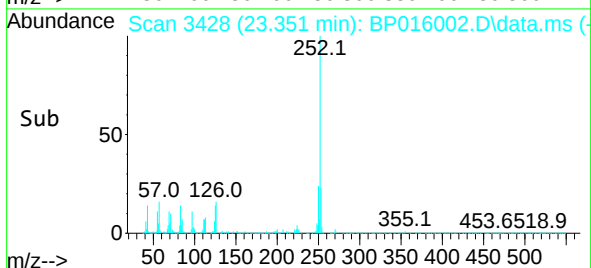

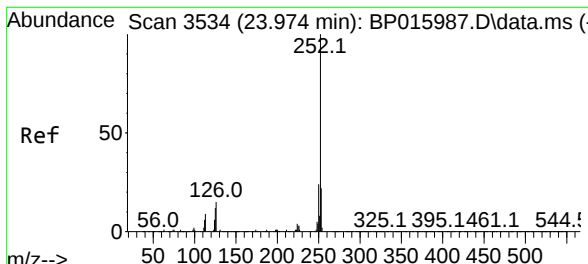

#93
Benzo(a)pyrene
Concen: 4.425 ng/ul
RT: 23.968 min Scan# 3534
Delta R.T. -0.012 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22




Instrument :
BNA_P
ClientSampleId :
DCGF6

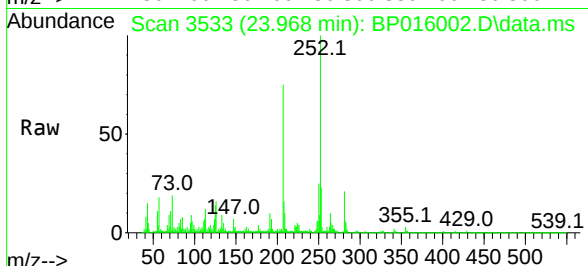


Tgt Ion: 252 Resp: 498500
Ion Ratio Lower Upper
252 100
253 23.3 17.7 26.5
125 13.5 8.2 12.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

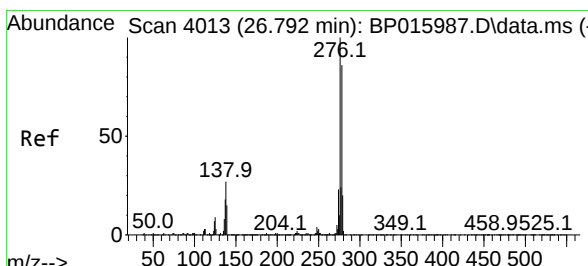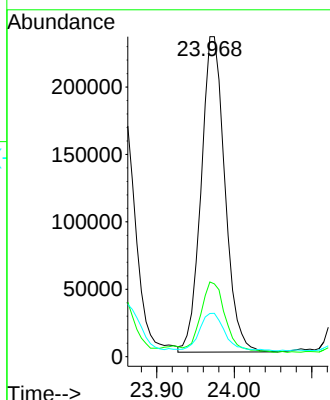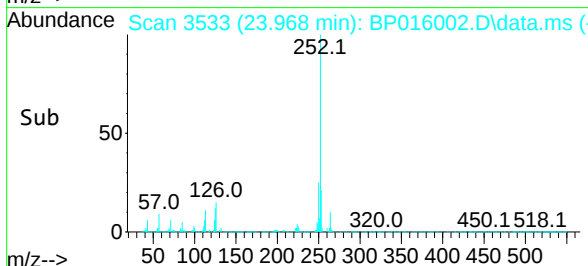


#94
Indeno(1,2,3-cd)pyrene
Concen: 2.534 ng/ul
RT: 26.792 min Scan# 4013
Delta R.T. 0.000 min
Lab File: BP016002.D
Acq: 05 Jul 2023 06:22

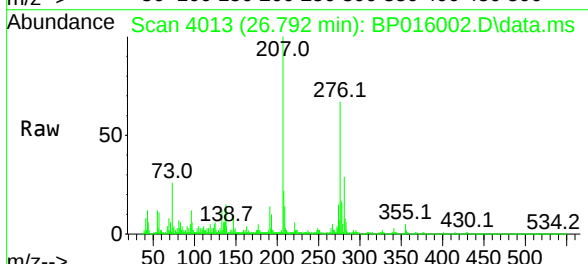


Tgt Ion: 276 Resp: 387572
Ion Ratio Lower Upper
276 100
138 29.2 15.7 23.5#
277 24.7 19.6 29.4

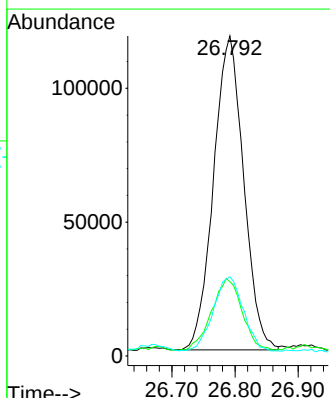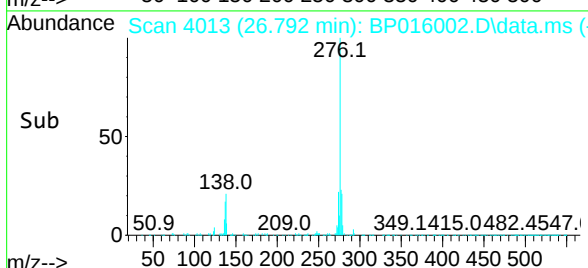

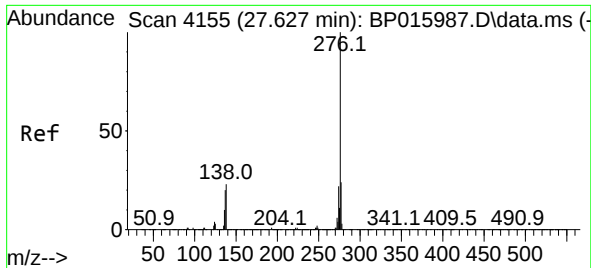

#96
 Benzo(g,h,i)perylene
 Concen: 2.886 ng/ul
 RT: 27.627 min Scan# 4155
 Delta R.T. 0.000 min
 Lab File: BP016002.D
 Acq: 05 Jul 2023 06:22

Instrument :
 BNA_P
 ClientSampleId :
 DCGF6

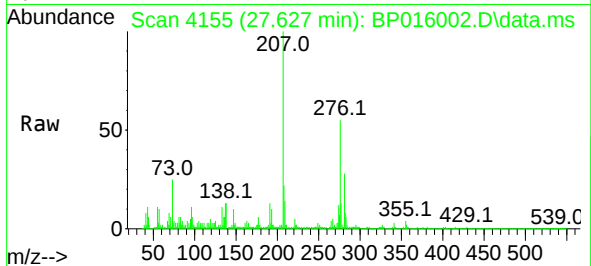

Tgt Ion:276 Resp: 363039
 Ion Ratio Lower Upper
 276 100
 138 23.0 15.1 22.7
 277 24.2 18.8 28.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

