

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016004.D
 Acq On : 05 Jul 2023 07:29
 Operator : MA/JU
 Sample : 03244-19
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGF8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :Sohil Jodhani 07/05/2023

Quant Time: Jul 05 08:47:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 02 06:12:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	308376	20.000	ng/ul	0.00
20) Naphthalene-d8	10.869	136	1339912	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.692	164	768982	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1453617	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	979261	20.000	ng/ul	# 0.00
88) Perylene-d12	24.092	264	1118142	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	34541	4.030	ng/uL	0.00
4) Pyridine-d5	3.822	84	179400	8.303	ng/ul	0.00
7) Phenol-d5	7.234	99	647025	24.522	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.363	67	469928	28.788	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	543131	27.269	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	497682	23.877	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	268631	26.233	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	298977	25.016	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	484307	22.740	ng/ul	0.02
31) 4-Chloroaniline-d4	11.046	131	466613	17.055	ng/ul	0.02
46) Dimethylphthalate-d6	14.104	166	1601858	26.951	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	1781624	26.665	ng/ul	0.00
54) 4-Nitrophenol-d4	15.010	143	139688m	17.809	ng/ul	0.06
60) Fluorene-d10	15.692	176	1276911	26.091	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	99520	11.132	ng/ul	0.02
73) Anthracene-d10	17.557	188	1564024	23.555	ng/ul	0.00
81) Pyrene-d10	19.786	212	1685709	26.362	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1527063	27.074	ng/ul	0.00
Target Compounds					Qvalue	
72) Phenanthrene	17.498	178	385010	4.875	ng/ul	98
74) Anthracene	17.604	178	92464m	1.165	ng/ul	
80) Fluoranthene	19.463	202	1025502	12.904	ng/ul	95
82) Pyrene	19.816	202	797783	9.841	ng/ul#	92
85) Benzo(a)anthracene	21.533	228	436504	6.337	ng/ul	97
87) Chrysene	21.586	228	527318	8.068	ng/ul	98
90) Benzo(b)fluoranthene	23.310	252	782696	10.894	ng/ul#	97
91) Benzo(k)fluoranthene	23.351	252	289818m	3.993	ng/ul	
93) Benzo(a)pyrene	23.980	252	492204	7.840	ng/ul#	95
94) Indeno(1,2,3-cd)pyrene	26.804	276	398195	4.672	ng/ul	97
95) Dibenzo(a,h)anthracene	26.798	278	114716m	1.639	ng/ul	
96) Benzo(g,h,i)perylene	27.639	276	370683	5.287	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016004.D
Acq On : 05 Jul 2023 07:29
Operator : MA/JU
Sample : 03244-19
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
DCGF8

Quant Time: Jul 05 08:47:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 02 06:12:16 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

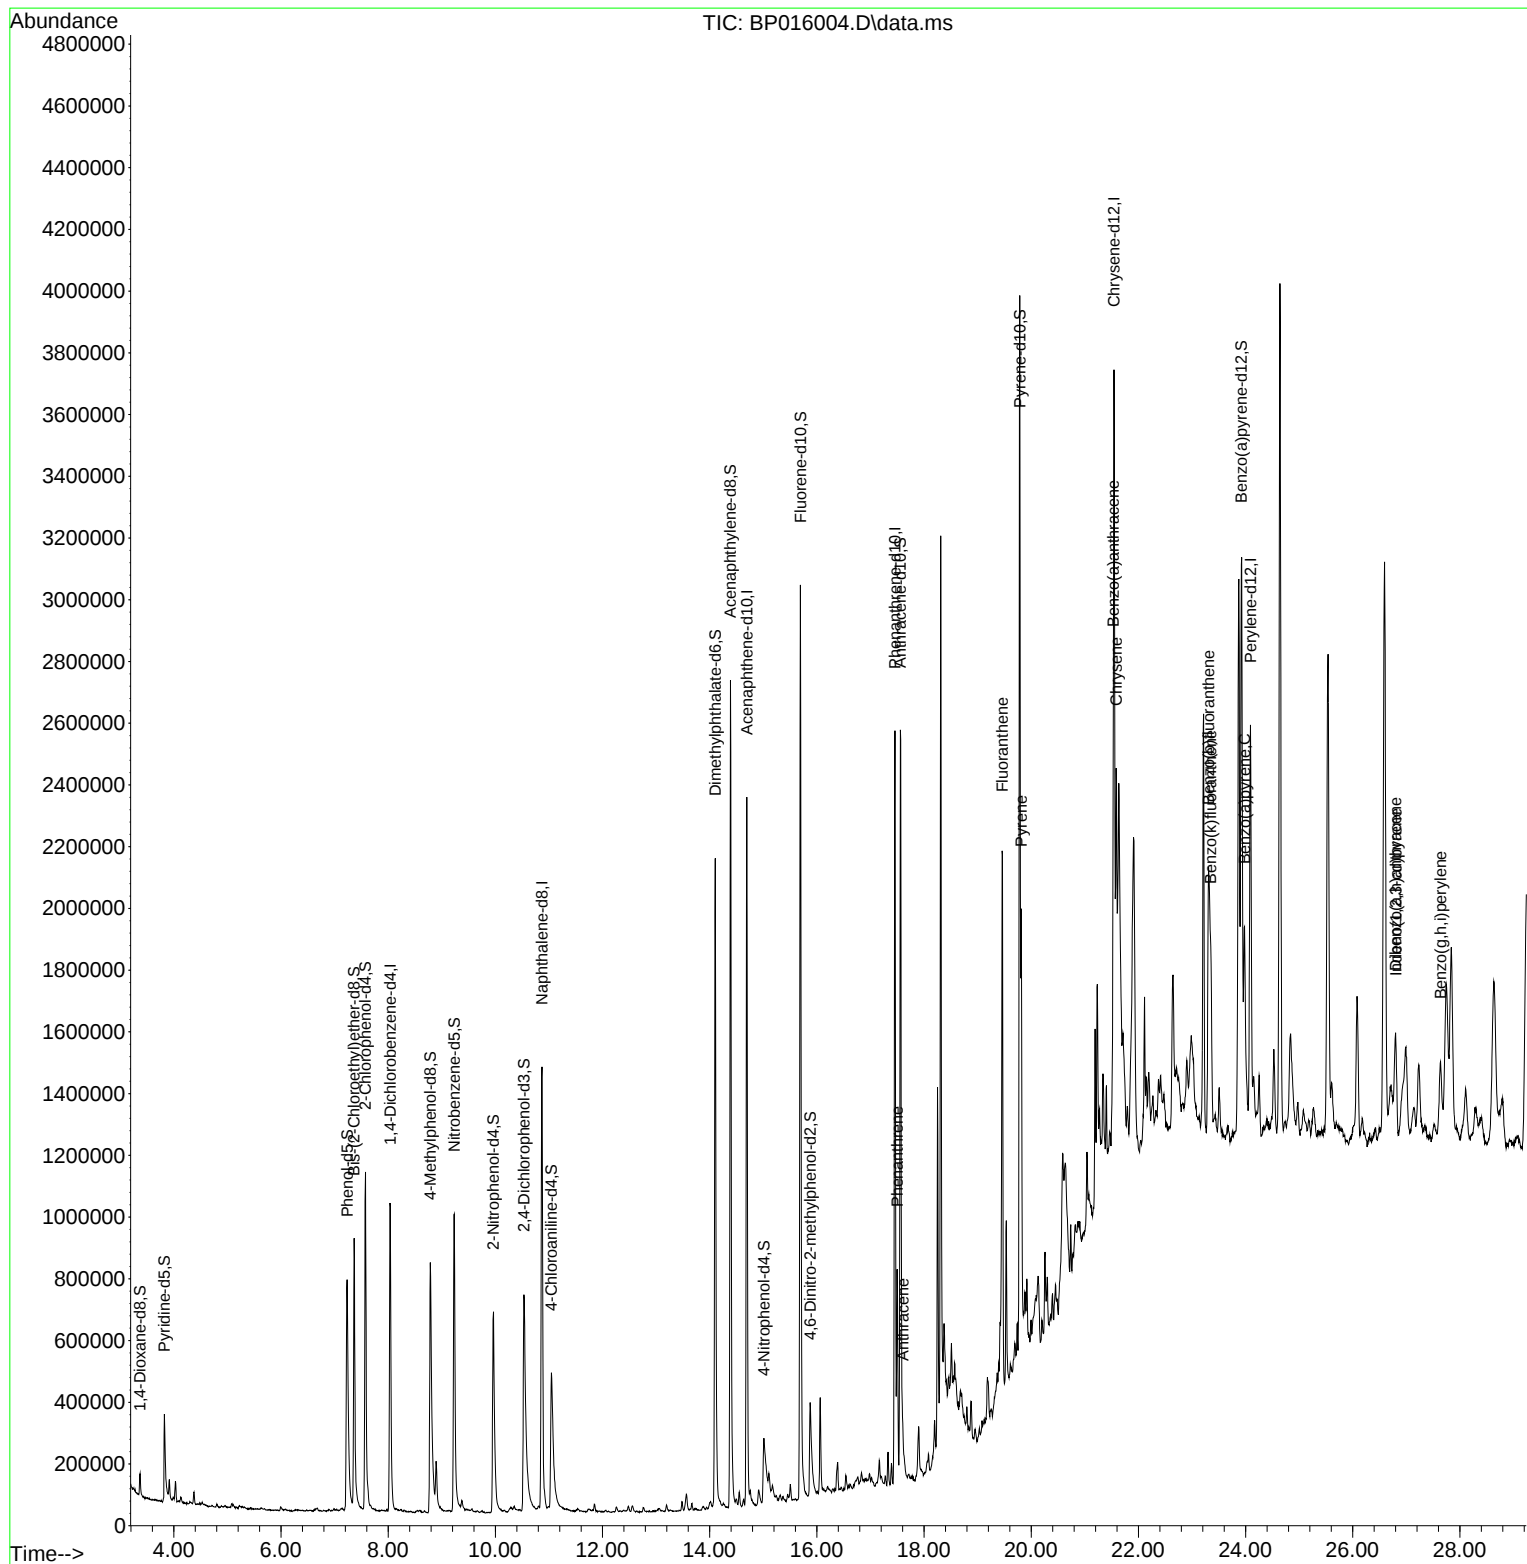

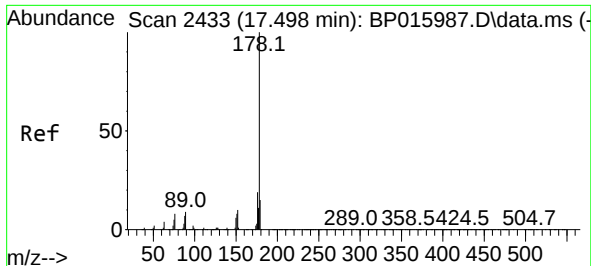

#72
Phenanthrene
Concen: 4.875 ng/ul
RT: 17.498 min Scan# 2433
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29




Instrument :
BNA_P
Client SampleId :
DCGF8

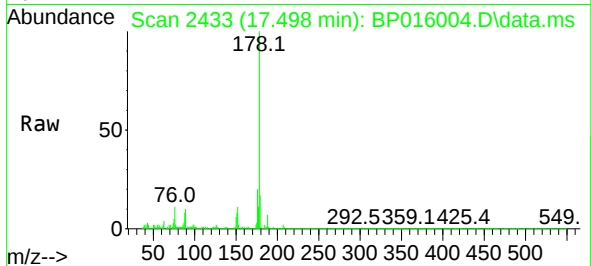


Tgt Ion:178 Resp: 385010
Ion Ratio Lower Upper
178 100
179 16.7 12.4 18.6
176 19.8 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

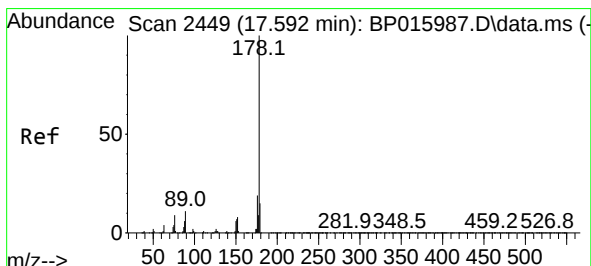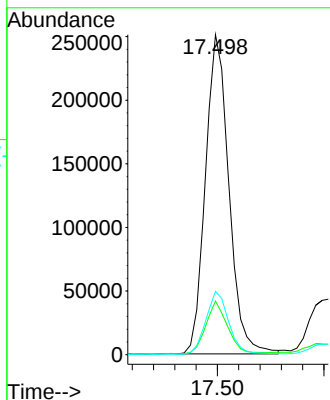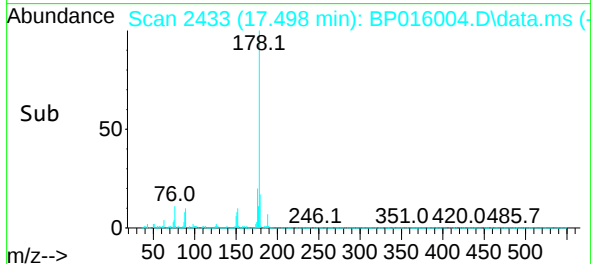


#74
Anthracene
Concen: 1.165 ng/ul m
RT: 17.604 min Scan# 2451
Delta R.T. 0.006 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29

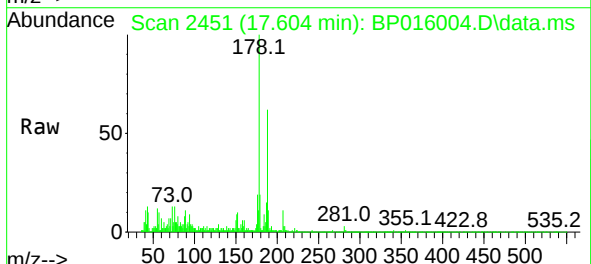

Tgt Ion:178 Resp: 92464
Ion Ratio Lower Upper
178 100
179 18.7 12.1 18.1#
176 19.1 14.6 22.0

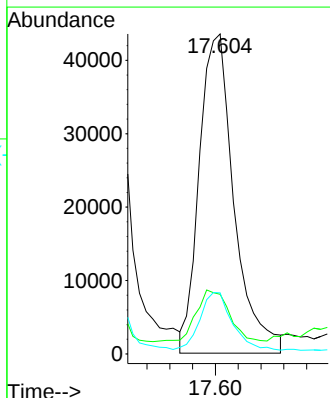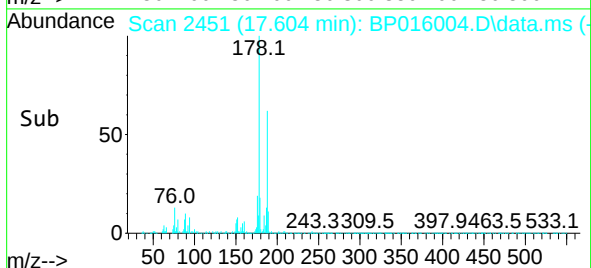

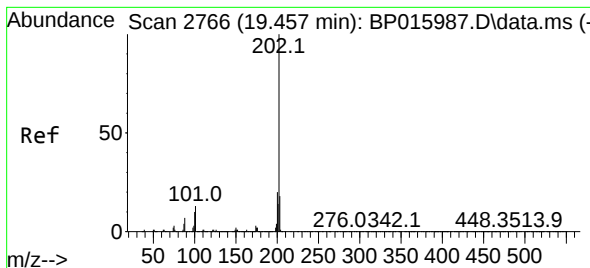





#80
Fluoranthene
Concen: 12.904 ng/ul
RT: 19.463 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29

Instrument :
BNA_P
ClientSampleId :
DCGF8

Tgt Ion:202 Resp: 102550
Ion Ratio Lower Upper
202 100
101 12.4 8.3 12.5
100 9.5 6.6 9.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

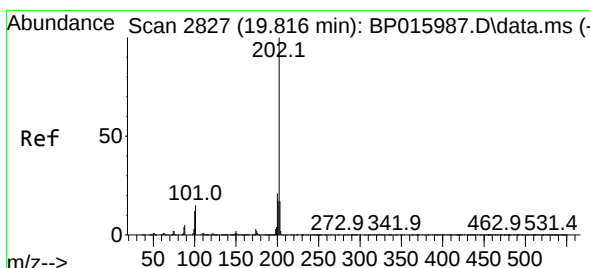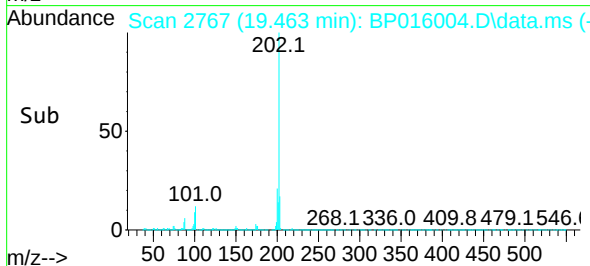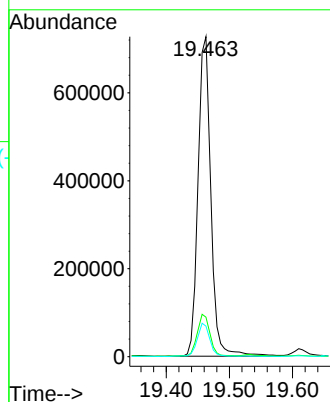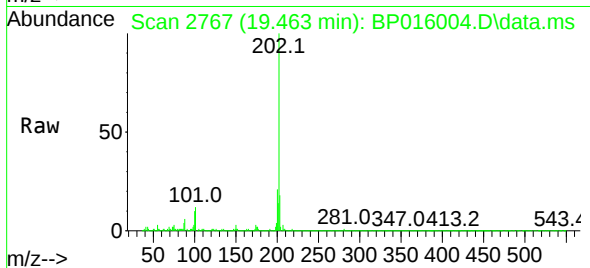

#82
Pyrene
Concen: 9.841 ng/ul
RT: 19.816 min Scan# 2827
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29


Tgt Ion:202 Resp: 797783
Ion Ratio Lower Upper
202 100
101 14.6 9.3 13.9#
100 12.5 7.6 11.4#

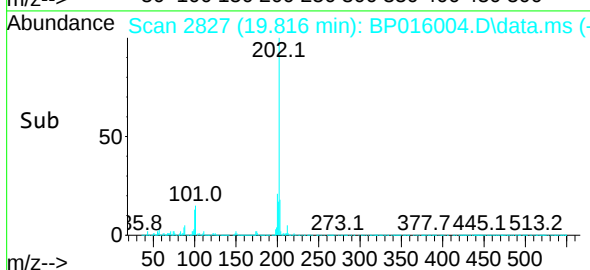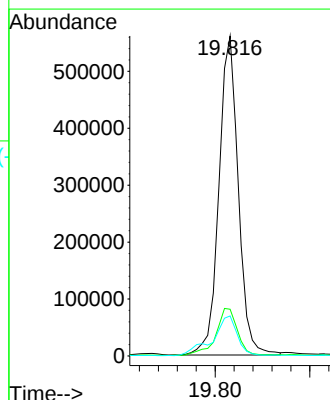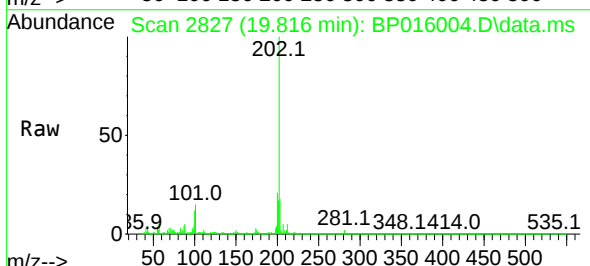

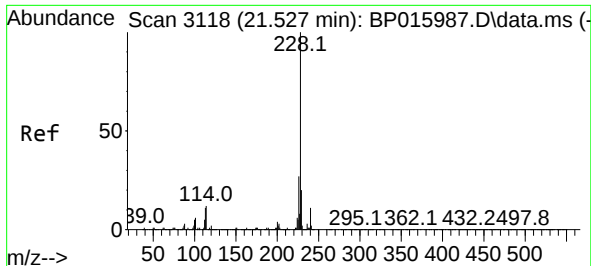

#85
Benzo(a)anthracene
Concen: 6.337 ng/u1
RT: 21.533 min Scan# 3119
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29




Instrument :
BNA_P
ClientSampleId :
DCGF8

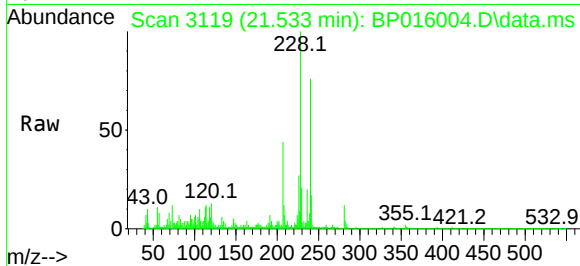


Tgt Ion:228 Resp: 436504
Ion Ratio Lower Upper
228 100
229 21.4 15.3 22.9
226 27.1 21.4 32.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

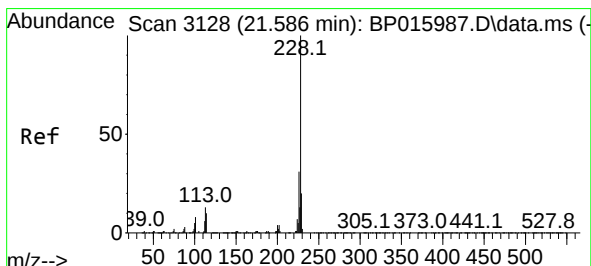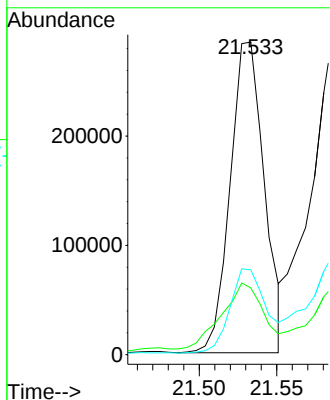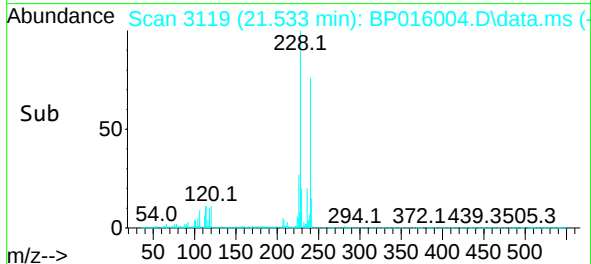


#87
Chrysene
Concen: 8.068 ng/u1
RT: 21.586 min Scan# 3128
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29

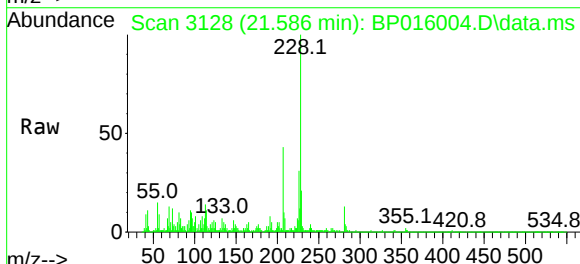


Tgt Ion:228 Resp: 527318
Ion Ratio Lower Upper
228 100
226 31.1 24.3 36.5
229 21.3 15.5 23.3

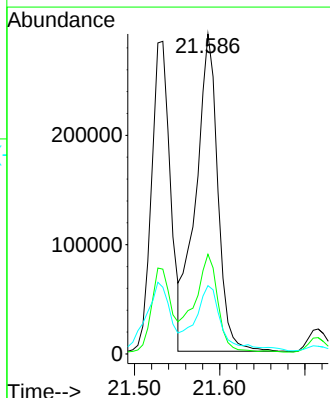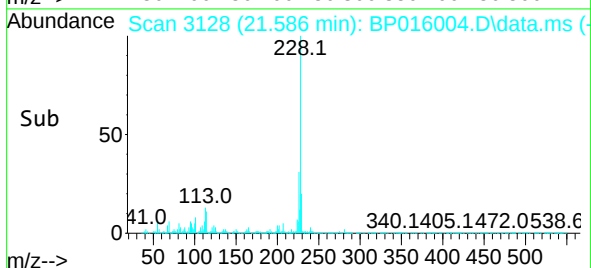

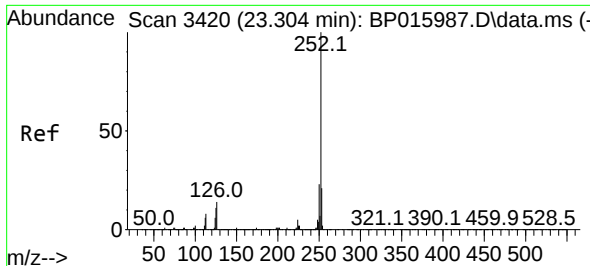

#90
Benzo(b)fluoranthene
Concen: 10.894 ng/ul
RT: 23.310 min Scan# 3421
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29




Instrument :
BNA_P
ClientSampleId :
DCGF8

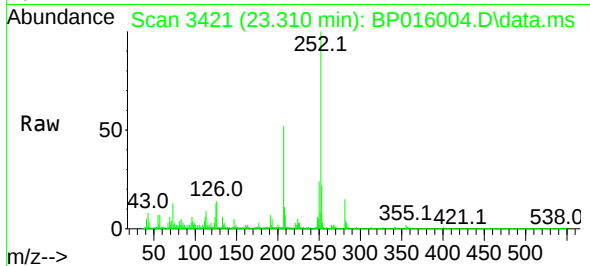

Tgt Ion:252 Resp: 782690
Ion Ratio Lower Upper
252 100
253 21.9 17.3 25.9
125 12.8 7.5 11.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

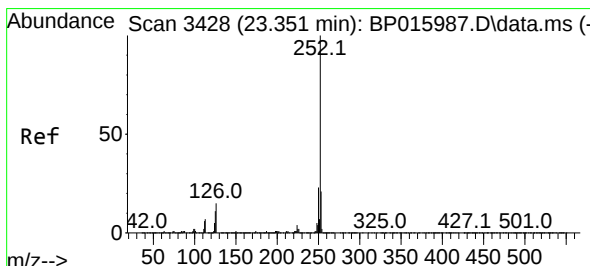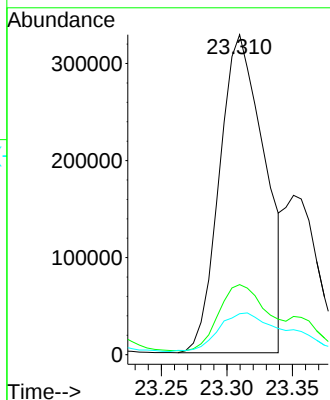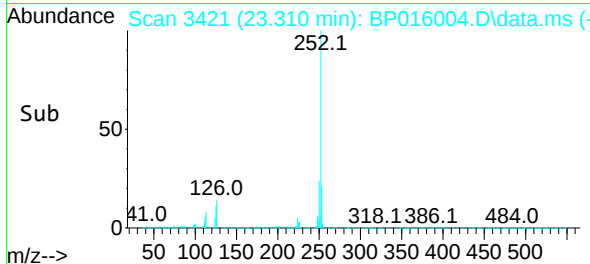

#91
Benzo(k)fluoranthene
Concen: 3.993 ng/ul m
RT: 23.351 min Scan# 3428
Delta R.T. -0.006 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29


Tgt Ion:252 Resp: 289818
Ion Ratio Lower Upper
252 100
253 24.0 17.0 25.4
125 15.7 7.3 10.9

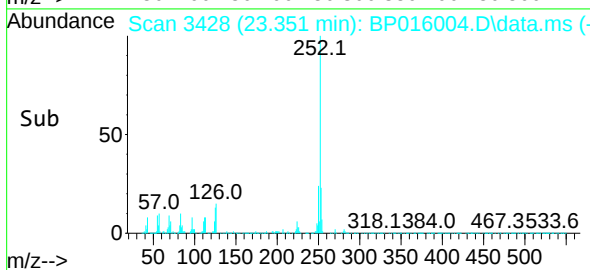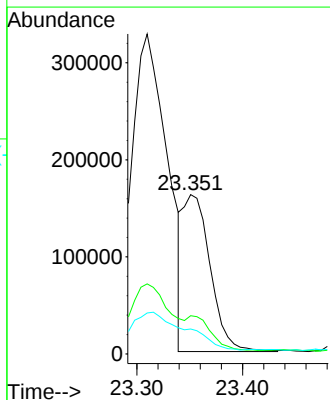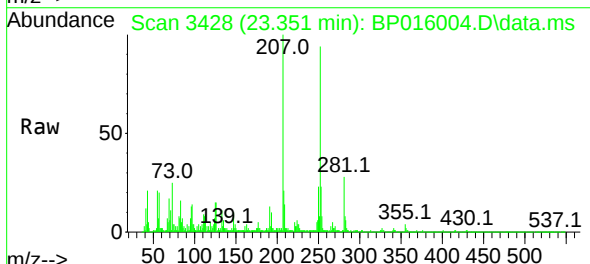

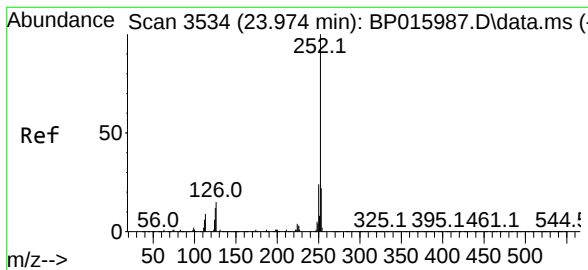

#93
Benzo(a)pyrene
Concen: 7.840 ng/ul
RT: 23.980 min Scan# 3534
Delta R.T. 0.000 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29




Instrument :
BNA_P
ClientSampleId :
DCGF8

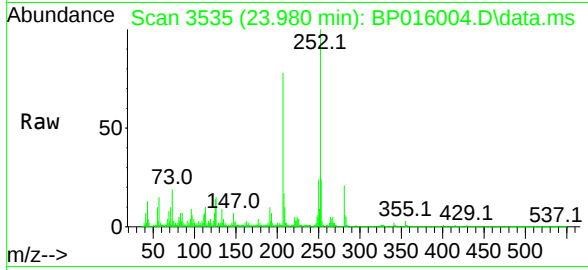


Tgt Ion:252 Resp: 492204
Ion Ratio Lower Upper
252 100
253 23.6 17.7 26.5
125 13.8 8.2 12.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :Sohil Jodhani 07/05/2023

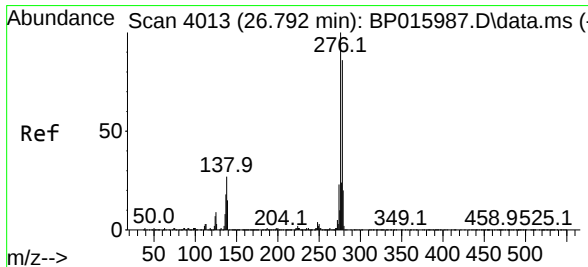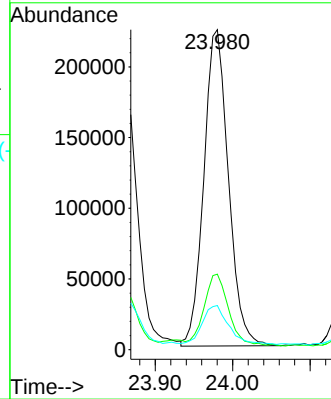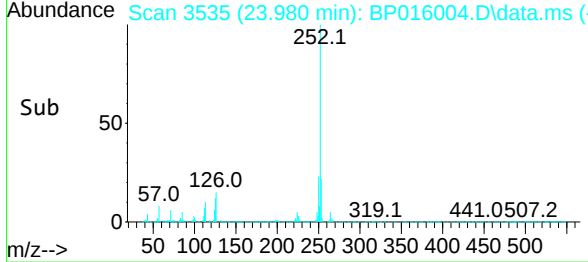


#94
Indeno(1,2,3-cd)pyrene
Concen: 4.672 ng/ul
RT: 26.804 min Scan# 4015
Delta R.T. 0.012 min
Lab File: BP016004.D
Acq: 05 Jul 2023 07:29

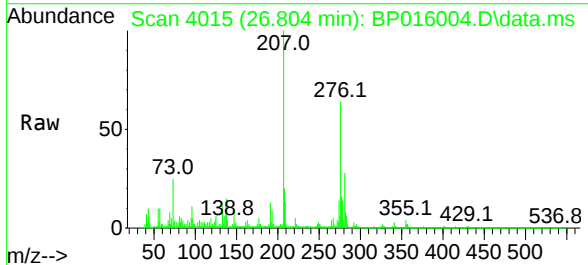

Tgt Ion:276 Resp: 398195
Ion Ratio Lower Upper
276 100
138 22.8 15.7 23.5
277 24.4 19.6 29.4

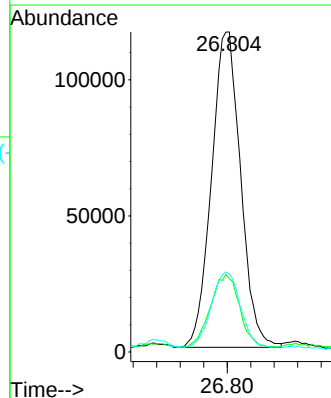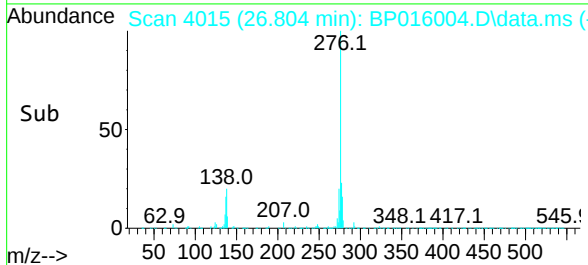

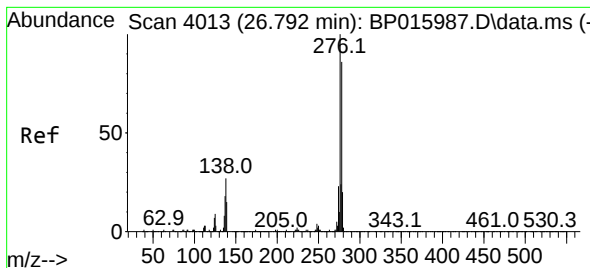

#95

Dibenzo(a,h)anthracene

Concen: 1.639 ng/ul m

RT: 26.798 min Scan# 4013

Delta R.T. 0.000 min

Lab File: BP016004.D

Acq: 05 Jul 2023 07:29

Instrument :

BNP_P

ClientSampleId :

DCGF8

Tgt Ion: 278 Resp: 114710





Ion	Ratio	Lower	Upper
278	100		
139	26.6	10.5	15.7
279	27.8	18.4	27.6

Manual Integrations

APPROVED

Reviewed By : Yogesh Patel 07/05/2023

Supervised By : Sohil Jodhani 07/05/2023

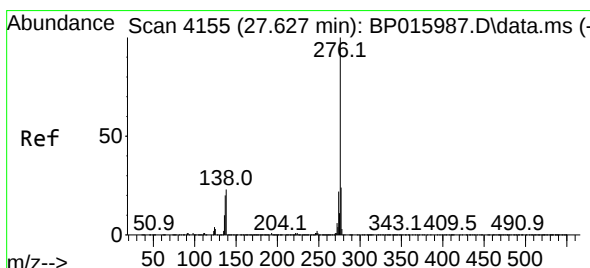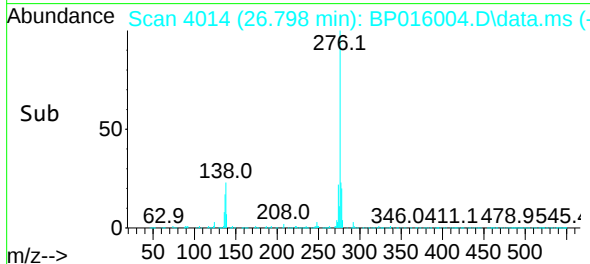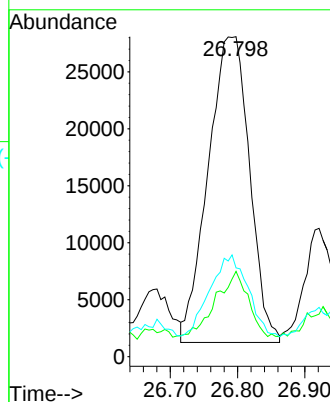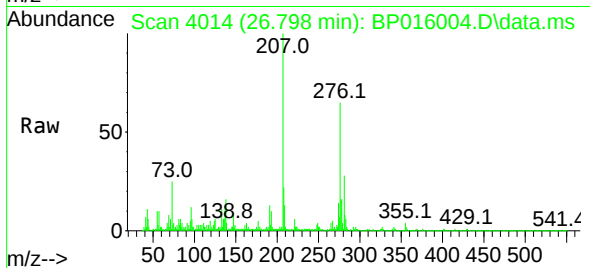

#96

Benzo(g,h,i)perylene

Concen: 5.287 ng/ul

RT: 27.639 min Scan# 4157

Delta R.T. 0.012 min

Lab File: BP016004.D

Acq: 05 Jul 2023 07:29

Tgt Ion: 276 Resp: 370683

Ion	Ratio	Lower	Upper
276	100		
138	24.3	15.1	22.7
277	24.2	18.8	28.2

