

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP015989.D
 Acq On : 04 Jul 2023 23:03
 Operator : MA/JU
 Sample : PB153764BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK764

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	43	rVB	108621	157812	2.54%	0.212%
2	3.811	104	106	129	rBV	1106441	1974534	31.84%	2.652%
3	4.134	158	161	167	rVB2	23535	32743	0.53%	0.044%
4	5.287	355	357	363	rVB6	6353	6910	0.11%	0.009%
5	7.228	680	687	704	rBV	969706	2467292	39.78%	3.314%
6	7.364	704	710	732	rVB	1122431	2084398	33.61%	2.800%
7	7.575	739	746	766	rBV	1362667	2587576	41.72%	3.476%
8	8.040	818	825	841	rBV	767885	1538496	24.81%	2.067%
9	8.781	944	951	978	rBV	1262921	3204923	51.68%	4.305%
10	9.228	1020	1027	1052	rBV	1240127	2577909	41.57%	3.463%
11	9.963	1143	1152	1179	rBV	877975	2216107	35.73%	2.977%
12	10.528	1237	1248	1284	rBV	811000	3094076	49.89%	4.156%
13	10.869	1297	1306	1326	rBV	1197078	2343905	37.79%	3.148%
14	11.040	1327	1335	1360	rBV	927509	3000282	48.38%	4.030%
15	12.499	1578	1583	1593	rBV4	18122	41817	0.67%	0.056%
16	13.499	1748	1753	1757	rBV7	4193	8150	0.13%	0.011%
17	13.569	1757	1765	1772	rBV2	34038	65988	1.06%	0.089%
18	13.663	1777	1781	1788	rVV10	3770	7735	0.12%	0.010%
19	14.104	1849	1856	1881	rBV	2445578	4473851	72.14%	6.009%
20	14.387	1897	1904	1927	rBV2	3101069	5304433	85.53%	7.125%
21	14.693	1949	1956	1967	rBV	1793799	2843468	45.85%	3.819%
22	15.004	2002	2009	2039	rBV	289674	1476396	23.81%	1.983%
23	15.428	2077	2081	2085	rBV7	5398	8161	0.13%	0.011%
24	15.693	2119	2126	2144	rBV	3032125	6050249	97.56%	8.127%
25	15.875	2150	2157	2178	rBV	344345	1119700	18.05%	1.504%
26	17.457	2419	2426	2437	rBV	1756547	2878115	46.41%	3.866%
27	17.563	2437	2444	2468	rVB	2906847	5916190	95.40%	7.947%
28	19.363	2747	2750	2757	rVB2	38721	53007	0.85%	0.071%
29	19.439	2760	2763	2768	rVV	43101	56345	0.91%	0.076%
30	19.786	2816	2822	2839	rBV	3602627	6201770	100.00%	8.330%
31	21.557	3118	3123	3134	rBV	1327514	2396131	38.64%	3.219%
32	23.922	3519	3525	3545	rVB2	2203599	5646198	91.04%	7.584%
33	24.092	3548	3554	3574	rVB	994212	2613641	42.14%	3.511%




Sum of corrected areas: 74448308

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015989.D
Acq On : 04 Jul 2023 23:03
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

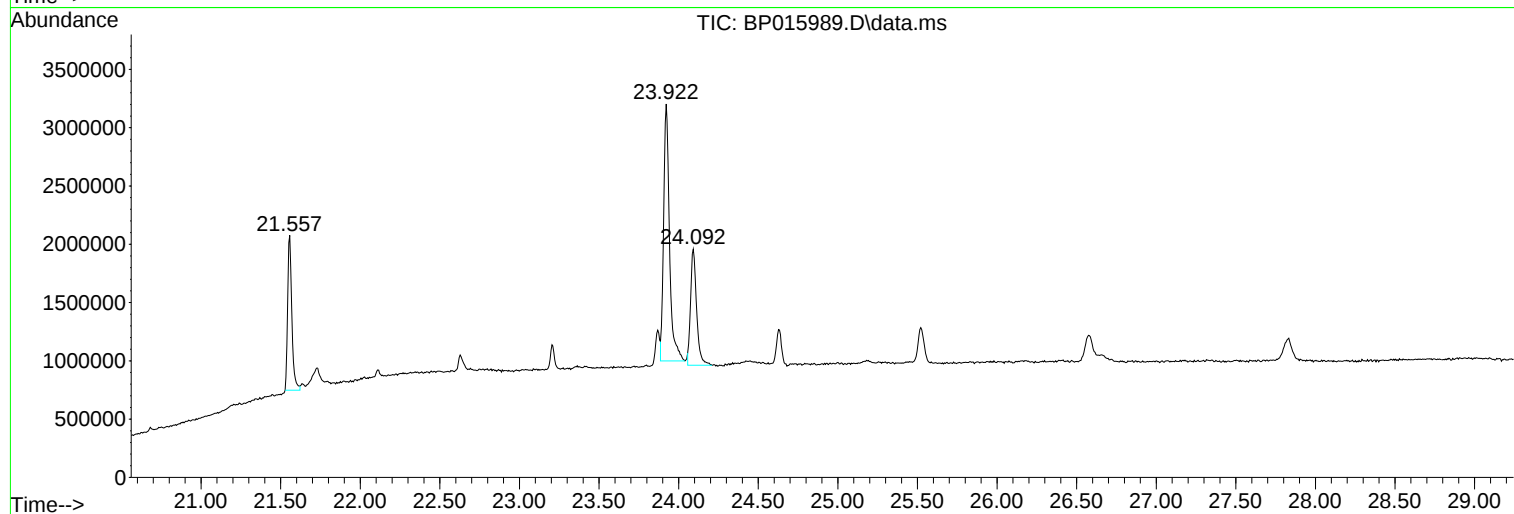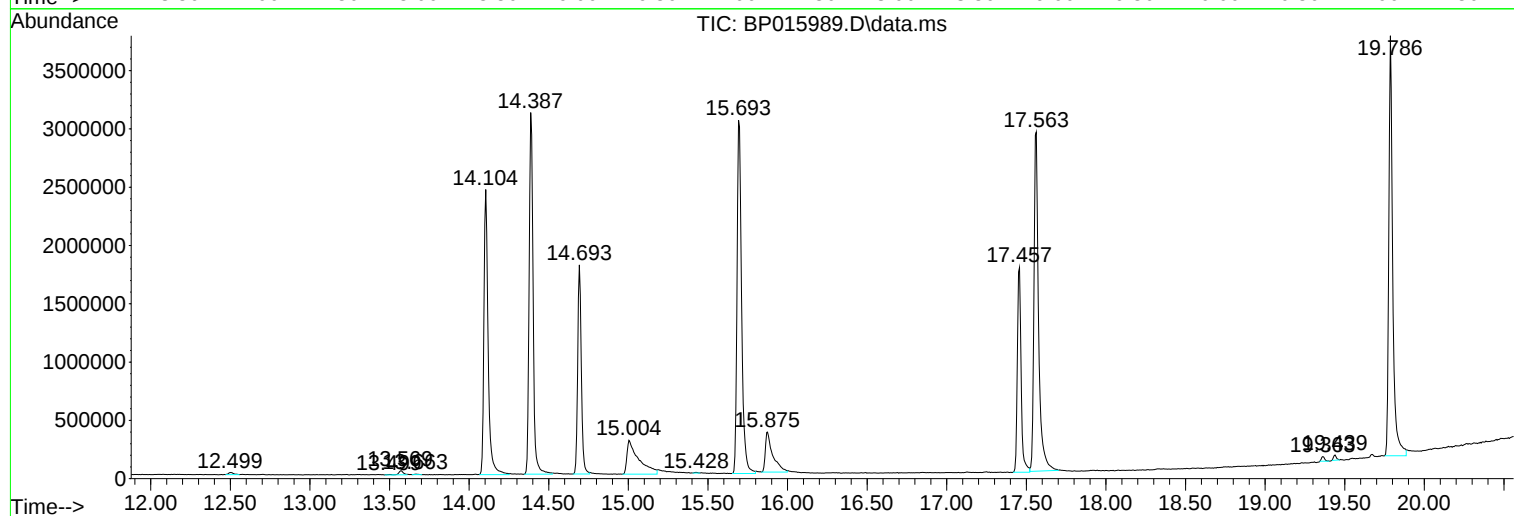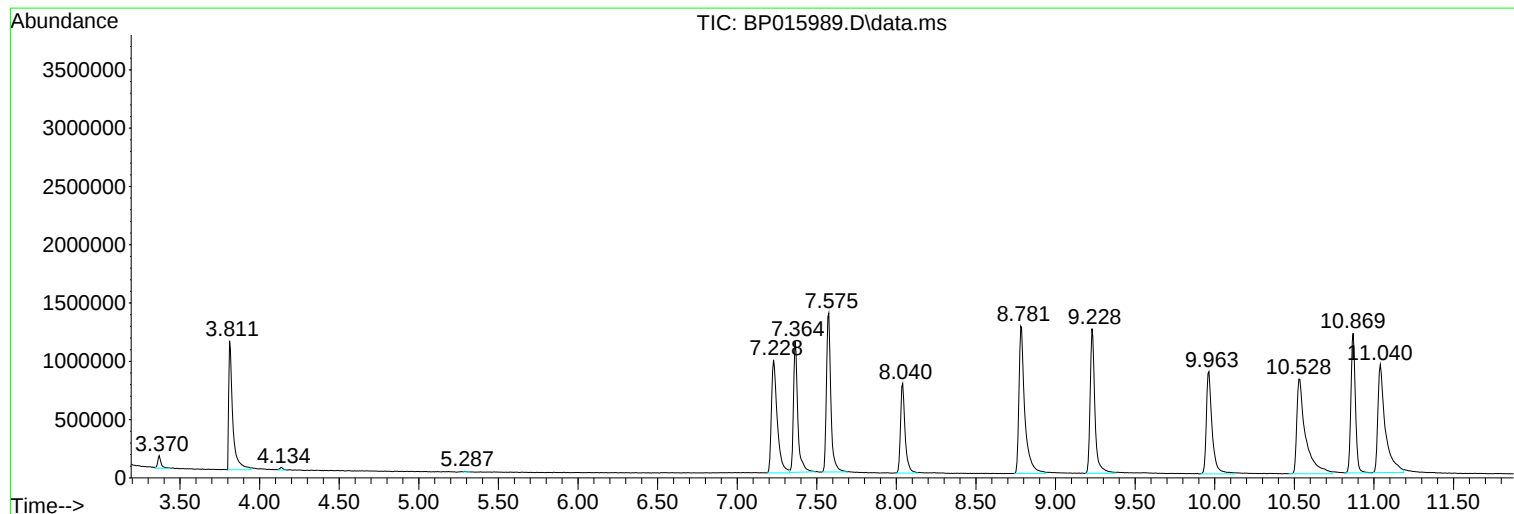

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015989.D
Acq On : 04 Jul 2023 23:03
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP015989.D
Acq On : 04 Jul 2023 23:03
Operator : MA/JU
Sample : PB153764BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------