

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016012.D
 Acq On : 05 Jul 2023 14:08
 Operator : MA/JU
 Sample : PB153588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	40	rVB	74794	109548	2.36%	0.189%
2	3.811	104	106	135	rBV	720746	1403319	30.19%	2.420%
3	4.134	157	161	165	rVB	13580	20712	0.45%	0.036%
4	6.570	571	575	579	rBV7	3144	5054	0.11%	0.009%
5	7.240	681	689	705	rBV	624690	1743965	37.52%	3.007%
6	7.369	705	711	732	rVB	705820	1452813	31.26%	2.505%
7	7.575	739	746	761	rBV	901969	1844928	39.69%	3.182%
8	8.040	818	825	839	rBV	760607	1572179	33.82%	2.711%
9	8.793	945	953	985	rBV	784128	2336377	50.26%	4.029%
10	9.240	1021	1029	1049	rBV	824854	1841230	39.61%	3.175%
11	9.969	1142	1153	1177	rBV	514454	1551449	33.38%	2.675%
12	10.122	1177	1179	1182	rVB4	4204	4841	0.10%	0.008%
13	10.546	1242	1251	1285	rBV	519980	2212630	47.60%	3.816%
14	10.875	1299	1307	1326	rBV	1097945	2357837	50.73%	4.066%
15	11.052	1329	1337	1366	rBV	565174	2077129	44.69%	3.582%
16	12.010	1493	1500	1501	rBV7	3490	5177	0.11%	0.009%
17	12.046	1504	1506	1512	rVB7	4241	5910	0.13%	0.010%
18	12.510	1581	1585	1596	rVB3	13661	34740	0.75%	0.060%
19	13.440	1738	1743	1746	rVB6	2911	4769	0.10%	0.008%
20	13.581	1761	1767	1772	rBV5	16346	31986	0.69%	0.055%
21	14.040	1841	1845	1850	rVB3	4421	6158	0.13%	0.011%
22	14.110	1850	1857	1882	rBV	1611441	3294943	70.89%	5.682%
23	14.299	1888	1889	1896	rVB7	3783	5048	0.11%	0.009%
24	14.393	1898	1905	1928	rBV	2344280	3977793	85.58%	6.860%
25	14.698	1950	1957	1971	rBV	1805251	2949040	63.44%	5.086%
26	15.034	2004	2014	2038	rBV3	168699	951411	20.47%	1.641%
27	15.593	2106	2109	2114	rVB7	7438	13436	0.29%	0.023%
28	15.704	2121	2128	2152	rBV	2216832	4648219	100.00%	8.016%
29	15.898	2155	2161	2185	rVV3	169255	685296	14.74%	1.182%
30	16.493	2260	2262	2267	rVB6	4383	4873	0.10%	0.008%
31	17.128	2367	2370	2376	rBV8	5708	12934	0.28%	0.022%
32	17.463	2420	2427	2438	rBV	1819124	2998723	64.51%	5.171%
33	17.569	2439	2445	2473	rVB2	2046280	4624265	99.48%	7.974%
34	18.328	2572	2574	2579	rBV6	7928	14037	0.30%	0.024%
35	19.375	2749	2752	2756	rBV3	31230	40764	0.88%	0.070%
36	19.451	2762	2765	2769	rBV2	26490	39952	0.86%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016012.D
Acq On : 05 Jul 2023 14:08
Operator : MA/JU
Sample : PB153588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.798	2818	2824	2845	rBV	2303487	4531395	97.49%	7.814%
38	21.563	3120	3124	3136	rBV	1238382	2302257	49.53%	3.970%
39	23.939	3522	3528	3548	rVV2	1449308	3635670	78.22%	6.270%
40	24.116	3551	3558	3579	rVB	879549	2635542	56.70%	4.545%




Sum of corrected areas: 57988349

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016012.D
Acq On : 05 Jul 2023 14:08
Operator : MA/JU
Sample : PB153588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

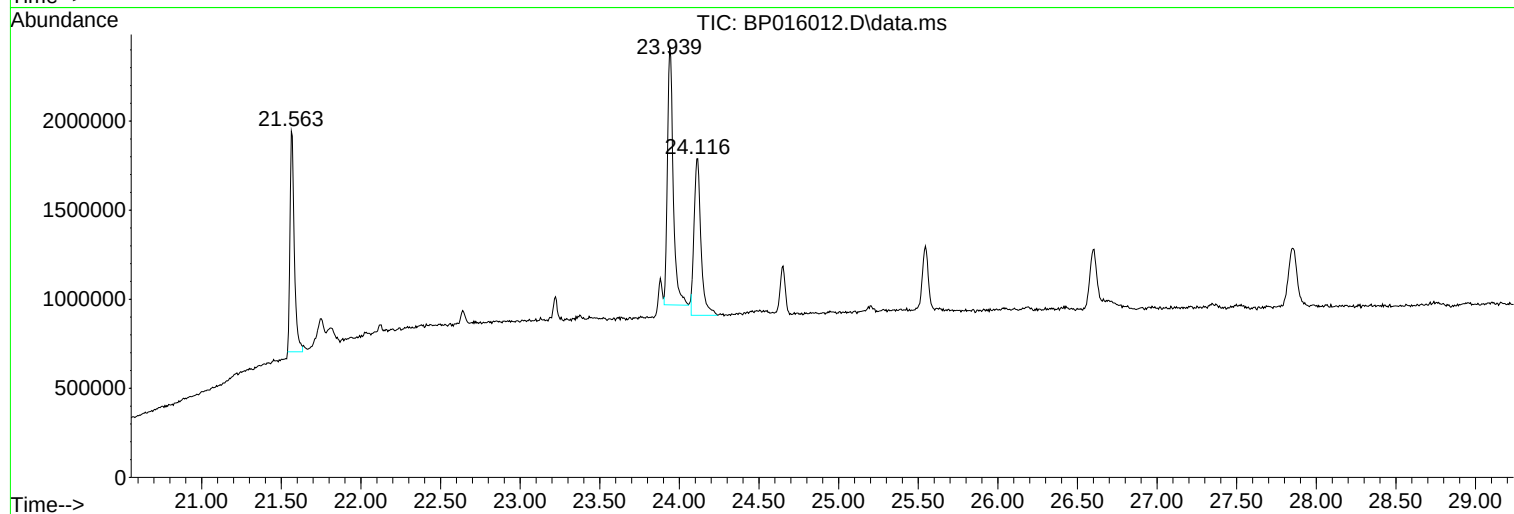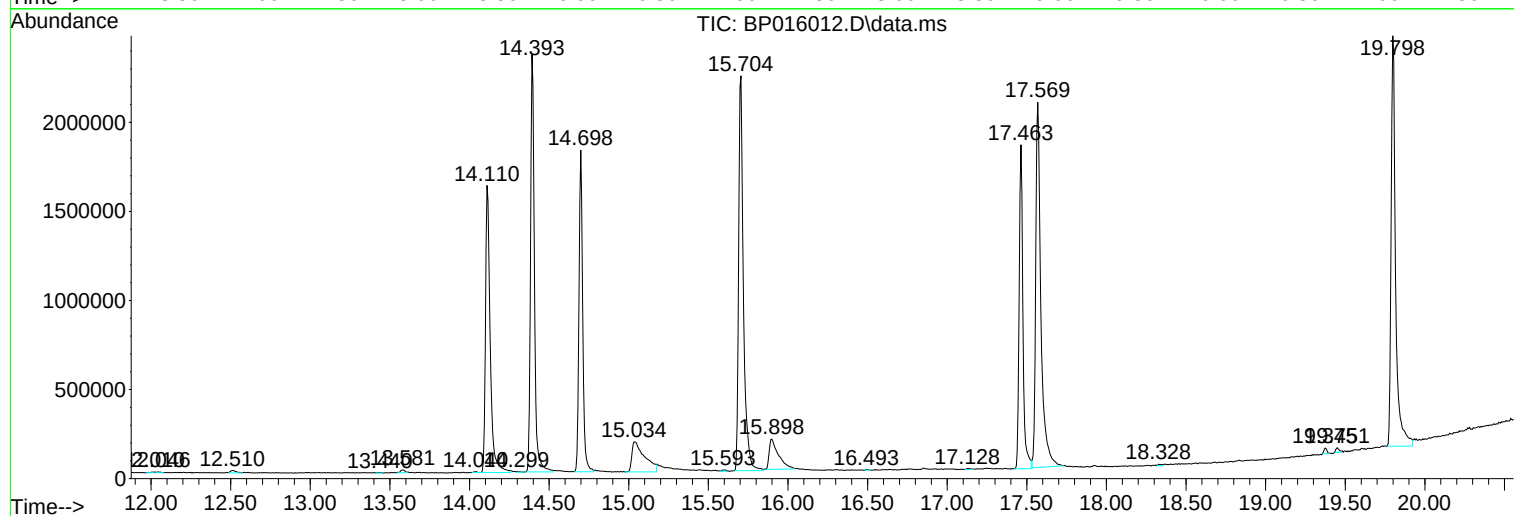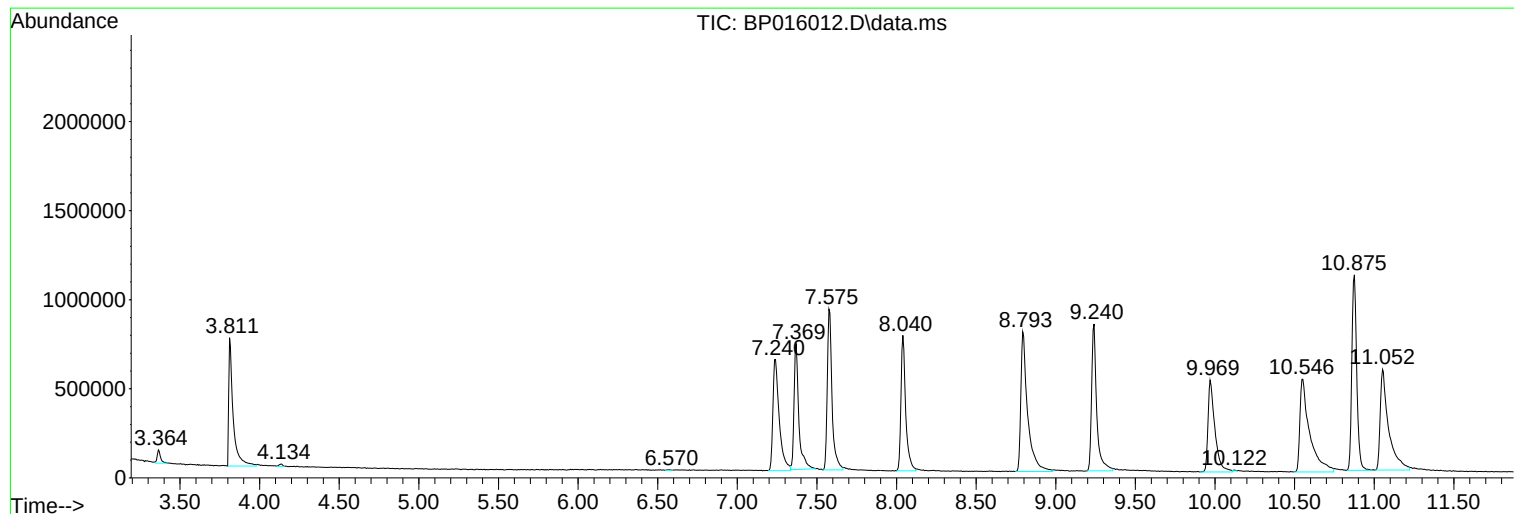

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016012.D
Acq On : 05 Jul 2023 14:08
Operator : MA/JU
Sample : PB153588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016012.D
Acq On : 05 Jul 2023 14:08
Operator : MA/JU
Sample : PB153588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc