

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
 Data File : BP016022.D
 Acq On : 05 Jul 2023 19:51
 Operator : MA/JU
 Sample : PB153780BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	40	rVB	84687	129736	2.75%	0.209%
2	3.817	103	107	131	rBV	833866	1579192	33.42%	2.542%
3	4.134	158	161	166	rVB2	16737	24412	0.52%	0.039%
4	4.511	223	225	232	rBV8	5653	11542	0.24%	0.019%
5	7.234	680	688	705	rBV	733872	1962562	41.53%	3.159%
6	7.363	705	710	738	rVV	838307	1712750	36.25%	2.757%
7	7.575	739	746	768	rVV	1053470	2082469	44.07%	3.352%
8	8.040	818	825	849	rBV	875114	1814985	38.41%	2.921%
9	8.793	944	953	982	rBV	886303	2609206	55.22%	4.200%
10	9.234	1021	1028	1048	rBV	936200	2063608	43.67%	3.321%
11	9.963	1142	1152	1179	rBV	594967	1740956	36.84%	2.802%
12	10.546	1239	1251	1295	rBV	590195	2499348	52.89%	4.023%
13	10.869	1298	1306	1324	rVV	1261899	2644686	55.97%	4.257%
14	11.046	1328	1336	1375	rBV	651726	2410213	51.01%	3.879%
15	12.510	1577	1585	1595	rBV3	14797	36974	0.78%	0.060%
16	13.575	1759	1766	1775	rVV4	21506	46180	0.98%	0.074%
17	14.110	1849	1857	1888	rBV	1715304	3506302	74.20%	5.644%
18	14.387	1897	1904	1927	rBV2	2372402	4160052	88.04%	6.696%
19	14.545	1929	1931	1936	rVB6	6002	10101	0.21%	0.016%
20	14.692	1949	1956	1974	rBV	1970303	3159526	66.86%	5.085%
21	15.034	2006	2014	2057	rBV3	169085	1143011	24.19%	1.840%
22	15.698	2120	2127	2150	rBV	2292583	4725379	100.00%	7.606%
23	15.892	2154	2160	2186	rVV2	165713	684331	14.48%	1.101%
24	17.457	2420	2426	2438	rBV	1753353	2964713	62.74%	4.772%
25	17.563	2438	2444	2469	rVB2	1997386	4333595	91.71%	6.975%
26	19.792	2817	2823	2842	rBV	2407917	4536386	96.00%	7.302%
27	21.557	3118	3123	3133	rBV2	1384118	2607254	55.18%	4.197%
28	23.927	3520	3526	3545	rVB	1708490	4245741	89.85%	6.834%
29	24.098	3549	3555	3572	rVB	982931	2683920	56.80%	4.320%




Sum of corrected areas: 62129130

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016022.D
Acq On : 05 Jul 2023 19:51
Operator : MA/JU
Sample : PB153780BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

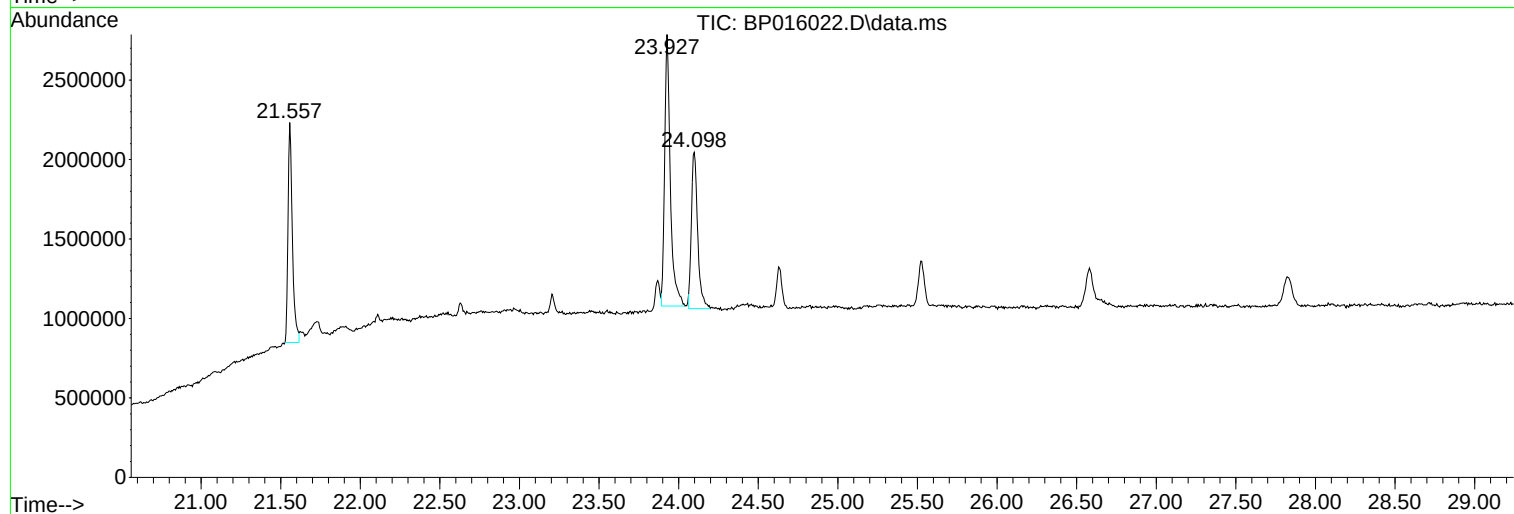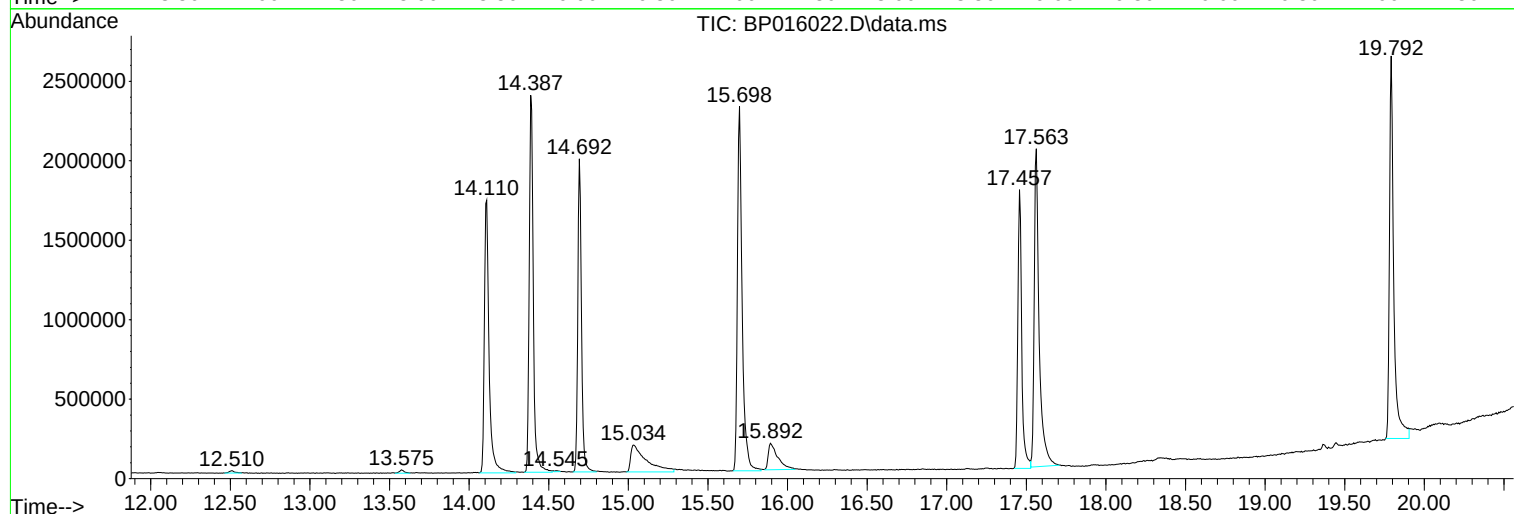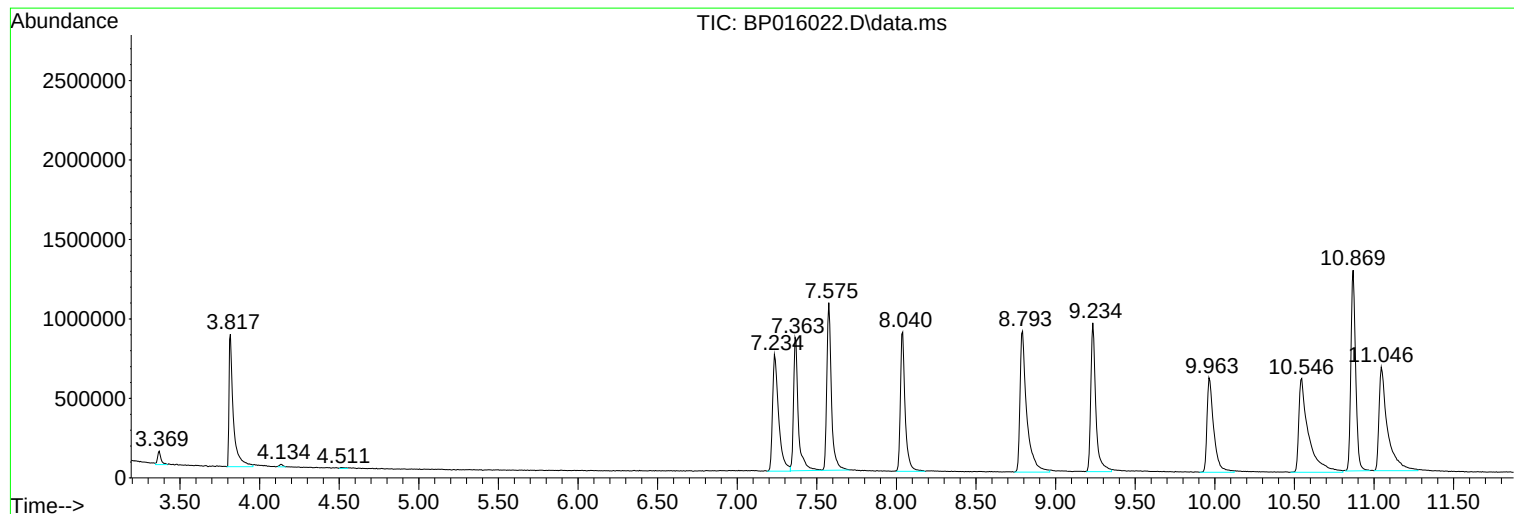

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016022.D
Acq On : 05 Jul 2023 19:51
Operator : MA/JU
Sample : PB153780BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070423\
Data File : BP016022.D
Acq On : 05 Jul 2023 19:51
Operator : MA/JU
Sample : PB153780BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------