




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016028.D
 Acq On : 06 Jul 2023 11:33
 Operator : MA/JU
 Sample : 03257-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY2

Manual IntegrationsAPPROVED

Quant Time: Jul 06 23:25:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

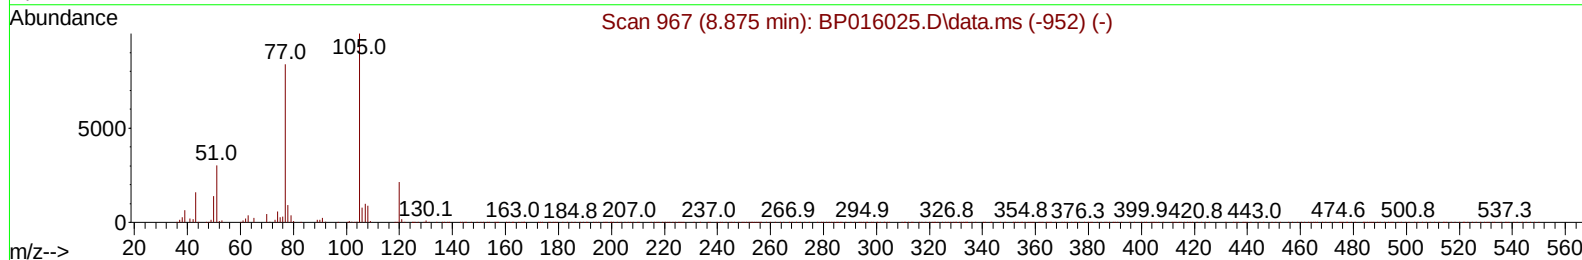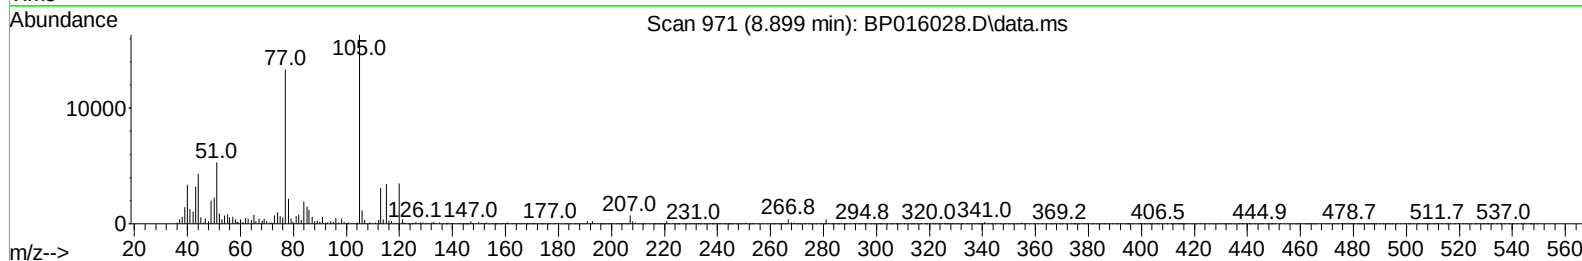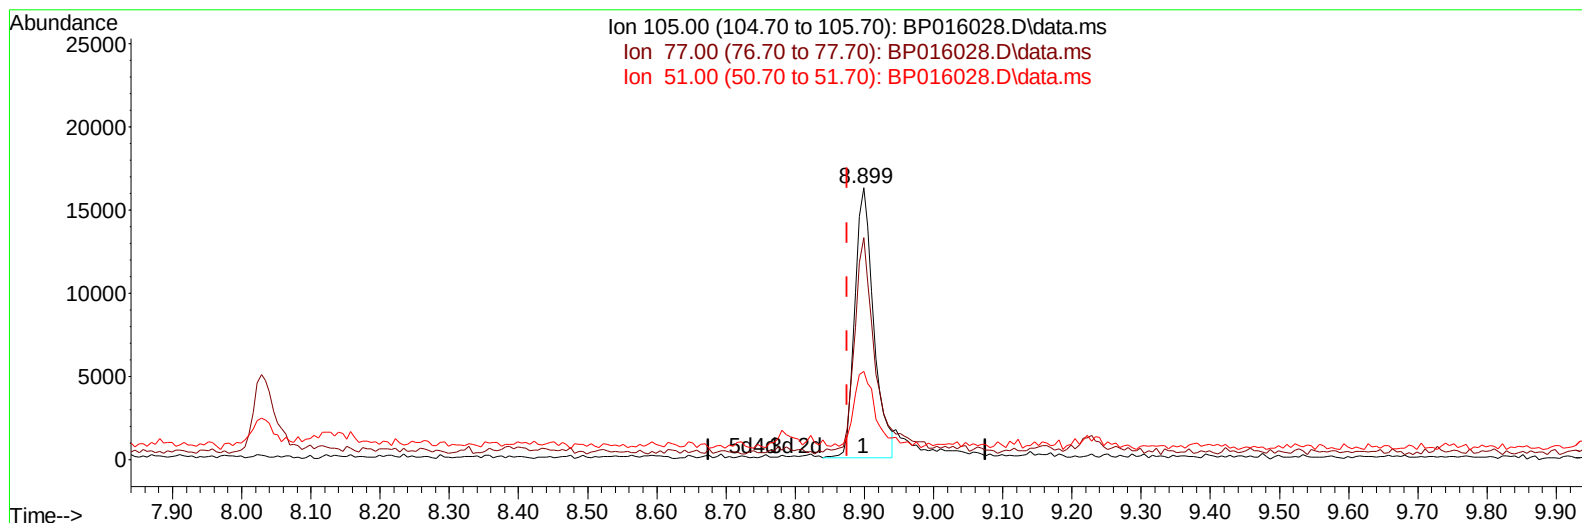

TIC: BP016028.D\data.ms

(16) Acetophenone

8.899min (+ 0.024) 1.12 ng/ul

response 31014

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	81.20	81.66
51.00	31.40	32.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016028.D
 Acq On : 06 Jul 2023 11:33
 Operator : MA/JU
 Sample : 03257-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY2

Manual IntegrationsAPPROVED

Quant Time: Jul 06 23:25:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

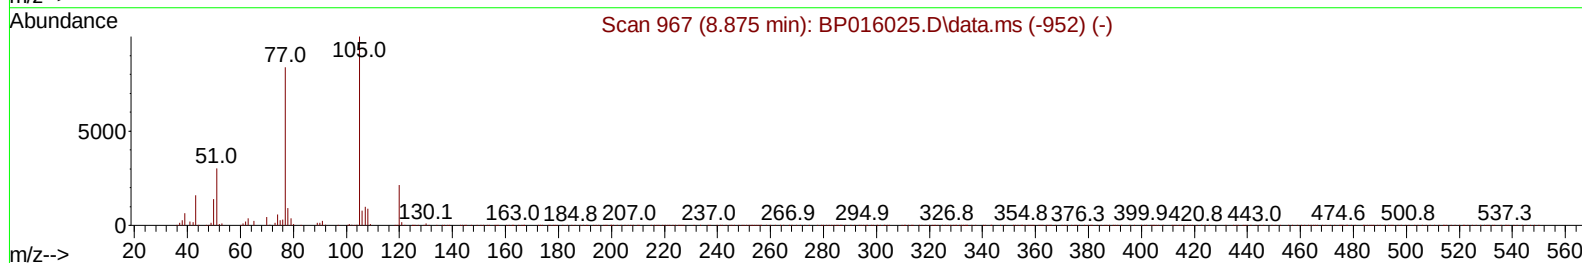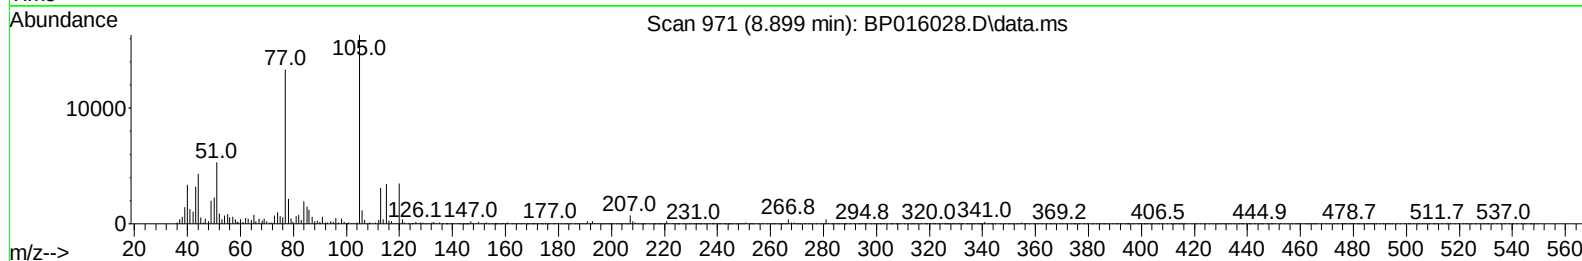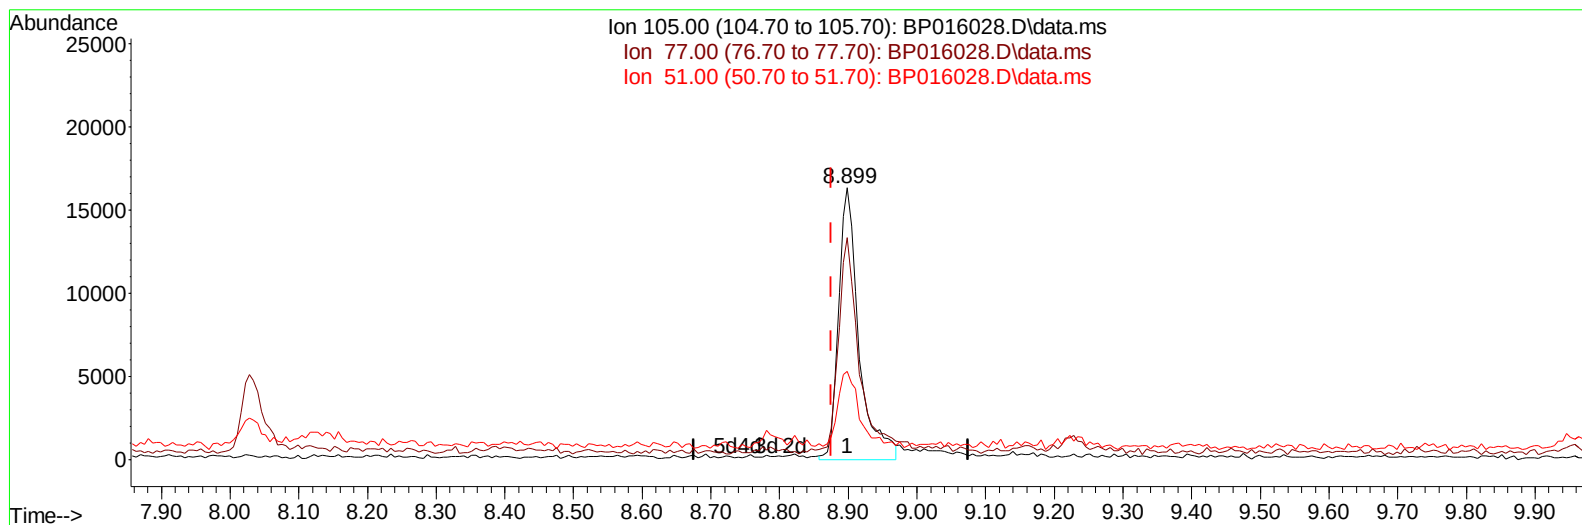

TIC: BP016028.D\data.ms

(16) Acetophenone

8.899min (+ 0.024) 1.22 ng/ul m

response 33531

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	81.20	81.66
51.00	31.40	32.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016028.D
Acq On : 06 Jul 2023 11:33
Operator : MA/JU
Sample : 03257-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY2

Manual IntegrationsAPPROVED

Quant Time: Jul 06 23:46:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

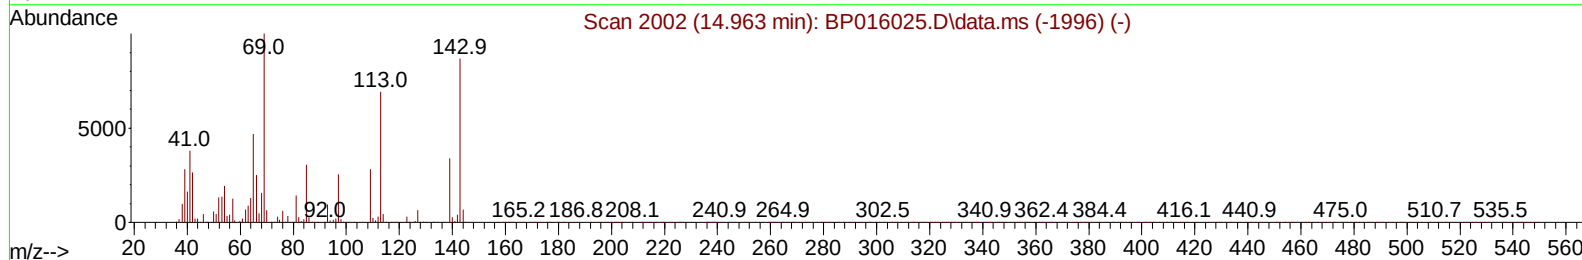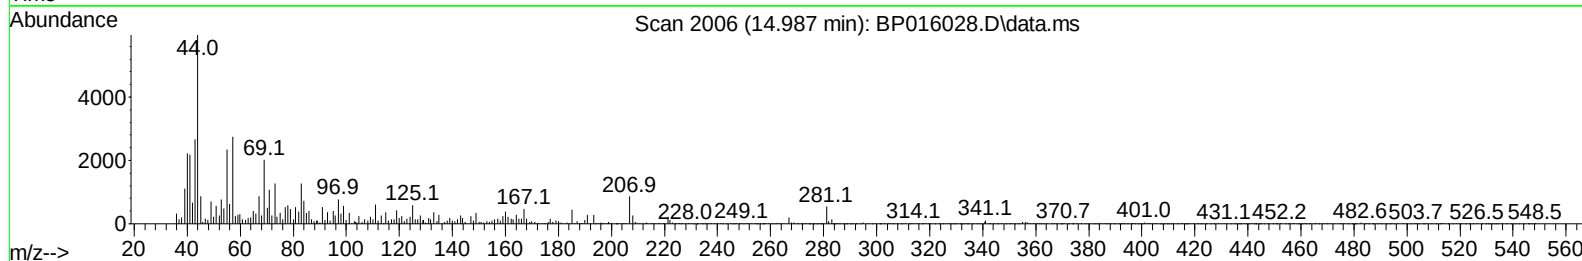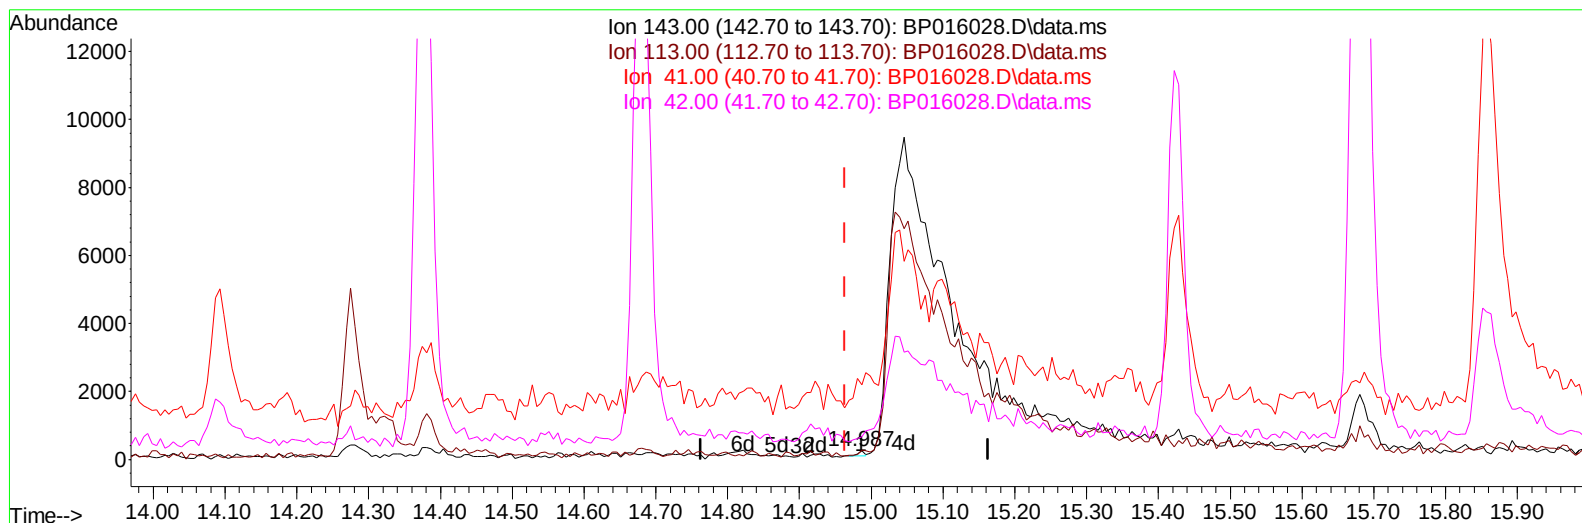

TIC: BP016028.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.987min (+ 0.024) 0.01 ng/ul

response 84

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	105.91
41.00	45.70	861.02#
42.00	31.20	262.20#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016028.D
Acq On : 06 Jul 2023 11:33
Operator : MA/JU
Sample : 03257-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY2

Manual IntegrationsAPPROVED

Quant Time: Jul 06 23:46:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

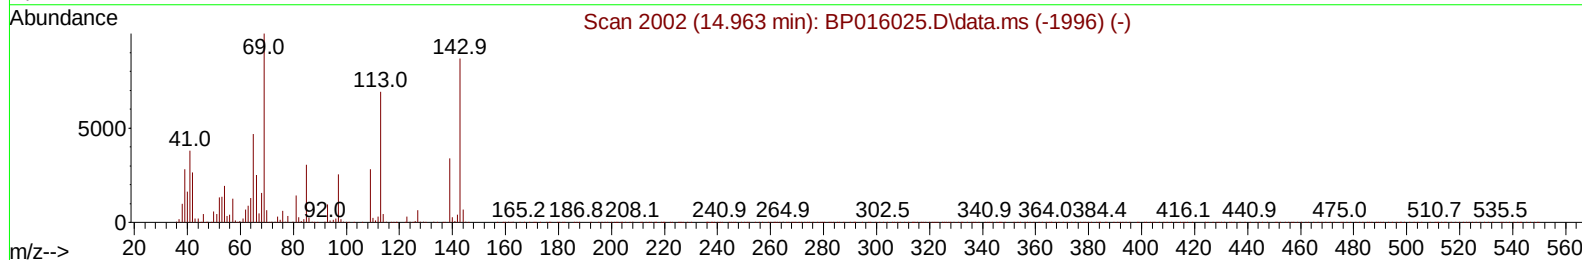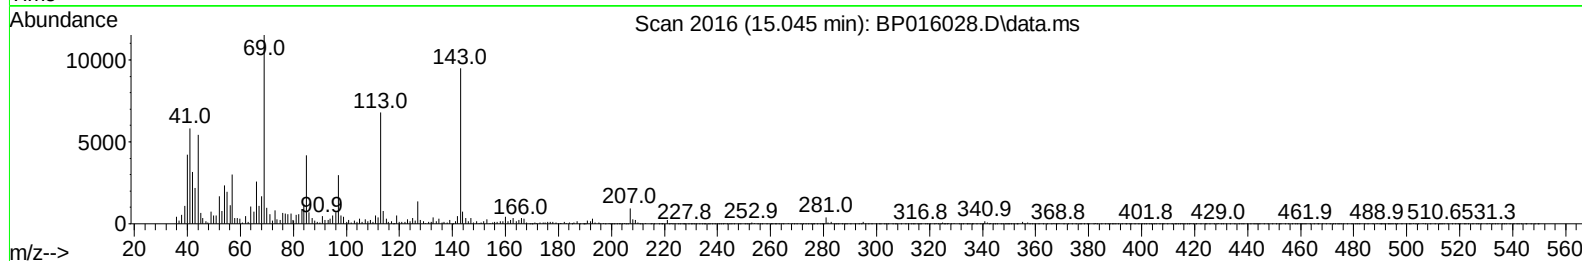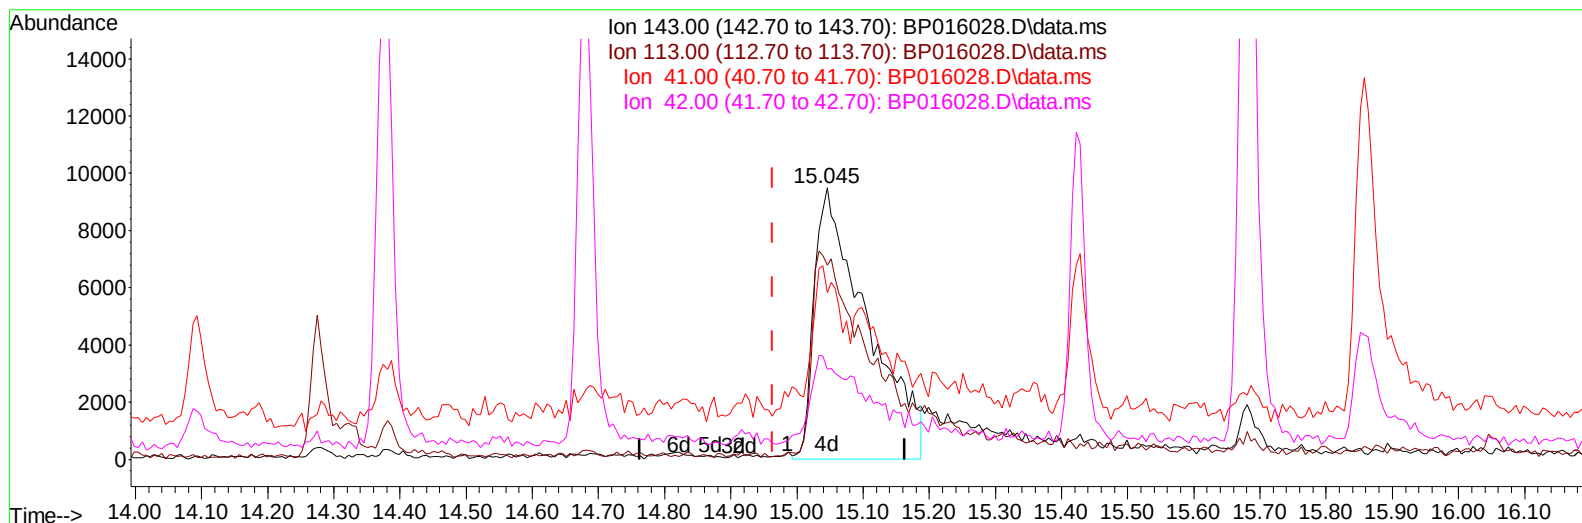

TIC: BP016028.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.045min (+ 0.082) 7.18 ng/ul m

response 52413

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	71.48#
41.00	45.70	61.52#
42.00	31.20	33.22

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016028.D
 Acq On : 06 Jul 2023 11:33
 Operator : MA/JU
 Sample : 03257-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

Quant Time: Jul 06 23:47:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.028	152		248226	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136		1110225	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.681	164		715555	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188		1600247	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240		1562287	20.000	ng/ul	# 0.00
88) Perylene-d12	24.080	264		1670374	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.358	96		27259	3.951	ng/uL	0.00
4) Pyridine-d5	3.817	84		125667	7.226	ng/ul	0.01
7) Phenol-d5	7.246	99		132348	6.231	ng/ul	0.03
9) Bis-(2-Chloroethyl)eth...	7.358	67		409213	31.143	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132		391053	24.391	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113		287597	17.141	ng/ul	0.01
21) Nitrobenzene-d5	9.228	128		242421	28.571	ng/ul	0.01
24) 2-Nitrophenol-d4	9.957	143		281769	28.454	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.528	165		437314	24.782	ng/ul	0.02
31) 4-Chloroaniline-d4	11.040	131		580678	25.616	ng/ul	0.02
46) Dimethylphthalate-d6	14.093	166		1709120	30.902	ng/ul	0.00
49) Acenaphthylene-d8	14.375	160		1867546	30.038	ng/ul	0.00
54) 4-Nitrophenol-d4	15.045	143		52413m	7.181	ng/ul	0.08
60) Fluorene-d10	15.681	176		1482307	32.550	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200		298033	30.284	ng/ul	0.00
73) Anthracene-d10	17.551	188		2493030	34.106	ng/ul	0.00
81) Pyrene-d10	19.775	212		3075337	30.146	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.910	264		2984737	35.422	ng/ul	0.00
Target Compounds							
16) Acetophenone	8.899	105		33531m	1.216	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016028.D
Acq On : 06 Jul 2023 11:33
Operator : MA/JU
Sample : 03257-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY2

Manual IntegrationsAPPROVED

Quant Time: Jul 06 23:47:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

