

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016051.D
 Acq On : 07 Jul 2023 02:02
 Operator : MA/JU
 Sample : 03284-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :

BNA_P

ClientSampleId :

DCGZ7




Manual IntegrationsAPPROVED

Quant Time: Jul 07 02:54:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

Supervised By :mohammad
 ahmed

07/07/2023

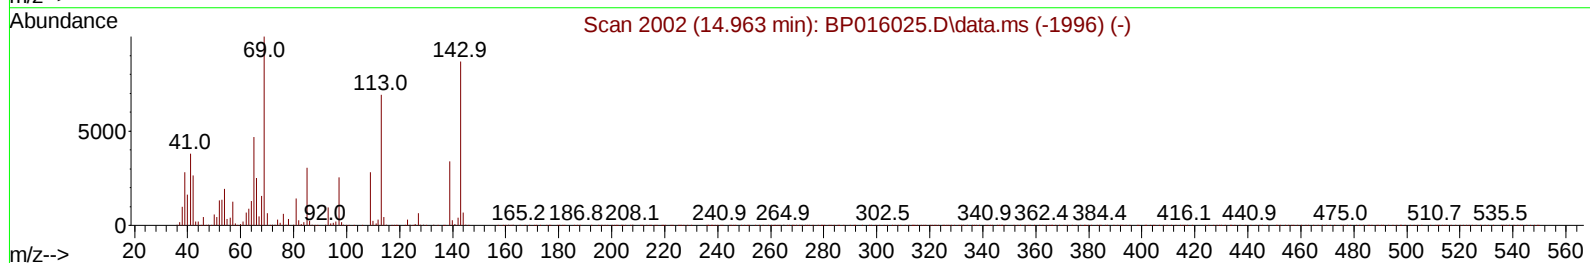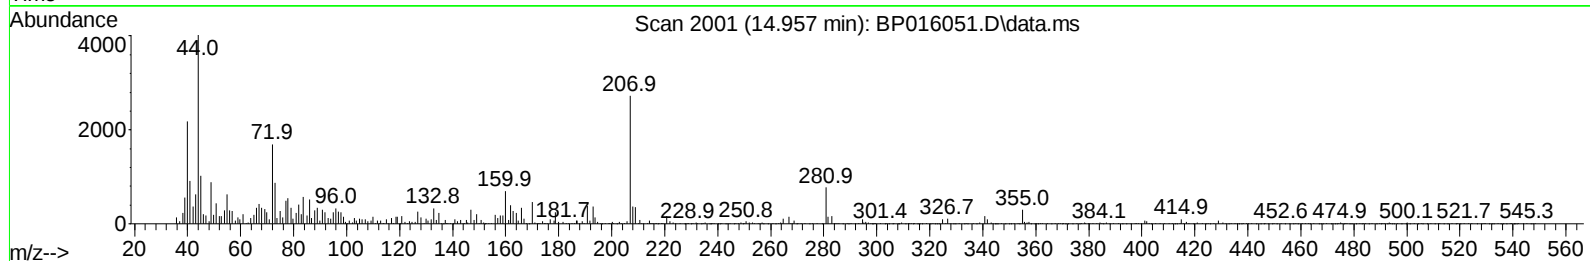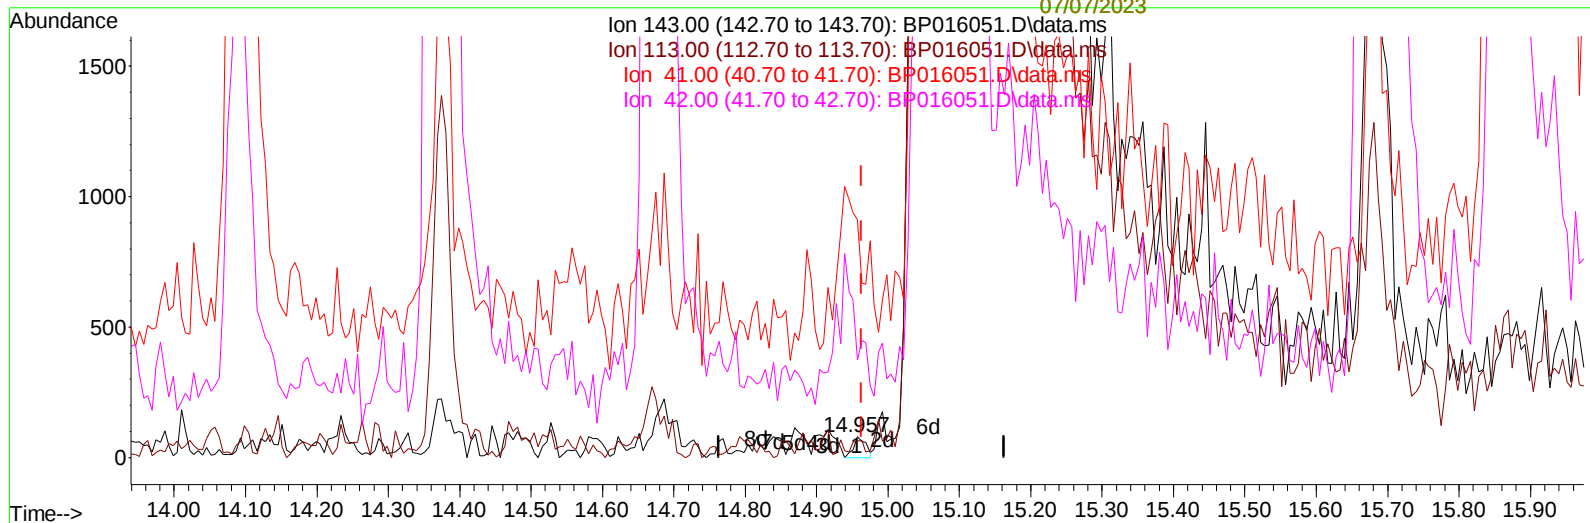

TIC: BP016051.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.957min (-0.006) 0.01 ng/u1

response 95

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	78.75
41.00	45.70	1141.25#
42.00	31.20	468.75#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
DCGZ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

Supervised By :mohammad
ahmed
07/07/2023

Quant Time: Jul 07 02:54:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

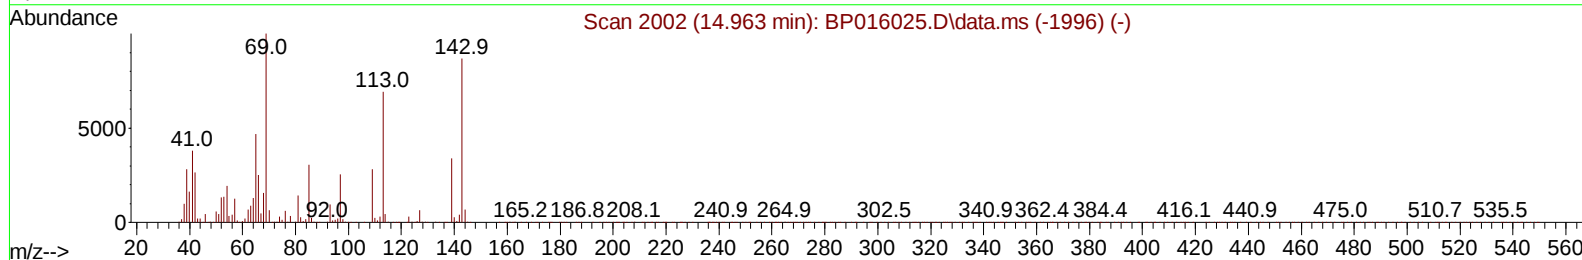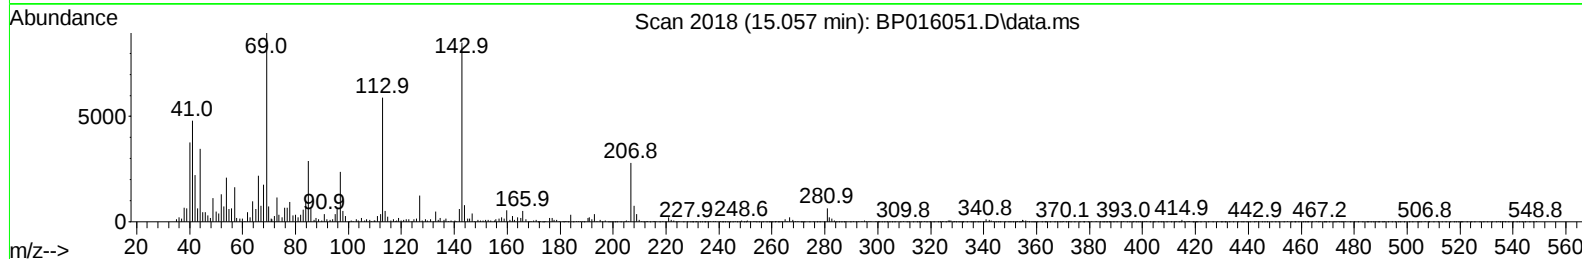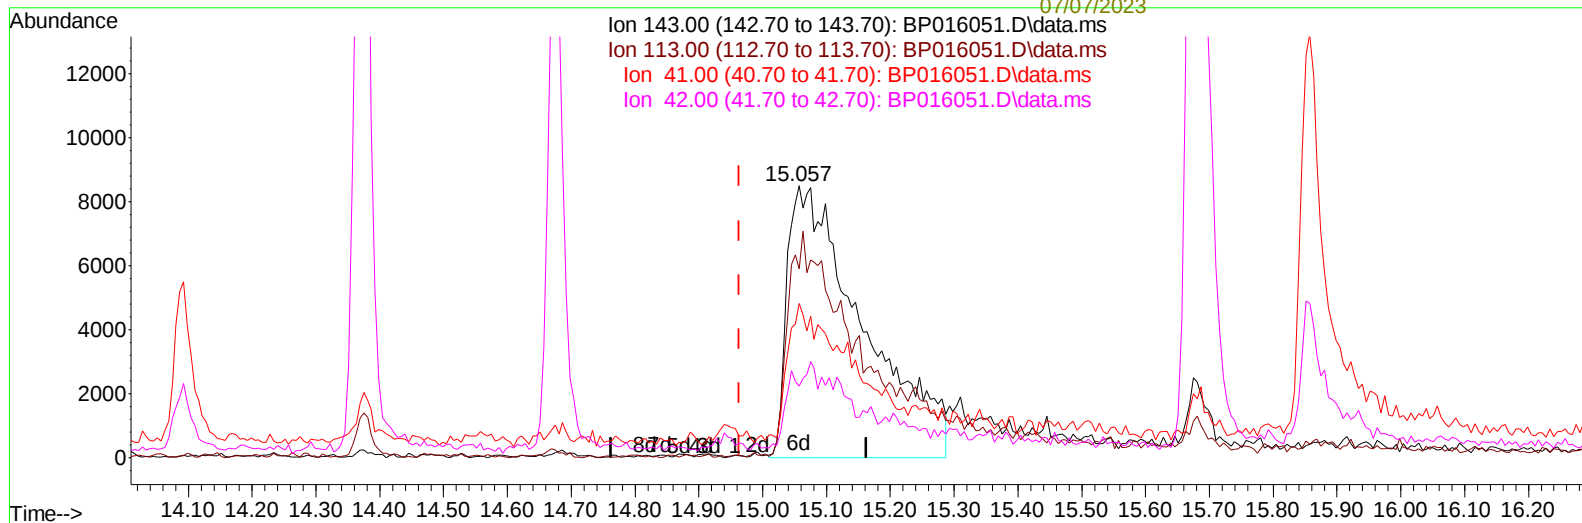

TIC: BP016051.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.057min (+ 0.094) 8.55 ng/ul m

response 69712

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	69.42#
41.00	45.70	56.63#
42.00	31.20	26.27

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016051.D
 Acq On : 07 Jul 2023 02:02
 Operator : MA/JU
 Sample : 03284-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGZ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

Supervised By :mohammad
 ahmed
 07/07/2023

Quant Time: Jul 07 02:55:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	266941	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	1198474	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	799719	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	1832527	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1767797	20.000	ng/ul	0.00
88) Perylene-d12	24.080	264	1828458	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	38740	5.221	ng/uL	0.00
4) Pyridine-d5	3.817	84	131116	7.010	ng/ul	0.01
7) Phenol-d5	7.240	99	208063	9.110	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.352	67	654473	46.316	ng/ul	0.00
11) 2-Chlorophenol-d4	7.569	132	617112	35.793	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	376337	20.858	ng/ul	0.00
21) Nitrobenzene-d5	9.222	128	397444	43.393	ng/ul	0.00
24) 2-Nitrophenol-d4	9.952	143	448195	41.927	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.534	165	660067	34.650	ng/ul	0.03
31) 4-Chloroaniline-d4	11.057	131	440864	18.016	ng/ul	0.04
46) Dimethylphthalate-d6	14.092	166	2902638	46.959	ng/ul	0.00
49) Acenaphthylene-d8	14.375	160	3104960	44.685	ng/ul	0.00
54) 4-Nitrophenol-d4	15.057	143	69712m	8.546	ng/ul	0.09
60) Fluorene-d10	15.681	176	2413868	47.427	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	420212	37.286	ng/ul	0.00
73) Anthracene-d10	17.545	188	3751503	44.817	ng/ul	0.00
81) Pyrene-d10	19.775	212	4850218	42.017	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	4390886	47.605	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGZ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

Supervised By :mohammad
ahmed
07/07/2023

Quant Time: Jul 07 02:55:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

