




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77

Manual IntegrationsAPPROVED

Quant Time: Jul 07 03:44:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

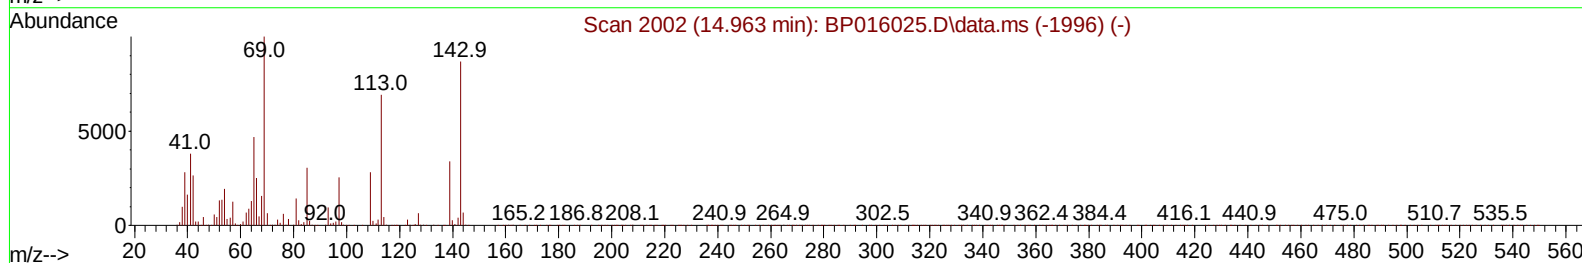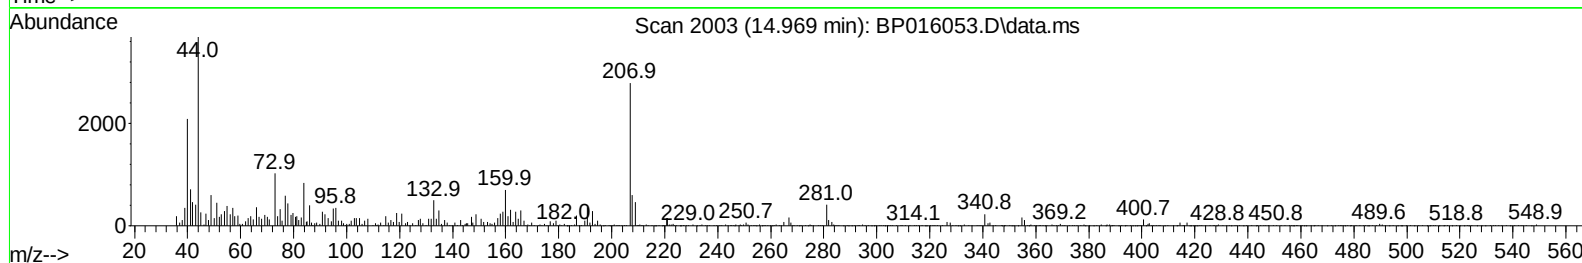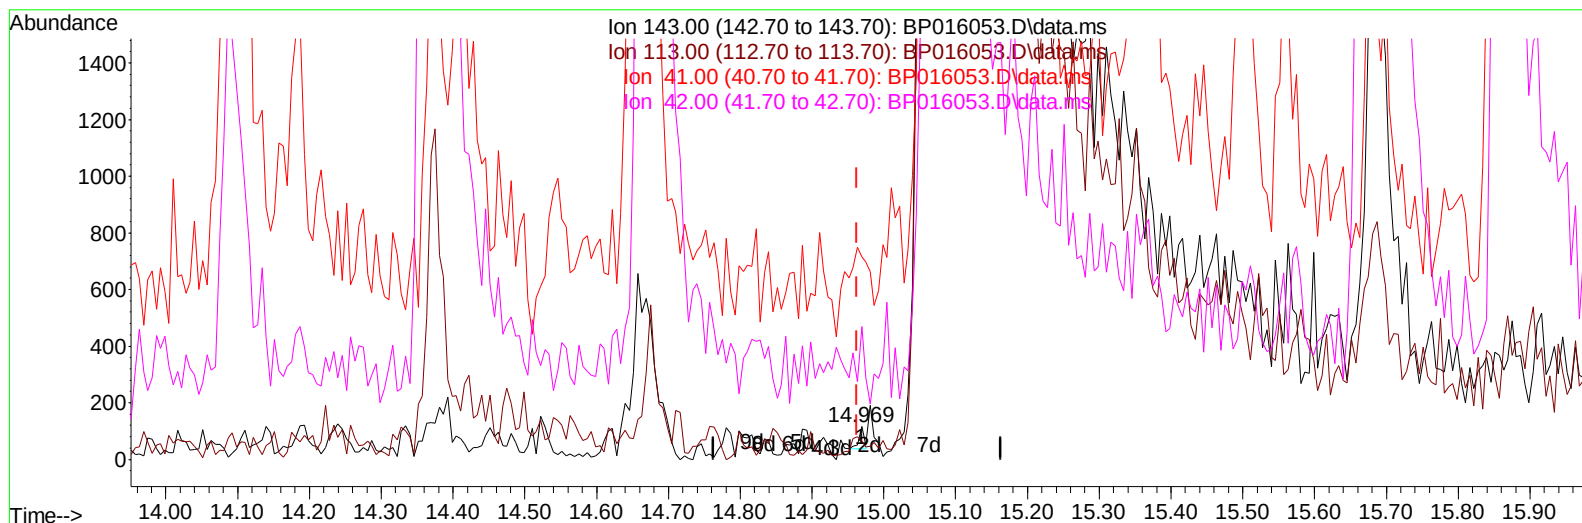

TIC: BP016053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.969min (+ 0.006) 0.00 ng/uL

response 40

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	48.12#
41.00	45.70	538.35#
42.00	31.20	352.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77

Manual IntegrationsAPPROVED

Quant Time: Jul 07 03:44:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

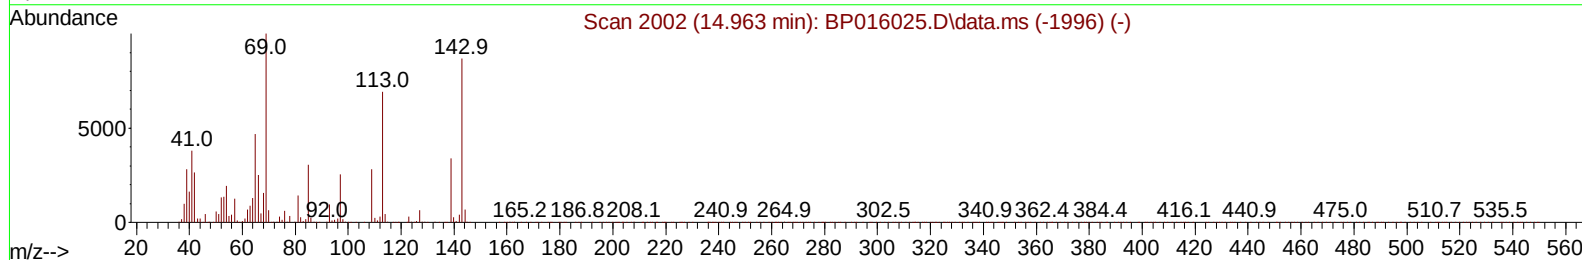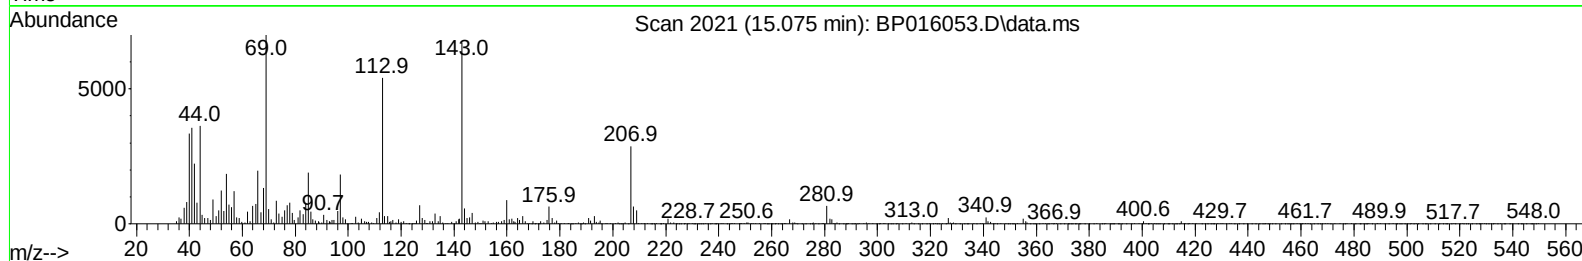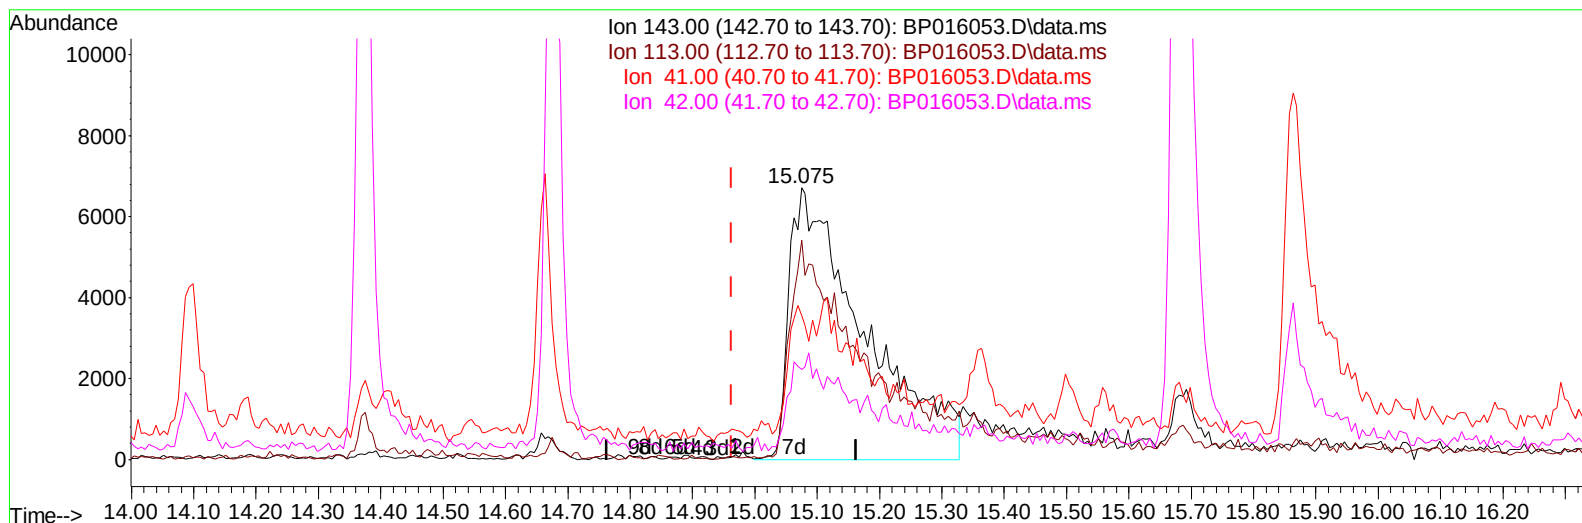

TIC: BP016053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.075min (+ 0.112) 6.94 ng/ul m

response 56008

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	80.65
41.00	45.70	53.00
42.00	31.20	33.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016053.D
 Acq On : 07 Jul 2023 03:10
 Operator : MA/JU
 Sample : 03237-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW77

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :mohammad ahmed 07/07/2023

Quant Time: Jul 07 03:45:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 06 23:18:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	270577	20.000	ng/ul	0.00
20) Naphthalene-d8	10.858	136	1196492	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.675	164	791548	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.440	188	1770831	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1692978	20.000	ng/ul	0.00
88) Perylene-d12	24.080	264	1698270	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	33906	4.508	ng/uL	0.00
4) Pyridine-d5	3.811	84	154626	8.156	ng/ul	0.00
7) Phenol-d5	7.252	99	153172	6.616	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.358	67	462963	32.323	ng/ul	0.00
11) 2-Chlorophenol-d4	7.575	132	446567	25.553	ng/ul	0.01
15) 4-Methylphenol-d8	8.781	113	332050	18.156	ng/ul	0.01
21) Nitrobenzene-d5	9.228	128	286630	31.346	ng/ul	0.01
24) 2-Nitrophenol-d4	9.958	143	311272	29.167	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.540	165	488688	25.696	ng/ul	0.04
31) 4-Chloroaniline-d4	11.046	131	685750	28.070	ng/ul	0.02
46) Dimethylphthalate-d6	14.093	166	2193605	35.855	ng/ul	0.00
49) Acenaphthylene-d8	14.375	160	2291296	33.316	ng/ul	0.00
54) 4-Nitrophenol-d4	15.075	143	56008m	6.937	ng/ul	0.11
60) Fluorene-d10	15.681	176	1825515	36.238	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	292043	26.816	ng/ul	0.01
73) Anthracene-d10	17.545	188	3150335	38.947	ng/ul	0.00
81) Pyrene-d10	19.775	212	3941731	35.656	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	3387742	39.545	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :mohammad ahmed 07/07/2023

Quant Time: Jul 07 03:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 06 23:18:26 2023
Response via : Initial Calibration

