

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016027.D
 Acq On : 06 Jul 2023 10:59
 Operator : MA/JU
 Sample : PB153581BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK581

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	39	rVB	69238	105921	1.53%	0.158%
2	3.805	102	105	127	rBV	639457	1228682	17.69%	1.830%
3	4.122	156	159	165	rVB3	15194	19858	0.29%	0.030%
4	7.222	679	686	703	rBV	529264	1566980	22.56%	2.333%
5	7.357	703	709	732	rVB	630605	1382358	19.91%	2.058%
6	7.563	737	744	766	rVV	771962	1668176	24.02%	2.484%
7	8.028	816	823	841	rBV	486221	1187077	17.09%	1.768%
8	8.781	943	951	990	rBV	745293	2146456	30.91%	3.196%
9	9.228	1018	1027	1052	rBV	729595	1762524	25.38%	2.624%
10	9.957	1143	1151	1180	rBV	524751	1494300	21.52%	2.225%
11	10.534	1241	1249	1297	rBV	455909	2063889	29.72%	3.073%
12	10.863	1297	1305	1322	rVV	835686	1822434	26.24%	2.714%
13	11.046	1327	1336	1366	rBV2	535317	2077617	29.92%	3.094%
14	12.504	1577	1584	1592	rBV3	13489	33113	0.48%	0.049%
15	13.563	1759	1764	1770	rBV2	21051	37696	0.54%	0.056%
16	14.098	1848	1855	1885	rBV	1817164	3661761	52.73%	5.453%
17	14.381	1895	1903	1925	rBV2	2447755	4107839	59.15%	6.117%
18	14.687	1946	1955	1974	rBV	1501899	2546733	36.67%	3.792%
19	14.987	1999	2006	2045	rBV2	271305	1507780	21.71%	2.245%
20	15.686	2118	2125	2143	rBV	2517496	5032206	72.46%	7.493%
21	15.863	2149	2155	2193	rBV	508754	1664044	23.96%	2.478%
22	17.239	2386	2389	2392	rBV4	6241	7862	0.11%	0.012%
23	17.445	2417	2424	2436	rBV	2085224	3164269	45.56%	4.712%
24	17.551	2436	2442	2470	rVB2	2518956	5671266	81.66%	8.445%
25	18.310	2566	2571	2582	rBV2	95151	258054	3.72%	0.384%
26	19.357	2746	2749	2754	rVB	49443	65055	0.94%	0.097%
27	19.433	2759	2762	2770	rVV	36043	62607	0.90%	0.093%
28	19.539	2777	2780	2785	rBV5	34336	55435	0.80%	0.083%
29	19.780	2815	2821	2844	rBV	3598102	6944678	100.00%	10.341%
30	21.551	3117	3122	3133	rBV	1765216	3429885	49.39%	5.107%
31	23.915	3517	3524	3544	rVB2	2546057	6924277	99.71%	10.311%
32	24.086	3546	3553	3574	rVB	1134392	3456383	49.77%	5.147%




Sum of corrected areas: 67157215

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016027.D
Acq On : 06 Jul 2023 10:59
Operator : MA/JU
Sample : PB153581BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

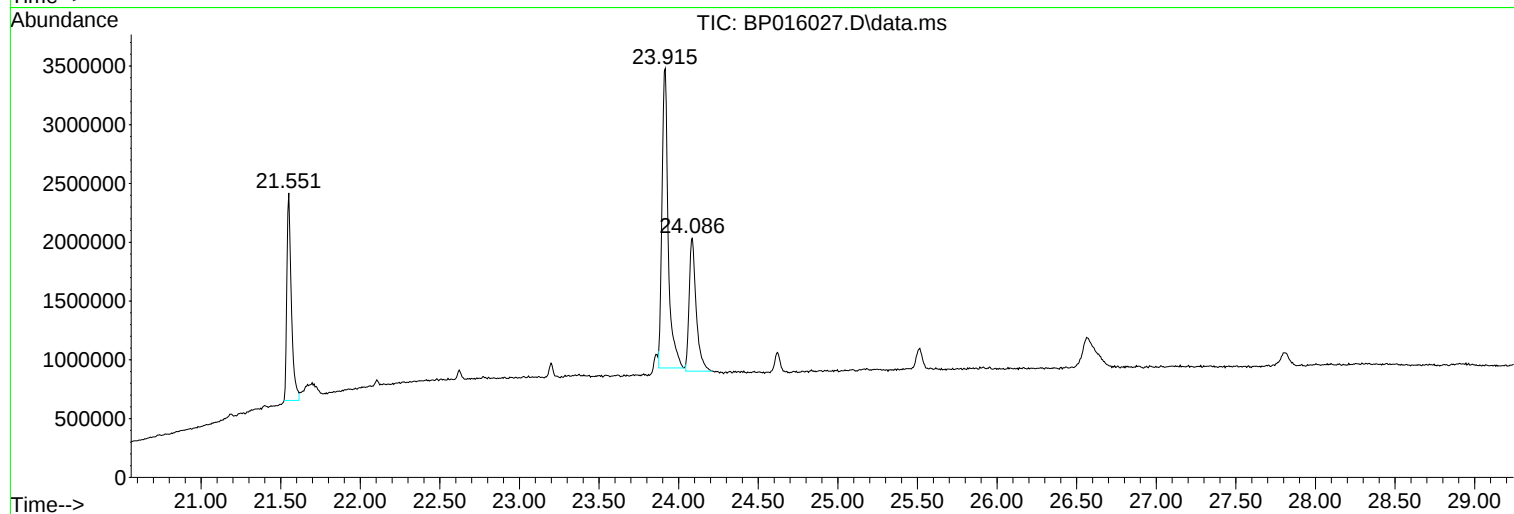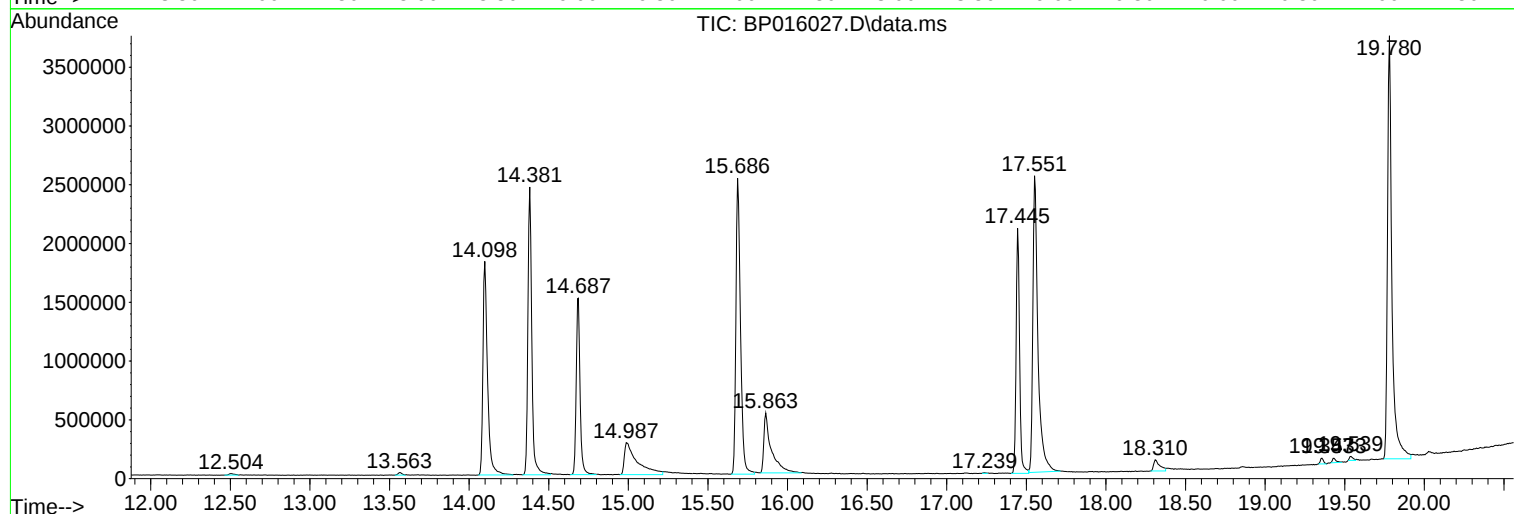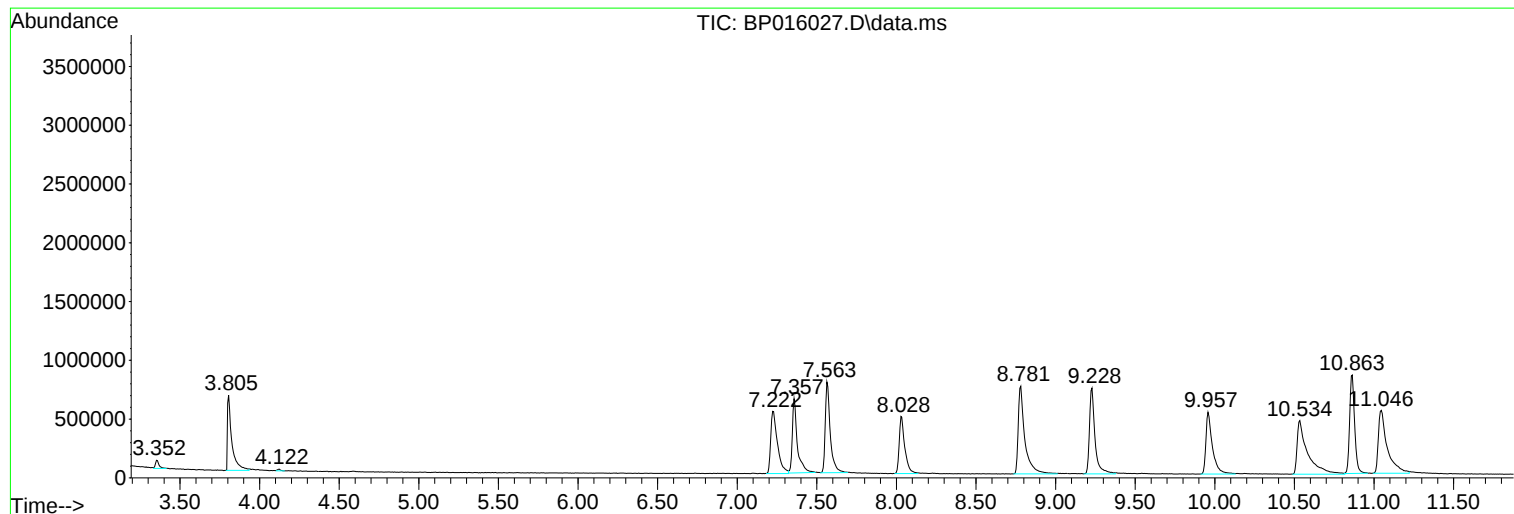

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016027.D
Acq On : 06 Jul 2023 10:59
Operator : MA/JU
Sample : PB153581BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016027.D
Acq On : 06 Jul 2023 10:59
Operator : MA/JU
Sample : PB153581BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK581

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc