

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016029.D
 Acq On : 06 Jul 2023 12:07
 Operator : MA/JU
 Sample : 03257-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	25	29	34	rVB	41404	55988	0.65%	0.077%
2	3.822	105	108	120	rBV	117672	258977	2.99%	0.355%
3	4.117	155	158	162	rBV3	11676	15580	0.18%	0.021%
4	7.105	661	666	672	rVB7	6326	9858	0.11%	0.014%
5	7.258	684	692	703	rBV	100166	299665	3.46%	0.411%
6	7.358	703	709	731	rVB	584888	1355057	15.65%	1.858%
7	7.575	739	746	767	rBV2	469822	1237404	14.29%	1.697%
8	8.034	817	824	834	rBV	568854	1307551	15.10%	1.793%
9	8.122	834	839	841	rBV5	22063	35647	0.41%	0.049%
10	8.787	942	952	968	rBV	348749	1056593	12.20%	1.449%
11	8.899	968	971	990	rVB3	62139	153716	1.78%	0.211%
12	9.163	1010	1016	1019	rBV4	15864	30742	0.36%	0.042%
13	9.228	1020	1027	1054	rVV	778173	1788158	20.65%	2.452%
14	9.957	1143	1151	1173	rBV	478331	1375476	15.89%	1.886%
15	10.110	1175	1177	1182	rVB6	5147	8663	0.10%	0.012%
16	10.534	1241	1249	1280	rBV	463098	1900693	21.95%	2.606%
17	10.857	1297	1304	1314	rBV	965732	2006155	23.17%	2.751%
18	11.040	1328	1335	1365	rBV	490748	1781322	20.57%	2.443%
19	11.616	1427	1433	1434	rBV6	6545	9909	0.11%	0.014%
20	12.498	1577	1583	1590	rBV	14515	31785	0.37%	0.044%
21	12.693	1609	1616	1626	rBV	22774	49417	0.57%	0.068%
22	13.281	1712	1716	1723	rVB5	12858	23307	0.27%	0.032%
23	13.551	1754	1762	1773	rBV2	46039	111123	1.28%	0.152%
24	13.657	1776	1780	1787	rVB10	4730	11640	0.13%	0.016%
25	13.910	1819	1823	1827	rBV7	4711	9120	0.11%	0.013%
26	14.098	1848	1855	1877	rBV	2050451	4036261	46.62%	5.535%
27	14.381	1895	1903	1929	rBV	2651040	4502507	52.00%	6.174%
28	14.540	1929	1930	1938	rVB8	7198	11072	0.13%	0.015%
29	14.681	1945	1954	1964	rBV	1883311	2986766	34.50%	4.095%
30	14.751	1964	1966	1974	rVB2	41544	61035	0.70%	0.084%
31	14.951	1995	2000	2002	rBV6	5267	8840	0.10%	0.012%
32	15.069	2013	2020	2026	rBV6	39322	135000	1.56%	0.185%
33	15.369	2066	2071	2077	rVB3	11004	22241	0.26%	0.030%
34	15.451	2080	2085	2092	rVV2	47662	81234	0.94%	0.111%
35	15.510	2092	2095	2100	rVB2	18478	28004	0.32%	0.038%
36	15.687	2116	2125	2149	rBV	2802312	5792963	66.91%	7.943%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016029.D
 Acq On : 06 Jul 2023 12:07
 Operator : MA/JU
 Sample : 03257-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	15.863	2149	2155	2182	rVV	586474	1796594	20.75%	2.463%
38	16.063	2187	2189	2196	rVB5	20112	33222	0.38%	0.046%
39	16.451	2251	2255	2259	rBV2	6874	13826	0.16%	0.019%
40	17.022	2348	2352	2355	rVB5	7095	9071	0.10%	0.012%
41	17.445	2418	2424	2435	rBV	2358970	3603080	41.61%	4.941%
42	17.551	2435	2442	2467	rVV2	3418222	7060102	81.54%	9.681%
43	17.716	2467	2470	2480	rVB	36149	66101	0.76%	0.091%
44	17.957	2509	2511	2517	rBV6	6174	11750	0.14%	0.016%
45	18.081	2527	2532	2544	rBV	781279	969202	11.19%	1.329%
46	18.304	2565	2570	2579	rBV	138968	310699	3.59%	0.426%
47	18.381	2580	2583	2591	rVB	62733	92649	1.07%	0.127%
48	19.139	2709	2712	2714	rBV2	28621	33722	0.39%	0.046%
49	19.357	2745	2749	2754	rVB2	57032	75842	0.88%	0.104%
50	19.428	2758	2761	2768	rVV	56729	86431	1.00%	0.119%
51	19.533	2775	2779	2792	rBV2	94831	230358	2.66%	0.316%
52	19.780	2815	2821	2849	rBV	4668511	8658233	100.00%	11.872%
53	21.551	3117	3122	3134	rBV	2102983	4004474	46.25%	5.491%
54	22.716	3316	3320	3326	rVB	725769	1014832	11.72%	1.392%
55	23.916	3517	3524	3544	rVB2	3237133	8160029	94.25%	11.189%
56	24.086	3547	3553	3578	rVB	1319300	4109270	47.46%	5.635%




Sum of corrected areas: 72928956

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016029.D
Acq On : 06 Jul 2023 12:07
Operator : MA/JU
Sample : 03257-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

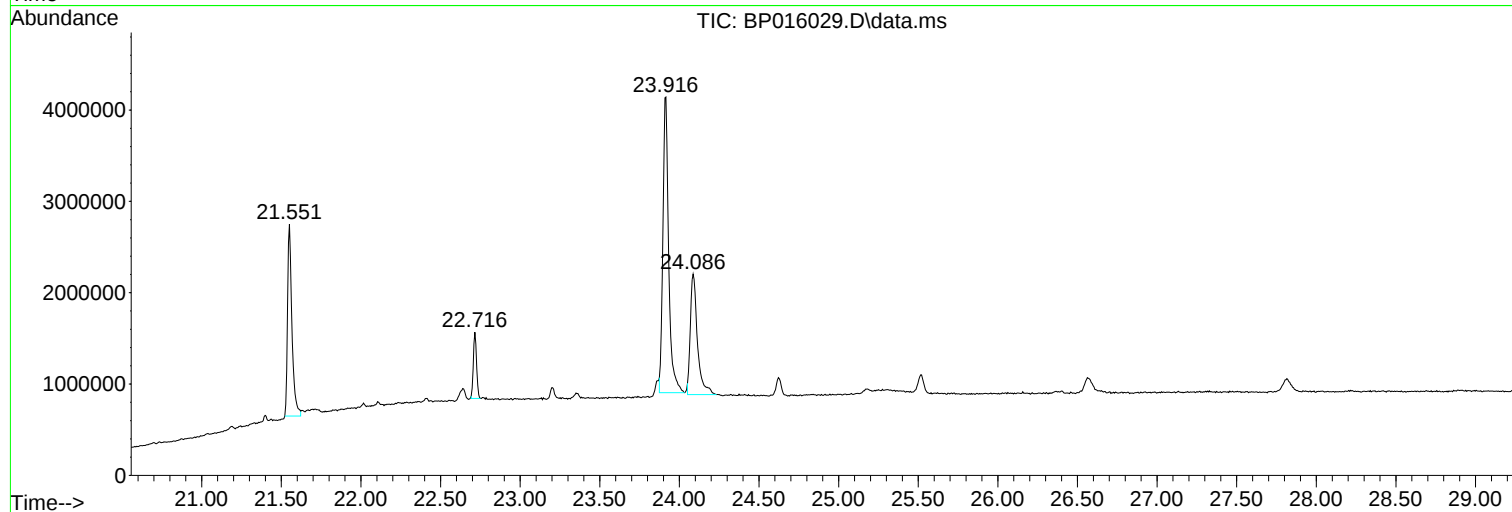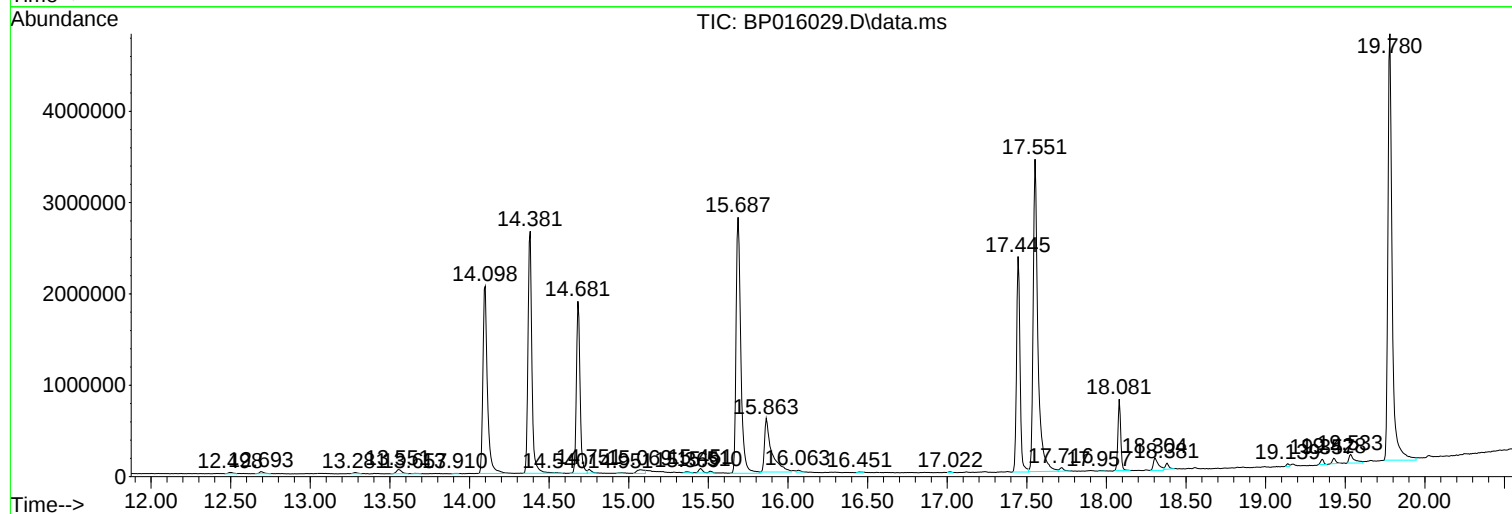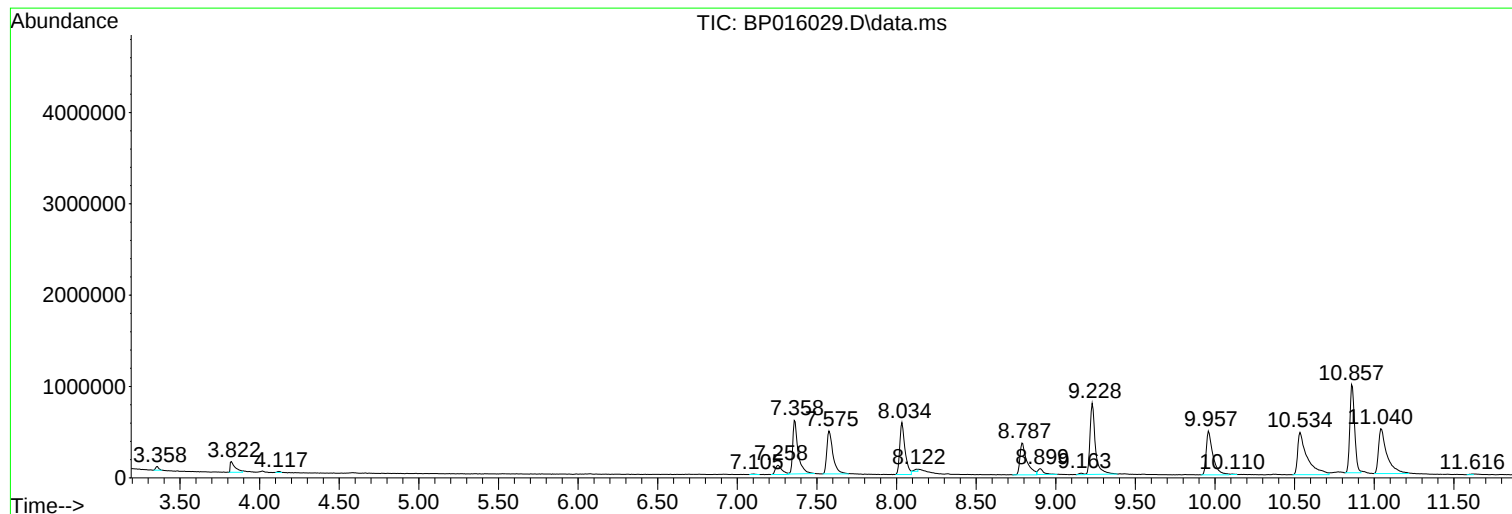

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016029.D
Acq On : 06 Jul 2023 12:07
Operator : MA/JU
Sample : 03257-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.081	5.38 ng/ul	969202	Phenanthrene-d10	17.445

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	99		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	92		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	91		
4	(1R,3aR,5aR,9aS)-1,4,4,7-Tetrame...	220	C15H24O	104188-25-2	50		
5	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	50		

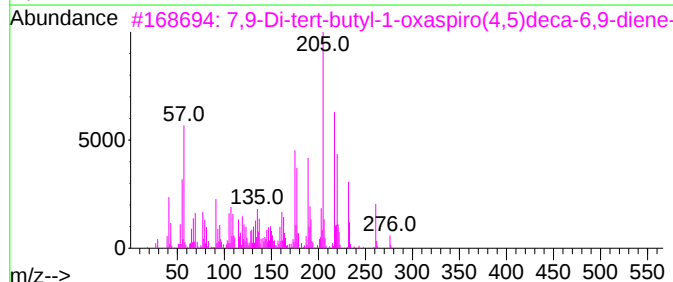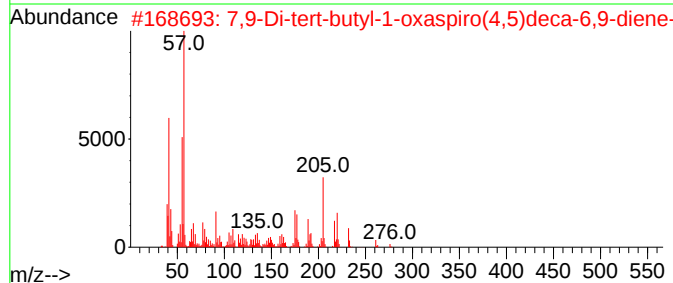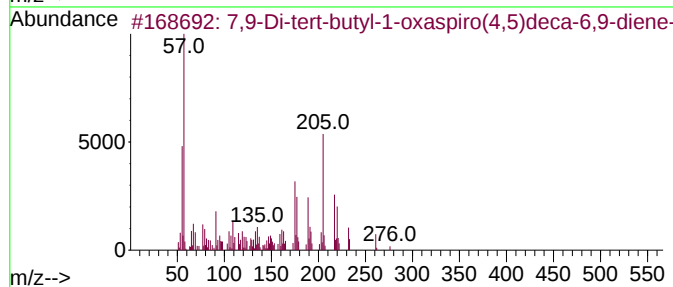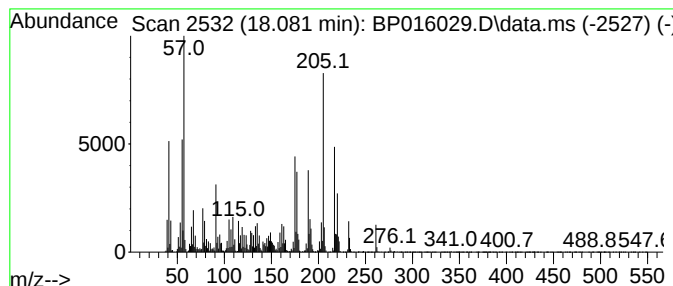

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016029.D
Acq On : 06 Jul 2023 12:07
Operator : MA/JU
Sample : 03257-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Hexanedioic acid, bis[2-(2-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.716	5.07 ng/ul	1014830	Chrysene-d12	21.551

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis[2-(2-butox...	434	C22H42O8	000141-17-3	93
2			Butane, 1,1'-[oxybis(2,1-ethaned...	218	C12H26O3	000112-73-2	37
3			1-Decanamine	157	C10H23N	002016-57-1	35
4			Succinic acid, di(2-butoxyethyl)...	318	C16H30O6	1010325-84-7	16
5			Propane, 1,1'-[ethylidenebis(oxy...	174	C10H22O2	005669-09-0	14

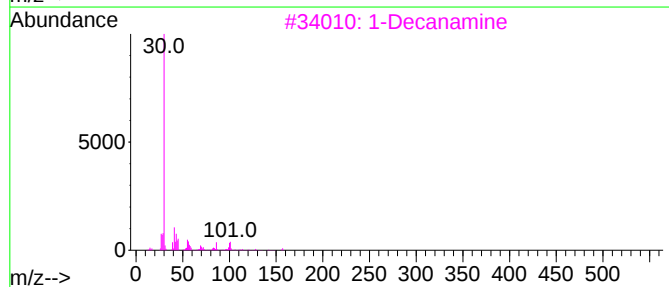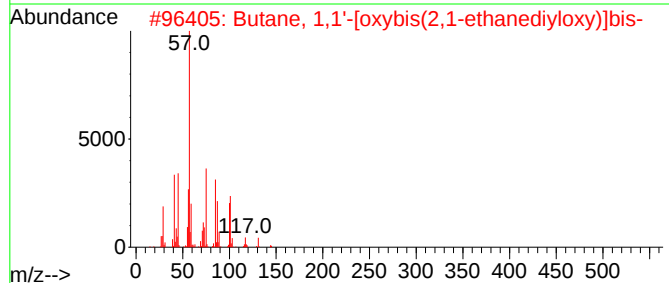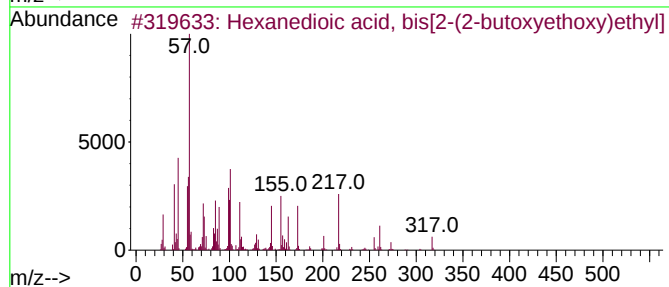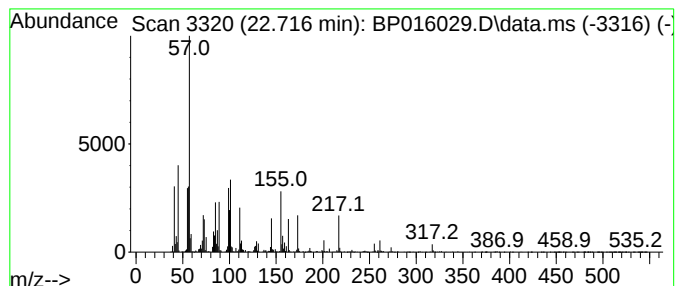

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016029.D
Acq On : 06 Jul 2023 12:07
Operator : MA/JU
Sample : 03257-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	18.081	5.4	ng/ul	969202	4	17.445	3603080	20.0
Hexanedioic aci...	22.716	5.1	ng/ul	1014830	5	21.551	4004470	20.0