

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016030.D
 Acq On : 06 Jul 2023 12:42
 Operator : MA/JU
 Sample : 03257-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	36	rVB	47153	75021	1.02%	0.119%
2	3.822	105	108	127	rBV	98832	235805	3.20%	0.373%
3	4.022	138	142	146	rVB2	14590	23711	0.32%	0.037%
4	4.122	155	159	164	rVB2	18323	28401	0.39%	0.045%
5	4.581	234	237	241	rBV3	9160	13529	0.18%	0.021%
6	4.658	248	250	256	rVB4	6783	8120	0.11%	0.013%
7	6.899	624	631	632	rBV7	5639	10763	0.15%	0.017%
8	7.105	662	666	669	rBV6	8000	11879	0.16%	0.019%
9	7.263	679	693	704	rBV	84228	267205	3.63%	0.422%
10	7.363	704	710	736	rVV	507561	1260810	17.12%	1.993%
11	7.581	739	747	773	rVV	408811	1125183	15.28%	1.779%
12	8.034	816	824	834	rBV	516648	1195055	16.23%	1.889%
13	8.128	835	840	868	rVB4	64577	364865	4.95%	0.577%
14	8.793	945	953	968	rBV	277533	873953	11.87%	1.382%
15	8.910	968	973	990	rVB	60723	167447	2.27%	0.265%
16	9.163	1008	1016	1020	rBV2	17180	33853	0.46%	0.054%
17	9.234	1020	1028	1054	rVV	644966	1569360	21.31%	2.481%
18	9.963	1144	1152	1178	rBV	407682	1284513	17.44%	2.031%
19	10.381	1219	1223	1227	rVB7	4993	7894	0.11%	0.012%
20	10.546	1243	1251	1281	rBV2	395316	1710325	23.23%	2.704%
21	10.863	1297	1305	1315	rBV	829555	1839212	24.98%	2.908%
22	11.051	1330	1337	1373	rBV	348070	1393742	18.93%	2.203%
23	11.634	1430	1436	1443	rBV8	8240	21269	0.29%	0.034%
24	12.416	1561	1569	1575	rBV8	9117	27552	0.37%	0.044%
25	12.504	1579	1584	1590	rVV3	11230	23552	0.32%	0.037%
26	12.692	1612	1616	1624	rBV	18811	35952	0.49%	0.057%
27	13.063	1673	1679	1684	rBV10	5272	11657	0.16%	0.018%
28	13.281	1713	1716	1726	rVB6	11561	19715	0.27%	0.031%
29	13.545	1756	1761	1776	rVV3	28734	78022	1.06%	0.123%
30	13.663	1776	1781	1791	rVB3	7494	18804	0.26%	0.030%
31	14.098	1848	1855	1878	rBV	1763259	3506128	47.61%	5.543%
32	14.381	1896	1903	1928	rBV	2276614	3820614	51.88%	6.040%
33	14.551	1928	1932	1938	rVB6	14253	23688	0.32%	0.037%
34	14.639	1942	1947	1948	rBV	52123	63000	0.86%	0.100%
35	14.681	1948	1954	1963	rVB	1568171	2640519	35.86%	4.175%
36	15.075	2016	2021	2023	rBV4	26672	45994	0.62%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016030.D
 Acq On : 06 Jul 2023 12:42
 Operator : MA/JU
 Sample : 03257-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	15.363	2067	2070	2076	rVB4	12504	25543	0.35%	0.040%
38	15.451	2080	2085	2090	rVV	32361	47856	0.65%	0.076%
39	15.504	2090	2094	2102	rVB3	27021	48822	0.66%	0.077%
40	15.686	2118	2125	2143	rBV	2454490	4978709	67.61%	7.871%
41	15.869	2150	2156	2182	rBV	490218	1625017	22.07%	2.569%
42	16.069	2186	2190	2196	rVB2	26579	45714	0.62%	0.072%
43	16.363	2236	2240	2247	rBV2	34764	73231	0.99%	0.116%
44	16.428	2247	2251	2256	rVV	29304	49718	0.68%	0.079%
45	16.480	2256	2260	2273	rVB	19094	54731	0.74%	0.087%
46	16.933	2335	2337	2341	rBV5	5769	7663	0.10%	0.012%
47	17.016	2347	2351	2355	rVB7	9994	15592	0.21%	0.025%
48	17.157	2371	2375	2379	rBV	40273	53691	0.73%	0.085%
49	17.204	2379	2383	2387	rVV2	25693	37987	0.52%	0.060%
50	17.445	2418	2424	2436	rBV	2106579	3328743	45.20%	5.263%
51	17.551	2436	2442	2464	rVB2	2875868	5762301	78.25%	9.110%
52	17.898	2498	2501	2507	rVB2	40329	50646	0.69%	0.080%
53	18.080	2527	2532	2545	rVB	816197	973123	13.22%	1.538%
54	18.304	2566	2570	2579	rBV3	100479	236707	3.21%	0.374%
55	18.380	2580	2583	2588	rVB	42836	60438	0.82%	0.096%
56	18.563	2611	2614	2618	rVB	40454	51900	0.70%	0.082%
57	19.169	2715	2717	2720	rBV	35505	37347	0.51%	0.059%
58	19.204	2720	2723	2728	rVB6	47548	49970	0.68%	0.079%
59	19.333	2742	2745	2746	rBV2	28733	31758	0.43%	0.050%
60	19.357	2746	2749	2754	rVV3	53478	69275	0.94%	0.110%
61	19.427	2758	2761	2766	rVV	50710	74186	1.01%	0.117%
62	19.527	2774	2778	2787	rBV	144196	296650	4.03%	0.469%
63	19.780	2815	2821	2843	rBV	4099858	7363728	100.00%	11.642%
64	21.551	3117	3122	3133	rBV	1892883	3693774	50.16%	5.840%
65	23.915	3517	3524	3545	rVB2	2764533	7005908	95.14%	11.076%
66	24.086	3547	3553	3568	rVB	1179823	3264355	44.33%	5.161%




Sum of corrected areas: 63252195

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016030.D
Acq On : 06 Jul 2023 12:42
Operator : MA/JU
Sample : 03257-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

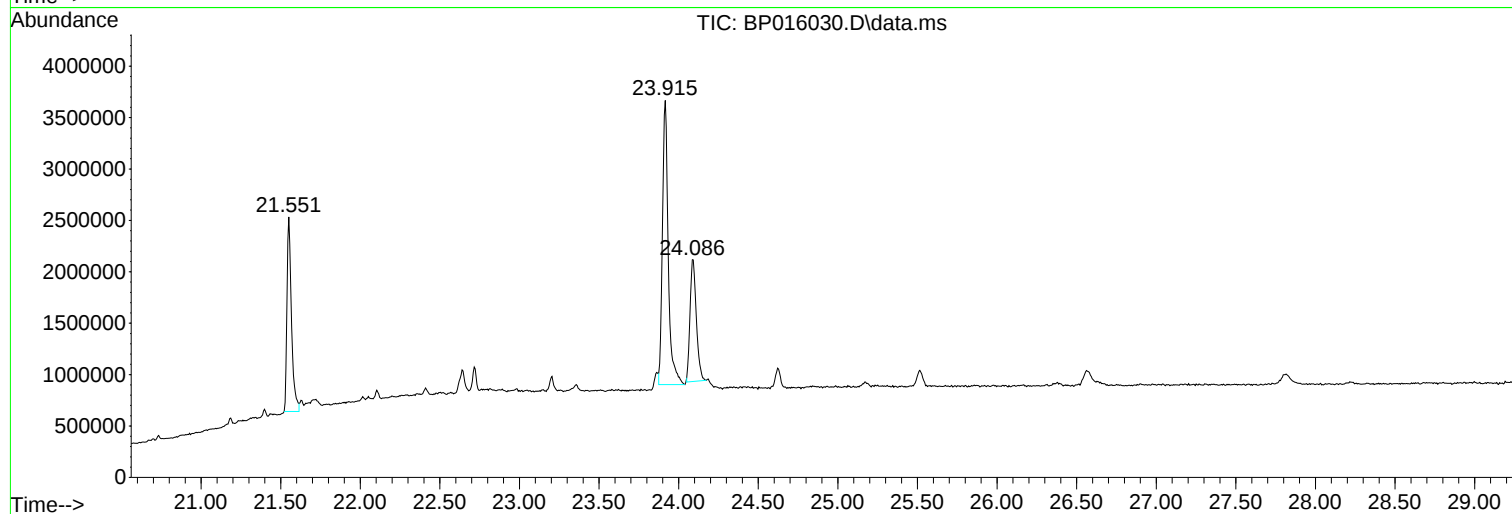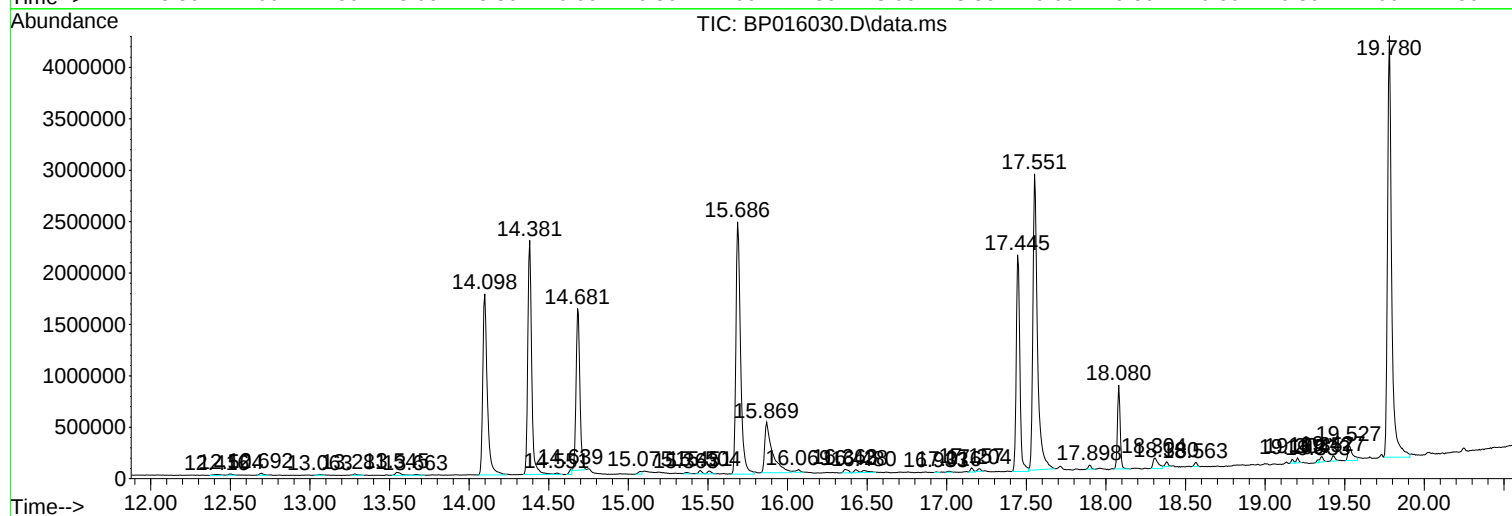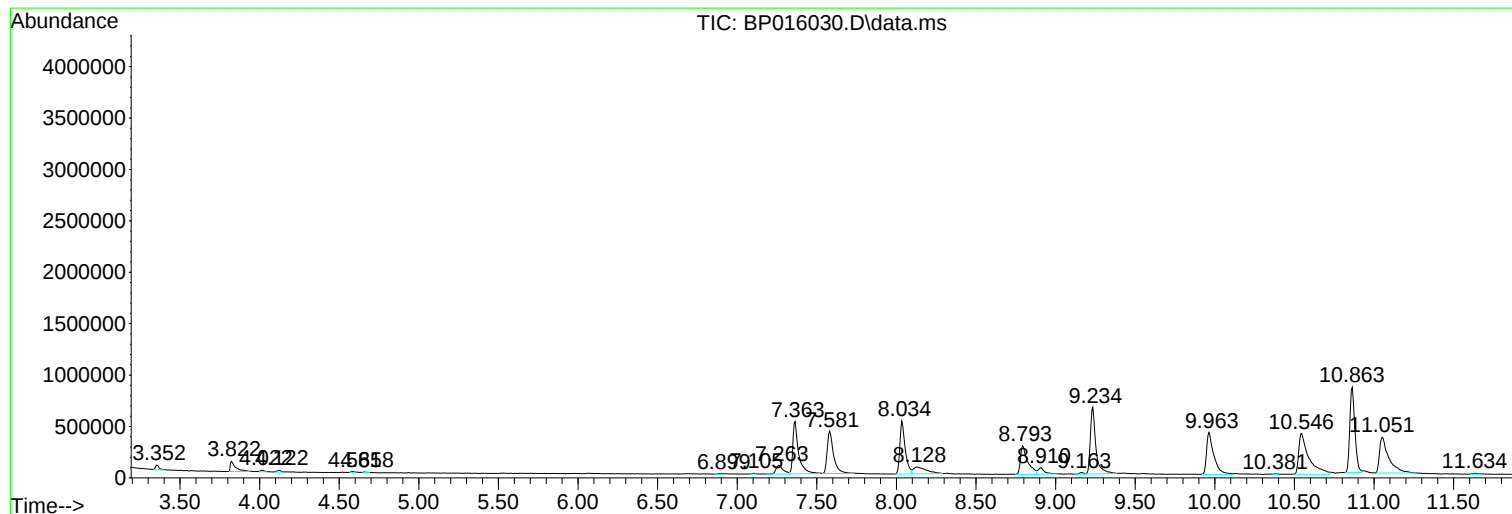

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016030.D
Acq On : 06 Jul 2023 12:42
Operator : MA/JU
Sample : 03257-15
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EXYY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
8.128	6.11 ng/ul	364865	1,4-Dichlorobenzene-d4			8.034
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Octane, 2,3-dimethyl-		142	C10H22	007146-60-3	59
2	Carbonic acid, isobutyl 2-ethylh...		230	C13H26O3	1000383-13-3	53
3	Heptane, 3,5-dimethyl-		128	C9H20	000926-82-9	45
4	1-Decene		140	C10H20	000872-05-9	43
5	Cyclobutanone, 2,2-dimethyl-		98	C6H10O	001192-14-9	43

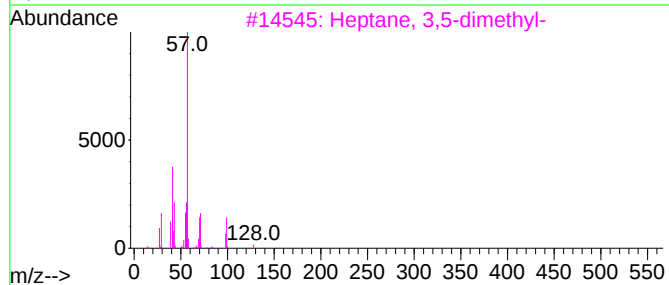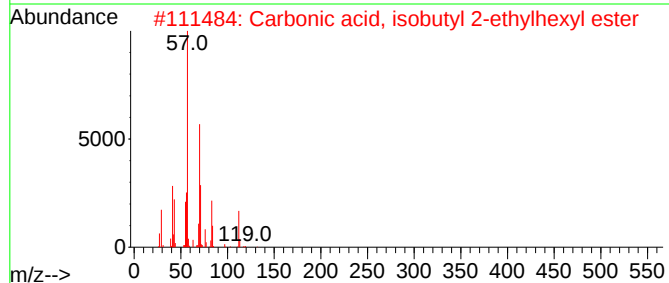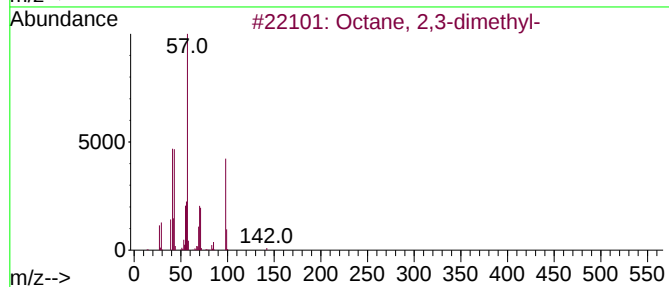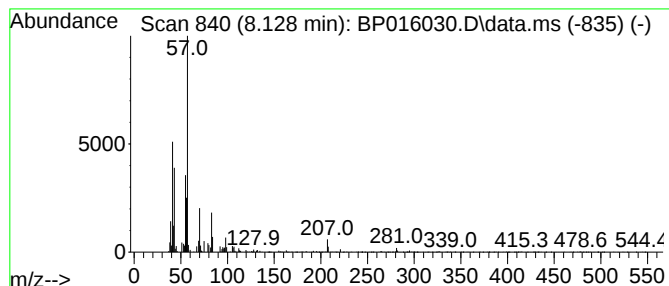

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016030.D
Acq On : 06 Jul 2023 12:42
Operator : MA/JU
Sample : 03257-15
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EXYY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
18.080	5.85 ng/ul	973123	Phenanthrene-d10	17.445	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	98
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	74
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	60
4	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	50
5	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	50

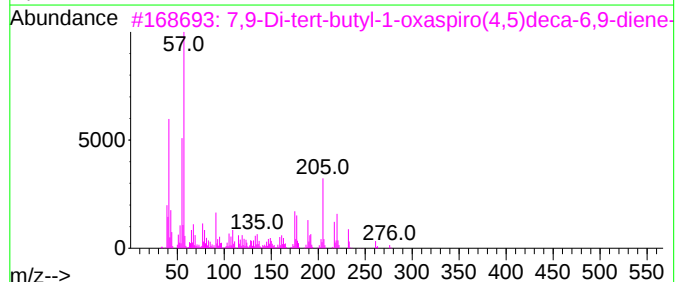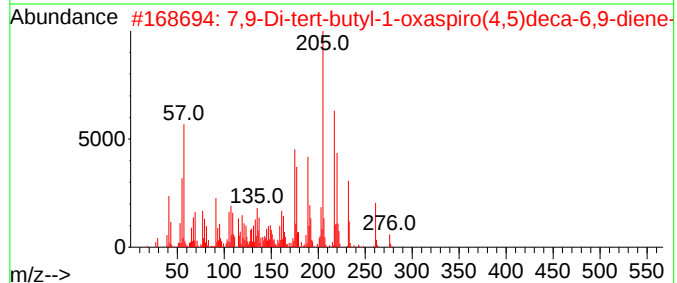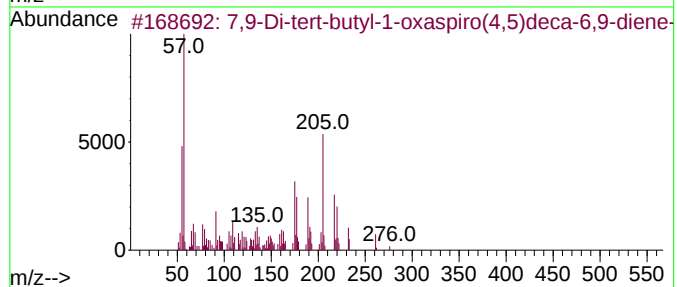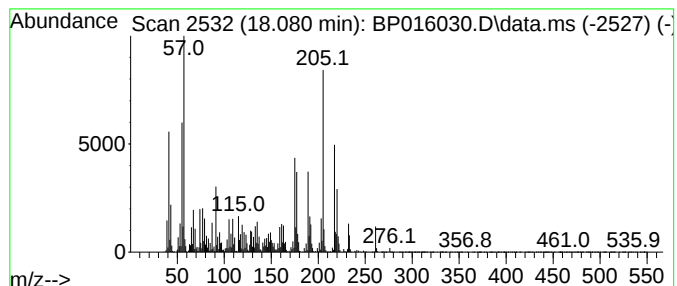

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016030.D
Acq On : 06 Jul 2023 12:42
Operator : MA/JU
Sample : 03257-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	8.128	6.1	ng/ul	364865	1	8.034	1195060	20.0
7,9-Di-tert-but...	18.080	5.8	ng/ul	973123	4	17.445	3328740	20.0