

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016040.D
 Acq On : 06 Jul 2023 19:46
 Operator : MA/JU
 Sample : PB153518BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK518

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	91194	137362	1.58%	0.174%
2	3.799	101	104	128	rBV	822970	1621851	18.63%	2.050%
3	4.117	155	158	165	rVB3	14100	19626	0.23%	0.025%
4	7.222	678	686	703	rBV	702814	2011812	23.11%	2.543%
5	7.358	703	709	731	rVB	768882	1695262	19.48%	2.143%
6	7.563	737	744	764	rBV	977073	2085800	23.96%	2.637%
7	8.028	815	823	840	rBV	489987	1216194	13.97%	1.537%
8	8.228	853	857	861	rVB7	6497	9666	0.11%	0.012%
9	8.775	942	950	981	rBV	970717	2703922	31.07%	3.418%
10	9.222	1019	1026	1046	rBV	905534	2180232	25.05%	2.756%
11	9.957	1140	1151	1172	rBV	654772	1861668	21.39%	2.353%
12	10.528	1241	1248	1285	rBV	566886	2477031	28.46%	3.131%
13	10.863	1297	1305	1325	rVB	853203	1841087	21.15%	2.327%
14	11.046	1328	1336	1369	rBV	651729	2577937	29.62%	3.259%
15	12.516	1580	1586	1591	rBV3	14416	32993	0.38%	0.042%
16	13.569	1759	1765	1769	rBV5	9846	20181	0.23%	0.026%
17	14.098	1848	1855	1879	rBV	2159841	4463183	51.28%	5.642%
18	14.381	1896	1903	1929	rBV	2955725	5027354	57.76%	6.355%
19	14.681	1948	1954	1969	rBV	1506585	2553218	29.33%	3.228%
20	14.987	2000	2006	2044	rBV	328045	1786845	20.53%	2.259%
21	15.687	2117	2125	2147	rBV	2928021	6242148	71.72%	7.891%
22	15.863	2149	2155	2194	rVV	582067	2016590	23.17%	2.549%
23	17.245	2386	2390	2395	rVB7	6306	9566	0.11%	0.012%
24	17.445	2418	2424	2436	rBV	2035324	3182260	36.56%	4.023%
25	17.557	2436	2443	2473	rVB2	2873586	7026122	80.72%	8.882%
26	18.345	2572	2577	2578	rBV5	20469	28754	0.33%	0.036%
27	19.357	2745	2749	2754	rBV2	61842	88970	1.02%	0.112%
28	19.433	2759	2762	2773	rVV	41793	82130	0.94%	0.104%
29	19.780	2815	2821	2847	rBV	4250890	8704061	100.00%	11.003%
30	21.557	3117	3123	3138	rBV	1669895	3730075	42.85%	4.715%
31	23.910	3517	3523	3545	rVB2	3054929	8091778	92.97%	10.229%
32	24.086	3547	3553	3576	rVB	1088409	3581421	41.15%	4.527%




Sum of corrected areas: 79107099

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016040.D
Acq On : 06 Jul 2023 19:46
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

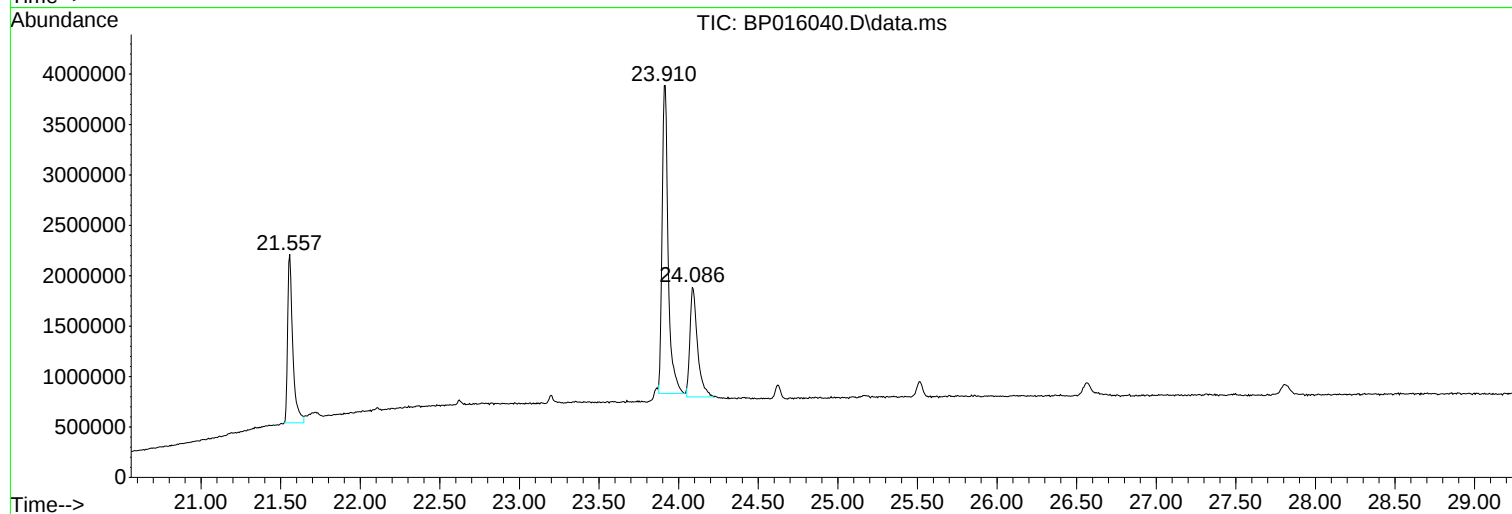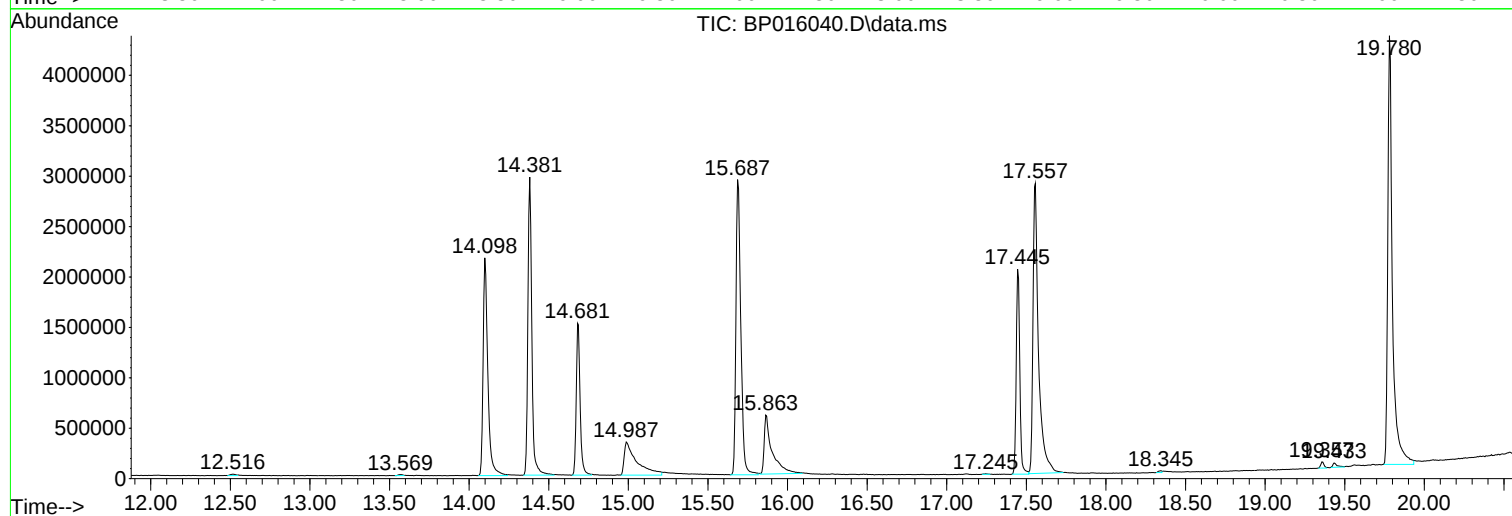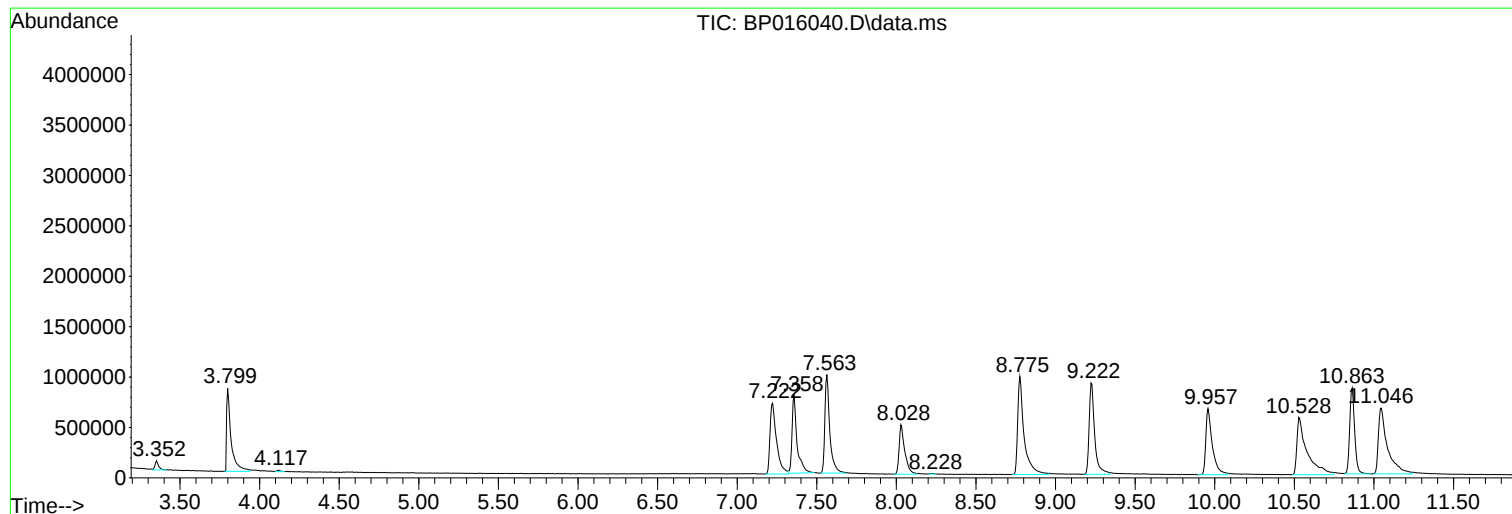

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016040.D
Acq On : 06 Jul 2023 19:46
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016040.D
Acq On : 06 Jul 2023 19:46
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------