

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016045.D
 Acq On : 06 Jul 2023 22:37
 Operator : MA/JU
 Sample : 03283-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	31	rBV	55217	70510	0.66%	0.084%
2	3.387	31	34	49	rVB	192327	295481	2.77%	0.352%
3	3.817	106	107	128	rBV	147237	354541	3.33%	0.423%
4	4.117	156	158	164	rVB2	16213	22551	0.21%	0.027%
5	7.093	661	664	672	rVB7	10545	21375	0.20%	0.025%
6	7.258	684	692	704	rBV2	96917	312376	2.93%	0.373%
7	7.358	704	709	739	rVV	570941	1581704	14.85%	1.886%
8	7.581	739	747	776	rVB	490078	1448126	13.59%	1.727%
9	8.034	817	824	854	rBV	625914	1684368	15.81%	2.009%
10	8.793	945	953	976	rBV	307893	1120759	10.52%	1.337%
11	9.228	1020	1027	1053	rBV	780799	1968016	18.47%	2.347%
12	9.546	1077	1081	1089	rVB4	17716	29504	0.28%	0.035%
13	9.963	1144	1152	1178	rBV	474756	1630477	15.30%	1.944%
14	10.552	1242	1252	1272	rBV	449355	1914694	17.97%	2.283%
15	10.857	1297	1304	1323	rBV	1054943	2558379	24.01%	3.051%
16	11.057	1330	1338	1374	rBV	350691	1546808	14.52%	1.845%
17	12.510	1581	1585	1593	rBV4	12330	28826	0.27%	0.034%
18	13.569	1759	1765	1771	rBV3	14908	29304	0.28%	0.035%
19	14.098	1847	1855	1875	rBV	2099045	4485821	42.11%	5.350%
20	14.375	1895	1902	1923	rBV	2863218	5036781	47.28%	6.007%
21	14.681	1947	1954	1974	rBV	2293161	3750678	35.21%	4.473%
22	15.110	2016	2027	2032	rBV8	32861	138390	1.30%	0.165%
23	15.457	2081	2086	2091	rVV2	16775	26897	0.25%	0.032%
24	15.522	2093	2097	2103	rVB5	10363	18233	0.17%	0.022%
25	15.687	2117	2125	2149	rBV	3204955	6754728	63.40%	8.056%
26	15.863	2149	2155	2184	rVV	685925	2333366	21.90%	2.783%
27	16.063	2184	2189	2202	rVB	135967	277482	2.60%	0.331%
28	16.281	2220	2226	2231	rBV8	7100	16089	0.15%	0.019%
29	17.445	2417	2424	2435	rBV	2938608	4708588	44.20%	5.615%
30	17.551	2435	2442	2468	rVB	3741374	8419696	79.03%	10.041%
31	17.904	2499	2502	2507	rBV7	12639	18758	0.18%	0.022%
32	18.086	2530	2533	2536	rBV5	12203	15338	0.14%	0.018%
33	18.304	2566	2570	2580	rBV4	86854	221197	2.08%	0.264%
34	18.381	2581	2583	2588	rVB	21748	29637	0.28%	0.035%
35	19.351	2744	2748	2754	rBV2	81844	121954	1.14%	0.145%
36	19.428	2757	2761	2770	rVV	62271	118524	1.11%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016045.D
Acq On : 06 Jul 2023 22:37
Operator : MA/JU
Sample : 03283-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYW5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.533	2775	2779	2786	rBV4	60013	123418	1.16%	0.147%
38	19.775	2814	2820	2843	rBV	5560632	10653411	100.00%	12.705%
39	21.545	3116	3121	3139	rBV	2422275	5451344	51.17%	6.501%
40	23.910	3516	3523	3544	rVB	3670572	9219678	86.54%	10.995%
41	24.080	3546	3552	3582	rVB	1627841	5293611	49.69%	6.313%




Sum of corrected areas: 83851418

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016045.D
Acq On : 06 Jul 2023 22:37
Operator : MA/JU
Sample : 03283-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

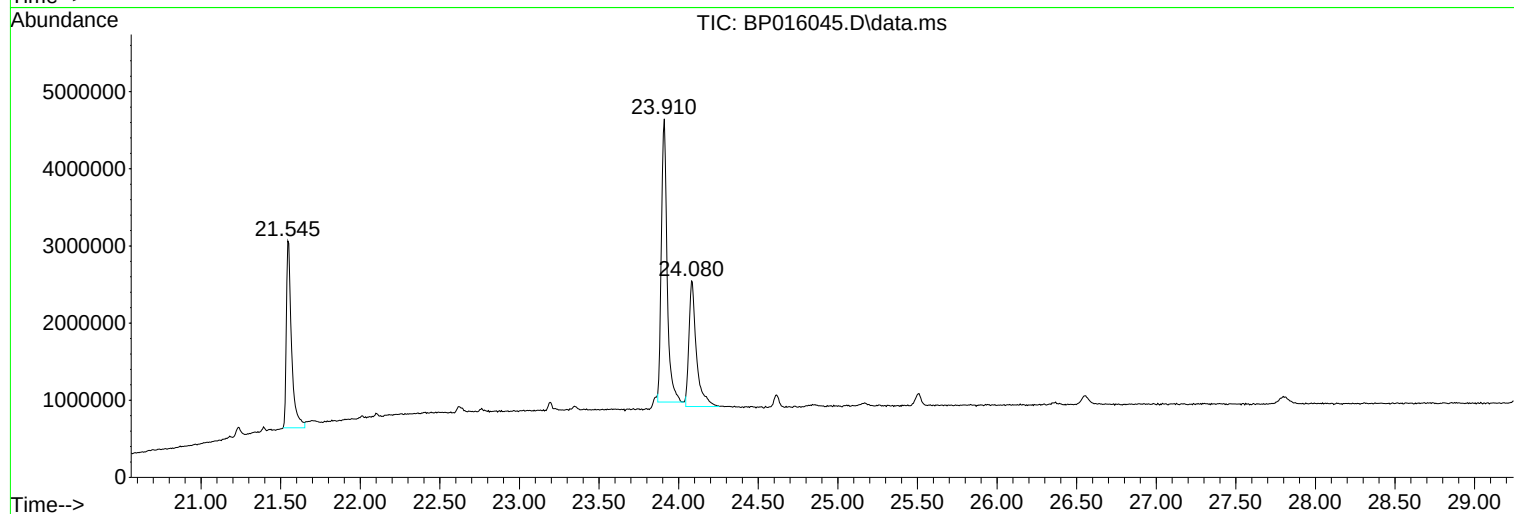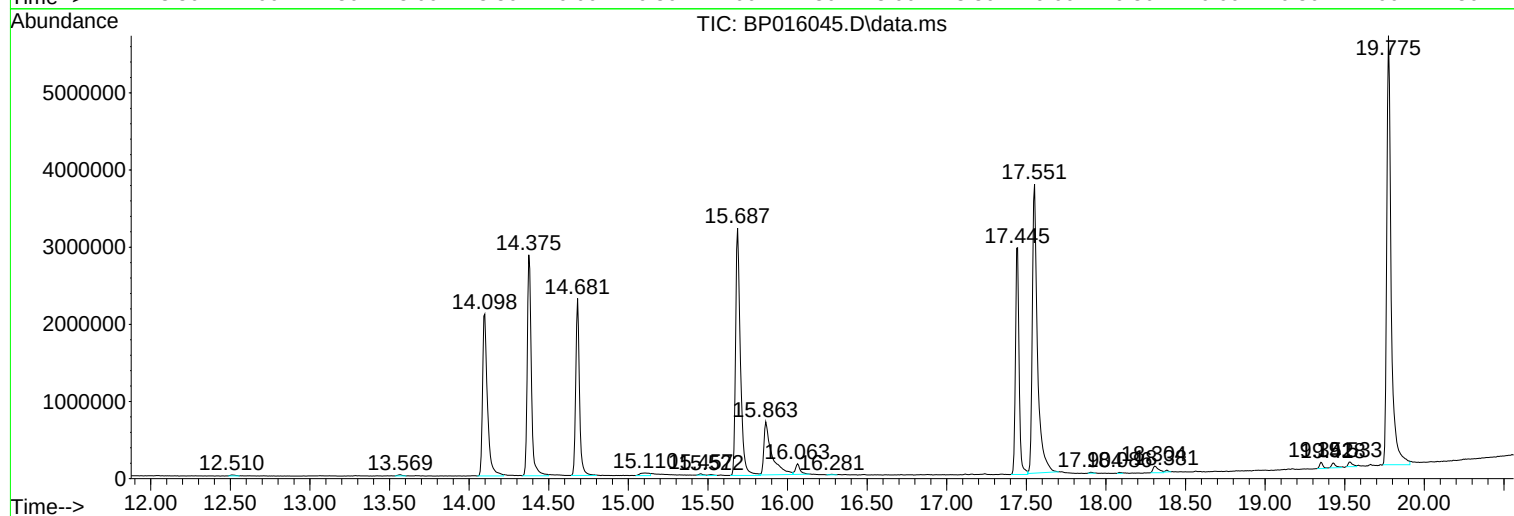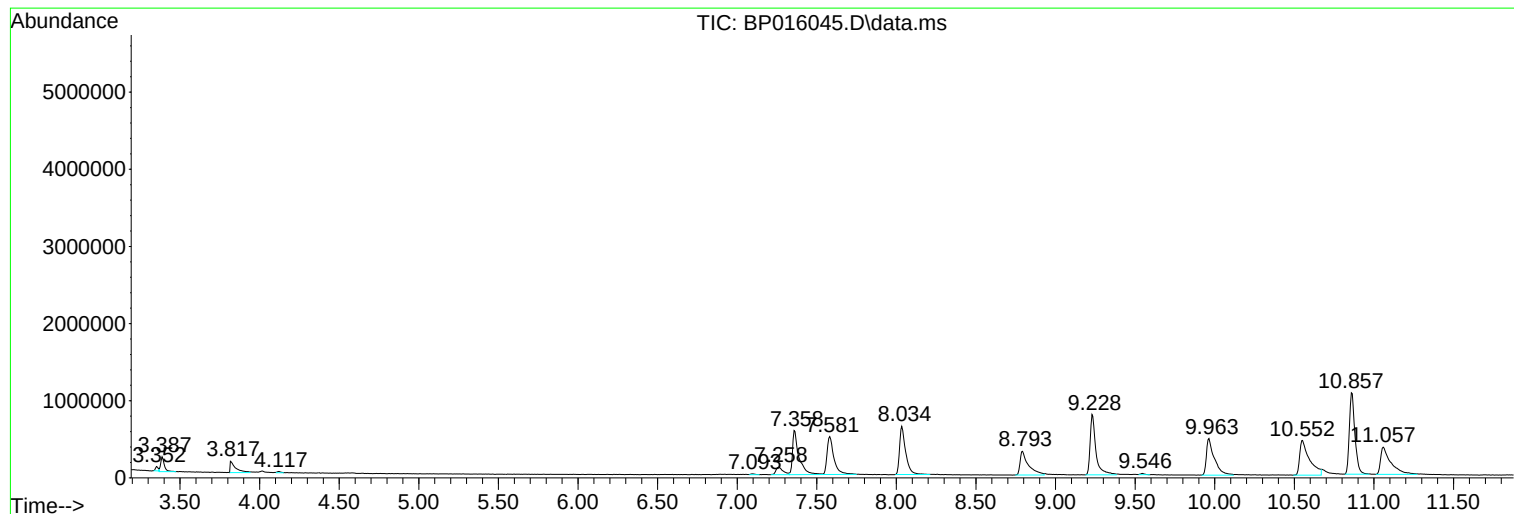

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016045.D
Acq On : 06 Jul 2023 22:37
Operator : MA/JU
Sample : 03283-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016045.D
Acq On : 06 Jul 2023 22:37
Operator : MA/JU
Sample : 03283-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc