

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016051.D
 Acq On : 07 Jul 2023 02:02
 Operator : MA/JU
 Sample : 03284-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCGZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	38	rVB	75483	114026	0.90%	0.114%
2	3.817	104	107	120	rBV	174075	386590	3.06%	0.387%
3	4.017	136	141	152	rVB	28712	55511	0.44%	0.056%
4	4.122	155	159	163	rVB	14928	22939	0.18%	0.023%
5	7.240	682	689	702	rBV	209316	602600	4.77%	0.603%
6	7.352	702	708	737	rVV	995275	2297627	18.20%	2.300%
7	7.569	737	745	766	rVV	901084	2245746	17.79%	2.248%
8	8.028	816	823	841	rBV	690440	1646539	13.04%	1.648%
9	8.781	943	951	982	rBV	533411	1722225	13.64%	1.724%
10	9.222	1017	1026	1052	rBV	1282948	2934437	23.24%	2.937%
11	9.546	1076	1081	1089	rVB7	11683	24891	0.20%	0.025%
12	9.952	1142	1150	1175	rBV	865443	2487947	19.71%	2.490%
13	10.534	1241	1249	1289	rBV	756373	3245963	25.71%	3.249%
14	10.857	1296	1304	1321	rVB	1136829	2494449	19.76%	2.497%
15	11.057	1330	1338	1374	rVB	355499	1481773	11.74%	1.483%
16	12.504	1578	1584	1593	rBV2	21401	51087	0.40%	0.051%
17	13.557	1757	1763	1771	rBV	32978	63279	0.50%	0.063%
18	14.092	1846	1854	1879	rBV	3244822	6359140	50.37%	6.364%
19	14.375	1894	1902	1927	rBV	4406104	7292026	57.76%	7.298%
20	14.675	1946	1953	1973	rBV	2208299	3619687	28.67%	3.623%
21	14.940	1993	1998	2003	rBV6	11727	27150	0.22%	0.027%
22	15.063	2010	2019	2020	rBV4	60636	136848	1.08%	0.137%
23	15.445	2081	2084	2089	rVB4	8690	13850	0.11%	0.014%
24	15.681	2116	2124	2139	rBV	4603267	9172637	72.65%	9.180%
25	15.857	2148	2154	2182	rBV	964194	2803974	22.21%	2.806%
26	16.057	2183	2188	2206	rVB	183732	360249	2.85%	0.361%
27	17.116	2364	2368	2371	rBV6	9211	12676	0.10%	0.013%
28	17.351	2401	2408	2413	rBV6	7530	18051	0.14%	0.018%
29	17.439	2417	2423	2435	rBV	2892156	4543110	35.98%	4.547%
30	17.545	2435	2441	2467	rVB2	4457152	9727074	77.05%	9.735%
31	18.086	2530	2533	2536	rVB5	13176	17486	0.14%	0.018%
32	18.298	2564	2569	2579	rBV2	151639	346986	2.75%	0.347%
33	18.381	2580	2583	2589	rVB	37915	55093	0.44%	0.055%
34	19.345	2743	2747	2753	rBV	93432	144417	1.14%	0.145%
35	19.422	2757	2760	2768	rVV	83629	137361	1.09%	0.137%
36	19.527	2774	2778	2786	rBV4	84755	178639	1.41%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGZ7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.775	2813	2820	2839	rBV	6687688	12625093	100.00%	12.636%
38	21.545	3116	3121	3138	rBV	2213653	5082307	40.26%	5.086%
39	23.904	3514	3522	3543	rVV2	4171493	10825312	85.74%	10.834%
40	24.080	3545	3552	3574	rVB	1414589	4540787	35.97%	4.545%




Sum of corrected areas: 99917582

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGZ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

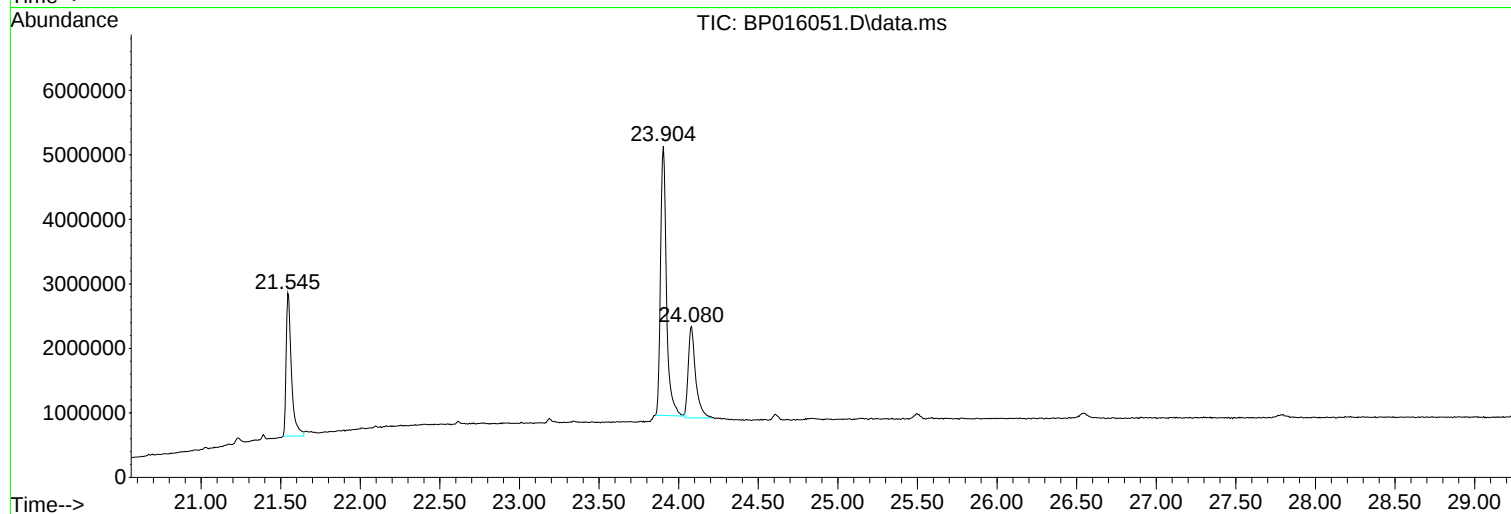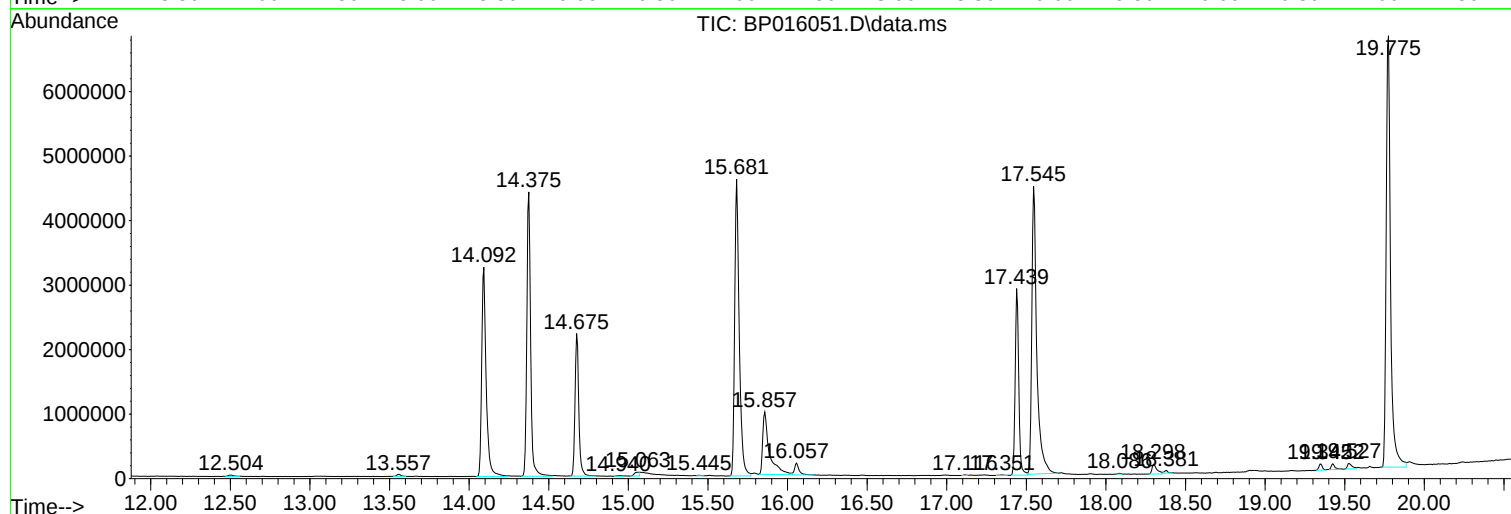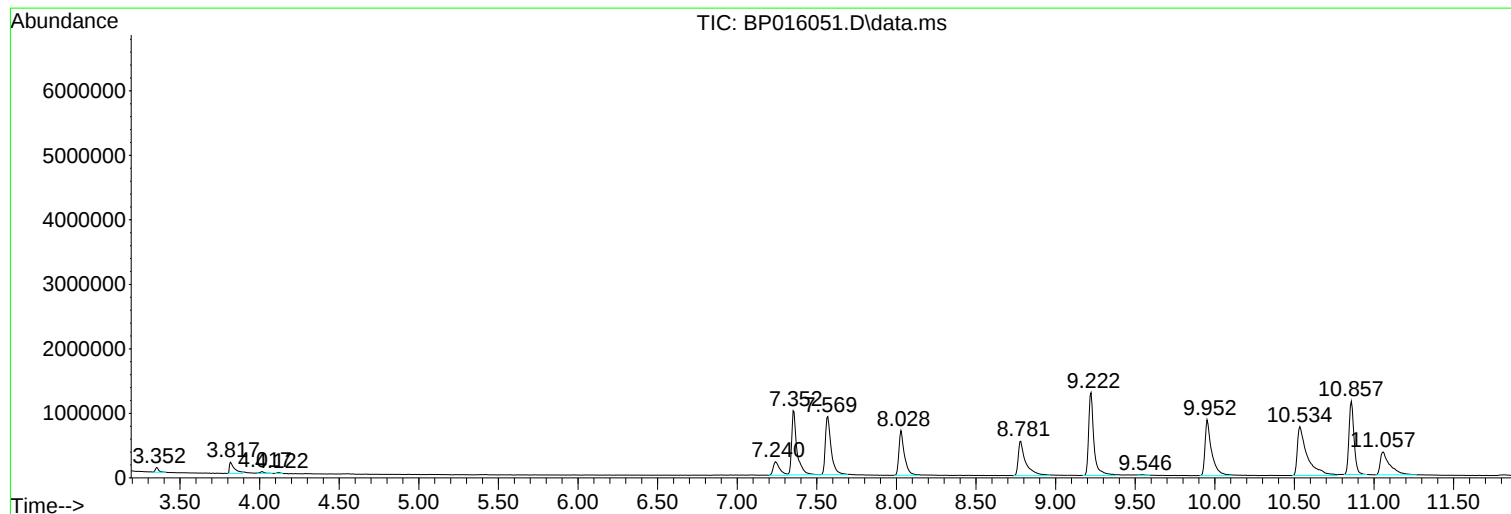

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGZ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016051.D
Acq On : 07 Jul 2023 02:02
Operator : MA/JU
Sample : 03284-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCGZ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------